

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
 Data File : BP019986.D
 Acq On : 25 Mar 2024 18:09
 Operator : MA/JU
 Sample : PB159760BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK760

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019986.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	32	rVB	34704	44128	1.46%	0.150%
2	3.646	91	95	110	rBV	112164	206350	6.84%	0.703%
3	3.934	141	144	152	rVB4	7425	10938	0.36%	0.037%
4	6.805	625	632	649	rBV	431021	803190	26.61%	2.736%
5	6.964	653	659	672	rBV	362811	626290	20.75%	2.133%
6	7.158	684	692	709	rVB	473520	787633	26.09%	2.683%
7	7.616	762	770	783	rBV	401302	699139	23.16%	2.381%
8	8.316	882	889	904	rBV	524369	946462	31.36%	3.224%
9	8.763	957	965	979	rBV	412575	788921	26.14%	2.687%
10	9.463	1076	1084	1101	rBV	352194	667680	22.12%	2.274%
11	9.999	1167	1175	1205	rBV	324878	963233	31.91%	3.281%
12	10.363	1227	1237	1249	rBV	505904	951509	31.52%	3.241%
13	10.546	1260	1268	1281	rBV2	32570	110144	3.65%	0.375%
14	11.999	1506	1515	1522	rVV4	6622	15347	0.51%	0.052%
15	13.122	1698	1706	1714	rBV7	8271	17977	0.60%	0.061%
16	13.663	1788	1798	1820	rBV	744693	1514299	50.17%	5.158%
17	13.922	1835	1842	1857	rBV	1040110	1672020	55.39%	5.695%
18	14.234	1889	1895	1910	rBV	886847	1307546	43.32%	4.454%
19	14.493	1933	1939	1953	rBV	264203	661664	21.92%	2.254%
20	15.263	2062	2070	2081	rBV	1146132	2101545	69.63%	7.158%
21	15.404	2087	2094	2108	rBV	407704	754735	25.00%	2.571%
22	16.081	2204	2209	2214	rBV9	5519	8869	0.29%	0.030%
23	16.745	2317	2322	2325	rVB6	2407	3671	0.12%	0.013%
24	16.857	2339	2341	2346	rVB5	3322	3378	0.11%	0.012%
25	17.069	2368	2377	2386	rBV	915437	1603633	53.13%	5.462%
26	17.175	2388	2395	2409	rVB2	1425483	2349609	77.84%	8.003%
27	19.104	2720	2723	2730	rVB3	20854	31298	1.04%	0.107%
28	19.192	2734	2738	2743	rVB2	11501	18798	0.62%	0.064%
29	19.563	2794	2801	2815	rVB	1542828	2875481	95.27%	9.794%
30	21.539	3130	3137	3148	rBV	1032957	1888153	62.56%	6.431%
31	24.592	3647	3656	3667	rVB	1300822	3018361	100.00%	10.281%
32	24.821	3685	3695	3707	rVB2	633565	1907254	63.19%	6.496%




Sum of corrected areas: 29359255

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019986.D
Acq On : 25 Mar 2024 18:09
Operator : MA/JU
Sample : PB159760BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

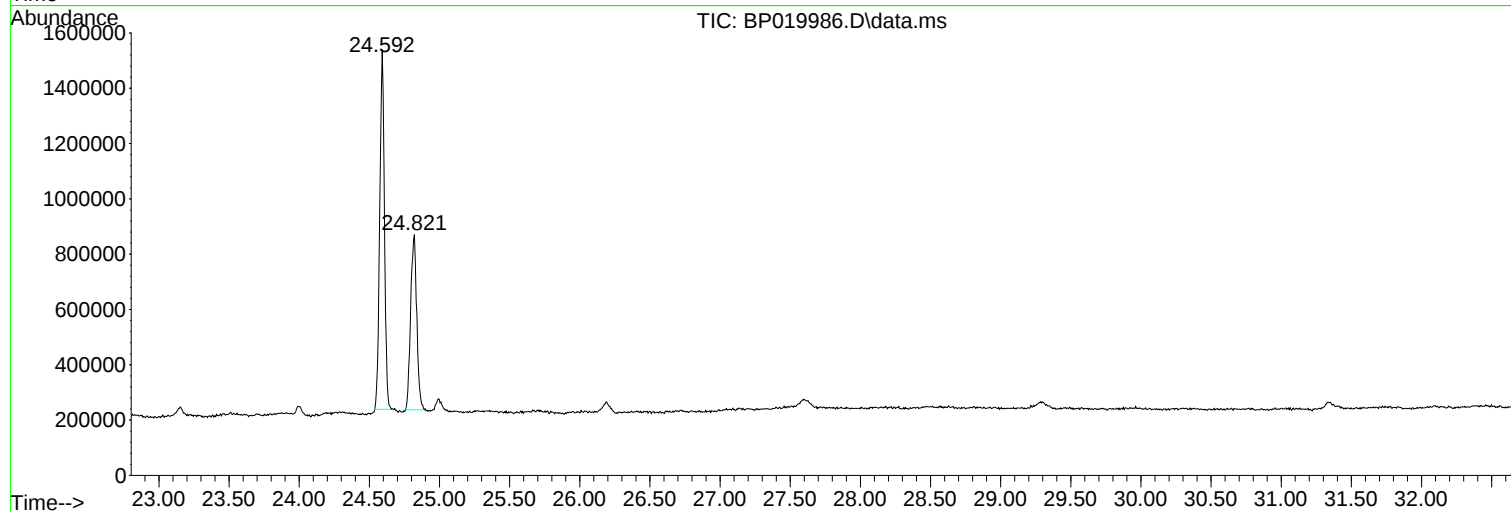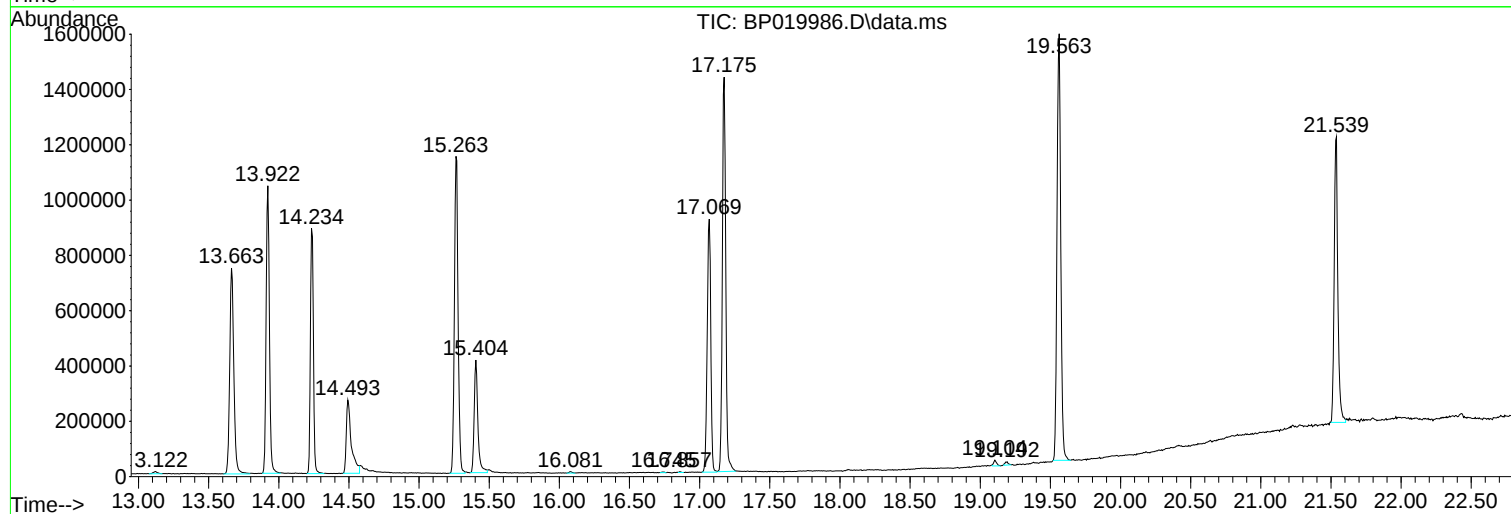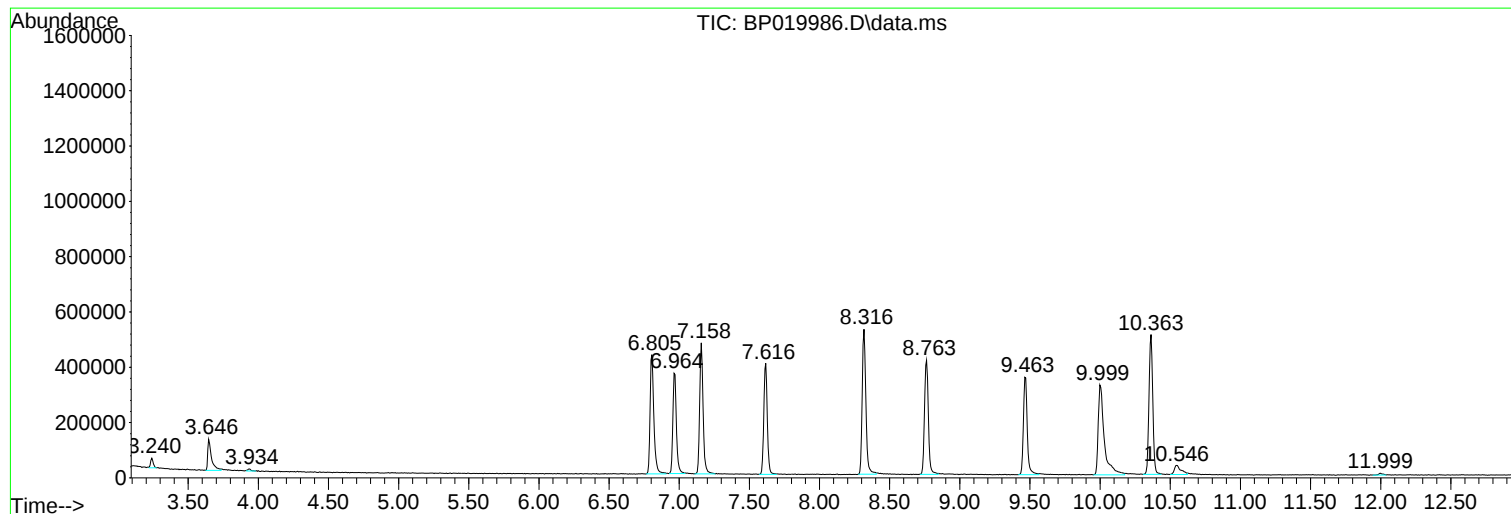

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019986.D
Acq On : 25 Mar 2024 18:09
Operator : MA/JU
Sample : PB159760BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019986.D
Acq On : 25 Mar 2024 18:09
Operator : MA/JU
Sample : PB159760BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK760

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------