
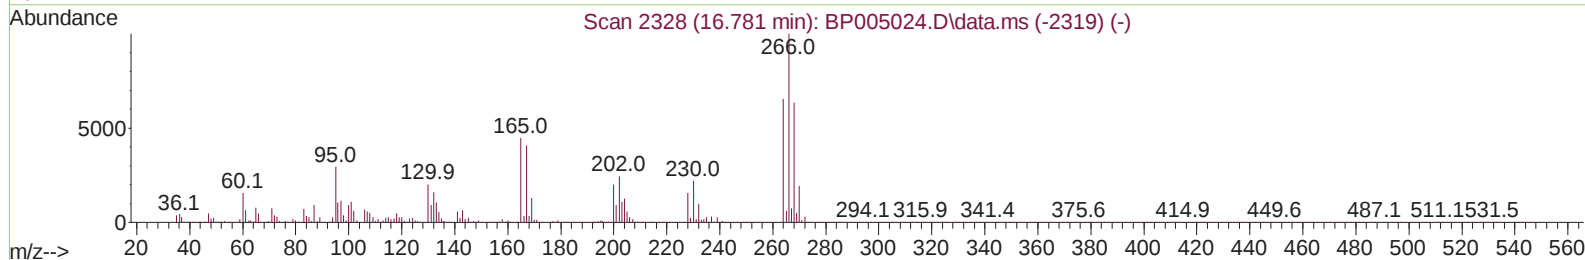
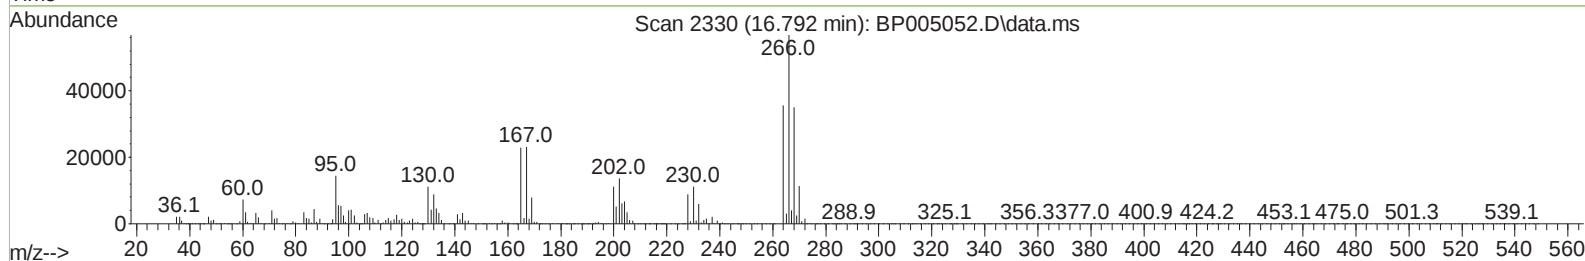


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005052.D
Acq On : 26 Mar 2021 08:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 10:07:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 10:07:03 2021
Response via : Initial Calibration

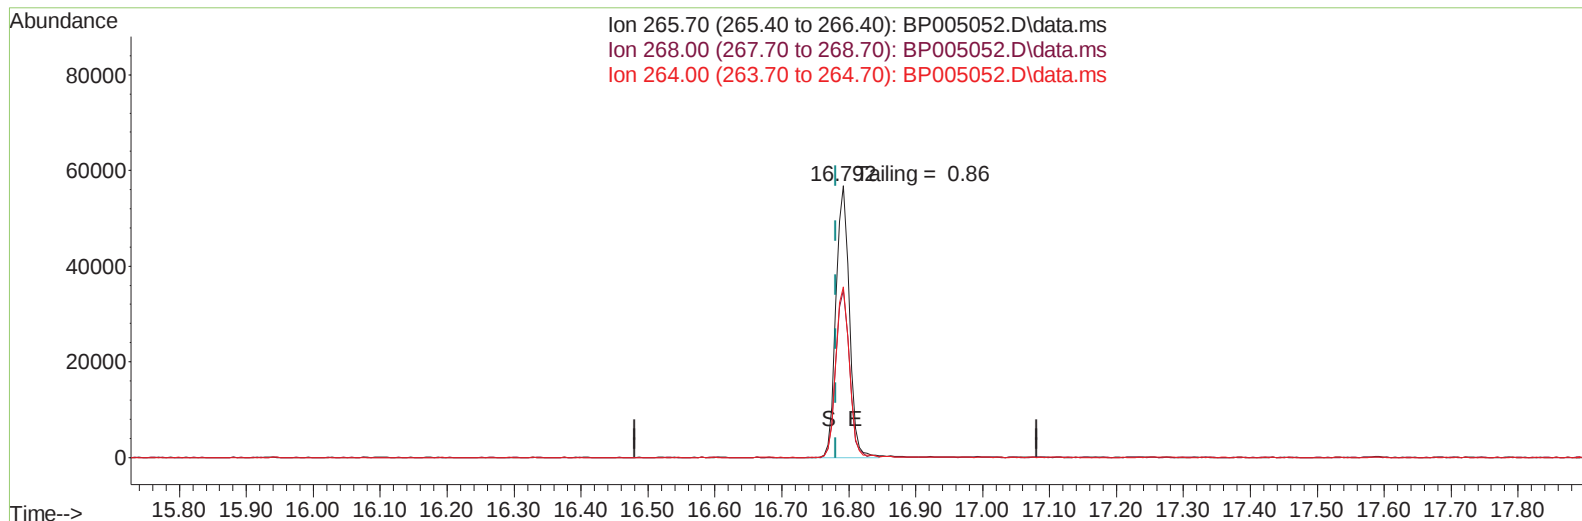

TIC: BP005052.D\data.ms

(70) Pentachlorophenol (C)




16.792min (+ 0.012) 63476.73 ng

response 79182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.56
264.00	63.30	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005052.D
Acq On : 26 Mar 2021 08:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 10:07:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 10:07:03 2021
Response via : Initial Calibration

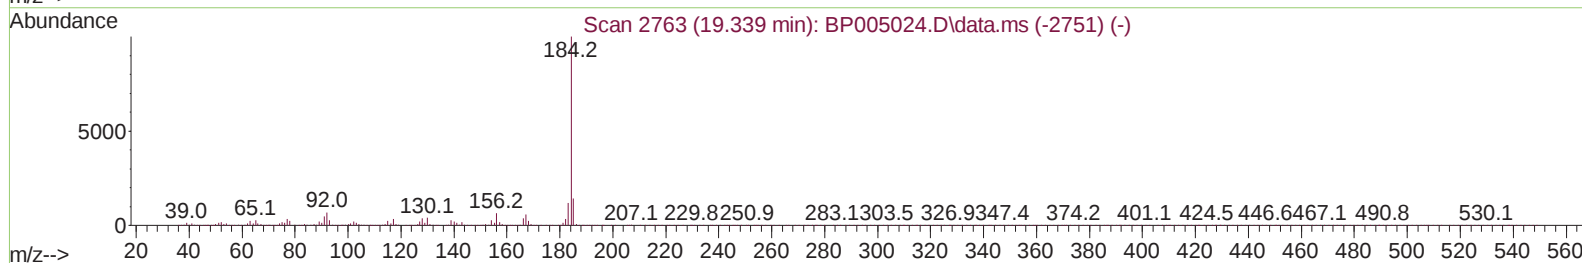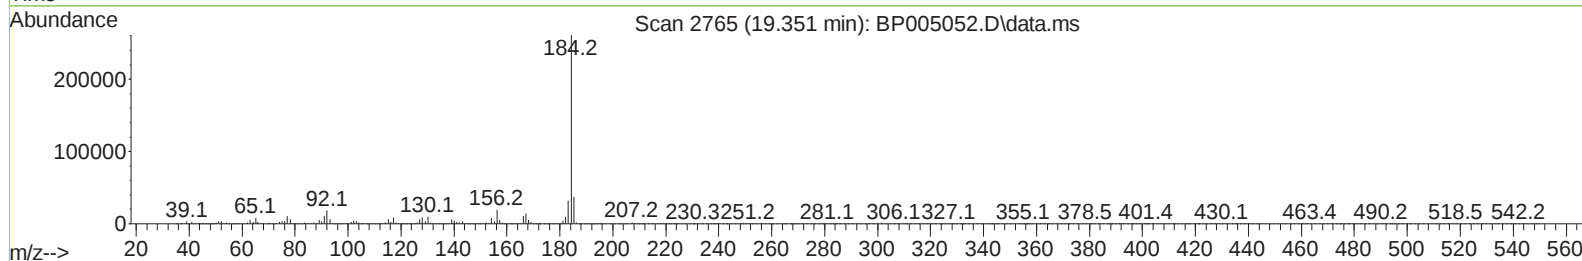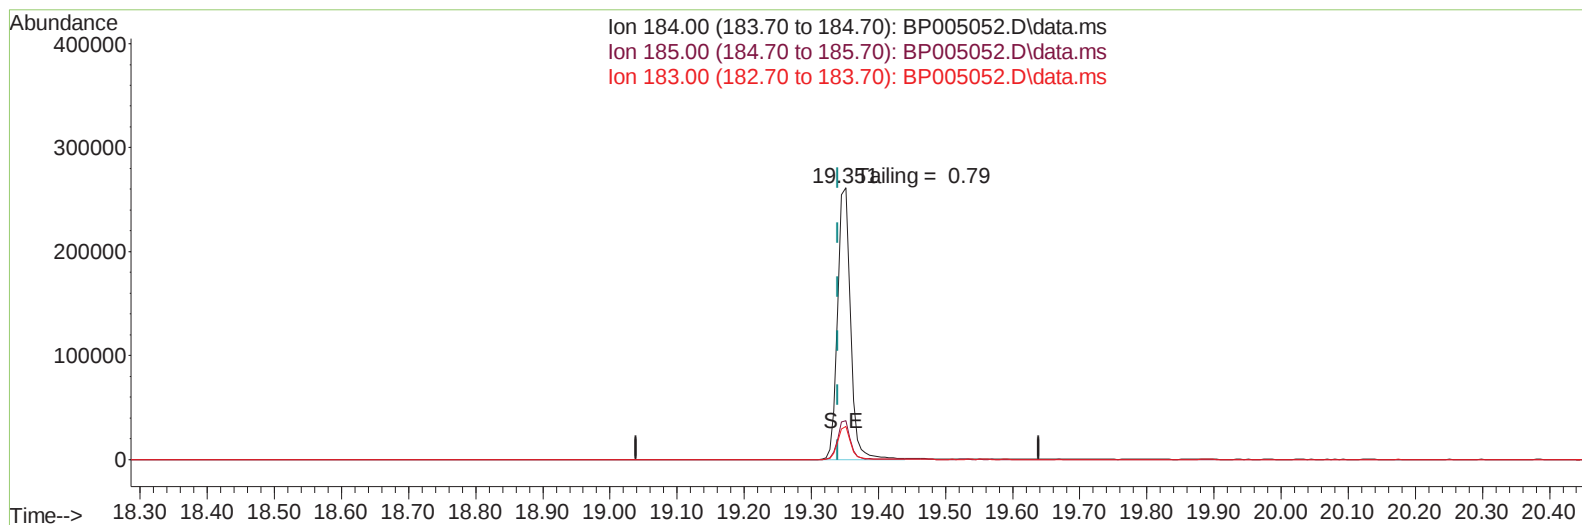

TIC: BP005052.D\data.ms

(77) Benzidine**19.351min (+ 0.012) 2924.17 ng****response 349142**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.36
183.00	12.00	12.20
0.00	0.00	0.00