

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
 Data File : BP005054.D
 Acq On : 26 Mar 2021 09:54
 Operator : CG/JU
 Sample : PB135082BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135082BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.311	372	378	392	rBV	731086	1032663	34.57%	9.194%
2	6.893	639	647	659	rBV	670799	1054661	35.31%	9.390%
3	7.716	780	787	795	rBV	121440	190898	6.39%	1.700%
4	8.875	976	984	999	rBV	412511	677958	22.70%	6.036%
5	10.505	1252	1261	1272	rBV	146059	251764	8.43%	2.242%
6	12.987	1676	1683	1694	rBV	1151854	1676965	56.14%	14.930%
7	14.369	1912	1918	1930	rBV	246577	364695	12.21%	3.247%
8	15.869	2165	2173	2188	rBV	1002133	1411305	47.25%	12.565%
9	17.134	2378	2388	2400	rBV	305324	469637	15.72%	4.181%
10	19.704	2819	2825	2836	rBV	2367869	2986935	100.00%	26.593%
11	21.227	3079	3084	3090	rBV	449427	556328	18.63%	4.953%
12	23.516	3466	3473	3485	rBV	286408	558098	18.68%	4.969%




Sum of corrected areas: 11231907

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005054.D
Acq On : 26 Mar 2021 09:54
Operator : CG/JU
Sample : PB135082BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135082BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

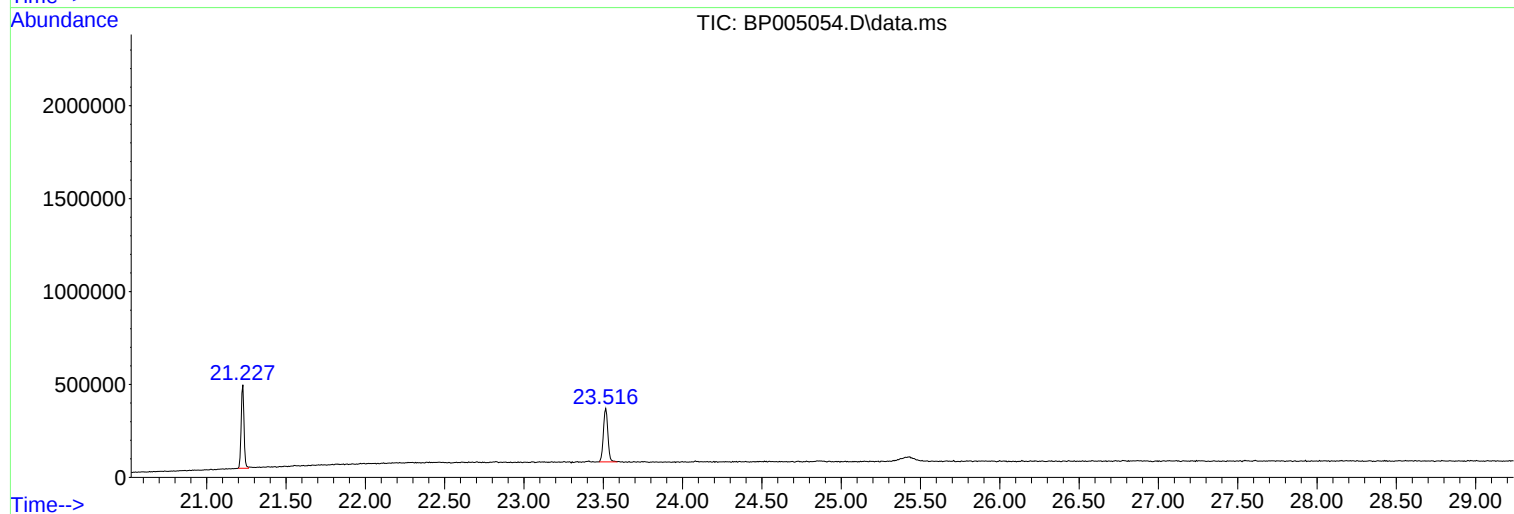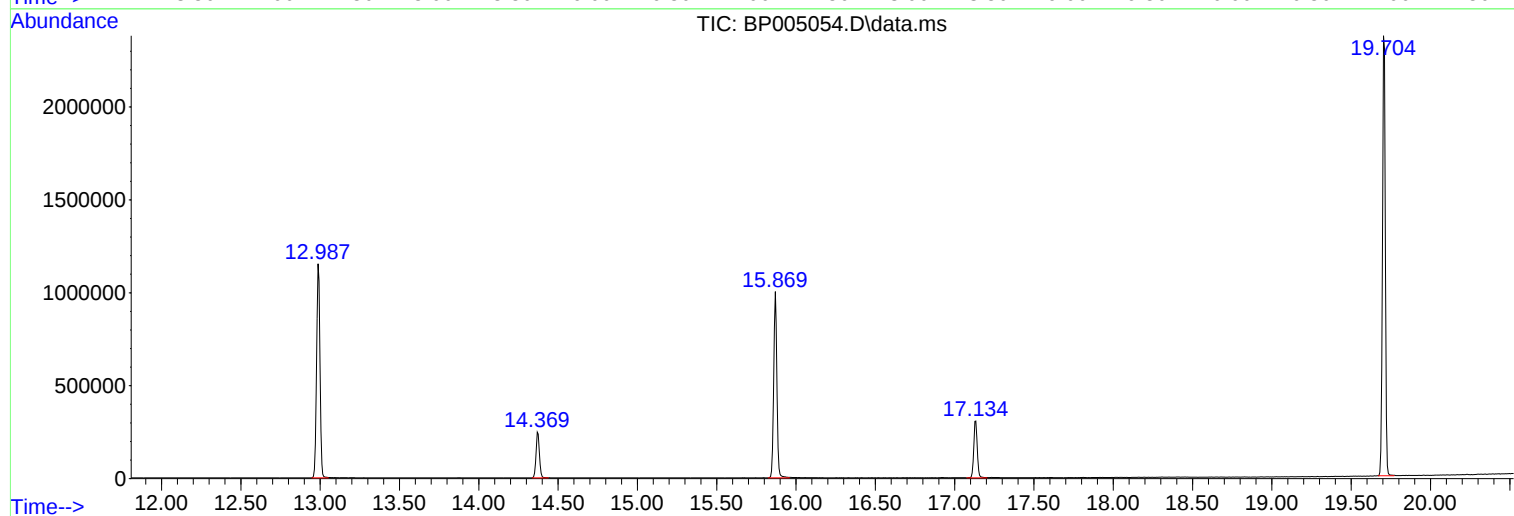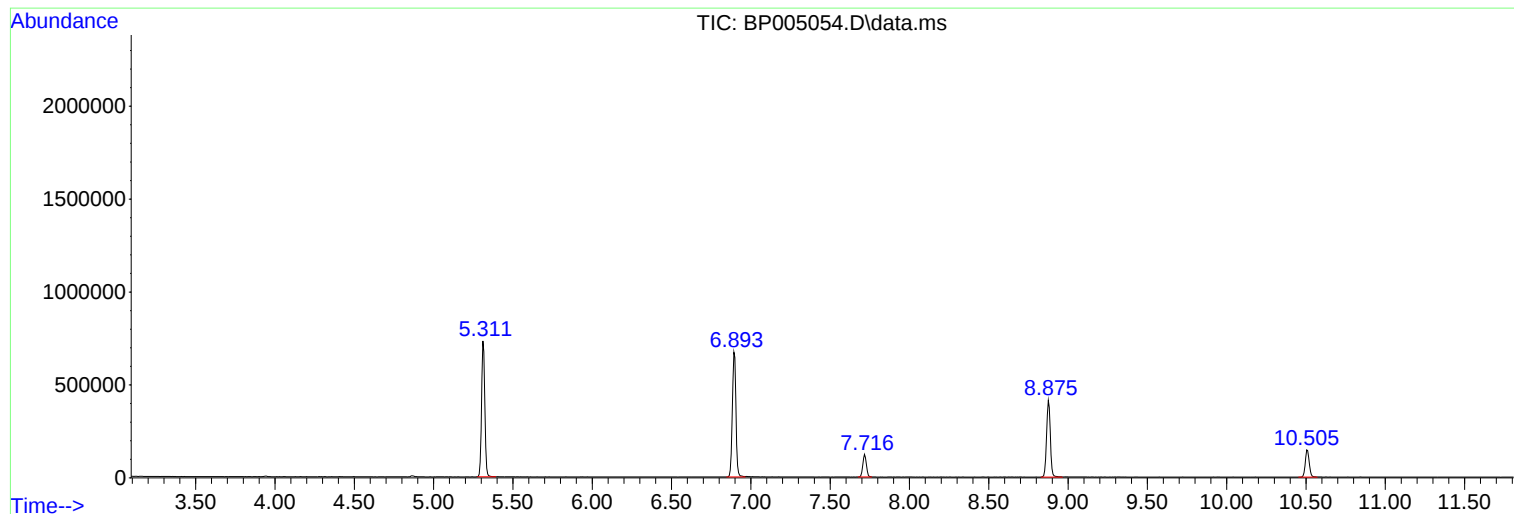

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005054.D
Acq On : 26 Mar 2021 09:54
Operator : CG/JU
Sample : PB135082BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135082BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005054.D
Acq On : 26 Mar 2021 09:54
Operator : CG/JU
Sample : PB135082BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135082BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------