

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
 Data File : BP005055.D
 Acq On : 26 Mar 2021 10:28
 Operator : CG/JU
 Sample : PB135109BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135109BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.311	372	378	389	rBV	702452	1025865	35.31%	9.454%
2	6.893	640	647	662	rBV	655672	1039489	35.78%	9.580%
3	7.717	780	787	796	rBV	121060	188834	6.50%	1.740%
4	8.875	975	984	1003	rBV	413211	667721	22.98%	6.154%
5	10.510	1254	1262	1274	rBV	140847	246544	8.49%	2.272%
6	12.987	1676	1683	1695	rBV	1097487	1580362	54.39%	14.564%
7	14.369	1910	1918	1930	rBV	223109	338919	11.66%	3.123%
8	15.869	2166	2173	2189	rBV	965779	1350214	46.47%	12.443%
9	17.128	2381	2387	2397	rBV	297280	433389	14.92%	3.994%
10	19.704	2819	2825	2838	rBV	2464058	2905490	100.00%	26.777%
11	21.228	3078	3084	3094	rBV	412376	537528	18.50%	4.954%
12	23.516	3466	3473	3486	rBV2	281741	536497	18.46%	4.944%




Sum of corrected areas: 10850852

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005055.D
Acq On : 26 Mar 2021 10:28
Operator : CG/JU
Sample : PB135109BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135109BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

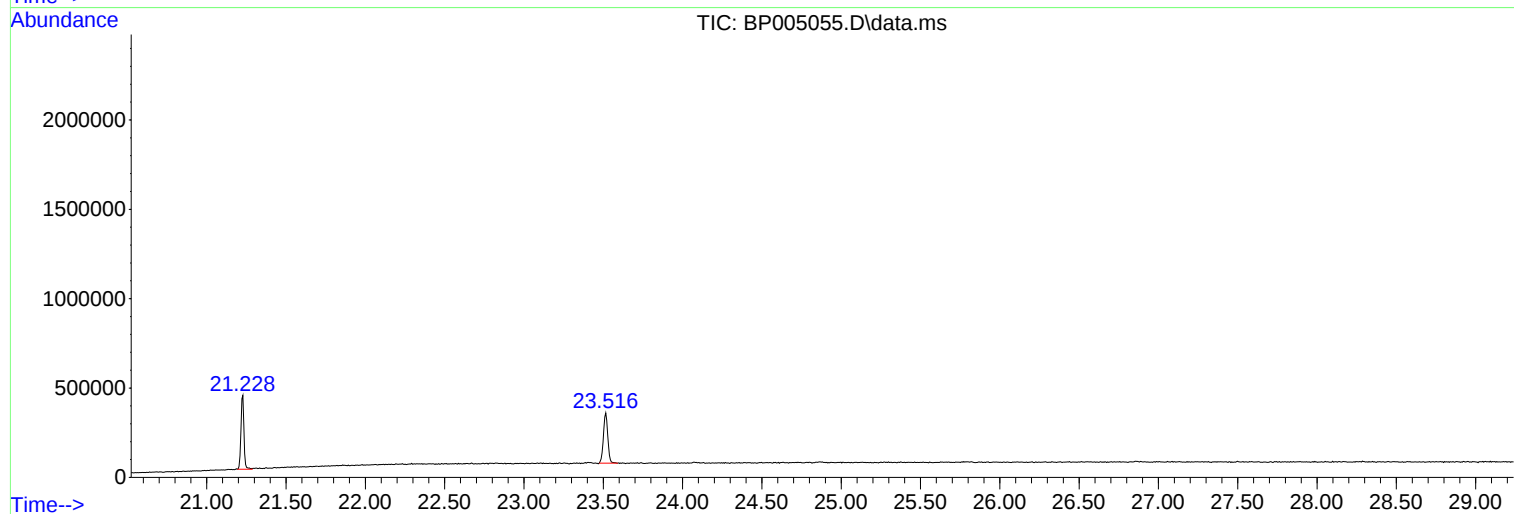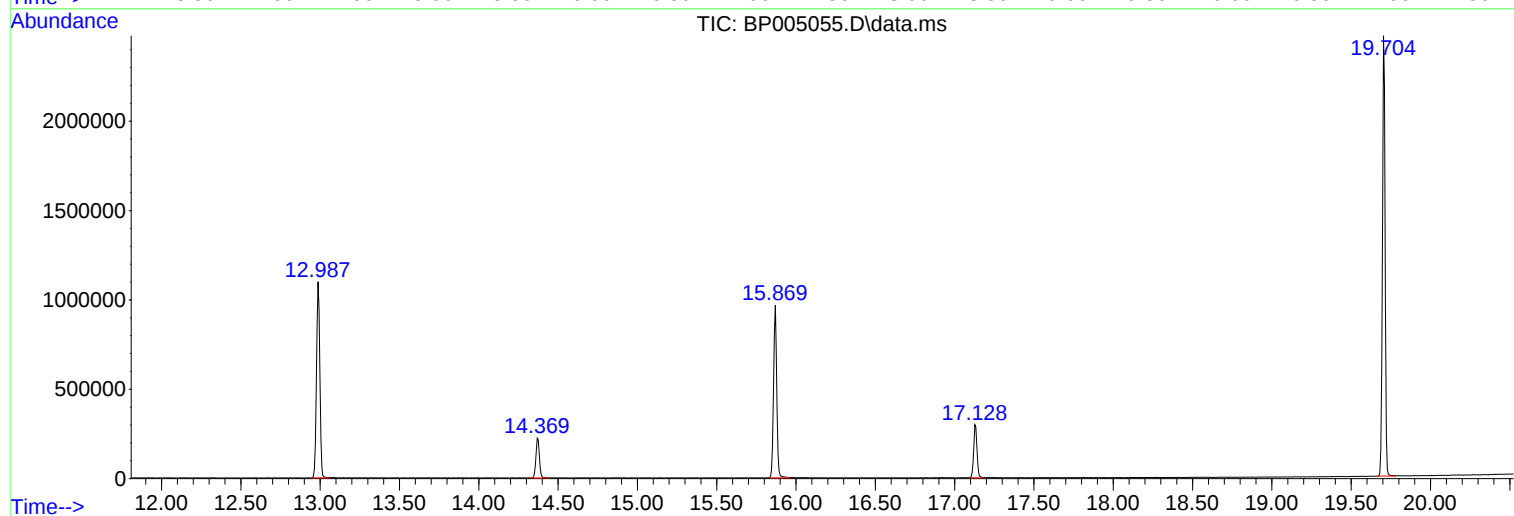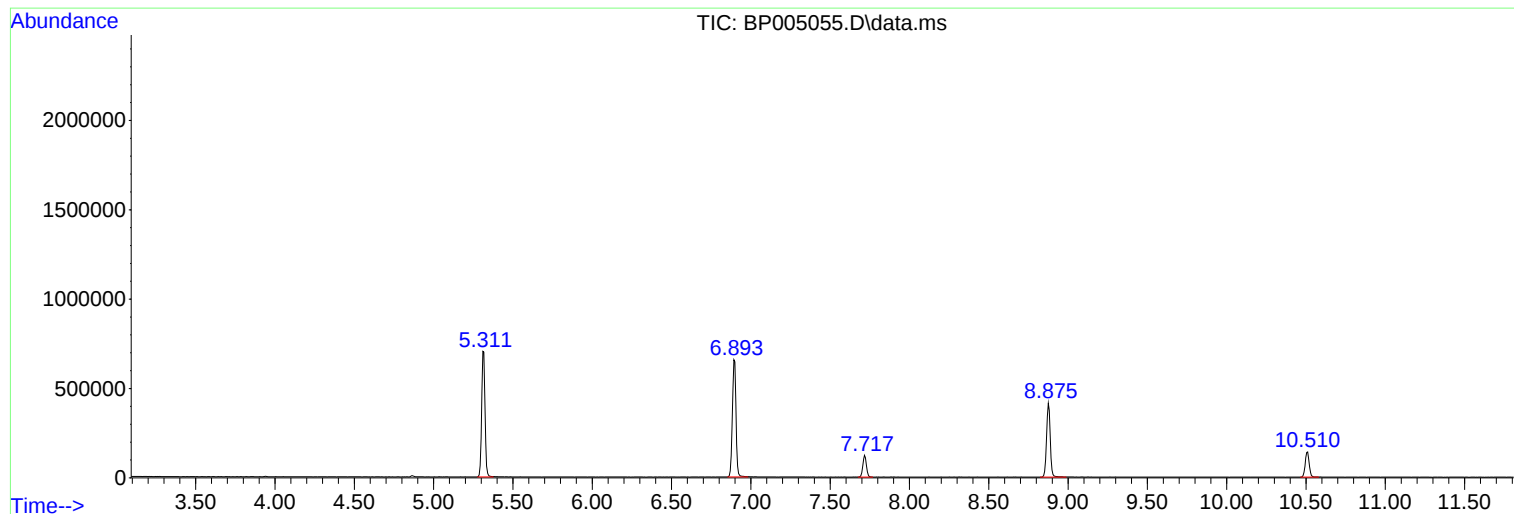

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005055.D
Acq On : 26 Mar 2021 10:28
Operator : CG/JU
Sample : PB135109BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135109BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005055.D
Acq On : 26 Mar 2021 10:28
Operator : CG/JU
Sample : PB135109BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135109BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------