
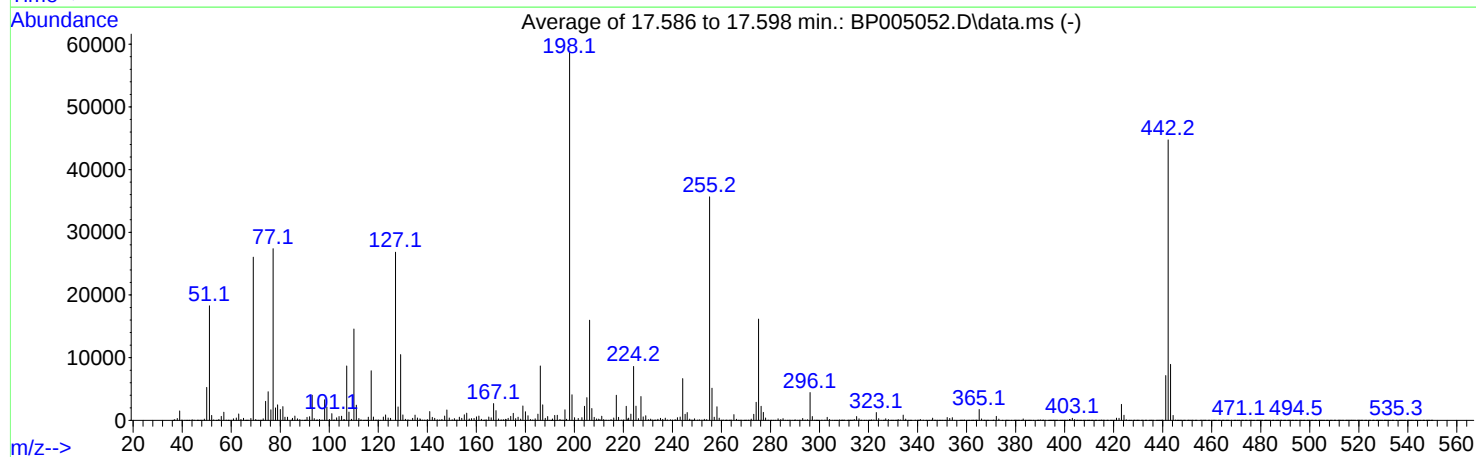


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
 Data File : BP005052.D
 Acq On : 26 Mar 2021 08:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 26 10:07:03 2021

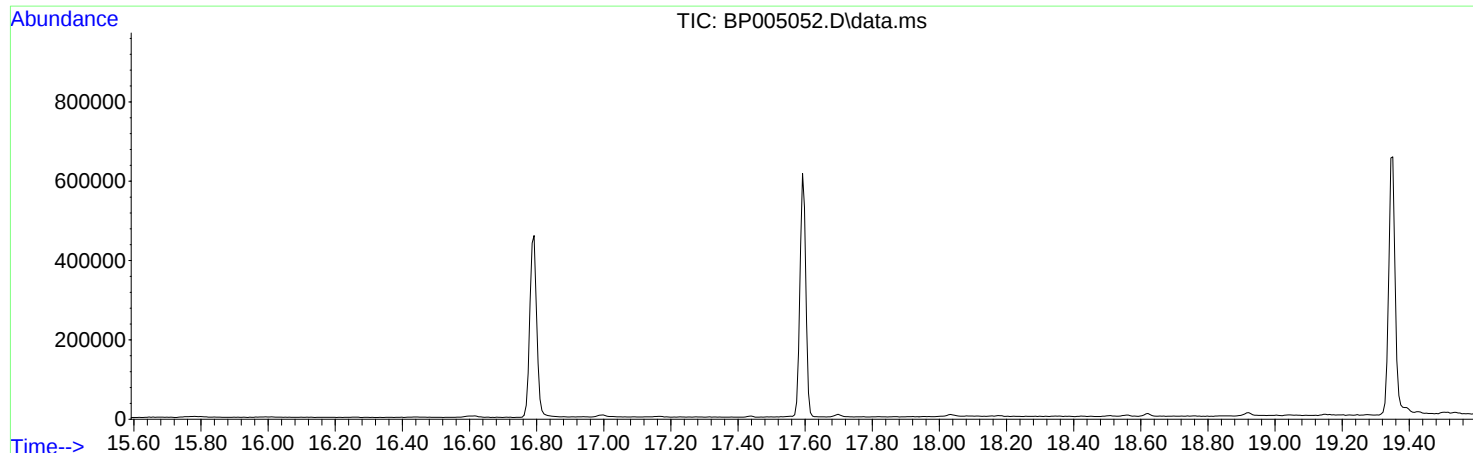




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	18269	PASS
68	69	0.00	2	1.2	313	PASS
69	198	0.00	100	44.4	26027	PASS
70	69	0.00	2	0.5	140	PASS
127	198	10	80	45.7	26837	PASS
197	198	0.00	2	0.3	176	PASS
198	198	100	100	100.0	58677	PASS
199	198	5	9	7.0	4084	PASS
275	198	10	60	27.5	16145	PASS
365	198	1	100	3.0	1734	PASS
441	198	0.01	100	12.2	7147	PASS
442	442	100	100	100.0	44733	PASS
443	442	15	24	20.0	8934	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005052.D
Acq On : 26 Mar 2021 08:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 26 10:07:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 10:07:03 2021
Response via : Initial Calibration

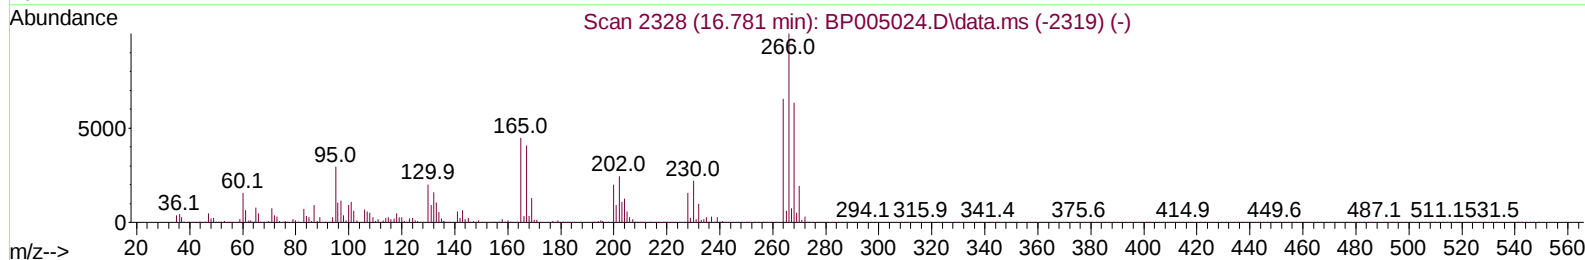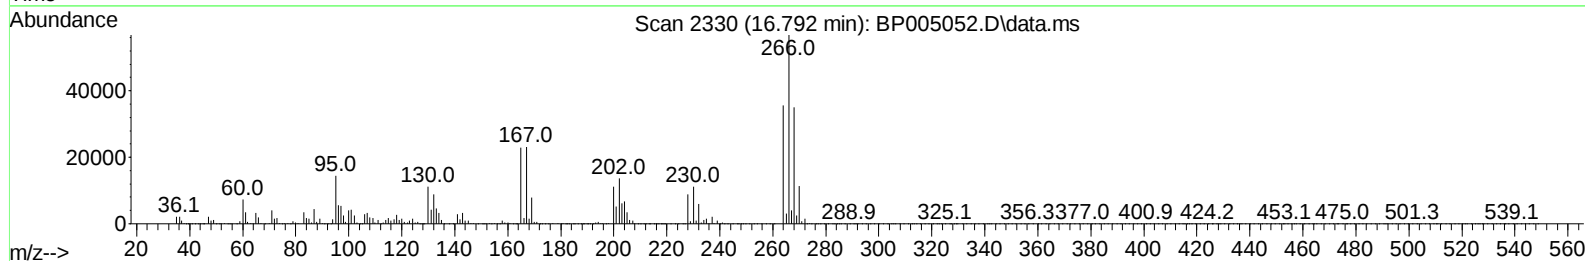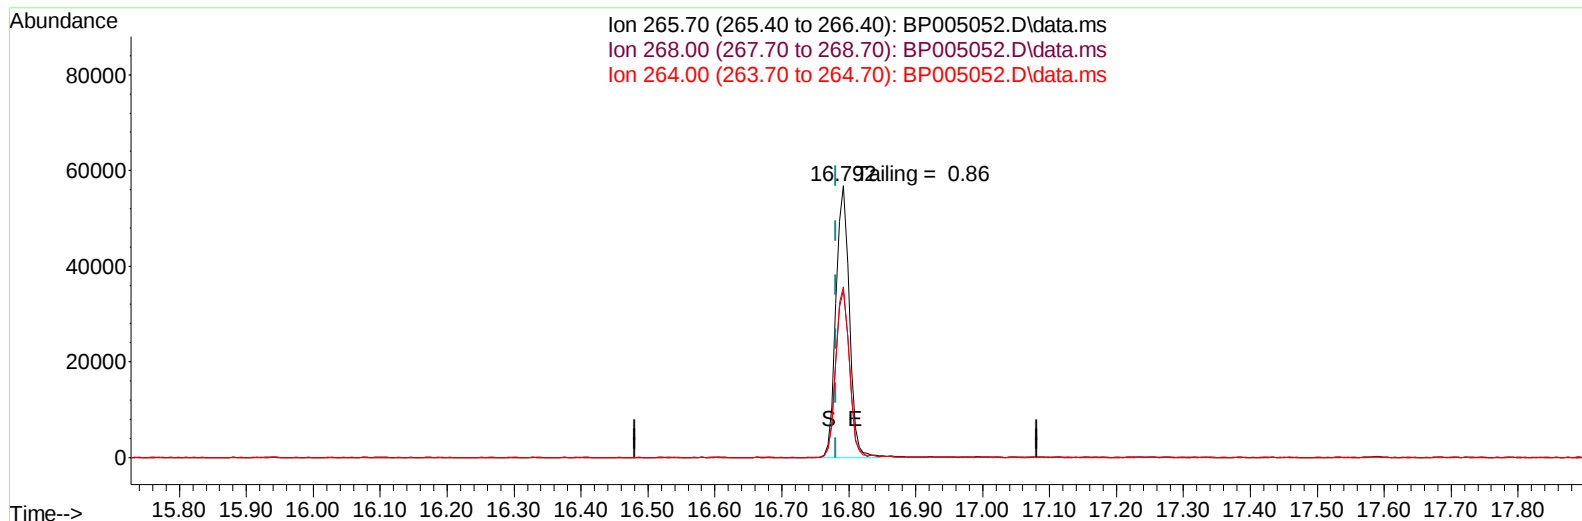

TIC: BP005052.D\data.ms

(70) Pentachlorophenol (C)

16.792min (+ 0.012) 63476.73 ng




response 79182

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	61.56
264.00	63.30	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032621\
Data File : BP005052.D
Acq On : 26 Mar 2021 08:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 26 10:07:52 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 10:07:03 2021
Response via : Initial Calibration

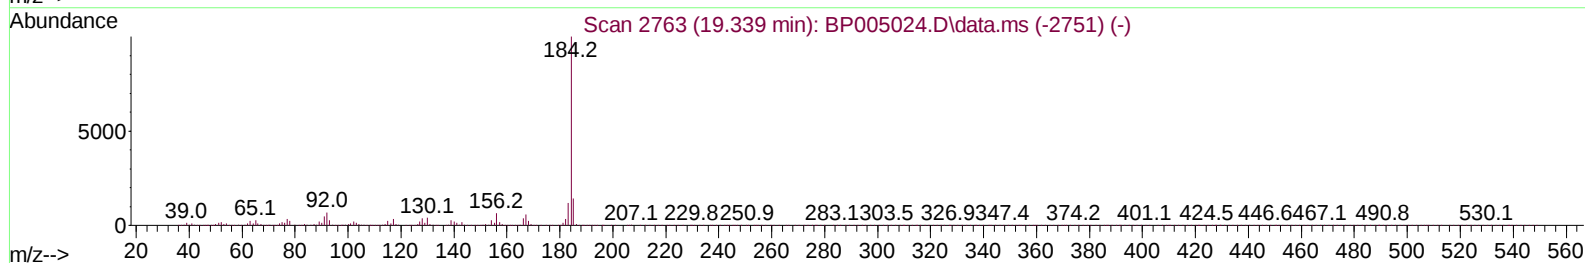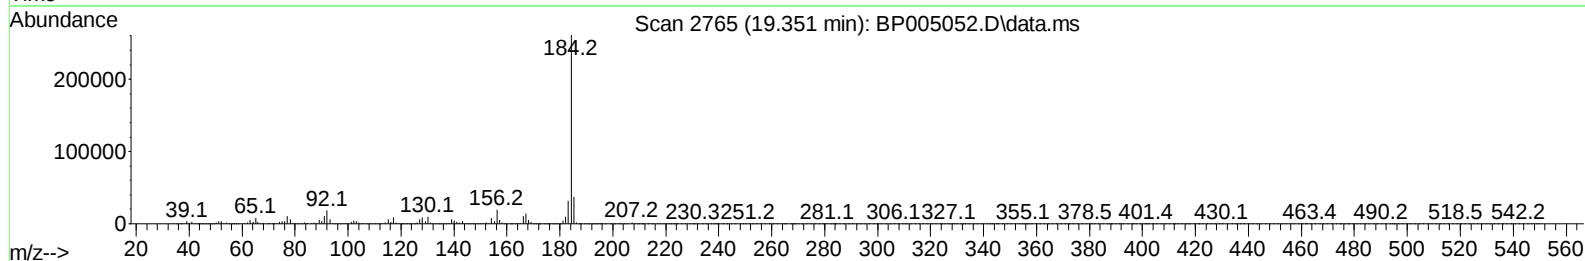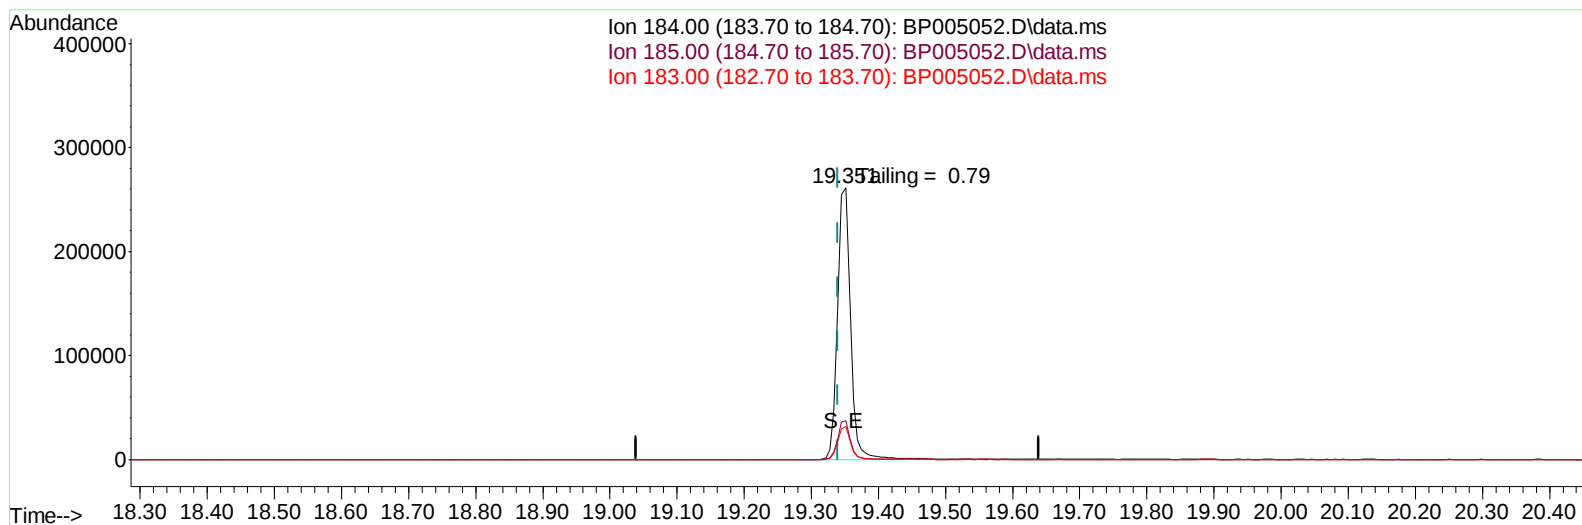

TIC: BP005052.D\data.ms

(77) Benzidine

19.351min (+ 0.012) 2924.17 ng

response 349142

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.36
183.00	12.00	12.20
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/26/2021	BNA_P	BP005052.D
Compound Name	Response	Retention Time
DDT	213012	20.551
DDD	3169	20.116
DDE	873	19.627
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4042	217054	1.86

Instrument :
BNA_P
ClientSampleId :
DFTPP