




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020001.D
Acq On : 26 Mar 2024 17:42
Operator : MA/JU
Sample : P1848-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOLY4

Manual IntegrationsAPPROVED

Quant Time: Mar 26 18:19:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :mohammad ahmed 03/29/2024

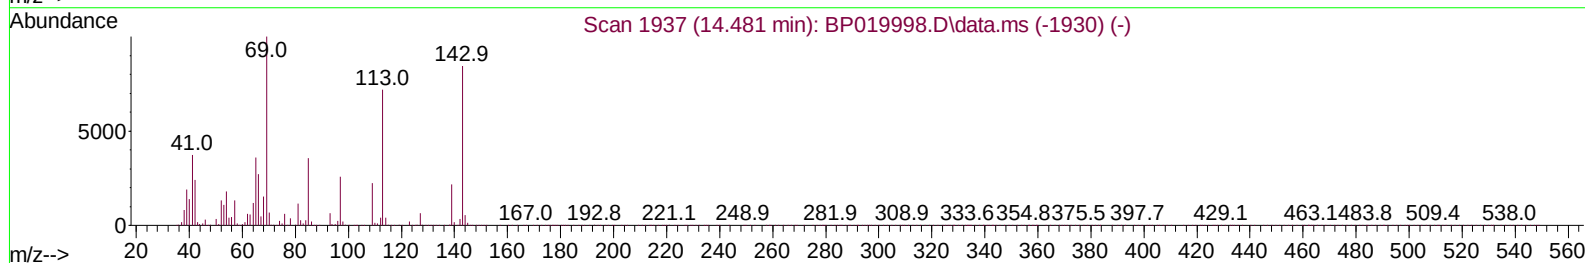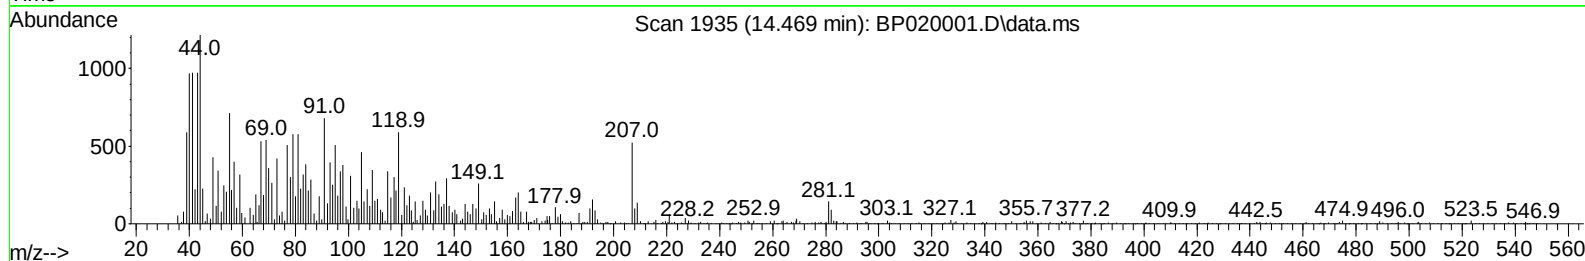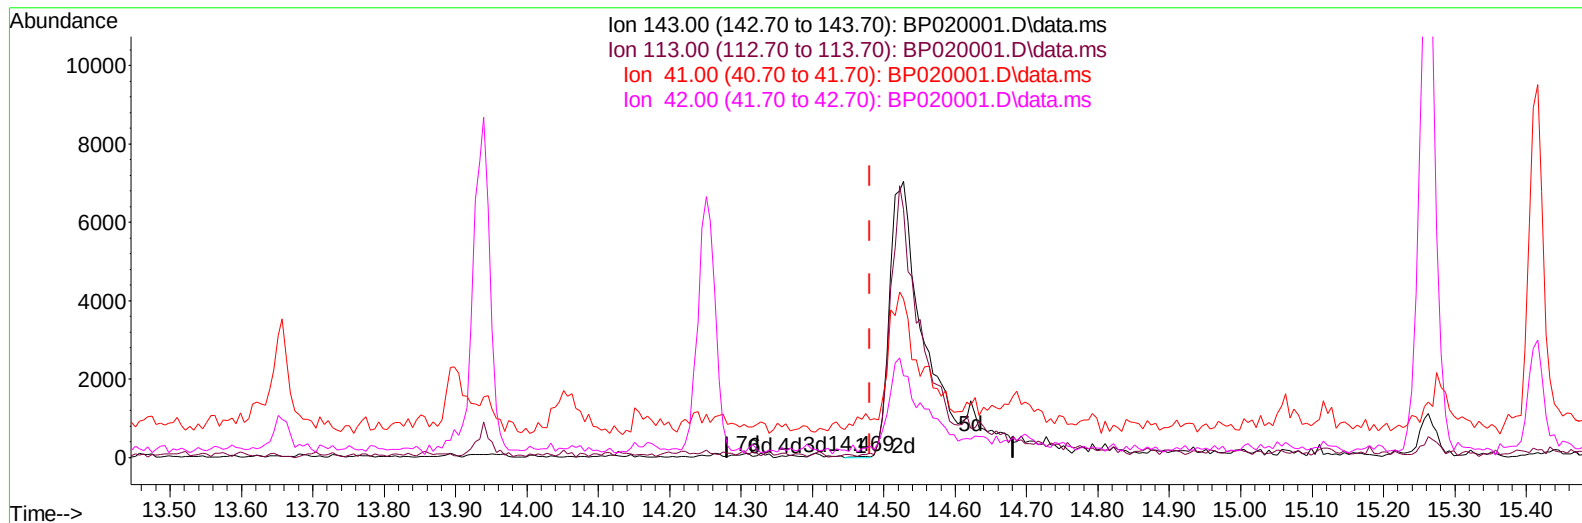

TIC: BP020001.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.469min (-0.012) 0.01 ng/u1

response 37

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	214.71#
41.00	40.90	2858.82#
42.00	28.50	650.00#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020001.D
Acq On : 26 Mar 2024 17:42
Operator : MA/JU
Sample : P1848-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY4

Manual IntegrationsAPPROVED

Quant Time: Mar 26 18:20:38 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :mohammad ahmed 03/29/2024

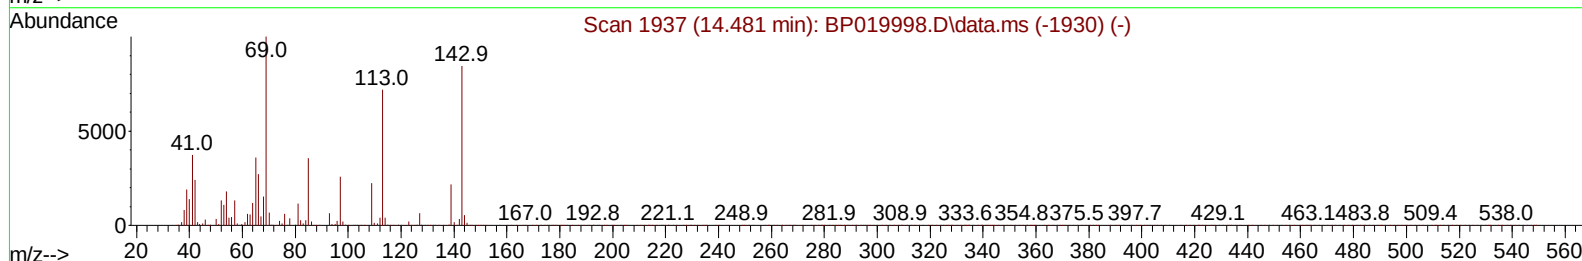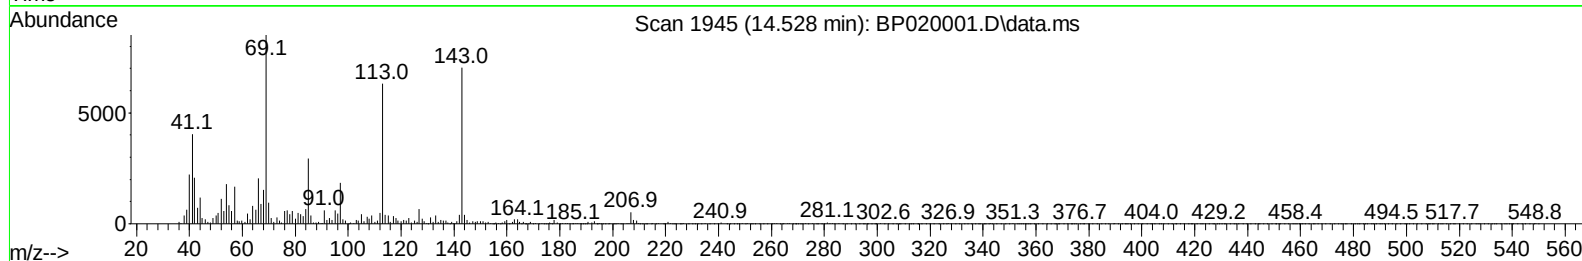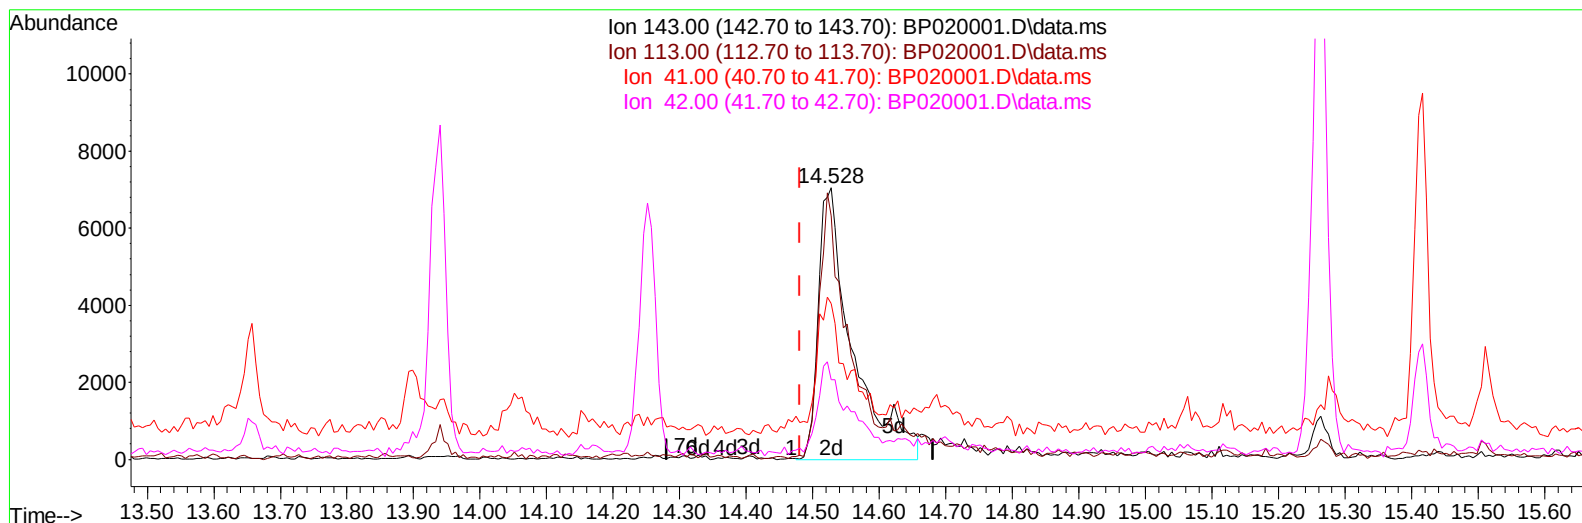

TIC: BP020001.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.047) 6.87 ng/ul m

response 25224

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	89.71
41.00	40.90	57.42#
42.00	28.50	29.48

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP020001.D
 Acq On : 26 Mar 2024 17:42
 Operator : MA/JU
 Sample : P1848-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY4

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/29/2024
 Supervised By :mohammad ahmed 03/29/2024

Quant Time: Mar 27 00:04:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 10:46:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.610	152	119026	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	508248	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.251	164	333245	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.063	188	631428	20.000	ng/ul	-0.01
79) Chrysene-d12	21.539	240	450329	20.000	ng/ul	0.00
88) Perylene-d12	24.810	264	487242	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	16079	5.919	ng/uL	0.00
4) Pyridine-d5	3.640	84	138297	16.860	ng/ul	0.00
7) Phenol-d5	6.805	99	83503	8.318	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.975	67	248866	38.052	ng/ul	0.00
11) 2-Chlorophenol-d4	7.152	132	207576	28.793	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113	160549	20.672	ng/ul	0.00
21) Nitrobenzene-d5	8.769	128	141869	36.418	ng/ul	0.01
24) 2-Nitrophenol-d4	9.475	143	152842	35.066	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.999	165	270918	34.034	ng/ul	0.00
31) 4-Chloroaniline-d4	10.516	131	651713	62.803	ng/ul	0.00
46) Dimethylphthalate-d6	13.657	166	1003962	42.969	ng/ul	0.00
49) Acenaphthylene-d8	13.939	160	1082487	39.661	ng/ul	0.00
54) 4-Nitrophenol-d4	14.528	143	25224m	6.867	ng/ul	0.05
60) Fluorene-d10	15.263	176	821116	41.255	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	143260	37.903	ng/ul	0.00
73) Anthracene-d10	17.169	188	1217960	43.575	ng/ul	0.00
81) Pyrene-d10	19.563	212	1254769	47.491	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.586	264	1089898	46.561	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020001.D
Acq On : 26 Mar 2024 17:42
Operator : MA/JU
Sample : P1848-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOLY4

Manual IntegrationsAPPROVED

Quant Time: Mar 27 00:04:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :mohammad ahmed 03/29/2024

