




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP020005.D
 Acq On : 26 Mar 2024 20:35
 Operator : MA/JU
 Sample : P1848-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY7

Manual IntegrationsAPPROVED

Quant Time: Mar 26 23:28:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 10:46:59 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
 Supervised By :mohammad ahmed 03/29/2024

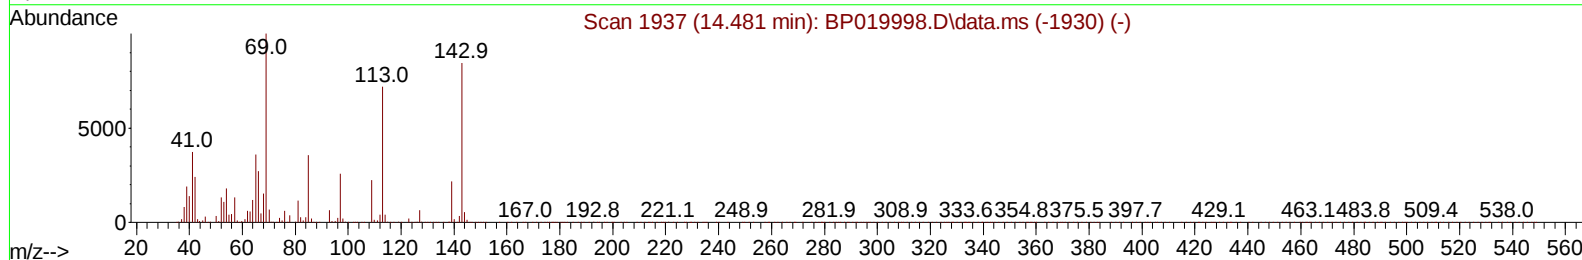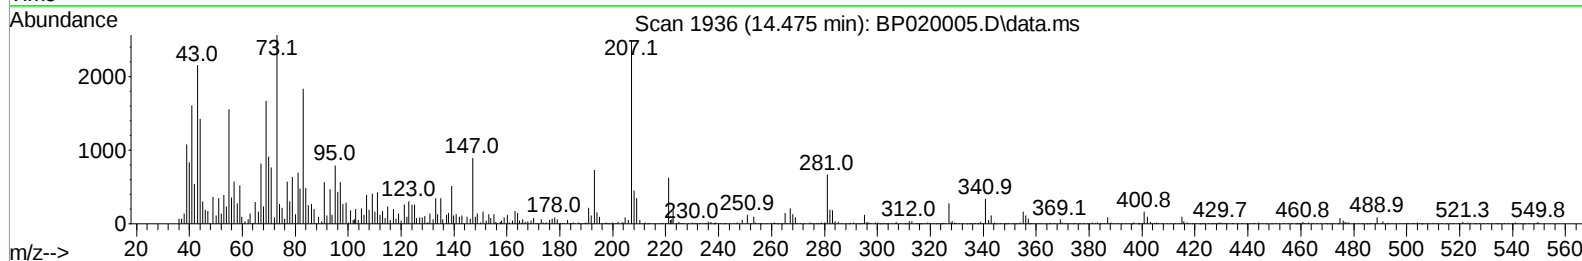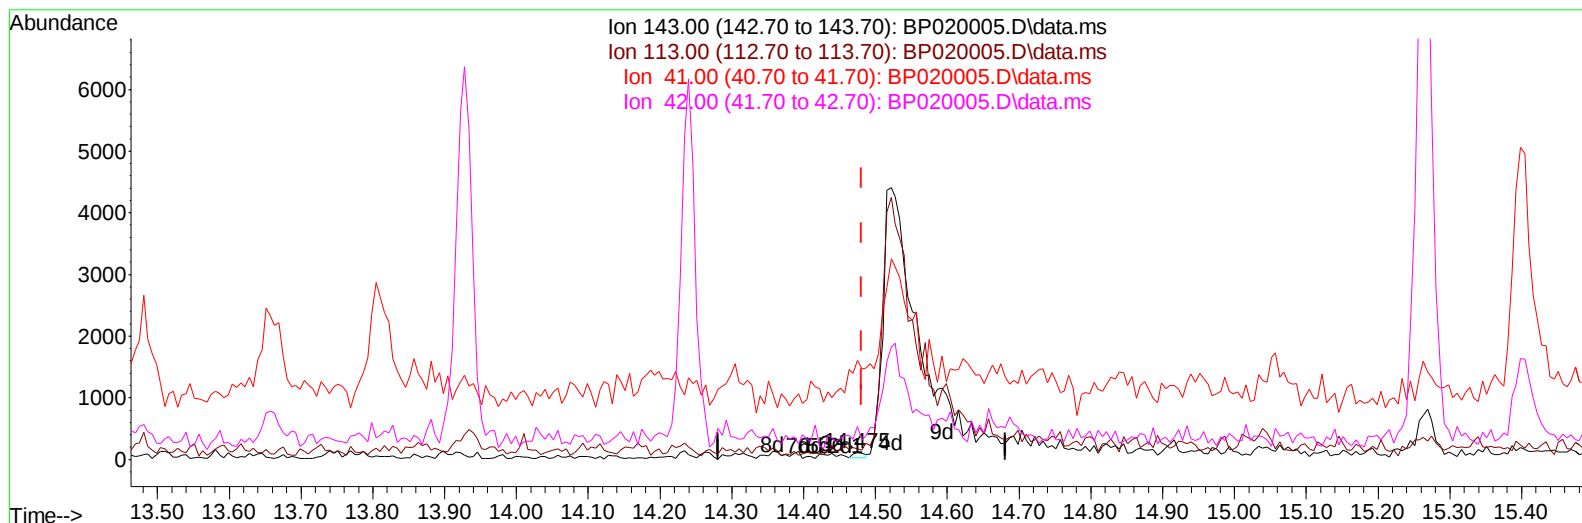

TIC: BP020005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.475min (-0.006) 0.03 ng/u1

response 91

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	153.91#
41.00	40.90	1393.04#
42.00	28.50	466.09#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020005.D
Acq On : 26 Mar 2024 20:35
Operator : MA/JU
Sample : P1848-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY7

Manual IntegrationsAPPROVED

Quant Time: Mar 26 23:28:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :mohammad ahmed 03/29/2024

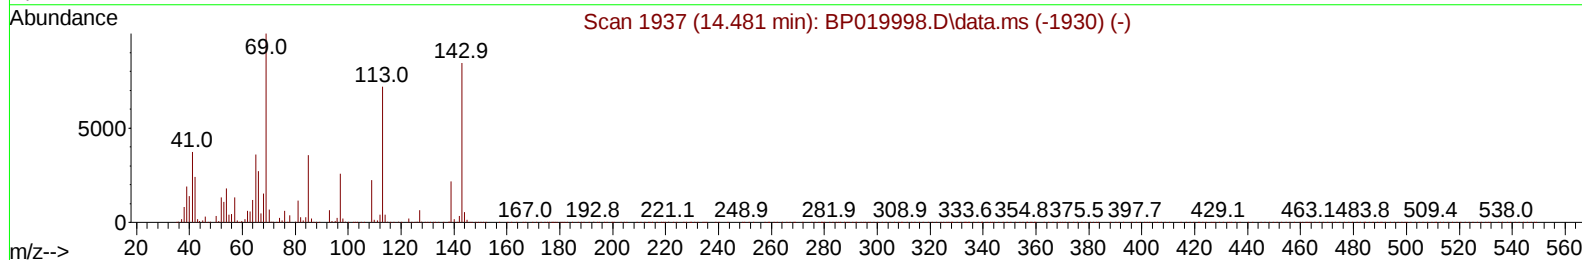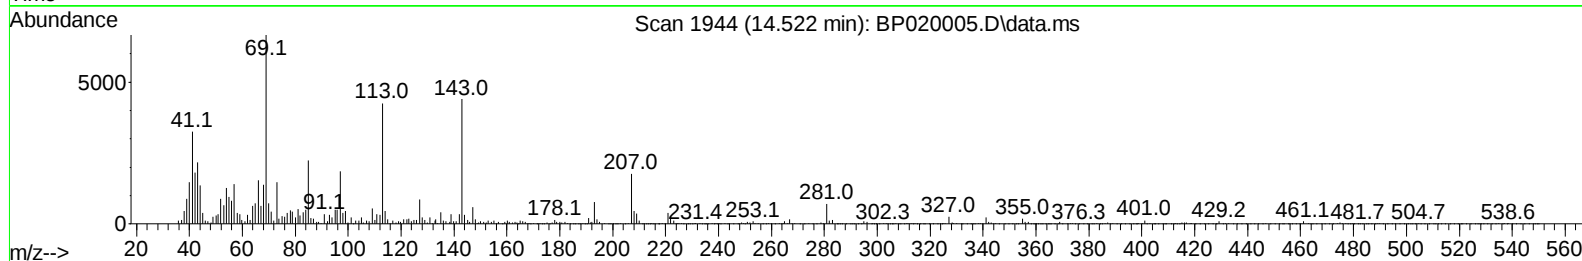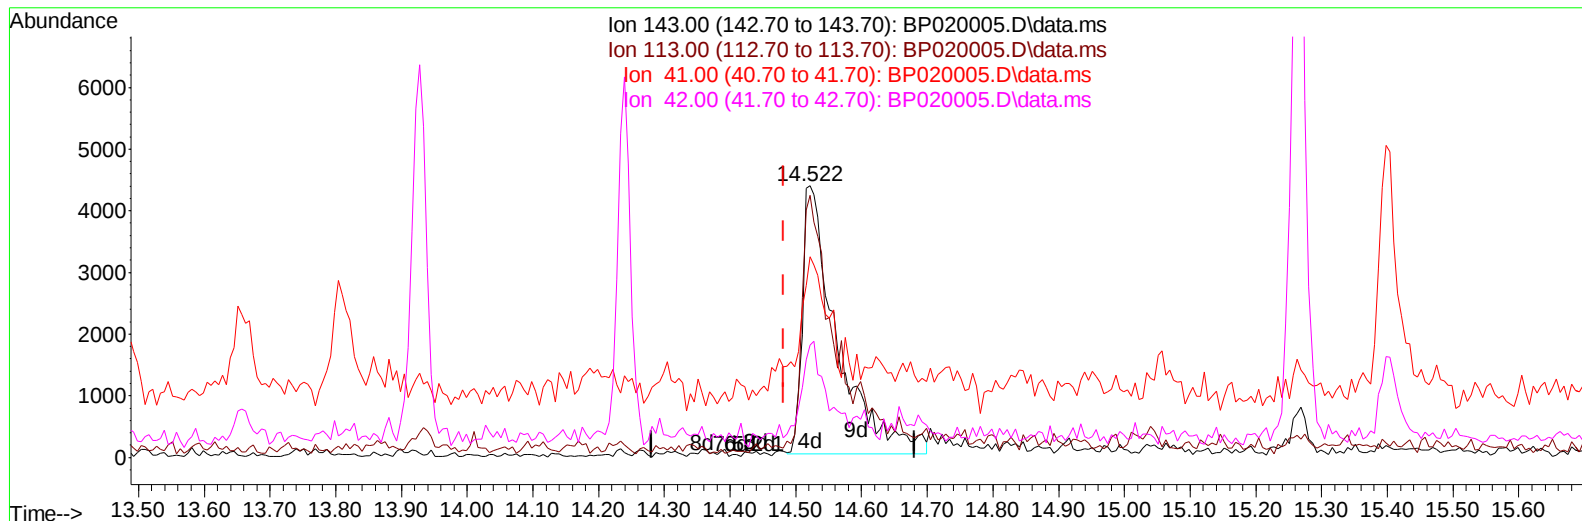

TIC: BP020005.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.041) 6.08 ng/ul m

response 15970

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	96.64
41.00	40.90	74.02#
42.00	28.50	41.31#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP020005.D
 Acq On : 26 Mar 2024 20:35
 Operator : MA/JU
 Sample : P1848-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY7

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/29/2024
 Supervised By :mohammad ahmed 03/29/2024

Quant Time: Mar 26 23:41:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 10:46:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	90388	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	381058	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.240	164	238383	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.063	188	433684	20.000	ng/ul	-0.01
79) Chrysene-d12	21.527	240	331272	20.000	ng/ul	-0.02
88) Perylene-d12	24.804	264	360007	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.240	96	12242	5.934	ng/uL	0.00
4) Pyridine-d5	3.646	84	63087	10.128	ng/ul	0.00
7) Phenol-d5	6.811	99	63164	8.286	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.969	67	194818	39.225	ng/ul	0.00
11) 2-Chlorophenol-d4	7.164	132	162791	29.735	ng/ul	0.01
15) 4-Methylphenol-d8	8.316	113	118795	20.142	ng/ul	0.01
21) Nitrobenzene-d5	8.763	128	108793	37.249	ng/ul	0.00
24) 2-Nitrophenol-d4	9.463	143	120569	36.895	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.005	165	198385	33.241	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	312436	40.158	ng/ul	0.00
46) Dimethylphthalate-d6	13.657	166	673987	40.326	ng/ul	0.00
49) Acenaphthylene-d8	13.928	160	759914	38.922	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	15970m	6.078	ng/ul	0.04
60) Fluorene-d10	15.263	176	559854	39.322	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.398	200	83221	32.058	ng/ul	-0.02
73) Anthracene-d10	17.181	188	814746	42.440	ng/ul	0.01
81) Pyrene-d10	19.563	212	873817	44.958	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.574	264	778716	45.024	ng/ul	-0.04

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020005.D
Acq On : 26 Mar 2024 20:35
Operator : MA/JU
Sample : P1848-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY7

Manual IntegrationsAPPROVED

Quant Time: Mar 26 23:41:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :mohammad ahmed 03/29/2024

