

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP019992.D
 Acq On : 26 Mar 2024 10:24
 Operator : MA/JU
 Sample : PB159439BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK439

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	35	rVB	47897	64452	1.92%	0.164%
2	3.640	91	94	116	rBV	558315	887855	26.52%	2.257%
3	3.940	141	145	151	rBV3	9201	14103	0.42%	0.036%
4	3.999	153	155	160	rVB6	3314	3989	0.12%	0.010%
5	4.146	177	180	187	rVB4	6918	11160	0.33%	0.028%
6	6.346	551	554	558	rBV6	2096	3805	0.11%	0.010%
7	6.811	625	633	651	rBV	657276	1162974	34.73%	2.956%
8	6.975	654	661	676	rVB	560512	928274	27.72%	2.360%
9	7.164	685	693	708	rBV	639488	1128569	33.71%	2.869%
10	7.622	761	771	783	rBV	530293	876766	26.19%	2.229%
11	8.322	881	890	907	rBV	709925	1426335	42.60%	3.626%
12	8.764	958	965	980	rBV	686973	1204697	35.98%	3.062%
13	9.475	1078	1086	1100	rBV	589042	1030318	30.77%	2.619%
14	9.999	1167	1175	1207	rBV	673728	1472123	43.97%	3.742%
15	10.363	1229	1237	1256	rVB	730202	1275648	38.10%	3.243%
16	10.522	1256	1264	1291	rBV	635342	1508852	45.06%	3.835%
17	11.999	1508	1515	1523	rBV4	9661	23375	0.70%	0.059%
18	13.122	1702	1706	1712	rVB6	4276	8081	0.24%	0.021%
19	13.663	1788	1798	1819	rBV	1229138	2197416	65.63%	5.586%
20	13.934	1836	1844	1860	rBV	1669428	2577984	76.99%	6.553%
21	14.246	1890	1897	1911	rBV	1265602	1722475	51.44%	4.378%
22	14.493	1932	1939	1954	rBV	407134	889553	26.57%	2.261%
23	15.269	2063	2071	2084	rBV	2183561	3115032	93.03%	7.918%
24	15.404	2087	2094	2109	rBV	525620	974645	29.11%	2.478%
25	16.081	2204	2209	2213	rBV5	8342	13928	0.42%	0.035%
26	16.745	2319	2322	2327	rBV7	2420	3981	0.12%	0.010%
27	16.863	2338	2342	2346	rBV7	3927	6892	0.21%	0.018%
28	17.063	2368	2376	2388	rBV	1051904	1949799	58.23%	4.956%
29	17.181	2389	2396	2411	rVV	2043240	3119780	93.18%	7.930%
30	18.022	2536	2539	2541	rBV4	2391	3535	0.11%	0.009%
31	18.051	2542	2544	2546	rBV3	3394	3369	0.10%	0.009%
32	19.110	2720	2724	2730	rVB4	22960	35348	1.06%	0.090%
33	19.192	2734	2738	2745	rBV	21655	37253	1.11%	0.095%
34	19.563	2795	2801	2813	rBV2	2069595	3348266	100.00%	8.511%
35	21.533	3130	3136	3147	rBV	982340	1729880	51.66%	4.397%
36	24.586	3646	3655	3676	rVB2	1106622	2922585	87.29%	7.429%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019992.D
Acq On : 26 Mar 2024 10:24
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	24.804	3685	3692	3712	rVB2	480309	1656668	49.48%	4.211%
----	--------	------	------	------	------	--------	---------	--------	--------




Sum of corrected areas: 39339765

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019992.D
Acq On : 26 Mar 2024 10:24
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

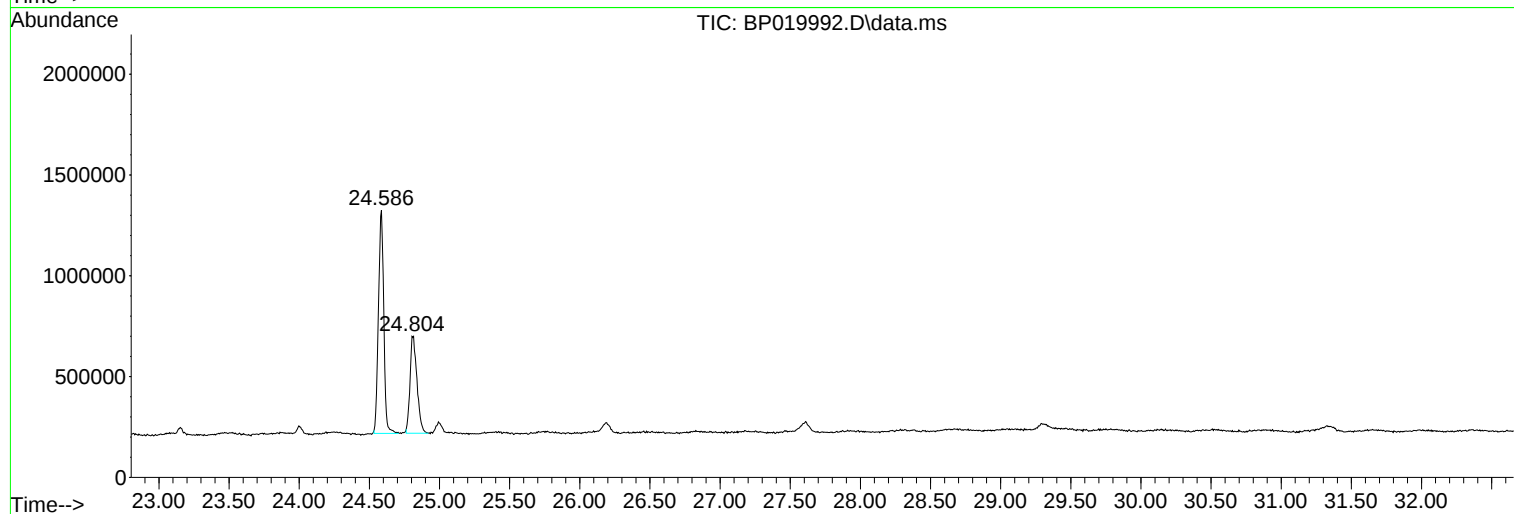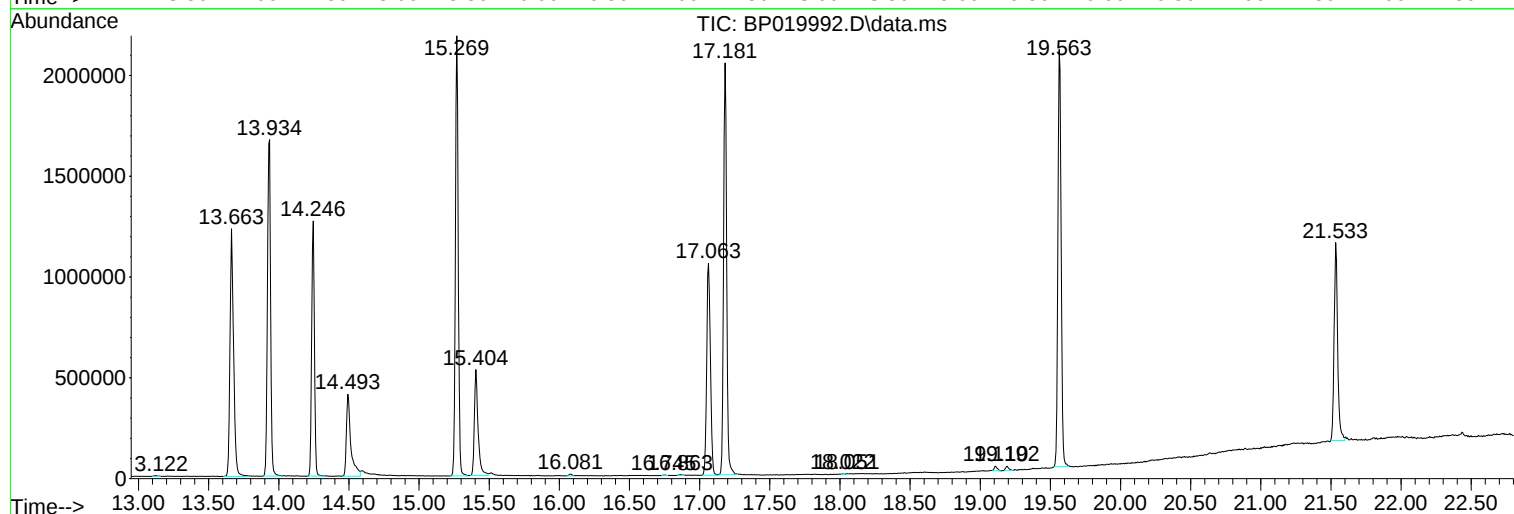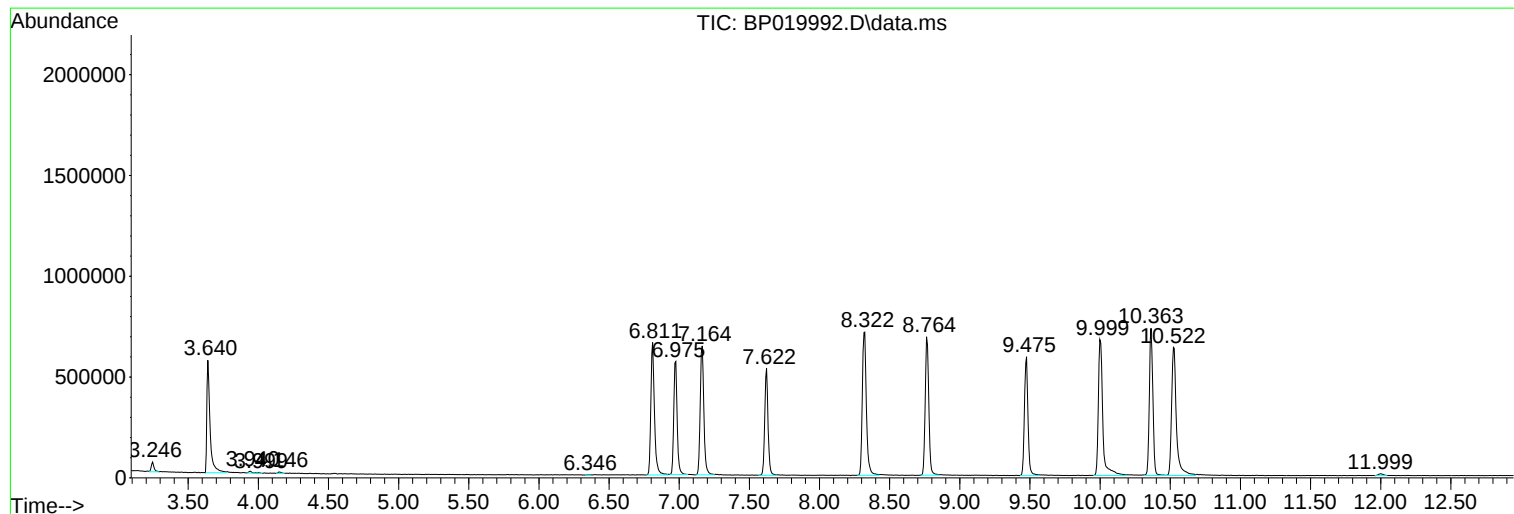

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019992.D
Acq On : 26 Mar 2024 10:24
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019992.D
Acq On : 26 Mar 2024 10:24
Operator : MA/JU
Sample : PB159439BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK439

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc