

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP019996.D
 Acq On : 26 Mar 2024 14:02
 Operator : MA/JU
 Sample : PB159472BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK472

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	18	22	30	rVB	48702	62506	1.70%	0.157%
2	3.611	86	89	110	rBV	549933	871829	23.77%	2.194%
3	3.905	136	139	142	rBV2	6223	6991	0.19%	0.018%
4	6.752	616	623	640	rBV	599821	1125072	30.68%	2.831%
5	6.934	645	654	667	rVV	526492	899675	24.53%	2.264%
6	7.111	677	684	696	rBV	656577	1079867	29.44%	2.717%
7	7.564	754	761	777	rBV	454182	826043	22.52%	2.079%
8	8.258	873	879	896	rBV	724687	1391220	37.93%	3.501%
9	8.722	950	958	968	rBV	674195	1179431	32.16%	2.968%
10	9.434	1070	1079	1095	rBV	554055	1008584	27.50%	2.538%
11	9.963	1160	1169	1176	rBV	757707	1297409	35.37%	3.265%
12	10.334	1224	1232	1245	rBV	729454	1201451	32.76%	3.023%
13	10.481	1250	1257	1283	rVV	624285	1465261	39.95%	3.687%
14	11.969	1502	1510	1519	rBV	10842	23598	0.64%	0.059%
15	12.340	1568	1573	1576	rBV7	1818	4389	0.12%	0.011%
16	13.651	1789	1796	1805	rBV	1521804	2264591	61.74%	5.699%
17	13.922	1833	1842	1858	rBV	1484697	2575812	70.23%	6.482%
18	14.234	1886	1895	1906	rBV	1042314	1715177	46.76%	4.316%
19	14.475	1930	1936	1949	rBV	460315	947530	25.83%	2.384%
20	15.263	2057	2070	2077	rBV	2202422	3215947	87.68%	8.093%
21	15.410	2087	2095	2107	rBV	582390	1101286	30.03%	2.771%
22	16.057	2201	2205	2210	rVV5	8998	12627	0.34%	0.032%
23	16.528	2282	2285	2288	rVB5	3391	3851	0.10%	0.010%
24	16.745	2317	2322	2326	rBV8	4159	7705	0.21%	0.019%
25	16.857	2335	2341	2344	rBV7	5426	10612	0.29%	0.027%
26	17.069	2370	2377	2388	rBV	1360835	2007999	54.75%	5.053%
27	17.175	2388	2395	2413	rVV2	1765943	3357742	91.55%	8.450%
28	17.522	2450	2454	2458	rBV7	3027	6226	0.17%	0.016%
29	17.634	2468	2473	2476	rBV7	3622	6947	0.19%	0.017%
30	18.057	2542	2545	2549	rBV6	3380	4603	0.13%	0.012%
31	19.122	2721	2726	2733	rVB4	26159	44444	1.21%	0.112%
32	19.192	2734	2738	2745	rVV2	19465	35621	0.97%	0.090%
33	19.575	2795	2803	2817	rBV	2203085	3667671	100.00%	9.229%
34	20.433	2945	2949	2958	rVB	135027	195644	5.33%	0.492%
35	21.545	3132	3138	3154	rBV	957194	1760967	48.01%	4.431%
36	24.598	3648	3657	3669	rVB2	1041289	2844059	77.54%	7.157%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019996.D
Acq On : 26 Mar 2024 14:02
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	24.833	3689	3697	3711	rVB	519752	1508329	41.12%	3.796%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 39738716

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019996.D
Acq On : 26 Mar 2024 14:02
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

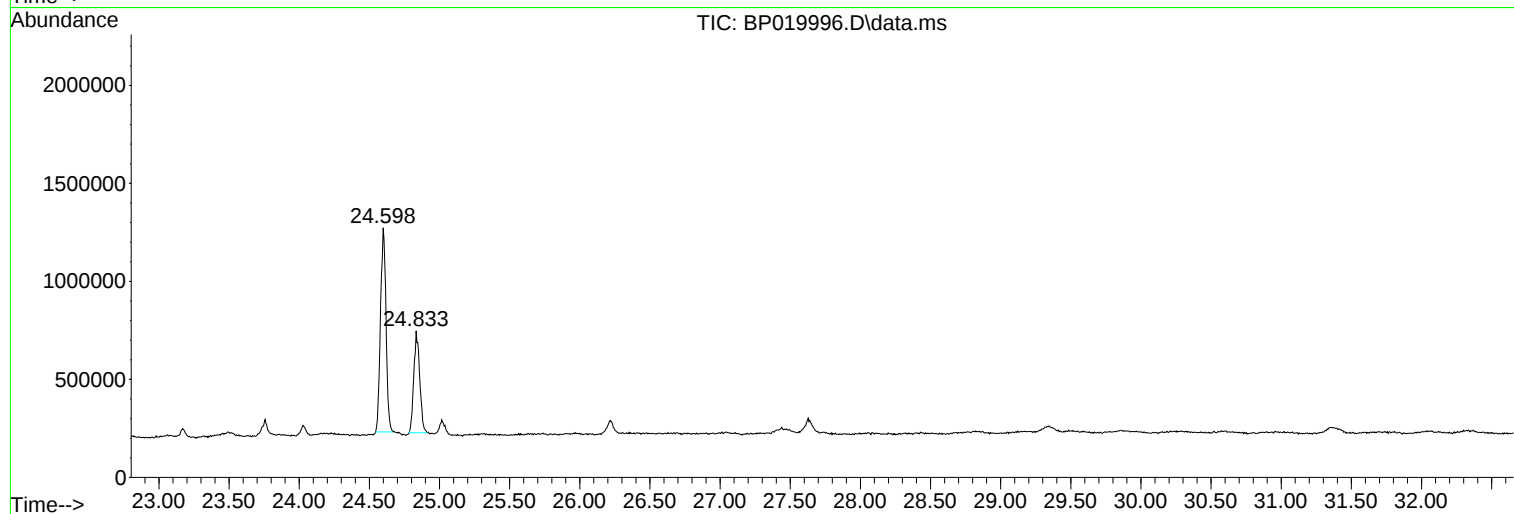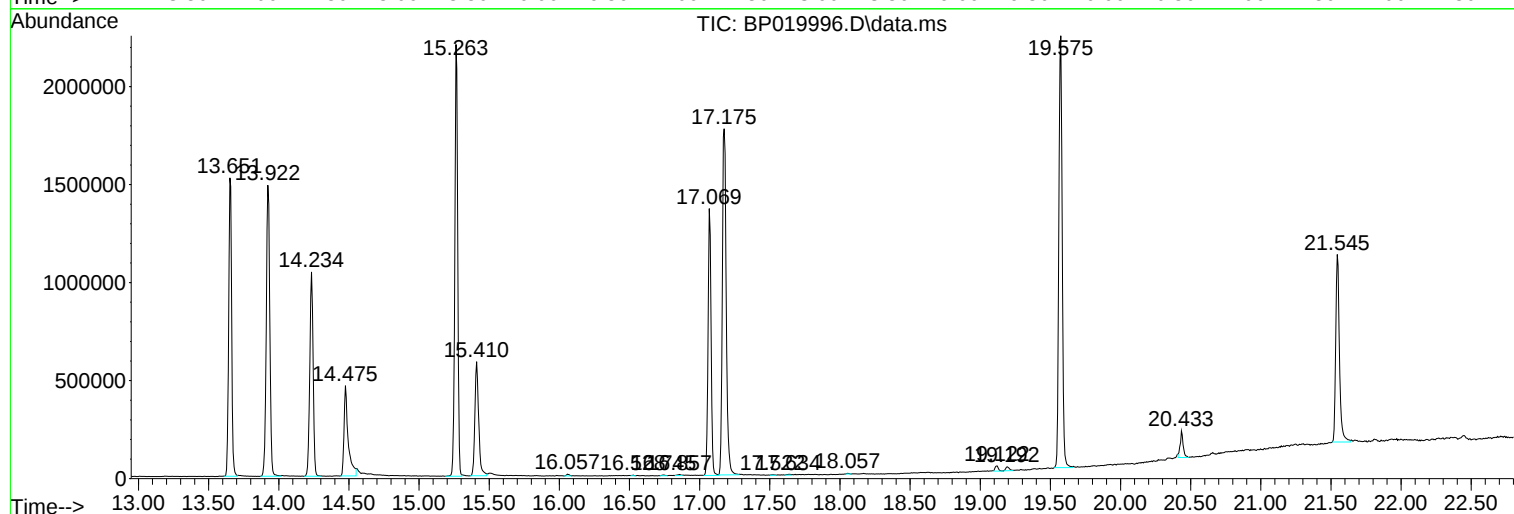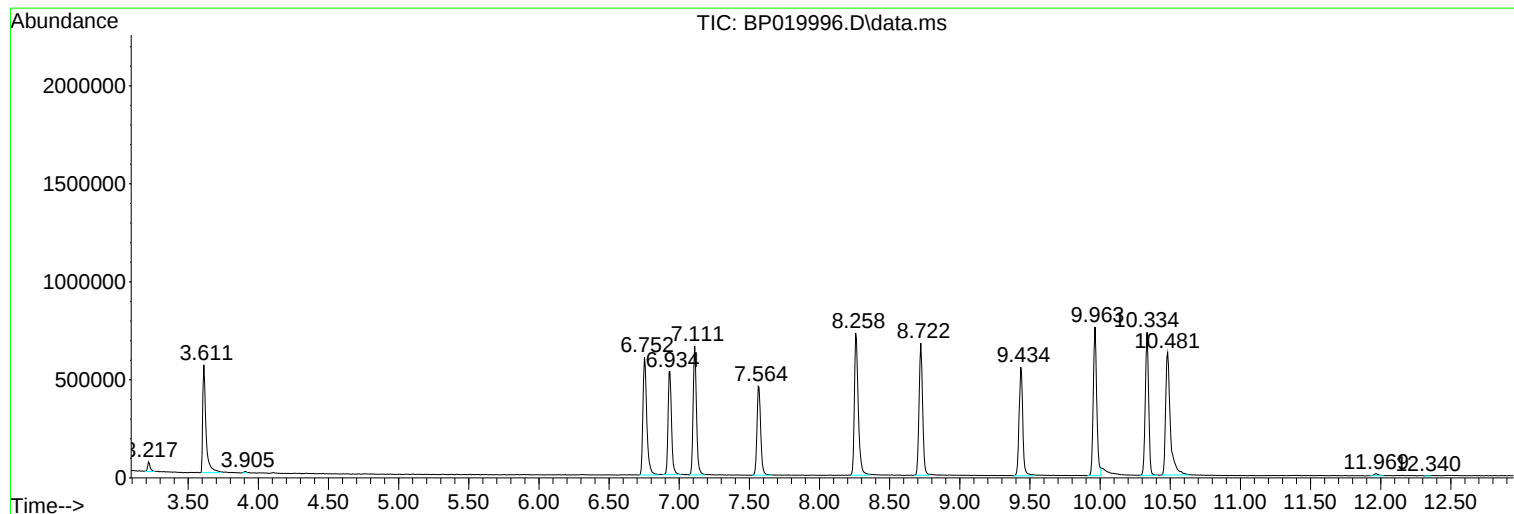

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019996.D
Acq On : 26 Mar 2024 14:02
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1










Instrument :
BNA_P
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
20.433	2.22 ng/ul	195644	Chrysene-d12		21.545	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	Heptadecane, 9-octyl-		352	C25H52	007225-64-1	93
2	Eicosane		282	C20H42	000112-95-8	93
3	Hexacosane		366	C26H54	000630-01-3	91
4	Octacosane		394	C28H58	000630-02-4	91
5	Heptacosane		380	C27H56	000593-49-7	91

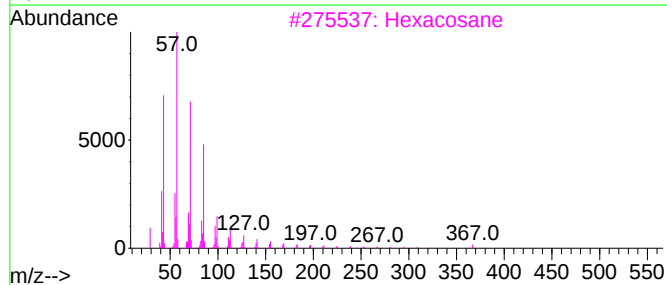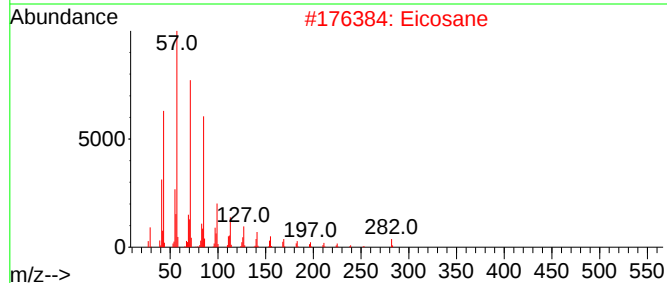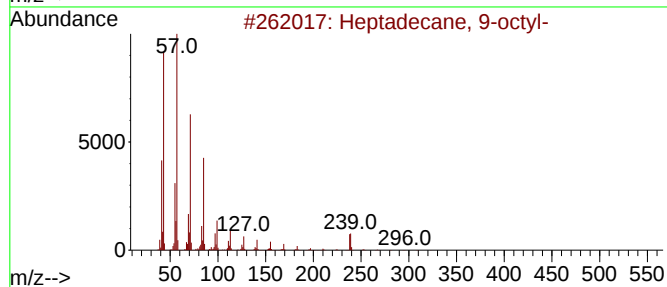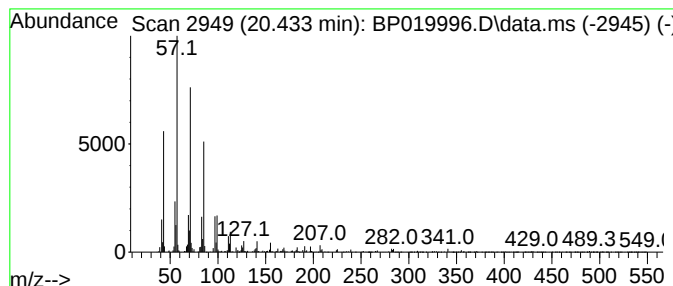

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019996.D
Acq On : 26 Mar 2024 14:02
Operator : MA/JU
Sample : PB159472BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK472

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.433	2.2	ng/u1	195644	5	21.545	1760970	20.0