

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP019997.D
 Acq On : 26 Mar 2024 14:45
 Operator : MA/JU
 Sample : PB159474BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK474

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	35	rVB	43815	58701	1.44%	0.144%
2	3.634	89	93	111	rBV	518887	840995	20.56%	2.059%
3	3.934	141	144	149	rVB3	7833	10025	0.25%	0.025%
4	4.140	176	179	183	rBV6	4407	6606	0.16%	0.016%
5	6.799	624	631	648	rBV	584470	1114654	27.25%	2.729%
6	6.963	653	659	672	rVB	557450	877874	21.46%	2.150%
7	7.146	683	690	704	rBV	568194	1068845	26.13%	2.617%
8	7.616	759	770	781	rBV	409531	707874	17.31%	1.733%
9	8.310	879	888	909	rBV2	702911	1429177	34.94%	3.500%
10	8.763	957	965	986	rBV	671503	1209954	29.58%	2.963%
11	9.469	1075	1085	1104	rBV	592943	1046740	25.59%	2.563%
12	9.993	1167	1174	1186	rBV	746715	1377127	33.67%	3.372%
13	10.357	1227	1236	1248	rBV	639406	1086091	26.56%	2.659%
14	10.516	1255	1263	1288	rBV	640116	1545387	37.79%	3.784%
15	11.987	1508	1513	1526	rVB3	11354	24821	0.61%	0.061%
16	13.128	1701	1707	1714	rVB2	10452	18334	0.45%	0.045%
17	13.663	1790	1798	1811	rBV	1615443	2481099	60.66%	6.075%
18	13.934	1837	1844	1866	rBV	1847567	2799319	68.45%	6.855%
19	14.245	1889	1897	1909	rBV	1106753	1620901	39.63%	3.969%
20	14.493	1933	1939	1955	rBV	546827	1093213	26.73%	2.677%
21	15.269	2062	2071	2086	rBV	2372221	3418704	83.59%	8.371%
22	15.398	2087	2093	2109	rBV	730787	1222230	29.88%	2.993%
23	15.516	2110	2113	2118	rVB3	12976	18161	0.44%	0.044%
24	16.075	2204	2208	2215	rVB6	9008	14862	0.36%	0.036%
25	16.757	2318	2324	2326	rBV7	4143	7925	0.19%	0.019%
26	16.863	2338	2342	2347	rBV8	4617	7093	0.17%	0.017%
27	17.063	2368	2376	2387	rBV	1050886	1940133	47.44%	4.751%
28	17.186	2389	2397	2409	rBV2	2272322	3685210	90.11%	9.024%
29	18.045	2540	2543	2547	rBV6	4365	7637	0.19%	0.019%
30	19.110	2720	2724	2731	rBV2	27298	46566	1.14%	0.114%
31	19.186	2732	2737	2745	rBV2	23557	46528	1.14%	0.114%
32	19.569	2795	2802	2813	rBV	2670973	4089865	100.00%	10.015%
33	20.410	2943	2945	2952	rVB4	31885	46436	1.14%	0.114%
34	21.527	3129	3135	3152	rBV2	891545	1657583	40.53%	4.059%
35	24.568	3643	3652	3666	rVB2	1078098	2862151	69.98%	7.008%
36	24.815	3685	3694	3707	rVB2	411346	1349923	33.01%	3.305%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019997.D
Acq On : 26 Mar 2024 14:45
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK474

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 40838744

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019997.D
Acq On : 26 Mar 2024 14:45
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK474

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

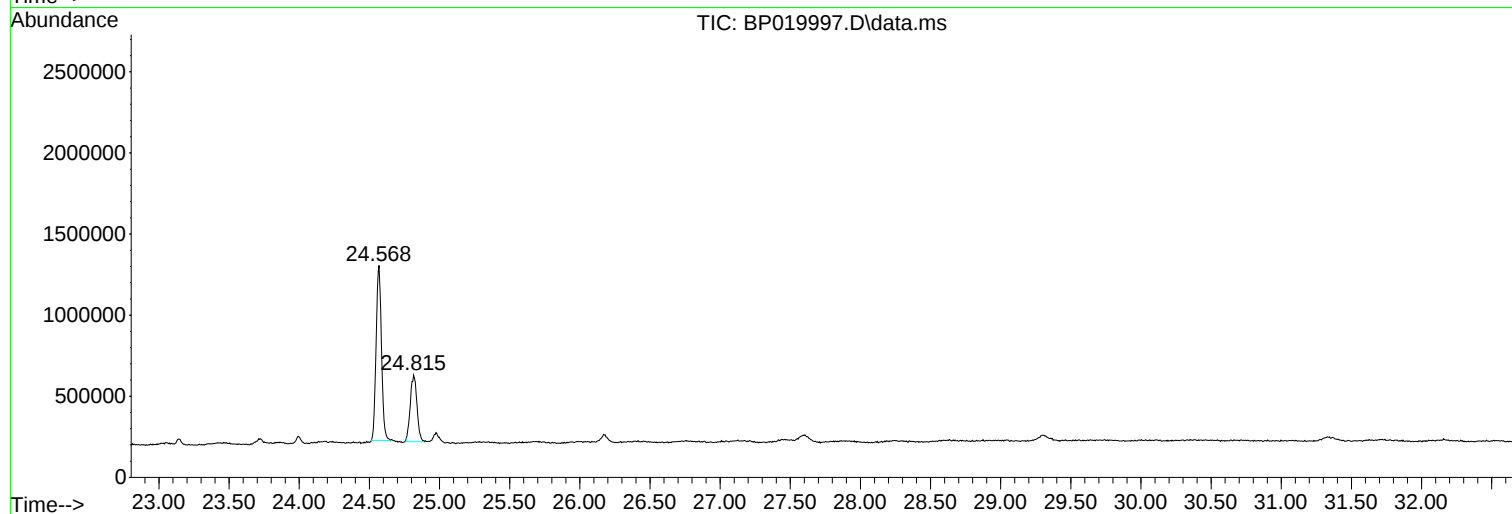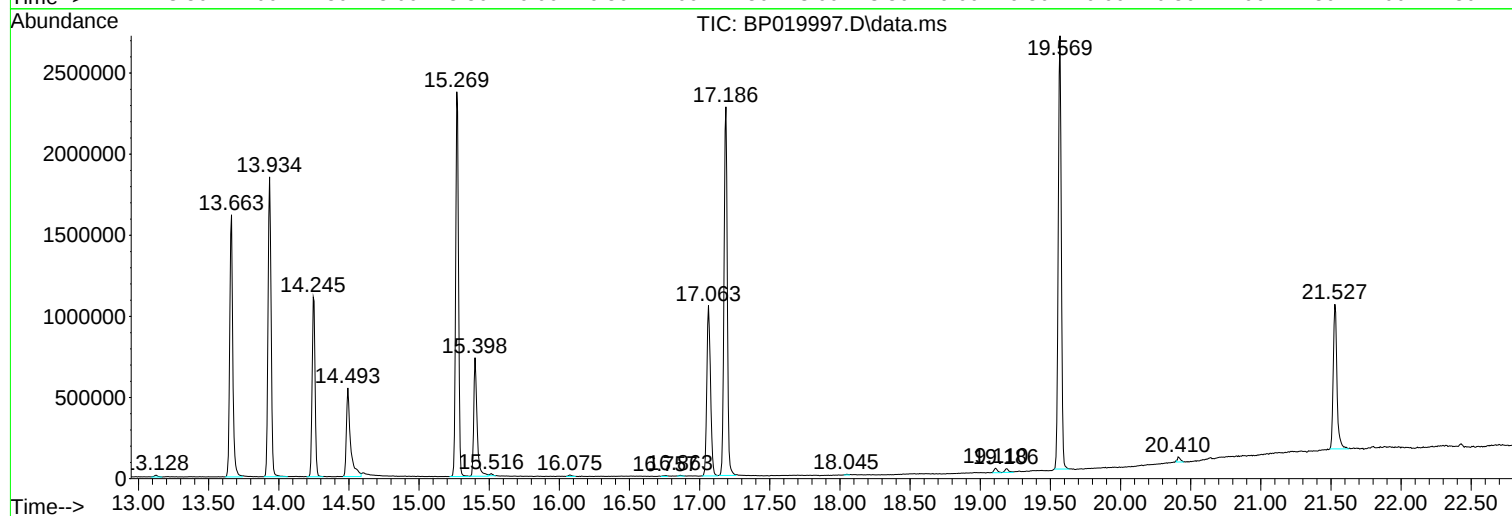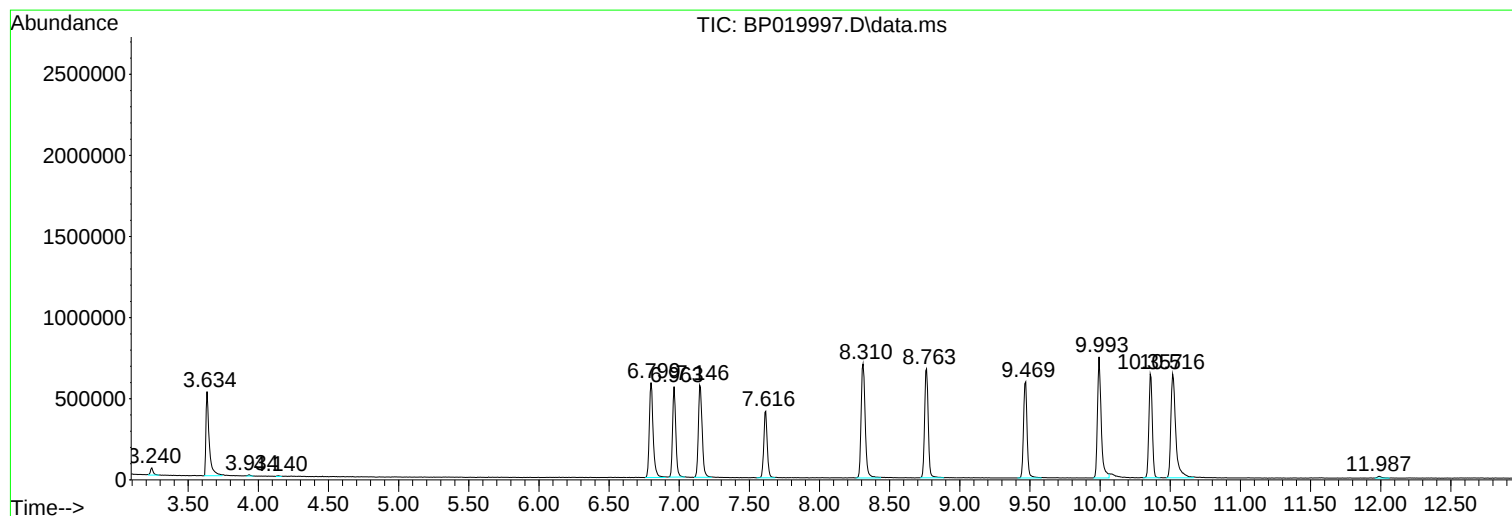

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019997.D
Acq On : 26 Mar 2024 14:45
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK474

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019997.D
Acq On : 26 Mar 2024 14:45
Operator : MA/JU
Sample : PB159474BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK474

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc