

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP019999.D
 Acq On : 26 Mar 2024 16:15
 Operator : MA/JU
 Sample : PB159783BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK783

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019999.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.234	22	25	35	rVB	33163	46118	1.55%	0.168%
2	3.634	89	93	115	rVB	247778	436424	14.63%	1.593%
3	3.922	139	142	147	rVB5	6877	10288	0.34%	0.038%
4	6.781	621	628	644	rBV	387901	748166	25.08%	2.731%
5	6.958	651	658	672	rBV	366792	571984	19.18%	2.088%
6	7.134	681	688	704	rBV	409492	710219	23.81%	2.592%
7	7.599	759	767	780	rBV	323529	578707	19.40%	2.112%
8	8.293	876	885	904	rBV	419555	886506	29.72%	3.236%
9	8.746	954	962	975	rBV	400053	736071	24.68%	2.687%
10	8.857	979	981	986	rVB6	2905	3861	0.13%	0.014%
11	9.457	1076	1083	1098	rBV	332092	618479	20.74%	2.257%
12	9.993	1166	1174	1187	rBV	277777	779105	26.12%	2.844%
13	10.352	1227	1235	1247	rBV	457776	791863	26.55%	2.890%
14	10.475	1254	1256	1263	rVB8	2023	3086	0.10%	0.011%
15	11.993	1507	1514	1520	rBV4	5722	10406	0.35%	0.038%
16	12.410	1581	1585	1590	rBV7	1844	3666	0.12%	0.013%
17	13.128	1703	1707	1712	rBV7	3502	6300	0.21%	0.023%
18	13.193	1714	1718	1723	rVB7	1829	3310	0.11%	0.012%
19	13.651	1790	1796	1808	rBV	1031904	1467431	49.20%	5.356%
20	13.934	1835	1844	1859	rBV	1008685	1584591	53.13%	5.784%
21	14.240	1887	1896	1909	rBV	656293	1142531	38.31%	4.170%
22	14.481	1930	1937	1957	rBV2	226762	726203	24.35%	2.651%
23	15.257	2057	2069	2086	rBV	1385857	2049877	68.73%	7.482%
24	15.416	2088	2096	2108	rBV	422258	758847	25.44%	2.770%
25	15.792	2154	2160	2165	rBV7	3706	5910	0.20%	0.022%
26	16.051	2200	2204	2212	rVB9	5582	8345	0.28%	0.030%
27	16.739	2318	2321	2326	rBV6	2552	3943	0.13%	0.014%
28	17.075	2371	2378	2387	rBV	994663	1432925	48.04%	5.230%
29	17.163	2387	2393	2416	rVB2	1390119	2401314	80.51%	8.765%
30	17.951	2525	2527	2530	rBV4	2624	3027	0.10%	0.011%
31	18.045	2539	2543	2550	rVB10	4438	6773	0.23%	0.025%
32	19.110	2720	2724	2730	rBV4	22643	29946	1.00%	0.109%
33	19.186	2732	2737	2742	rBV4	17988	32621	1.09%	0.119%
34	19.563	2794	2801	2817	rBV	2116417	2982534	100.00%	10.886%
35	21.533	3130	3136	3151	rBV2	722190	1579640	52.96%	5.766%
36	24.598	3647	3657	3670	rVB2	984438	2718349	91.14%	9.922%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019999.D
Acq On : 26 Mar 2024 16:15
Operator : MA/JU
Sample : PB159783BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	24.827	3687	3696	3714	rVB	455002	1517740	50.89%	5.540%
----	--------	------	------	------	-----	--------	---------	--------	--------




Sum of corrected areas: 27397106

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019999.D
Acq On : 26 Mar 2024 16:15
Operator : MA/JU
Sample : PB159783BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

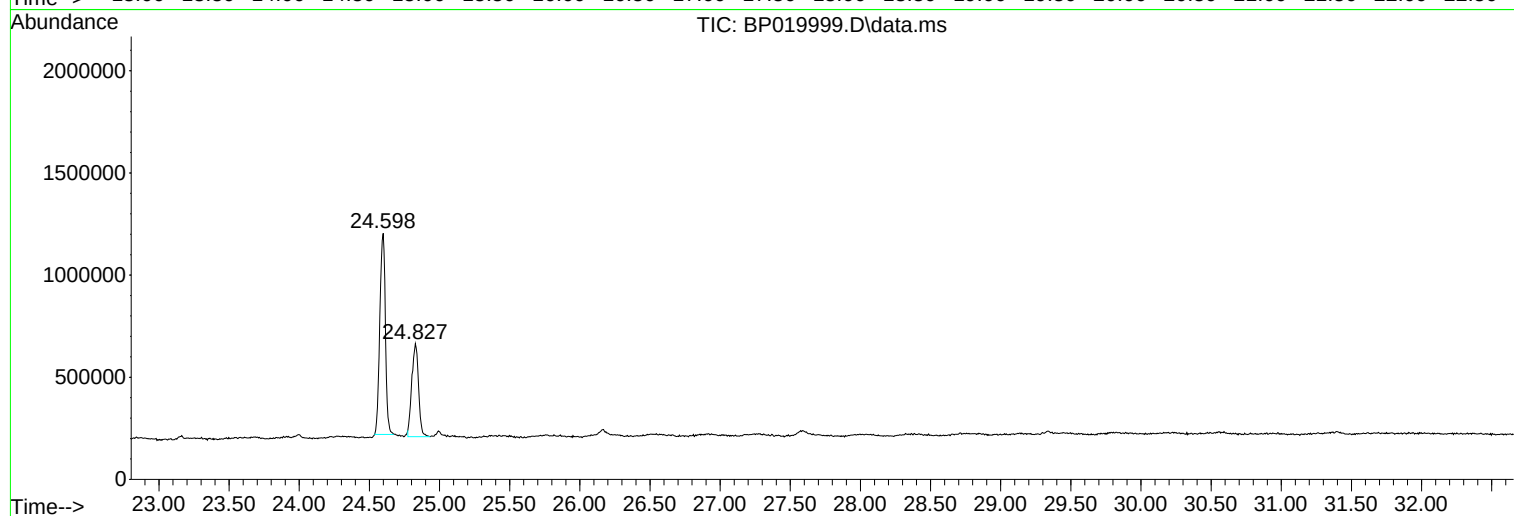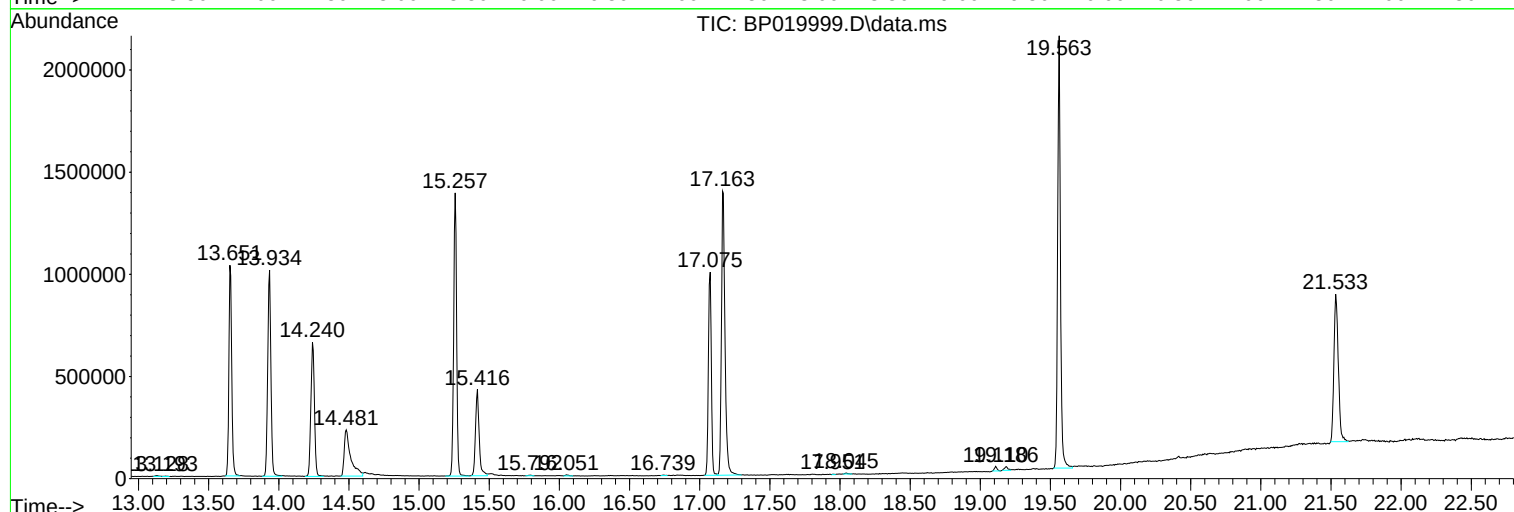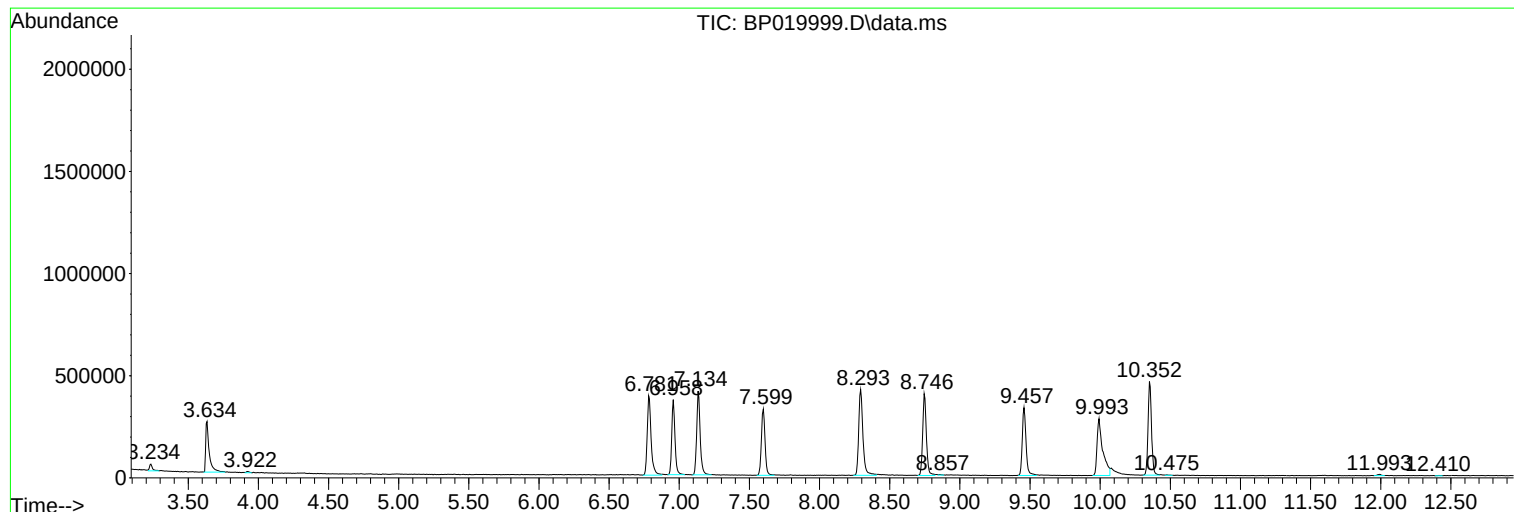

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019999.D
Acq On : 26 Mar 2024 16:15
Operator : MA/JU
Sample : PB159783BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP019999.D
Acq On : 26 Mar 2024 16:15
Operator : MA/JU
Sample : PB159783BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc