

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
 Data File : BP020000.D
 Acq On : 26 Mar 2024 16:59
 Operator : MA/JU
 Sample : PB159785BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK785

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020000.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	33	rVB	35993	45294	1.78%	0.170%
2	3.646	92	95	108	rBV	143924	244083	9.61%	0.917%
3	3.934	141	144	149	rBV3	6326	9863	0.39%	0.037%
4	5.893	473	477	481	rVB7	1825	2686	0.11%	0.010%
5	6.793	622	630	648	rBV	436243	870711	34.30%	3.270%
6	6.969	654	660	674	rVB	413045	671214	26.44%	2.521%
7	7.146	683	690	704	rBV	490819	842758	33.20%	3.165%
8	7.605	761	768	781	rBV	326062	591074	23.28%	2.220%
9	8.299	877	886	902	rBV	545736	1026801	40.45%	3.857%
10	8.405	902	904	908	rVB5	3735	3775	0.15%	0.014%
11	8.757	957	964	982	rBV	479342	861313	33.93%	3.235%
12	9.463	1077	1084	1099	rBV	409021	725702	28.59%	2.726%
13	9.999	1168	1175	1207	rBV	386160	1030148	40.58%	3.869%
14	10.199	1207	1209	1213	rVB5	2708	3120	0.12%	0.012%
15	10.369	1228	1238	1250	rBV	466328	806645	31.78%	3.030%
16	10.546	1262	1268	1288	rBV3	29540	102662	4.04%	0.386%
17	11.998	1509	1515	1524	rBV6	7249	15938	0.63%	0.060%
18	13.140	1702	1709	1716	rVB6	5295	11148	0.44%	0.042%
19	13.663	1792	1798	1808	rBV	947053	1454912	57.31%	5.465%
20	13.734	1808	1810	1814	rVB5	2813	3488	0.14%	0.013%
21	13.934	1833	1844	1861	rBV	982312	1745805	68.77%	6.557%
22	14.240	1888	1896	1908	rBV	611317	1065973	41.99%	4.004%
23	14.487	1932	1938	1959	rBV	215146	631049	24.86%	2.370%
24	14.675	1967	1970	1975	rVB6	4977	6528	0.26%	0.025%
25	14.834	1995	1997	2005	rBV9	1668	2870	0.11%	0.011%
26	15.269	2062	2071	2087	rBV	1352465	2100683	82.75%	7.890%
27	15.416	2087	2096	2108	rBV	322711	687157	27.07%	2.581%
28	15.510	2110	2112	2119	rVB7	8528	14888	0.59%	0.056%
29	16.063	2201	2206	2209	rBV6	5305	7766	0.31%	0.029%
30	16.751	2320	2323	2327	rVB6	2605	2866	0.11%	0.011%
31	17.081	2371	2379	2388	rBV	757922	1206793	47.54%	4.533%
32	17.175	2388	2395	2418	rVB	1441162	2292689	90.31%	8.611%
33	17.975	2526	2531	2534	rBV7	2951	6375	0.25%	0.024%
34	18.163	2561	2563	2570	rBV8	1961	3354	0.13%	0.013%
35	19.116	2721	2725	2731	rBV4	17954	26749	1.05%	0.100%
36	19.198	2735	2739	2745	rVV2	12599	21605	0.85%	0.081%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020000.D
Acq On : 26 Mar 2024 16:59
Operator : MA/JU
Sample : PB159785BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	19.575	2796	2803	2815	rBV	1625153	2538612	100.00%	9.535%
38	21.539	3131	3137	3152	rVB	595762	1223697	48.20%	4.596%
39	24.586	3647	3655	3670	rVB2	803225	2421413	95.38%	9.095%
40	24.827	3688	3696	3710	rVB	436293	1293502	50.95%	4.858%




Sum of corrected areas: 26623709

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020000.D
Acq On : 26 Mar 2024 16:59
Operator : MA/JU
Sample : PB159785BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

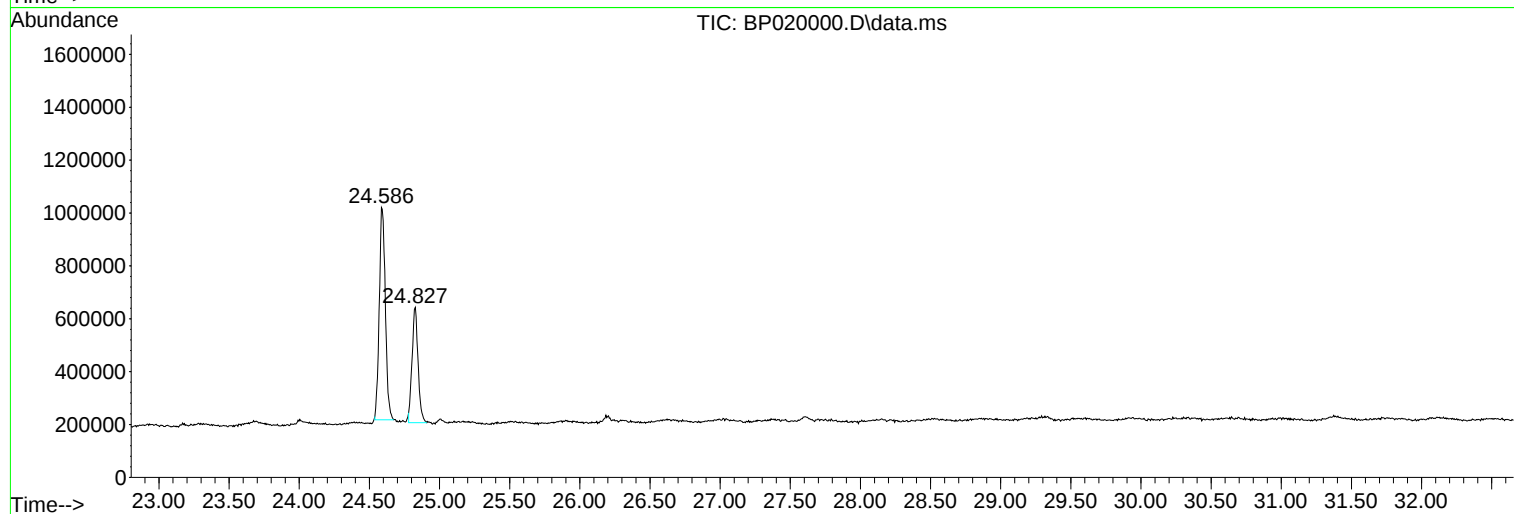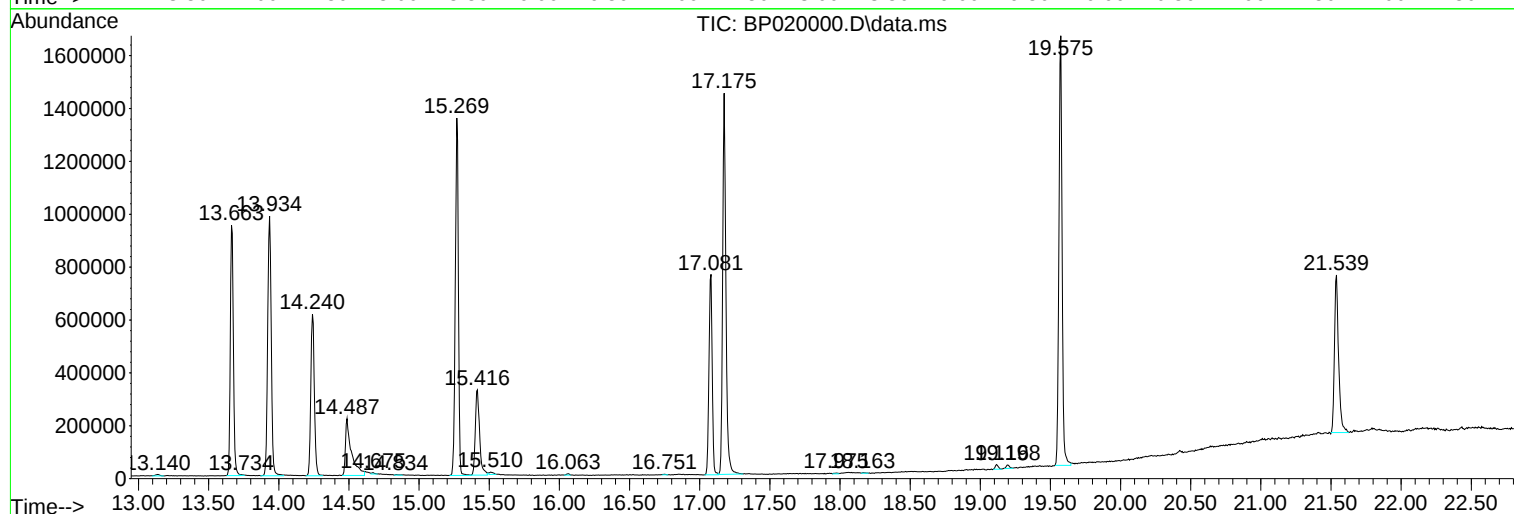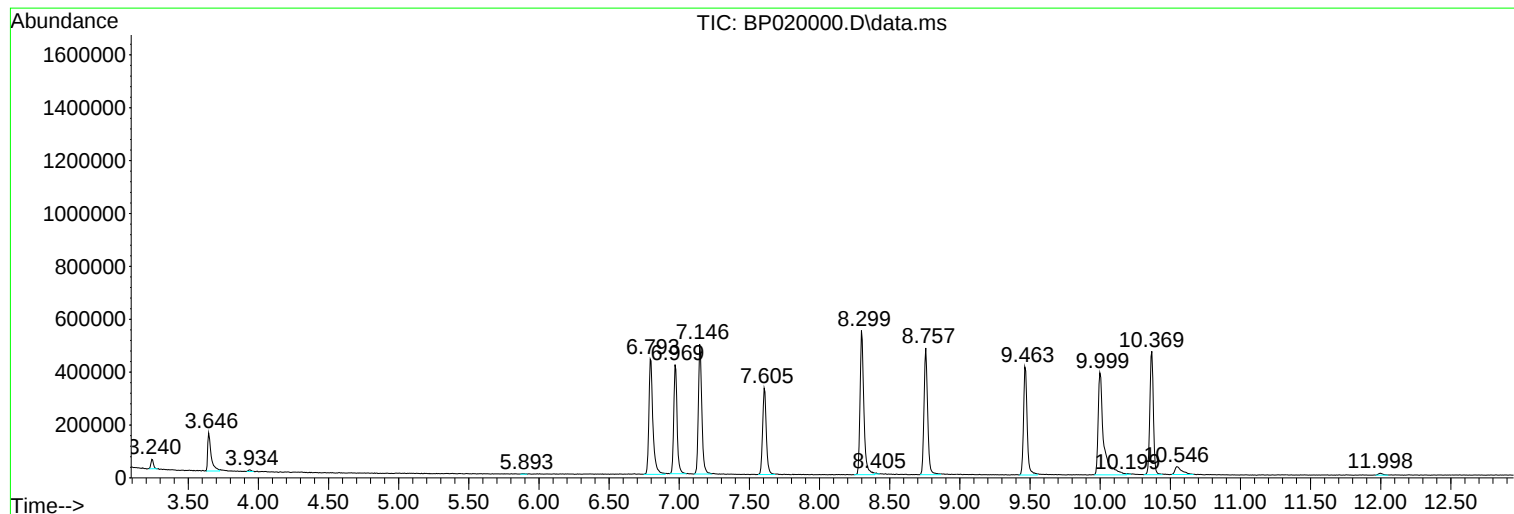

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020000.D
Acq On : 26 Mar 2024 16:59
Operator : MA/JU
Sample : PB159785BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032624\
Data File : BP020000.D
Acq On : 26 Mar 2024 16:59
Operator : MA/JU
Sample : PB159785BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK785

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------