
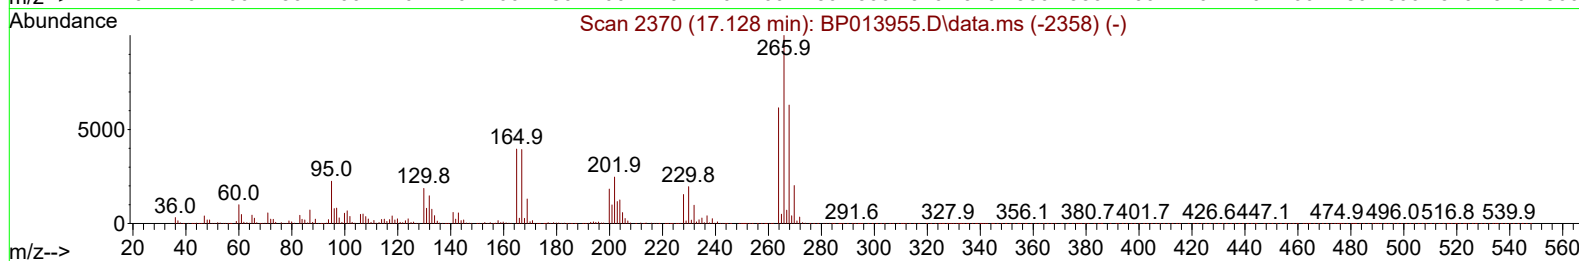
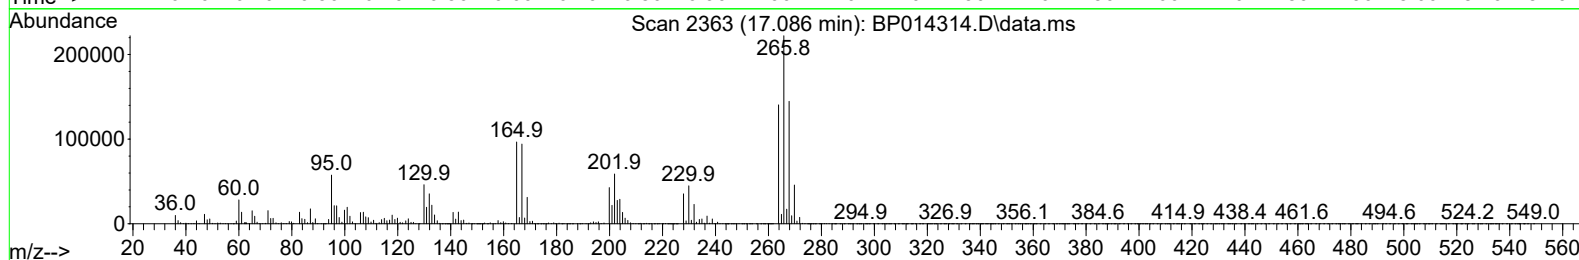


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
Data File : BP014314.D
Acq On : 27 Mar 2023 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 03:21:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 03:19:01 2023
Response via : Initial Calibration

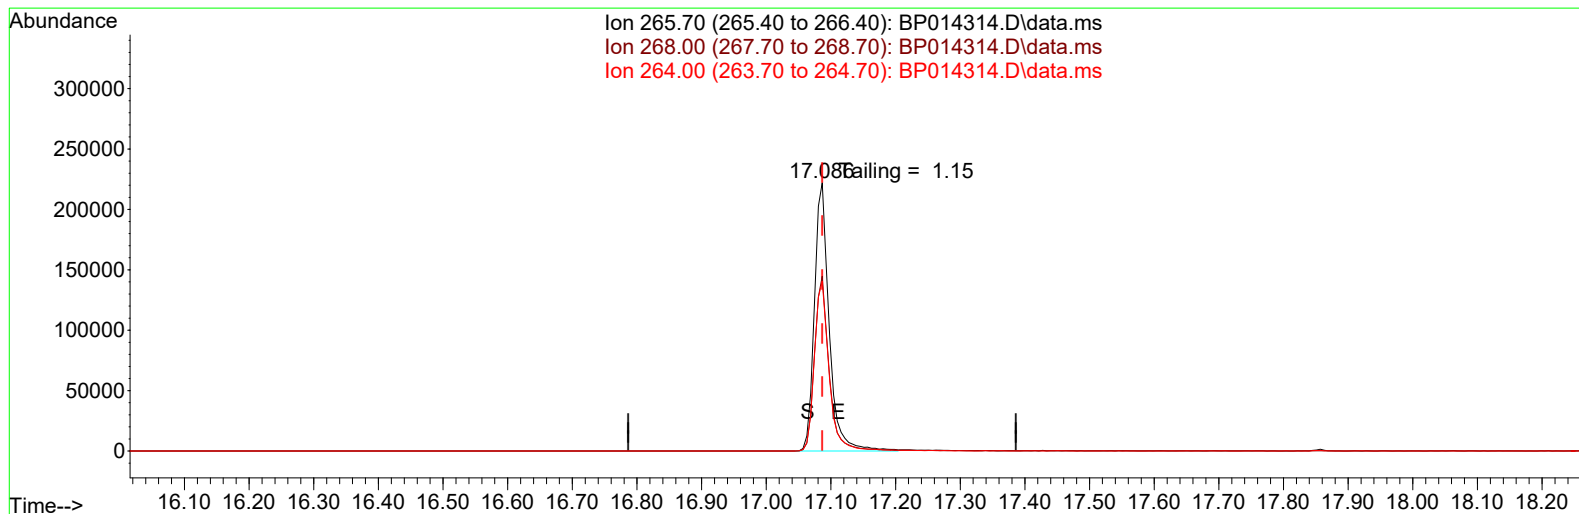

TIC: BP014314.D\data.ms

(70) Pentachlorophenol (C)




17.086min (+ 0.000) 3871430.94 ng

response 356283

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.12
264.00	61.50	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
 Data File : BP014314.D
 Acq On : 27 Mar 2023 15:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 03:21:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 25 03:19:01 2023
 Response via : Initial Calibration

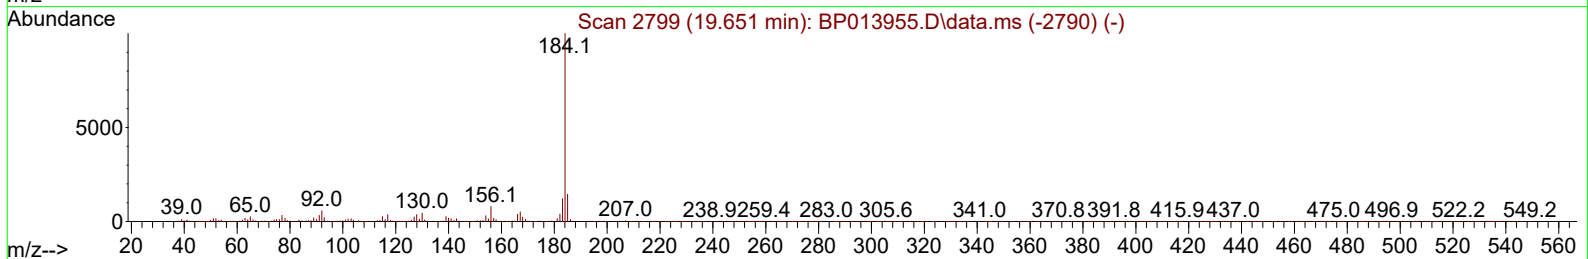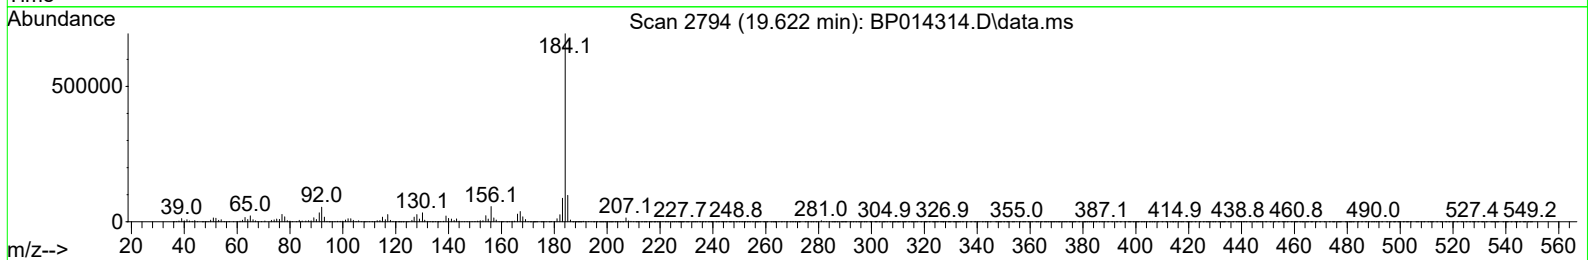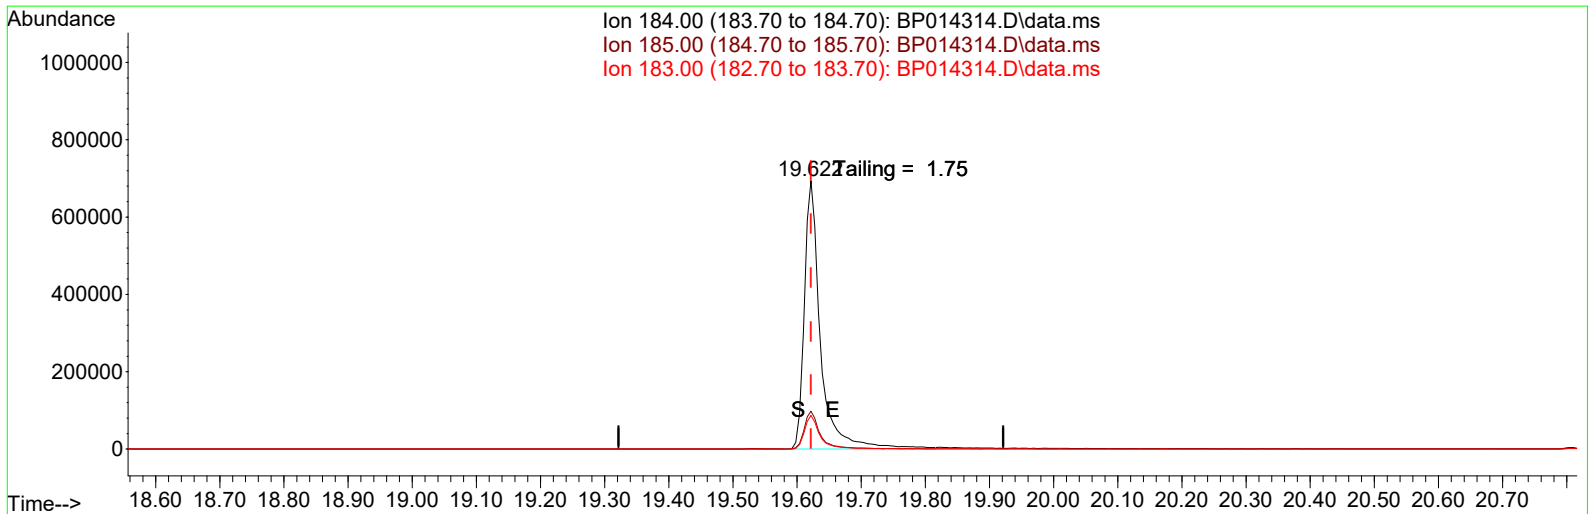

TIC: BP014314.D\data.ms

(77) Benzidine

19.622min (0.000) -20.00 ng

response 1221570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.07
183.00	12.10	12.53
0.00	0.00	0.00