

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
 Data File : BP014316.D
 Acq On : 27 Mar 2023 17:13
 Operator : CG/JU
 Sample : PB151659BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB151659BL

Quant Time: Mar 28 02:09:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 25 03:19:01 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	140054	20.000	ng	0.00
21) Naphthalene-d8	10.857	136	493734	20.000	ng	# 0.00
39) Acenaphthene-d10	14.681	164	273156	20.000	ng	0.00
64) Phenanthrene-d10	17.439	188	502270	20.000	ng	# 0.00
76) Chrysene-d12	21.521	240	454428	20.000	ng	0.00
86) Perylene-d12	24.045	264	534407	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.581	112	1235170	143.025	ng	0.00
7) Phenol-d6	7.199	99	1521080	134.153	ng	0.00
23) Nitrobenzene-d5	9.210	82	964721	89.306	ng	0.00
42) 2,4,6-Tribromophenol	16.175	330	463306	104.612	ng	0.00
45) 2-Fluorobiphenyl	13.304	172	1892321	89.753	ng	0.00
79) Terphenyl-d14	19.974	244	2427179	88.073	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
Data File : BP014316.D
Acq On : 27 Mar 2023 17:13
Operator : CG/JU
Sample : PB151659BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB151659BL

Quant Time: Mar 28 02:09:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 03:19:01 2023
Response via : Initial Calibration




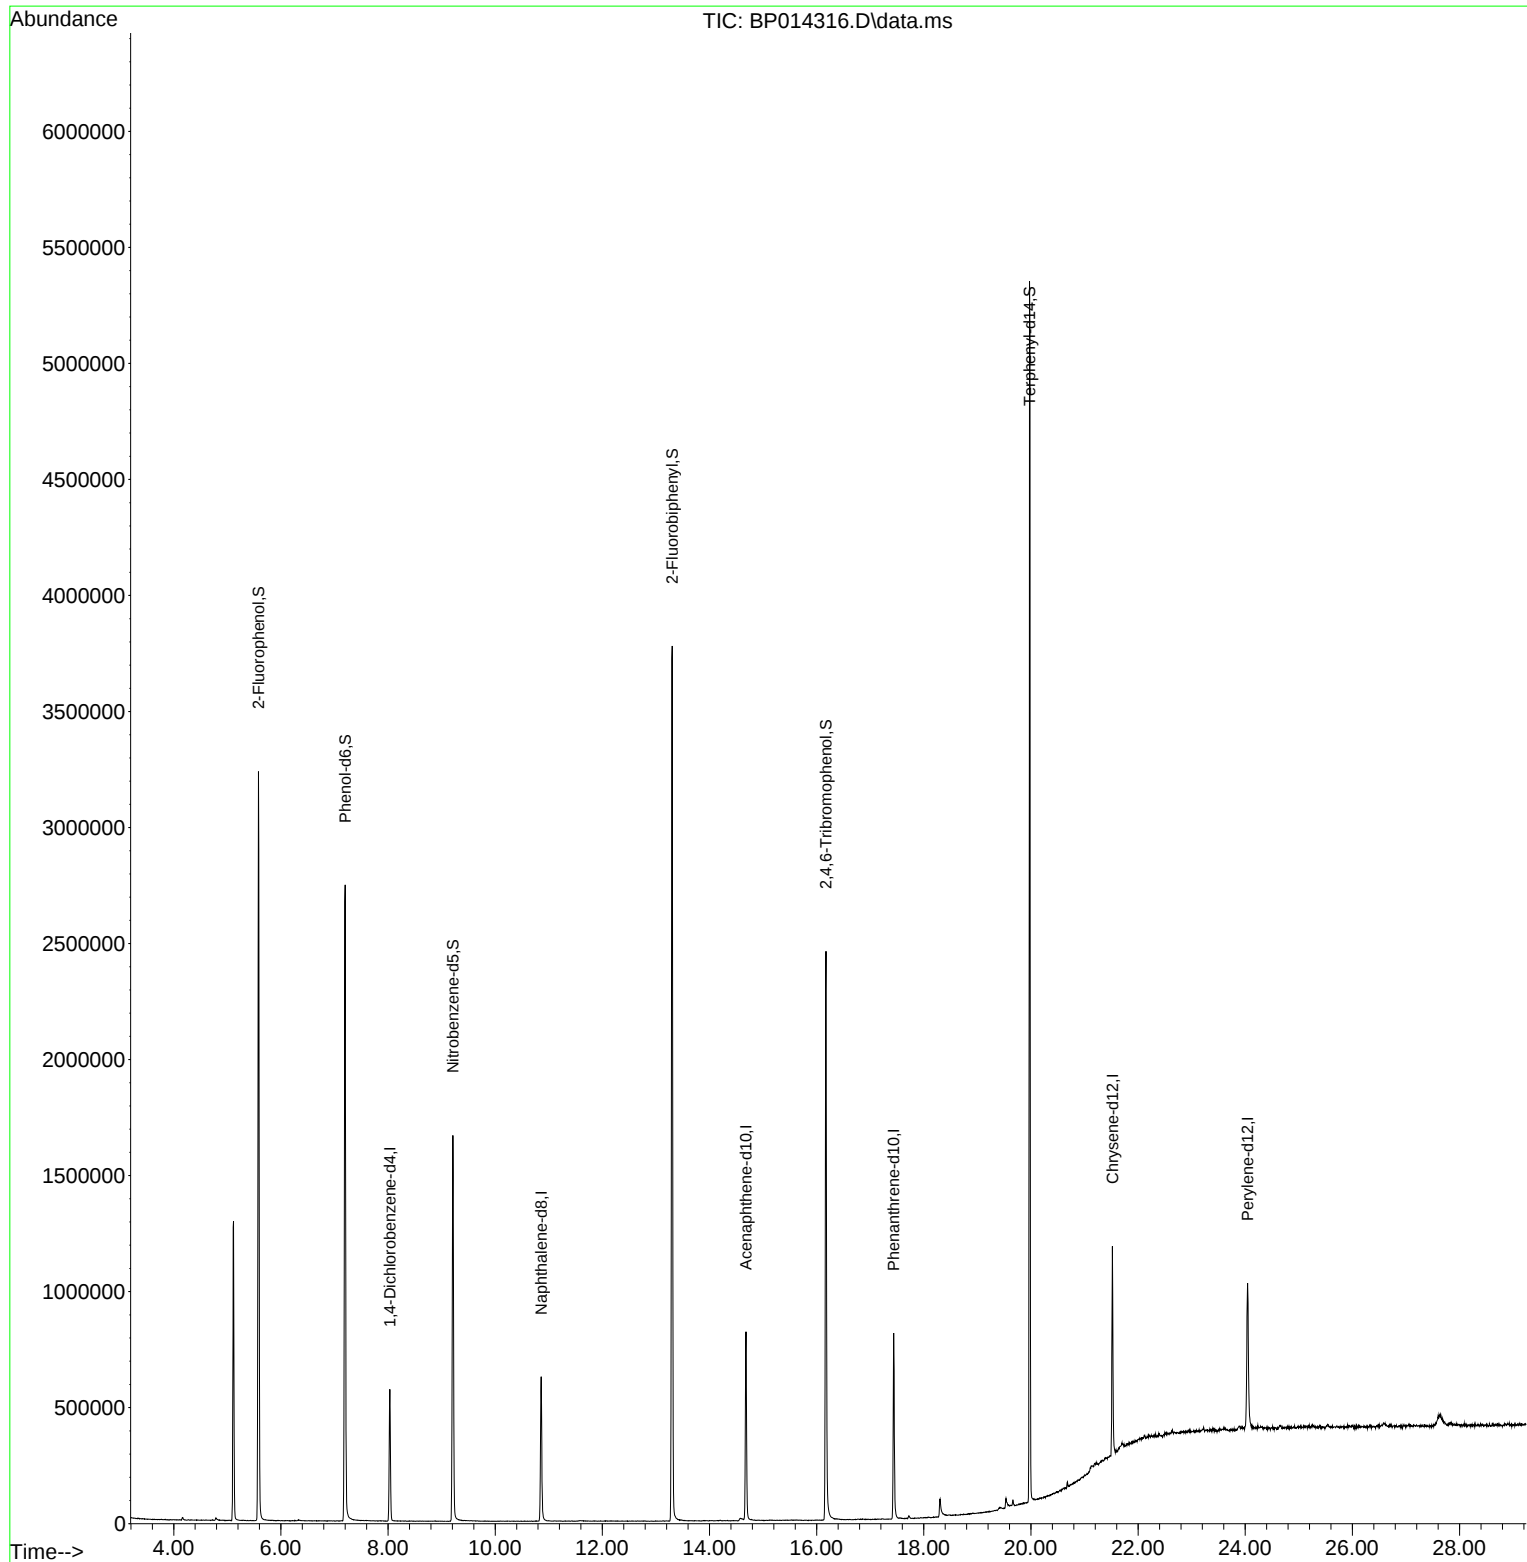




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.034 min Scan# 81
 Delta R.T. 0.006 min
 Lab File: BP014316.D
 Acq: 27 Mar 2023 17:13




Instrument :
 BNA_P
 ClientSampleId :
 PB151659BL


Tgt Ion:152 Resp: 140054
 Ion Ratio Lower Upper
 152 100
 150 157.5 122.3 183.5
 115 66.2 51.6 77.4

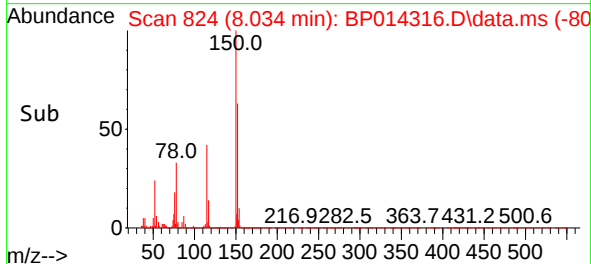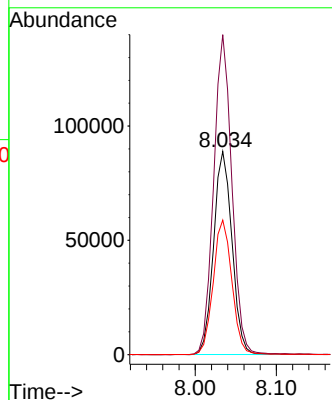

#5
 2-Fluorophenol
 Concen: 143.025 ng
 RT: 5.581 min Scan# 407
 Delta R.T. 0.006 min
 Lab File: BP014316.D
 Acq: 27 Mar 2023 17:13

Tgt Ion:112 Resp: 1235170
 Ion Ratio Lower Upper
 112 100
 64 65.1 46.7 70.1
 63 35.0 26.6 40.0


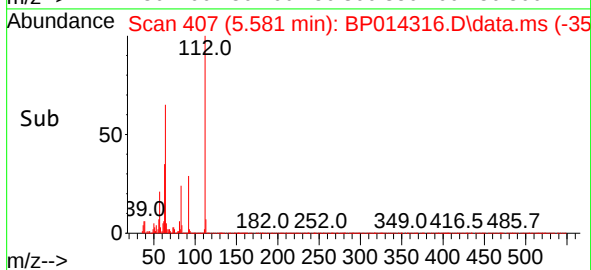
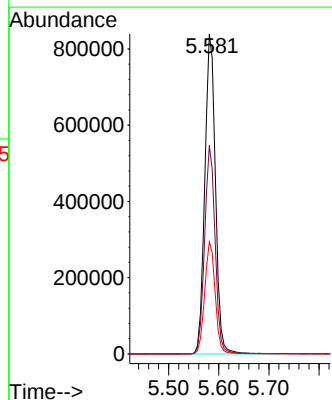
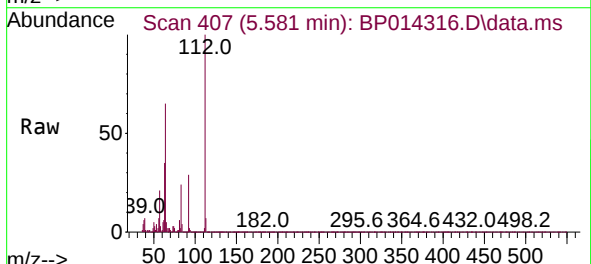




#7
Phenol-d6
Concen: 134.153 ng
RT: 7.199 min Scan# 68
Delta R.T. 0.006 min
Lab File: BP014316.D
Acq: 27 Mar 2023 17:13




Instrument :
BNA_P
ClientSampleId :
PB151659BL


Tgt Ion: 99 Resp: 1521080
Ion Ratio Lower Upper
99 100
42 18.9 15.0 22.6
71 41.0 34.3 51.5

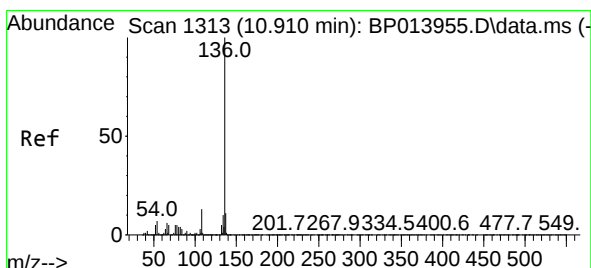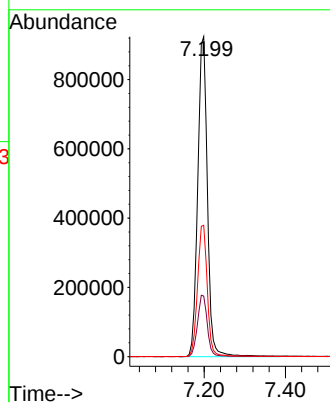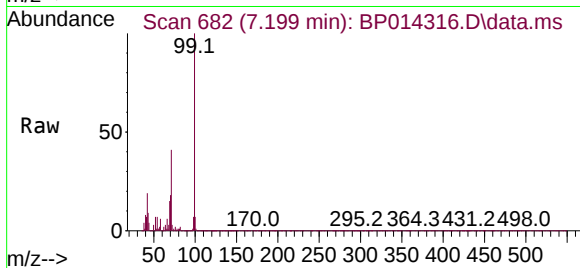

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.857 min Scan# 1304
Delta R.T. 0.006 min
Lab File: BP014316.D
Acq: 27 Mar 2023 17:13

Tgt Ion: 136 Resp: 493734
Ion Ratio Lower Upper
136 100
137 10.8 8.7 13.1
54 8.8 5.8 8.8#
68 6.2 4.0 6.0#


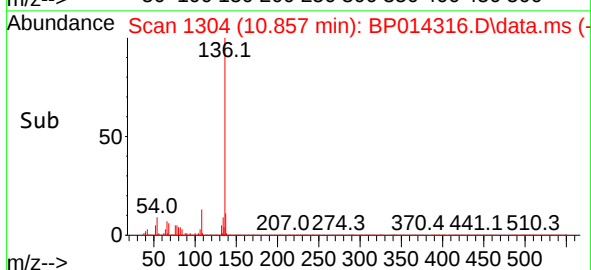
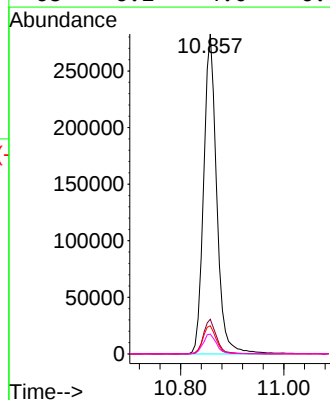
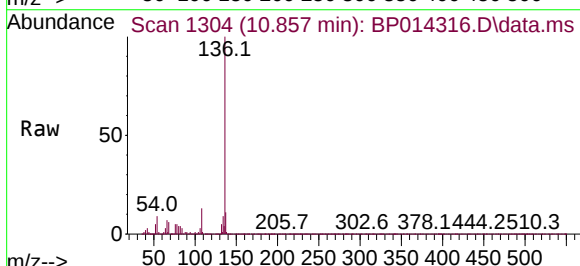




#23
Nitrobenzene-d5
Concen: 89.306 ng
RT: 9.210 min Scan# 10
Delta R.T. -0.000 min
Lab File: BP014316.D
Acq: 27 Mar 2023 17:13




Instrument :
BNA_P
ClientSampleId :
PB151659BL


Tgt Ion: 82 Resp: 964721
Ion Ratio Lower Upper
82 100
128 35.3 31.1 46.7
54 50.4 40.0 60.0

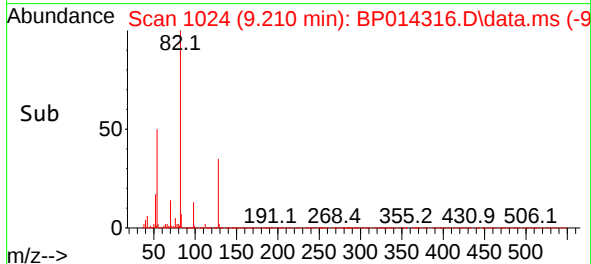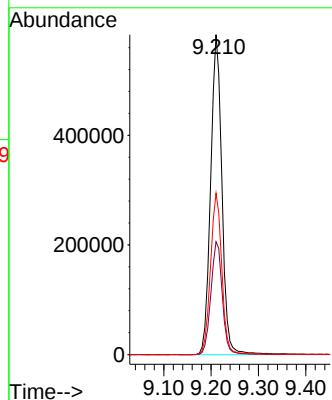

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.681 min Scan# 1954
Delta R.T. 0.006 min
Lab File: BP014316.D
Acq: 27 Mar 2023 17:13

Tgt Ion: 164 Resp: 273156
Ion Ratio Lower Upper
164 100
162 106.0 82.1 123.1
160 46.2 36.2 54.2

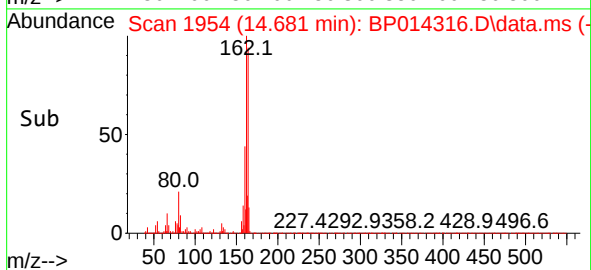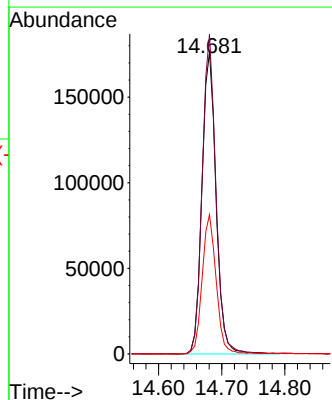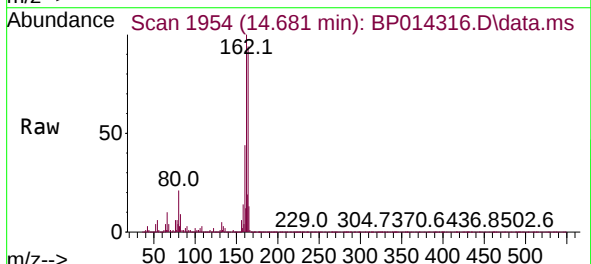

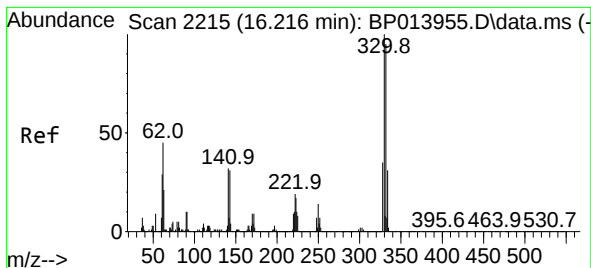

#42

2,4,6-Tribromophenol

Concen: 104.612 ng

RT: 16.175 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP014316.D

Acq: 27 Mar 2023 17:13

Instrument :

BNA_P

ClientSampleId :

PB151659BL





Tgt Ion:330 Resp: 463306

Ion Ratio Lower Upper

330 100

332 97.3 77.1 115.7

141 34.6 25.6 38.4

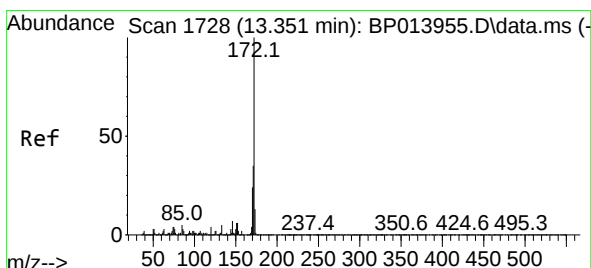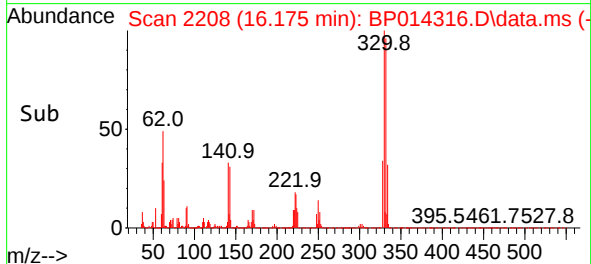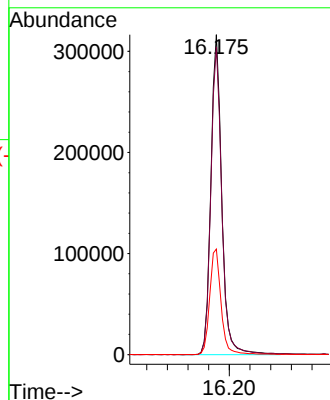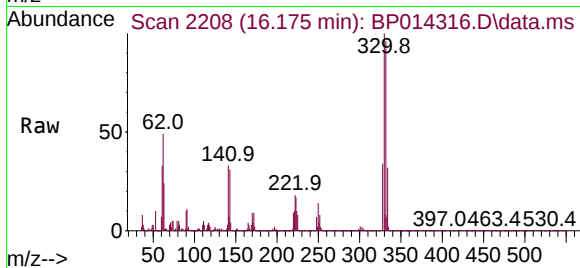

#45

2-Fluorobiphenyl

Concen: 89.753 ng

RT: 13.304 min Scan# 1720

Delta R.T. 0.006 min

Lab File: BP014316.D

Acq: 27 Mar 2023 17:13




Tgt Ion:172 Resp: 1892321


Ion Ratio Lower Upper

172 100

171 35.6 28.3 42.5

170 23.4 19.0 28.4

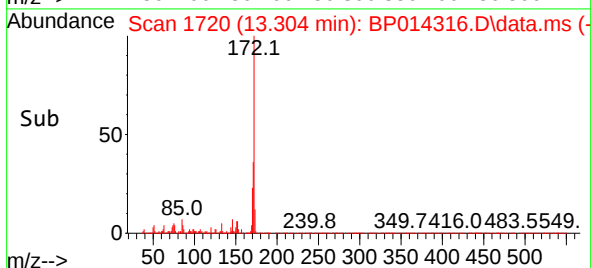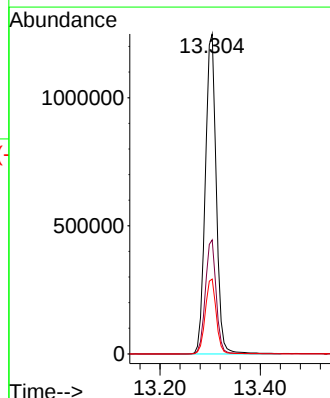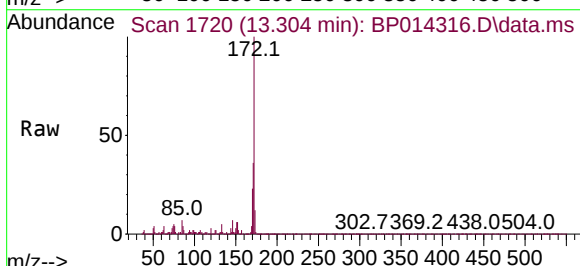

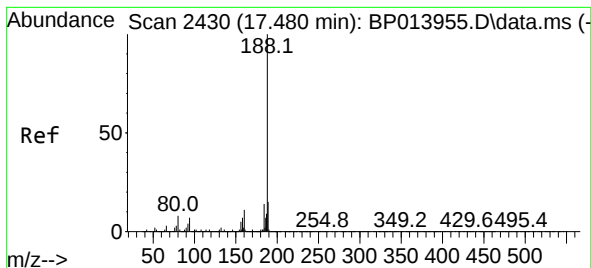

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.439 min Scan# 24

Delta R.T. 0.006 min

Lab File: BP014316.D

Acq: 27 Mar 2023 17:13

Instrument :

BNA_P

ClientSampleId :

PB151659BL





Tgt Ion:188 Resp: 502270

Ion Ratio Lower Upper

188 100

94 9.4 5.8 8.6#

80 10.4 6.6 9.8#

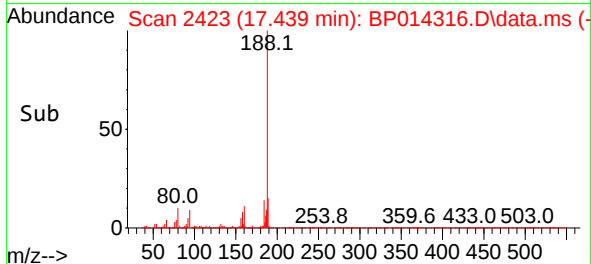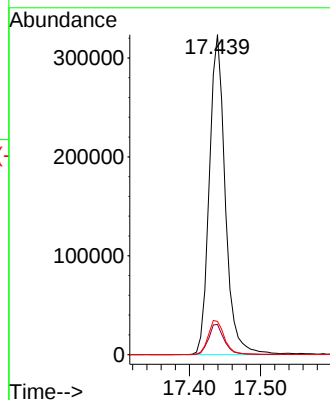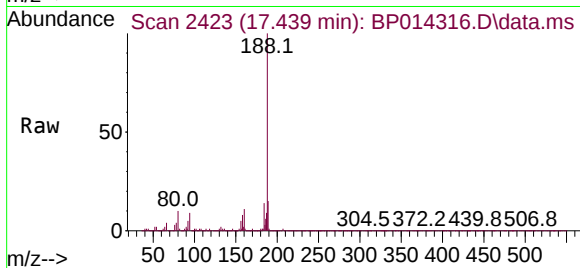

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.521 min Scan# 3117

Delta R.T. 0.006 min

Lab File: BP014316.D

Acq: 27 Mar 2023 17:13




Tgt Ion:240 Resp: 454428


Ion Ratio Lower Upper

240 100

120 9.3 6.4 9.6

236 25.9 21.2 31.8


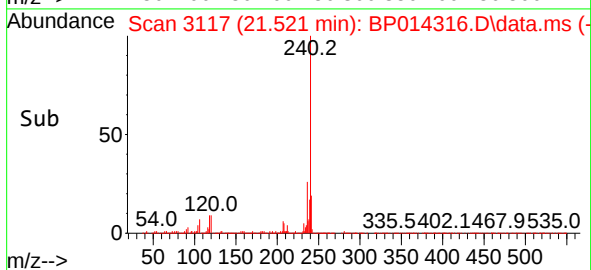
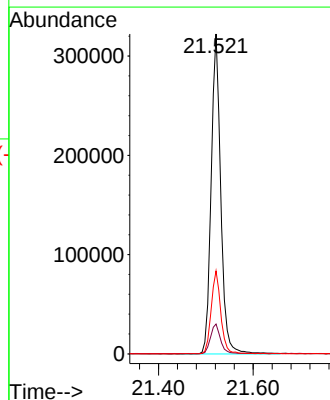
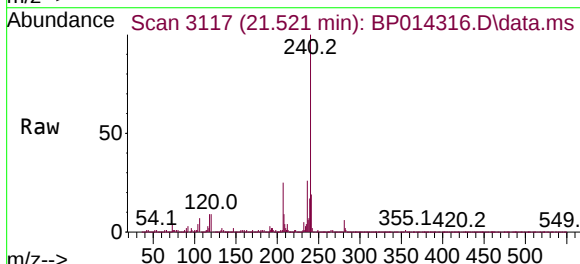




#79
 Terphenyl-d14
 Concen: 88.073 ng
 RT: 19.974 min Scan# 2861
 Delta R.T. -0.000 min
 Lab File: BP014316.D
 Acq: 27 Mar 2023 17:13

Instrument :
 BNA_P
 ClientSampleId :
 PB151659BL

Tgt Ion:244 Resp: 2427179
 Ion Ratio Lower Upper
 244 100
 212 7.6 6.0 9.0
 122 9.4 5.8 8.6#

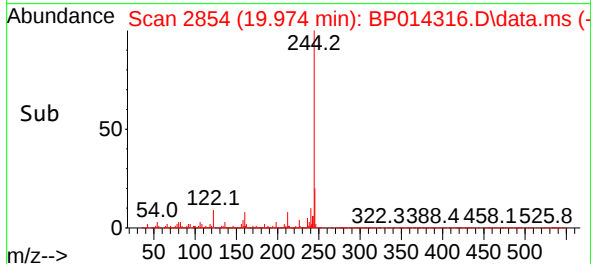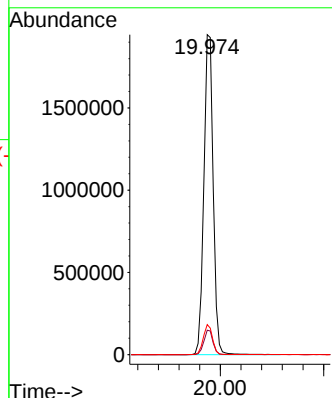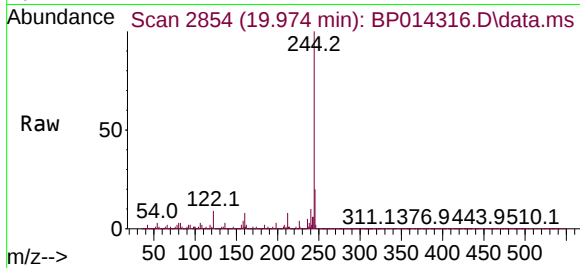

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.045 min Scan# 3546
 Delta R.T. 0.012 min
 Lab File: BP014316.D
 Acq: 27 Mar 2023 17:13

Tgt Ion:264 Resp: 534407
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.4 29.2
 265 21.6 17.8 26.8

