


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
Data File : BP014314.D
Acq On : 27 Mar 2023 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 25 03:19:01 2023

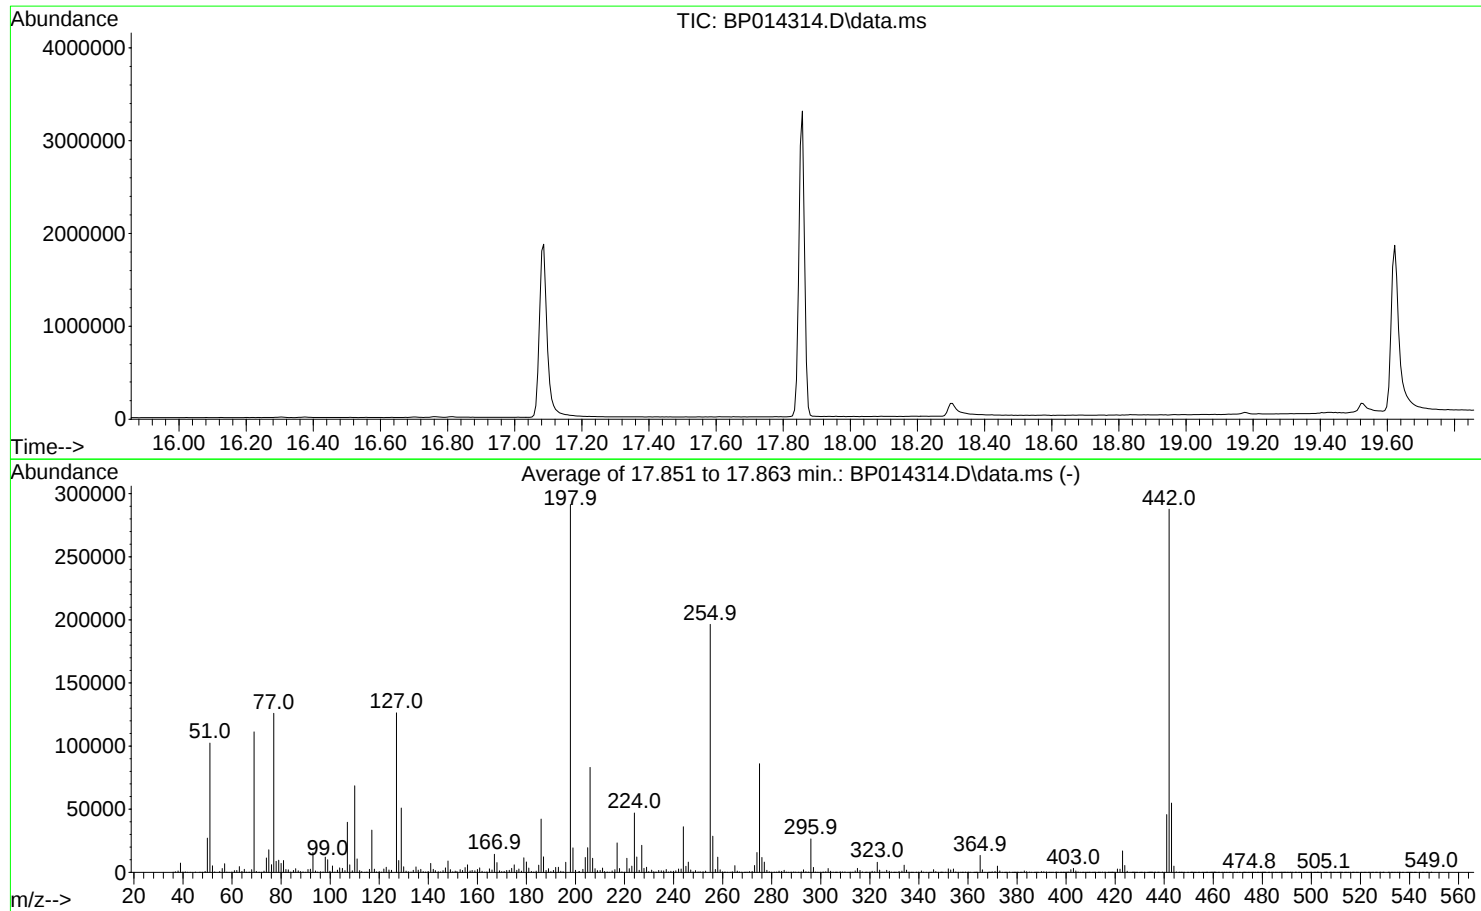




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.1	102358	PASS
68	69	0.00	2	1.9	2136	PASS
69	198	0.00	100	38.2	111232	PASS
70	69	0.00	2	0.6	701	PASS
127	198	10	80	43.3	126349	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	291474	PASS
199	198	5	9	6.6	19366	PASS
275	198	10	60	29.5	85979	PASS
365	198	1	100	4.6	13328	PASS
441	198	0.01	100	15.7	45765	PASS
442	442	100	100	100.0	287802	PASS
443	442	15	24	19.1	54875	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
Data File : BP014314.D
Acq On : 27 Mar 2023 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 28 03:21:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 03:19:01 2023
Response via : Initial Calibration

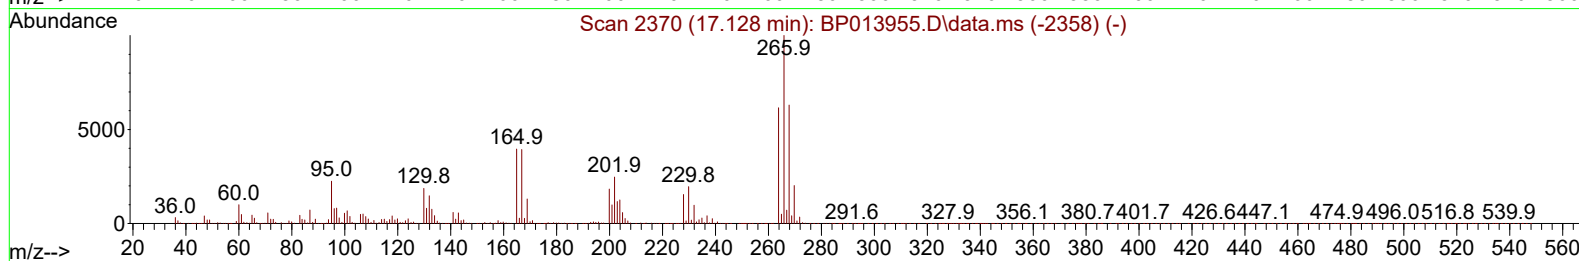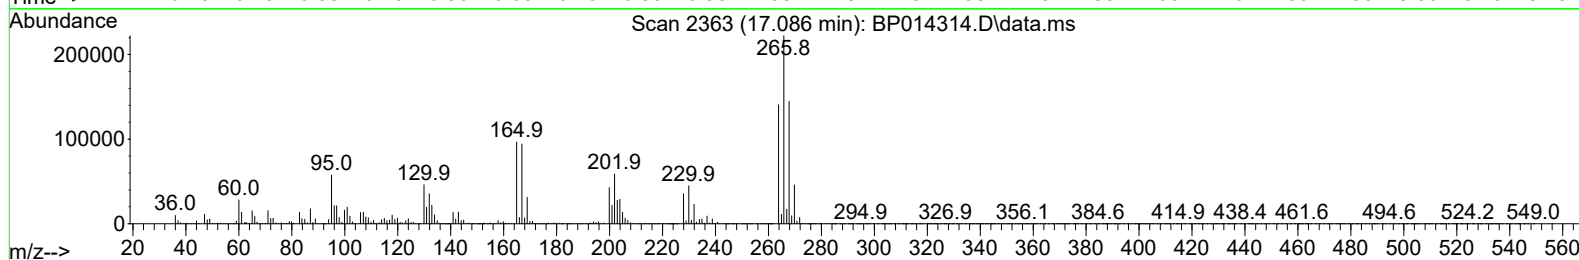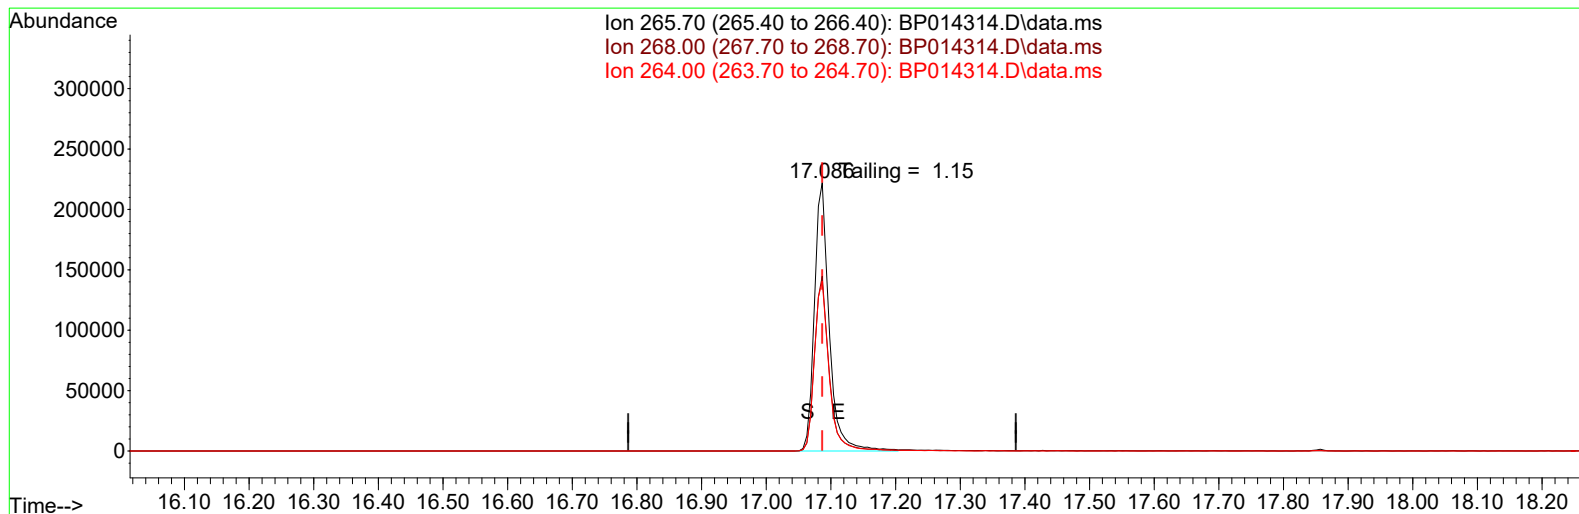

TIC: BP014314.D\data.ms

(70) Pentachlorophenol (C)

17.086min (+ 0.000) 3871430.94 ng




response 356283

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.12
264.00	61.50	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032723\
Data File : BP014314.D
Acq On : 27 Mar 2023 15:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 28 03:21:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP030623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 25 03:19:01 2023
Response via : Initial Calibration

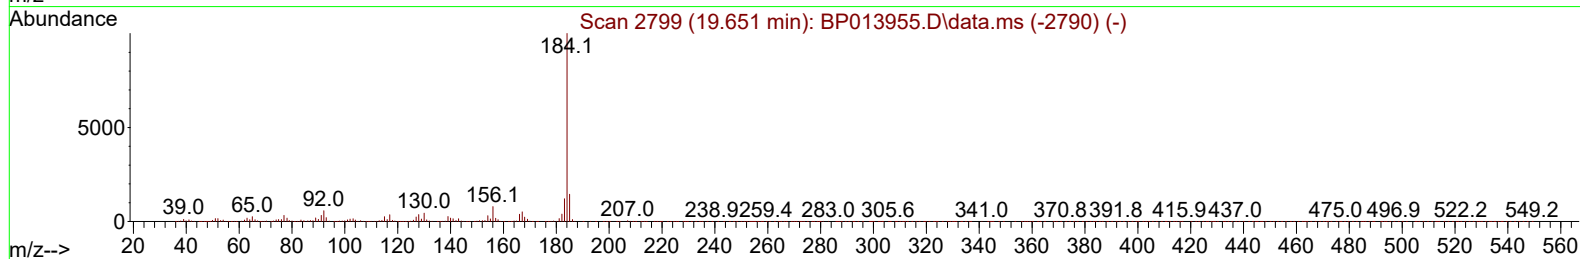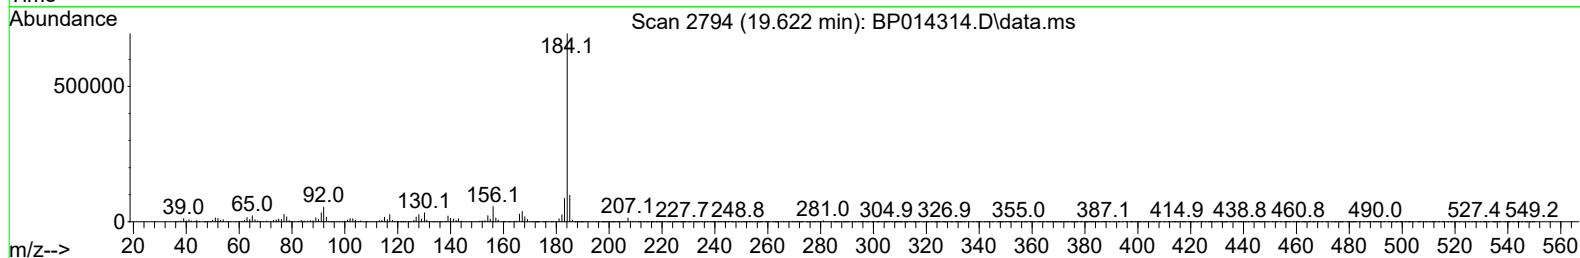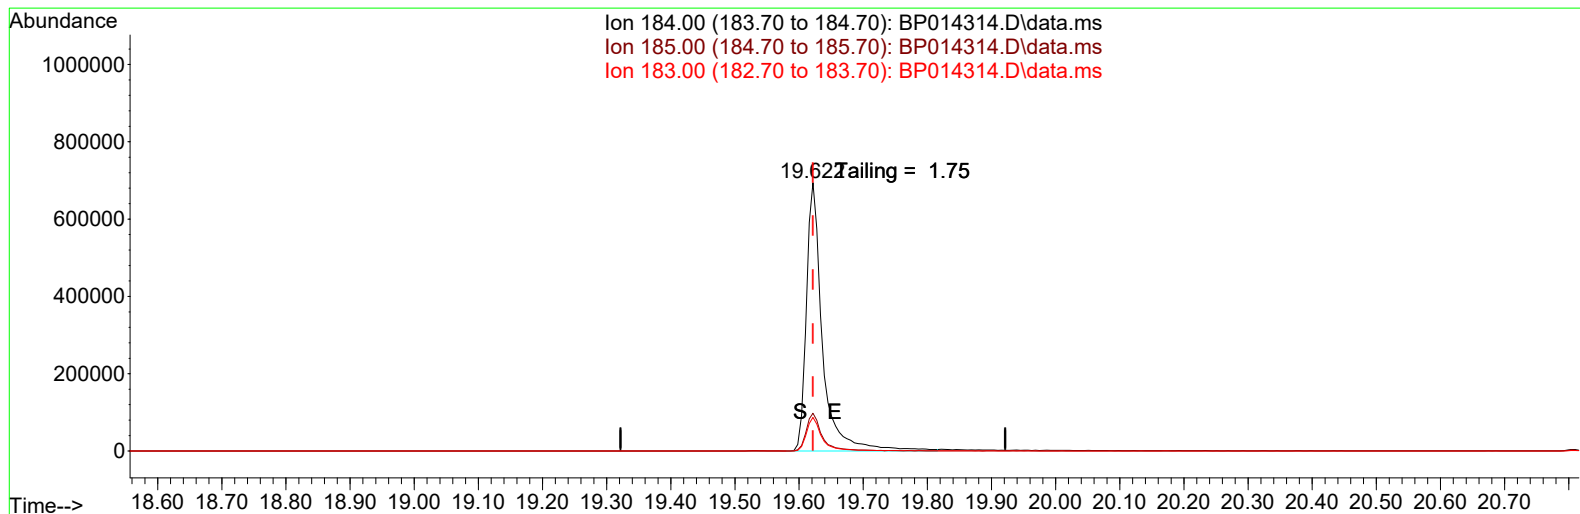

TIC: BP014314.D\data.ms

(77) Benzidine

19.622min (0.000) -20.00 ng

response 1221570

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.07
183.00	12.10	12.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/27/2023	BNA_P	<u>BP014314.D</u>
Compound Name	Response	Retention Time
DDT	885261	20.81
DDD	12825	20.38
DDE	630	19.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13455	898716	1.50

Instrument :
BNA_P
ClientSampleId :
DFTPP