
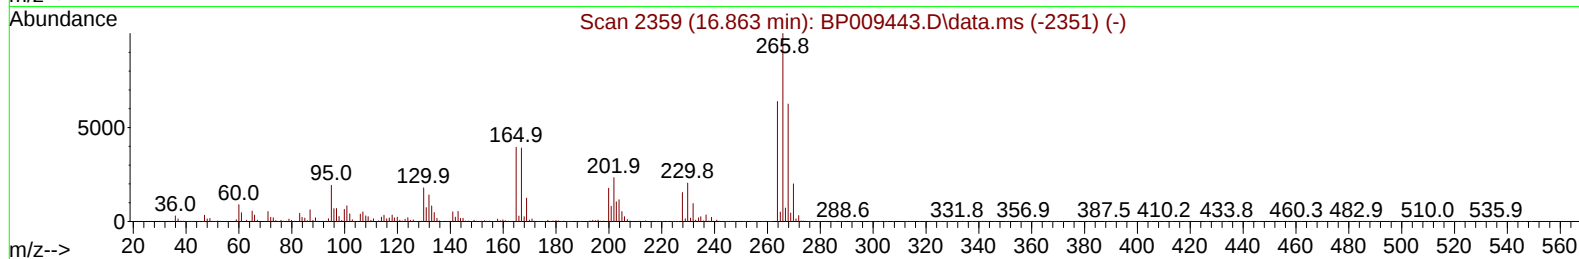
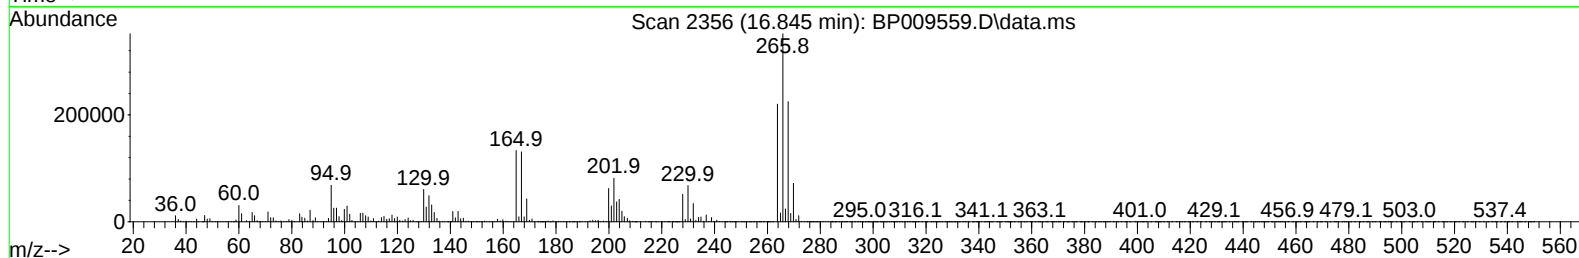


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
Data File : BP009559.D
Acq On : 28 Mar 2022 09:42
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 09:22:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 06:34:38 2022
Response via : Initial Calibration

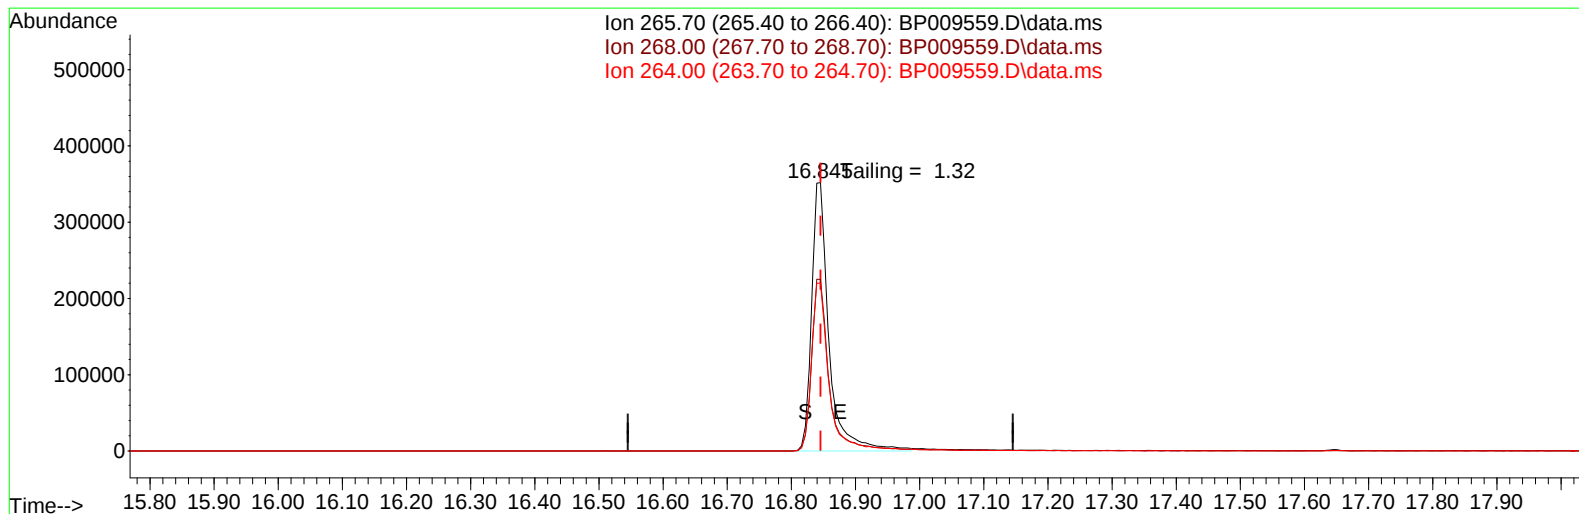

TIC: BP009559.D\data.ms

(70) Pentachlorophenol (C)




16.845min (-0.000) 1619870.00 ng

response 670711

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.95
264.00	63.60	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009559.D
 Acq On : 28 Mar 2022 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 09:22:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

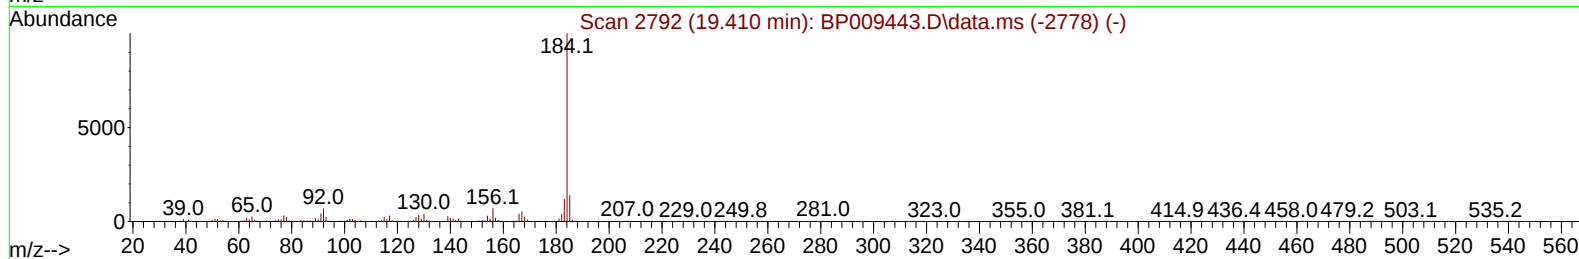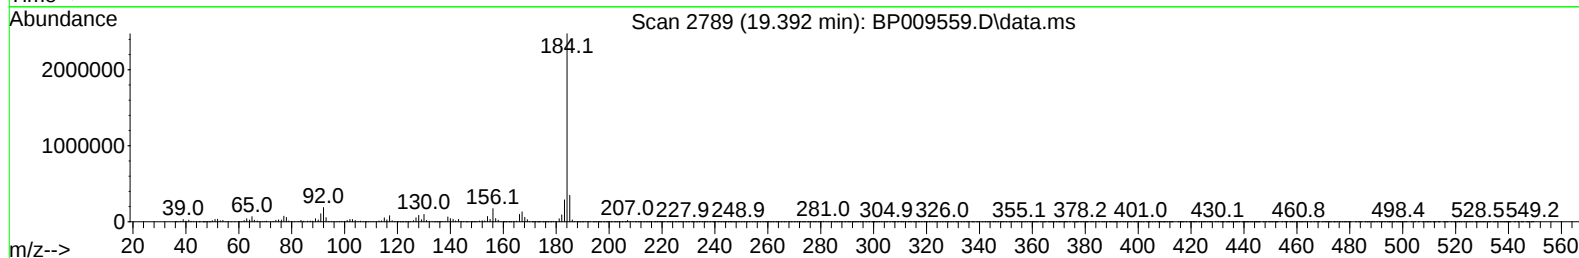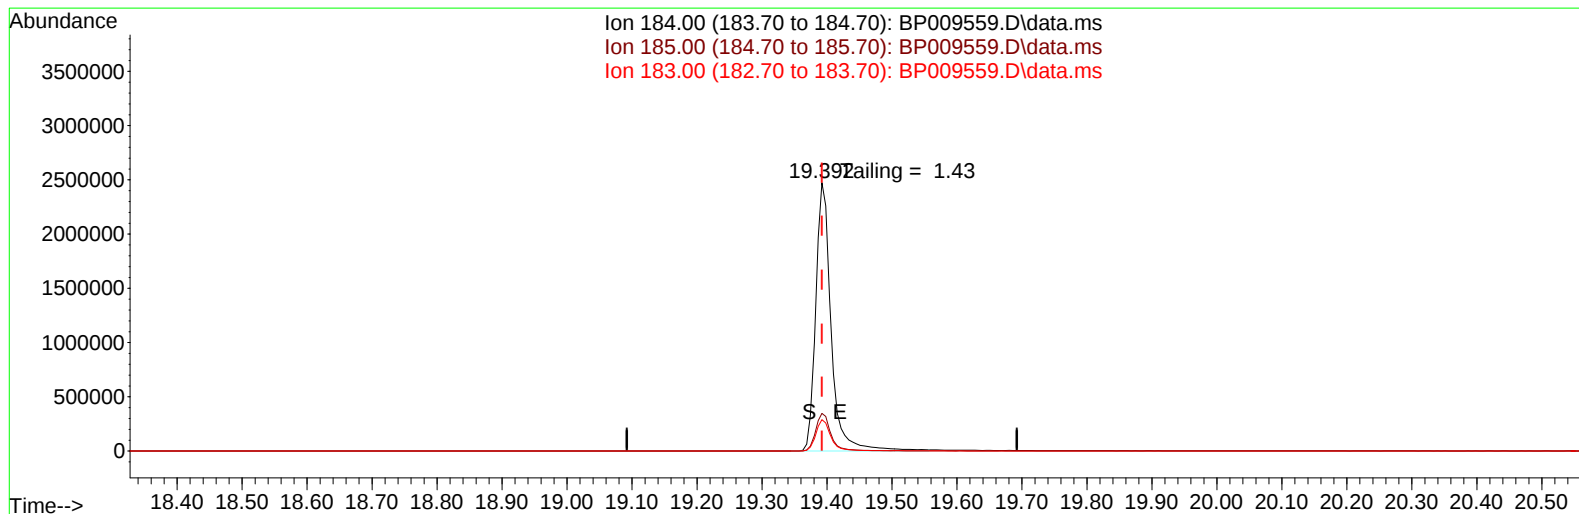

TIC: BP009559.D\data.ms

(77) Benzidine**19.392min (-0.000) 733666.92 ng****response 4100157**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	11.70	11.68
0.00	0.00	0.00