

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009579.D
 Acq On : 28 Mar 2022 22:51
 Operator : CG/JU
 Sample : N2098-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 V-2-0309-2B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009579.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.017	3	5	20	rVB	554886	736212	5.96%	0.681%
2	4.317	220	226	239	rBV	1059546	1639003	13.26%	1.516%
3	4.905	320	326	342	rBV	1109891	1784568	14.44%	1.651%
4	5.370	397	405	434	rBV	1832332	3377663	27.33%	3.124%
5	6.958	664	675	705	rBV	2560348	5070934	41.03%	4.690%
6	7.764	805	812	821	rBV	938718	1638259	13.25%	1.515%
7	7.858	822	828	839	rVB	238179	447253	3.62%	0.414%
8	8.028	848	857	870	rBV7	38101	142291	1.15%	0.132%
9	8.446	918	928	935	rBV2	80988	154082	1.25%	0.143%
10	8.922	997	1009	1020	rBV	1902584	3613874	29.24%	3.343%
11	9.005	1020	1023	1034	rVB3	63112	128594	1.04%	0.119%
12	9.358	1077	1083	1096	rVB4	59160	146061	1.18%	0.135%
13	10.558	1278	1287	1293	rBV	1191060	2293181	18.55%	2.121%
14	11.999	1523	1532	1540	rBV2	71172	144416	1.17%	0.134%
15	12.228	1561	1571	1579	rVB2	67696	143854	1.16%	0.133%
16	13.034	1700	1708	1728	rBV	5104571	8439565	68.28%	7.806%
17	13.246	1739	1744	1757	rVB	112084	185799	1.50%	0.172%
18	14.134	1889	1895	1909	rBV	205303	381859	3.09%	0.353%
19	14.410	1934	1942	1949	rVV	1886962	3099060	25.07%	2.867%
20	14.475	1949	1953	1963	rVB	152601	268819	2.17%	0.249%
21	14.816	2005	2011	2018	rVB	110730	197827	1.60%	0.183%
22	15.463	2117	2121	2134	rVB2	151393	304276	2.46%	0.281%
23	15.763	2168	2172	2181	rVB	68119	141680	1.15%	0.131%
24	15.910	2191	2197	2206	rBV	1177394	2028687	16.41%	1.876%
25	16.151	2233	2238	2240	rBV	132813	206328	1.67%	0.191%
26	16.834	2349	2354	2360	rVB2	94281	162219	1.31%	0.150%
27	16.998	2378	2382	2391	rVB2	181606	343040	2.78%	0.317%
28	17.175	2406	2412	2416	rBV	2387528	3811777	30.84%	3.526%
29	17.216	2416	2419	2426	rVV	2123253	3250035	26.30%	3.006%
30	17.310	2430	2435	2441	rVV	619167	983028	7.95%	0.909%
31	17.375	2442	2446	2452	rVB3	76720	140940	1.14%	0.130%
32	17.587	2478	2482	2492	rBV	178047	339618	2.75%	0.314%
33	17.698	2497	2501	2508	rVB3	136233	193137	1.56%	0.179%
34	17.881	2527	2532	2540	rVB	1695346	2524125	20.42%	2.335%
35	18.051	2557	2561	2564	rBV	250691	347305	2.81%	0.321%
36	18.098	2565	2569	2574	rVV	422413	640713	5.18%	0.593%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009579.D
 Acq On : 28 Mar 2022 22:51
 Operator : CG/JU
 Sample : N2098-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 V-2-0309-2B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.145	2574	2577	2580	rVV	136061	194403	1.57%	0.180%
38	18.175	2580	2582	2587	rVV	157370	225724	1.83%	0.209%
39	18.239	2588	2593	2597	rVV2	472821	846378	6.85%	0.783%
40	18.275	2597	2599	2606	rVB	219917	280785	2.27%	0.260%
41	18.539	2640	2644	2648	rBV	241525	327100	2.65%	0.303%
42	18.586	2648	2652	2658	rVB2	126711	195687	1.58%	0.181%
43	18.945	2709	2713	2716	rBV	183860	261743	2.12%	0.242%
44	18.986	2717	2720	2726	rVV5	118693	232733	1.88%	0.215%
45	19.081	2732	2736	2743	rVB	266137	446857	3.62%	0.413%
46	19.198	2751	2756	2764	rBV	5101371	7316925	59.20%	6.768%
47	19.345	2777	2781	2787	rBV	458924	680745	5.51%	0.630%
48	19.557	2807	2817	2825	rBV	4511361	7437465	60.18%	6.879%
49	19.628	2826	2829	2836	rVB2	205550	329586	2.67%	0.305%
50	19.757	2844	2851	2856	rBV	9360431	12359714	100.00%	11.432%
51	20.039	2897	2899	2903	rVB	264904	297001	2.40%	0.275%
52	20.139	2913	2916	2920	rBV	188265	228671	1.85%	0.212%
53	20.439	2963	2967	2972	rVB	1543072	1744964	14.12%	1.614%
54	20.780	3022	3025	3032	rVB	370797	475102	3.84%	0.439%
55	21.286	3105	3111	3116	rBV2	4080660	8378793	67.79%	7.750%
56	21.328	3116	3118	3128	rVB	1990515	2555934	20.68%	2.364%
57	21.410	3129	3132	3136	rBV	595389	740234	5.99%	0.685%
58	22.963	3390	3396	3409	rBV	2083325	6021431	48.72%	5.570%
59	23.580	3496	3501	3510	rVB	1597901	3543687	28.67%	3.278%
60	23.686	3514	3519	3525	rVV2	1759252	3540213	28.64%	3.275%


Sum of corrected areas: 108111957

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
Data File : BP009579.D
Acq On : 28 Mar 2022 22:51
Operator : CG/JU
Sample : N2098-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
V-2-0309-2B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

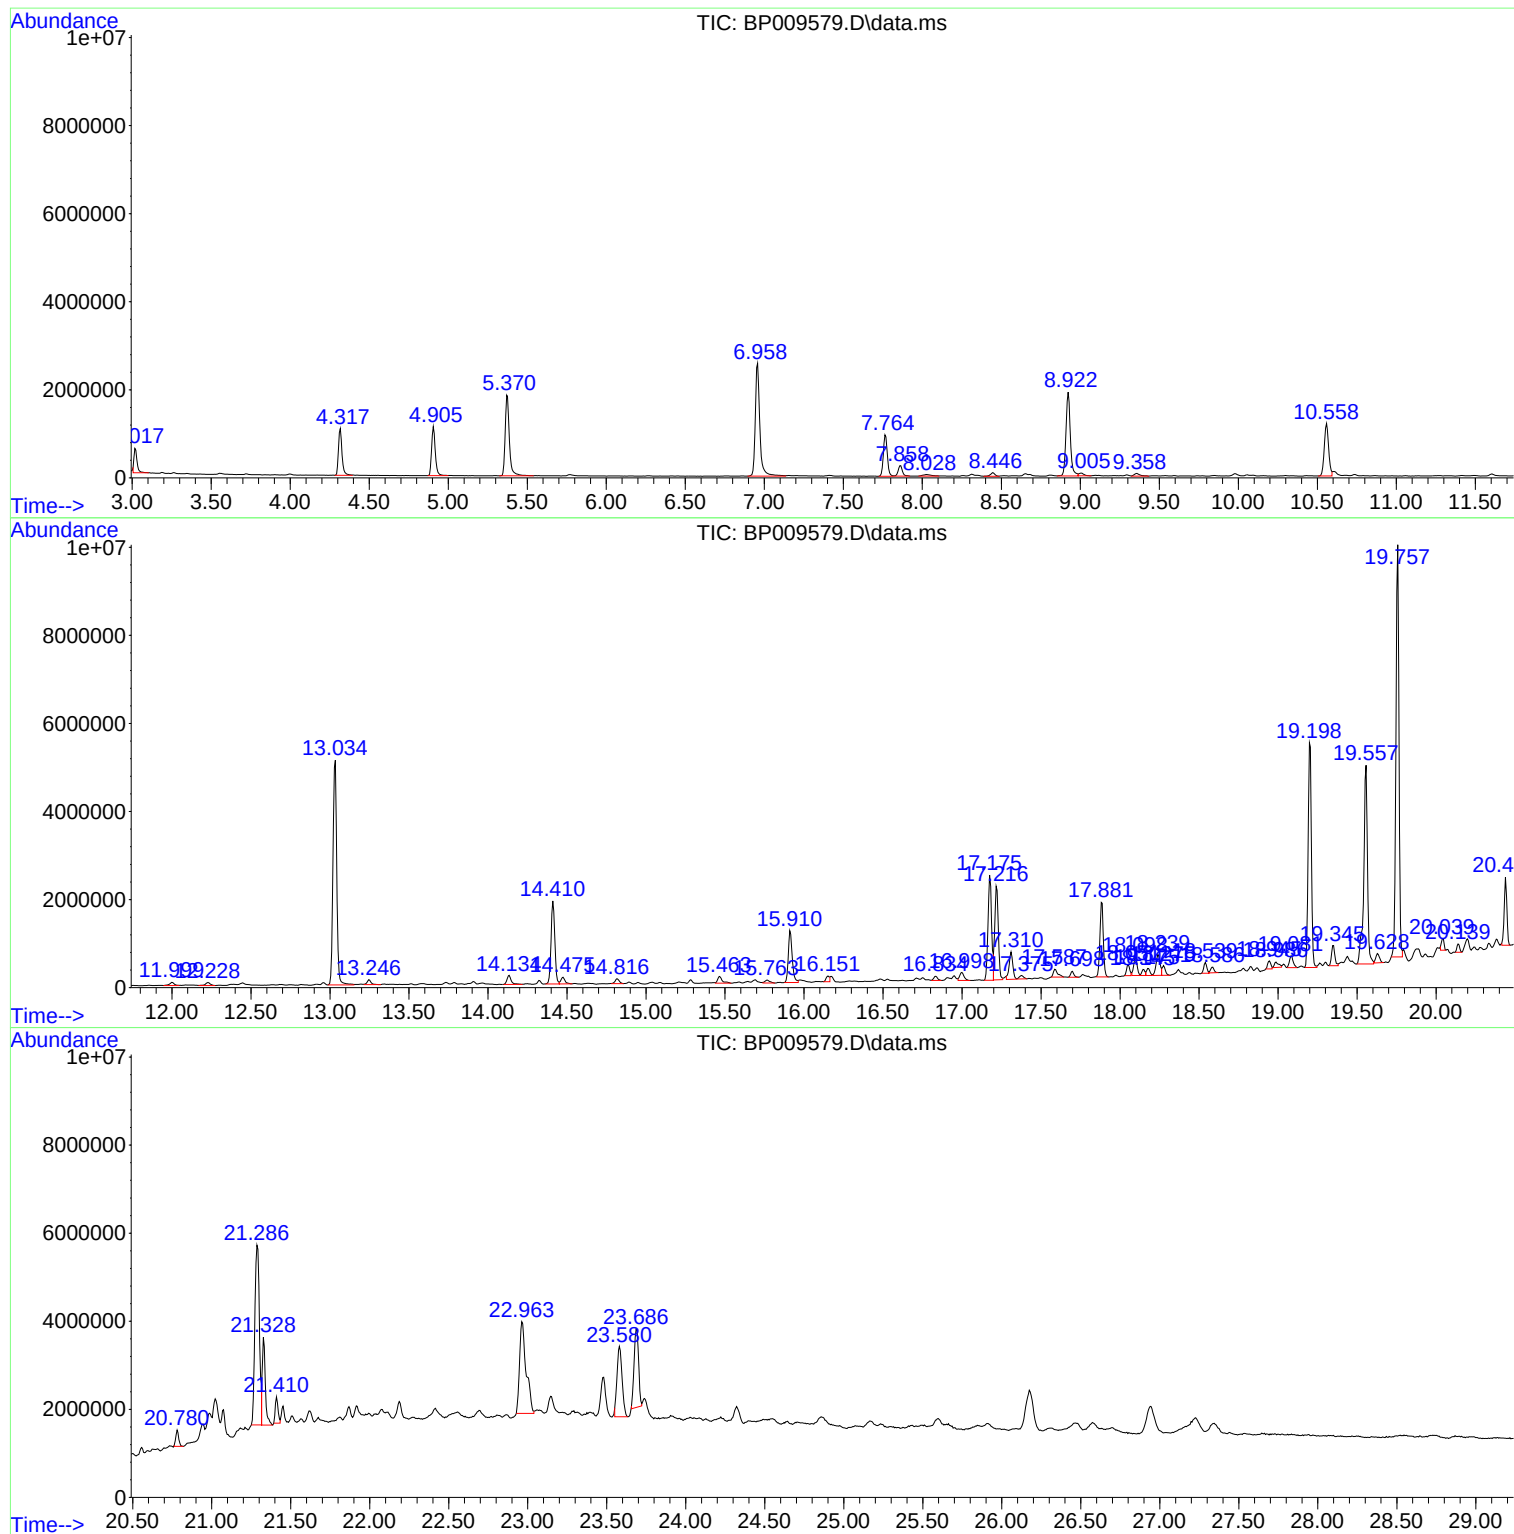

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
Data File : BP009579.D
Acq On : 28 Mar 2022 22:51
Operator : CG/JU
Sample : N2098-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
V-2-0309-2B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
Data File : BP009579.D
Acq On : 28 Mar 2022 22:51
Operator : CG/JU
Sample : N2098-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
V-2-0309-2B

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------