
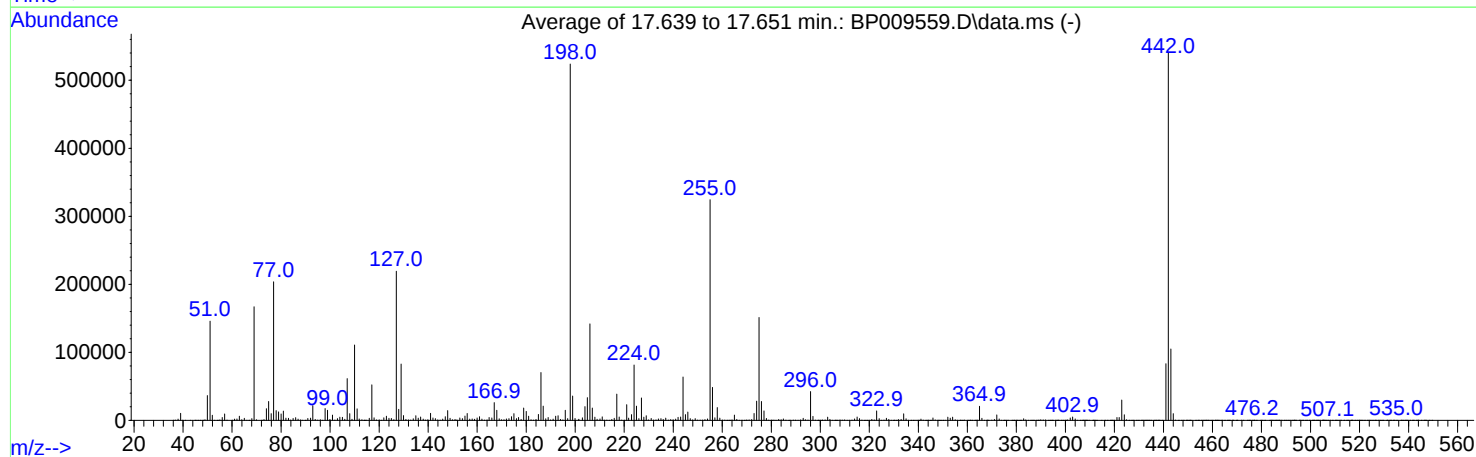


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009559.D
 Acq On : 28 Mar 2022 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 06:34:38 2022

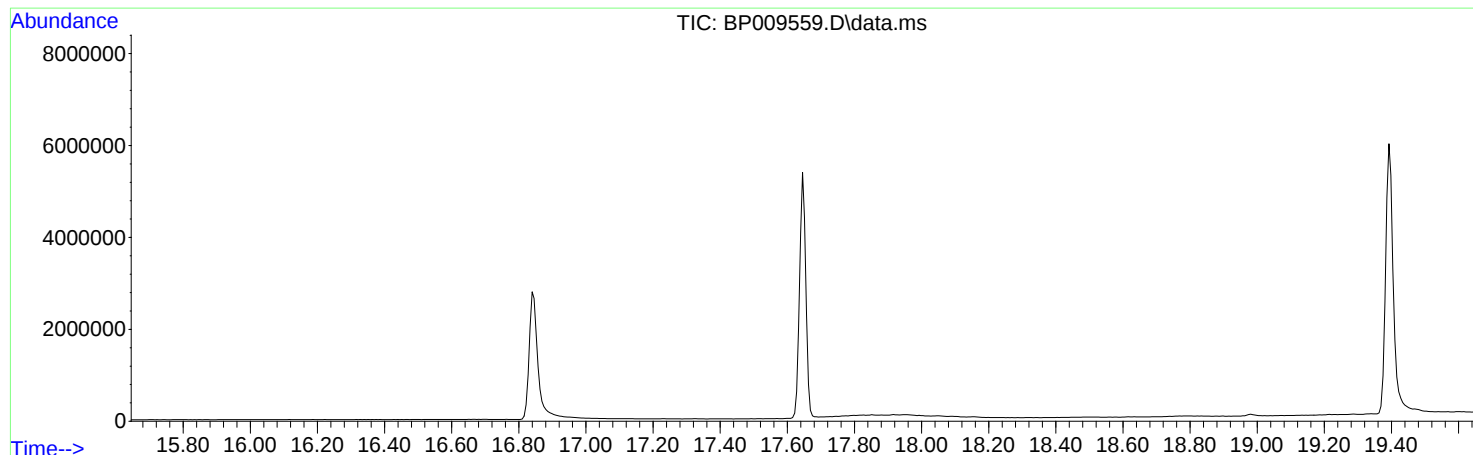


AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	145942	PASS
68	69	0.00	2	1.6	2699	PASS
69	198	0.00	100	31.9	167089	PASS
70	69	0.00	2	0.5	877	PASS
127	198	10	80	41.9	219254	PASS
197	198	0.00	2	0.5	2591	PASS
198	198	100	100	100.0	523777	PASS
199	198	5	9	6.8	35734	PASS
275	198	10	60	28.9	151380	PASS
365	198	1	100	3.9	20646	PASS
441	198	0.01	100	15.9	83291	PASS
442	442	100	100	100.0	540814	PASS
443	442	15	24	19.4	104854	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009559.D
 Acq On : 28 Mar 2022 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 09:22:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

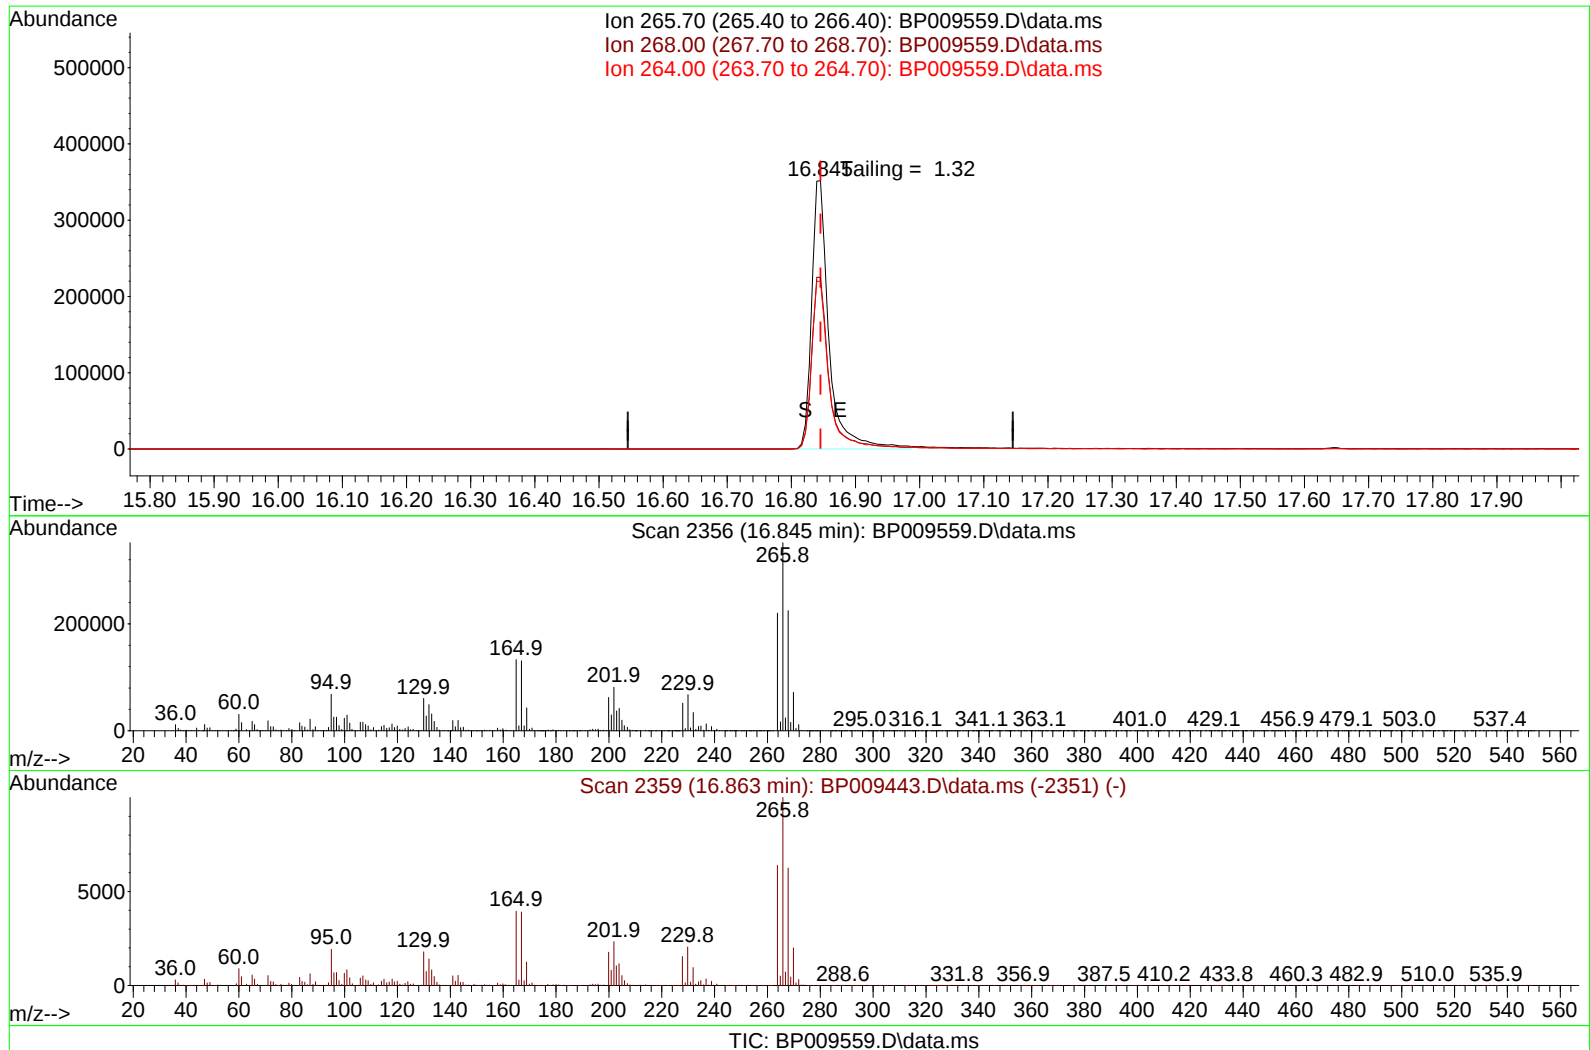

TIC: BP009559.D\data.ms

(70) Pentachlorophenol (C)

16.845min (-0.000) 1619870.00 ng




response 670711

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.95
264.00	63.60	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009559.D
 Acq On : 28 Mar 2022 09:42
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 09:22:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

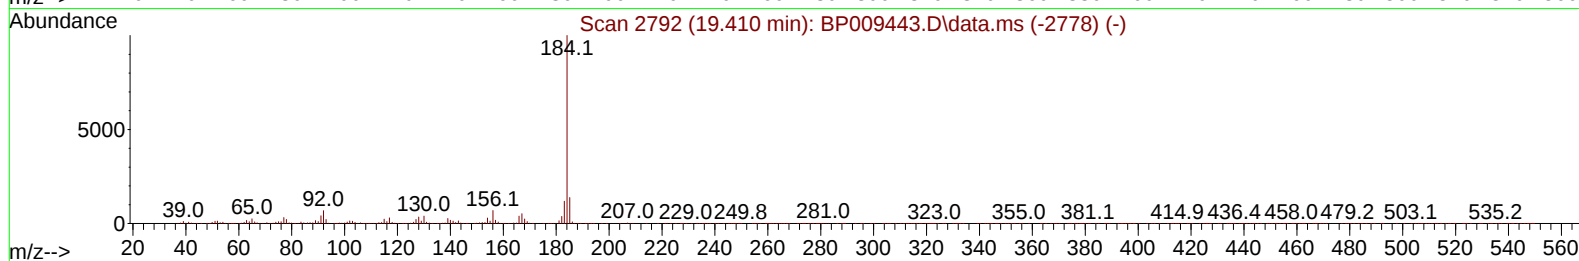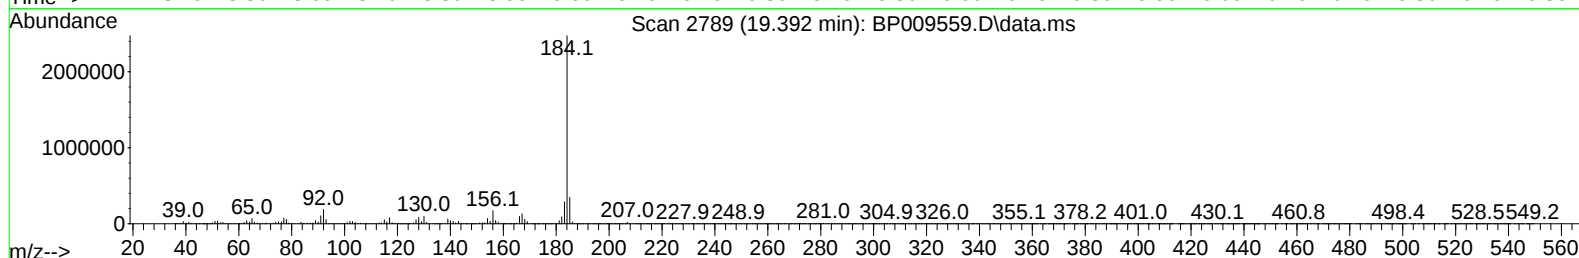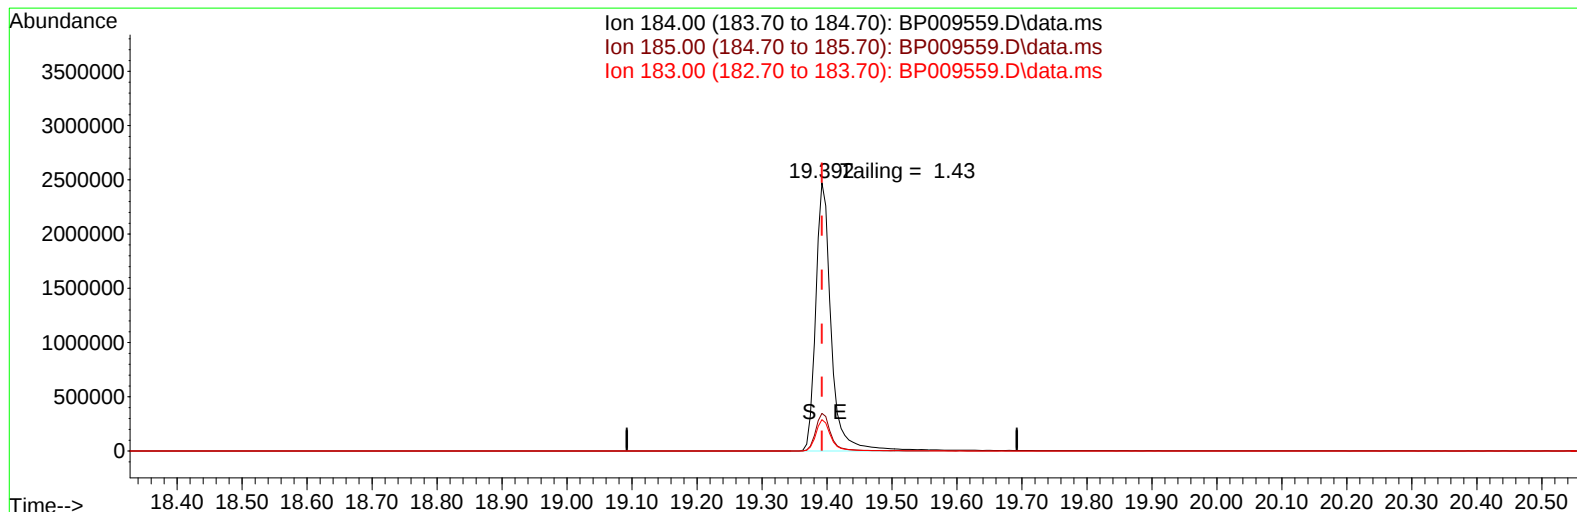

TIC: BP009559.D\data.ms

(77) Benzidine

19.392min (-0.000) 733666.92 ng

response 4100157

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.04
183.00	11.70	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2022	BNA_P	<u>BP009559.D</u>
Compound Name	Response	Retention Time
DDT	2018382	20.604
DDD	53607	20.175
DDE	7073	19.68
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
60680	2079062	2.92

Instrument :
BNA_P
ClientSampleId :
DFTPP