
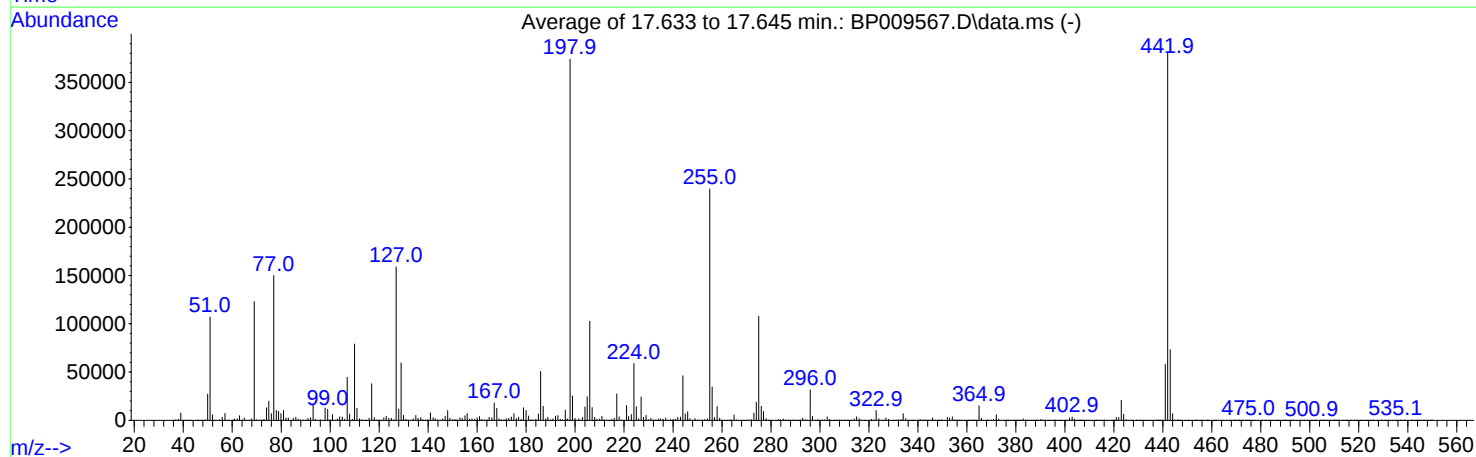


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009567.D
 Acq On : 28 Mar 2022 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 06:34:38 2022

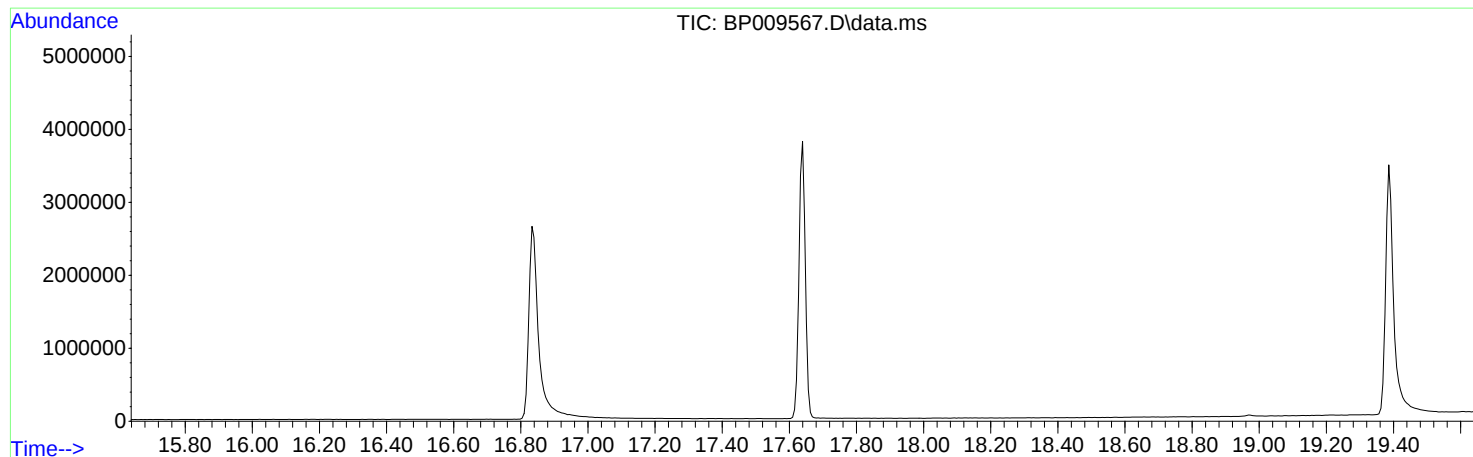


AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.6	107008	PASS
68	69	0.00	2	1.4	1729	PASS
69	198	0.00	100	32.9	122957	PASS
70	69	0.00	2	0.5	614	PASS
127	198	10	80	42.5	158963	PASS
197	198	0.00	2	0.4	1370	PASS
198	198	100	100	100.0	373931	PASS
199	198	5	9	6.8	25371	PASS
275	198	10	60	28.8	107768	PASS
365	198	1	100	4.0	15011	PASS
441	198	0.01	100	15.5	57981	PASS
442	442	100	100	100.0	380921	PASS
443	442	15	24	19.2	73291	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009567.D
 Acq On : 28 Mar 2022 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 09:27:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

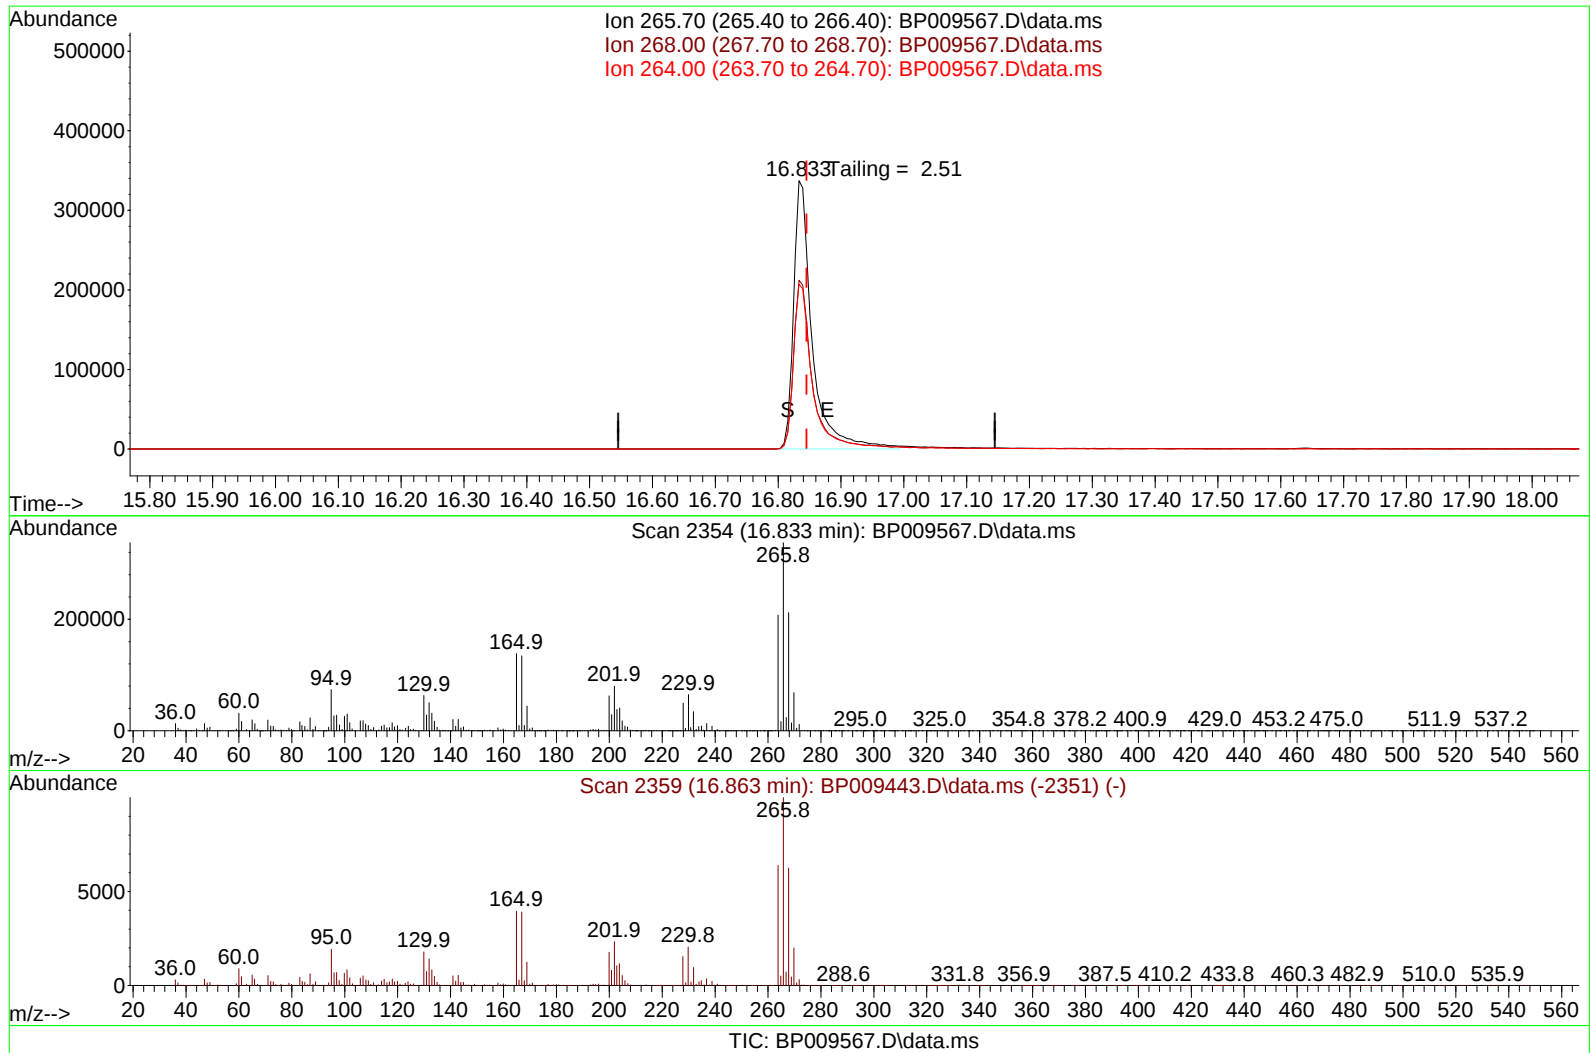

(70) Pentachlorophenol (C)

16.833min (-0.012) 238195.18 ng




response 710102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.85
264.00	63.60	61.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032822\
 Data File : BP009567.D
 Acq On : 28 Mar 2022 16:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 29 09:27:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

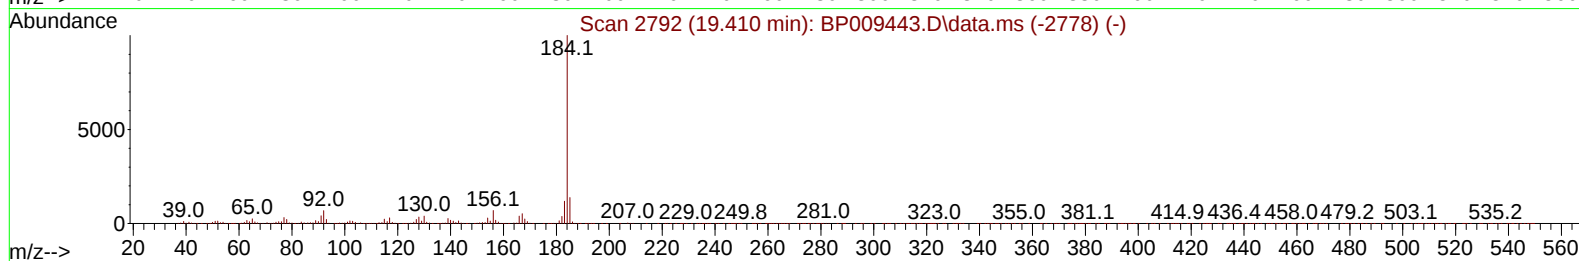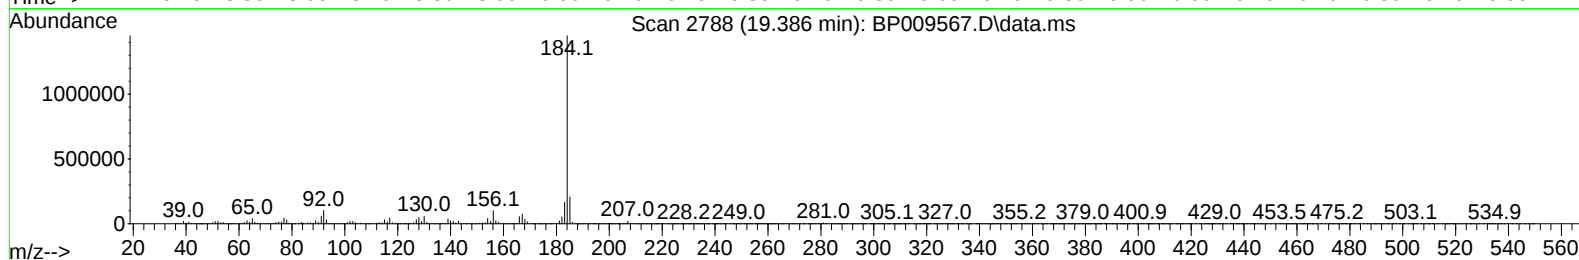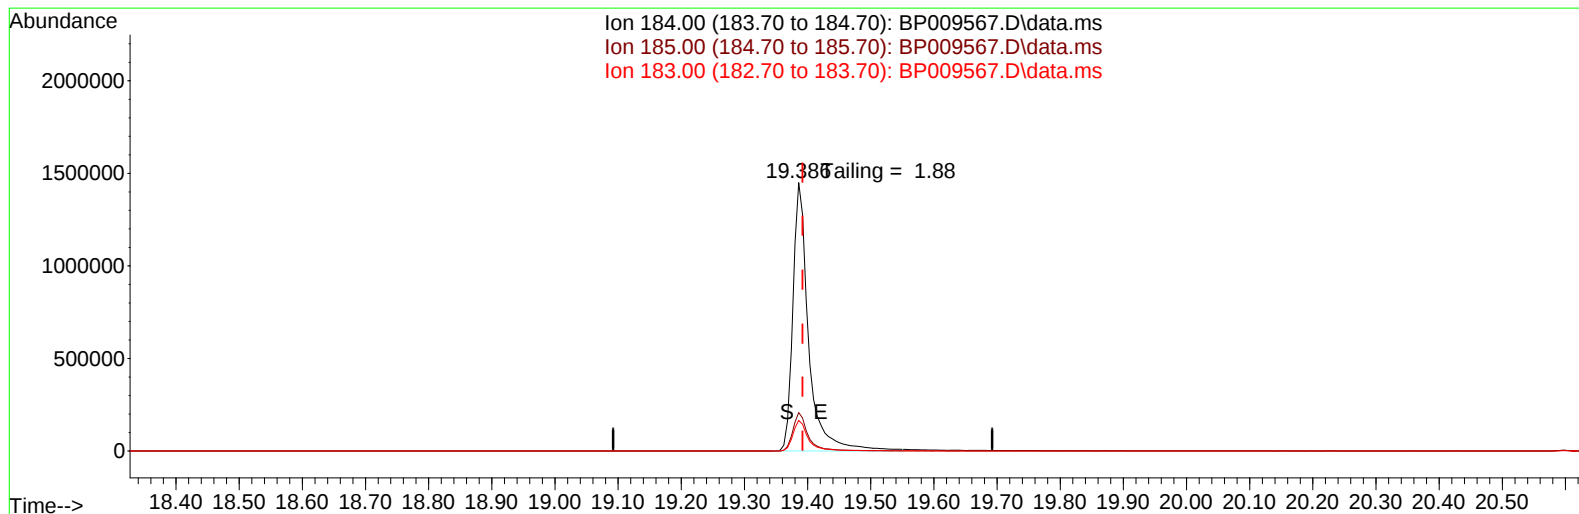

TIC: BP009567.D\data.ms

(77) Benzidine

19.386min (-0.006) 33254.26 ng

response 2543130

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.30
183.00	11.70	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/28/2022	BNA_P	<u>BP009567.D</u>
Compound Name	Response	Retention Time
DDT	1229247	20.598
DDD	19407	20.168
DDE	2688	19.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22095	1251342	1.77

Instrument :
BNA_P
ClientSampleId :
DFTPP