

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032823\
 Data File : BP014339.D
 Acq On : 28 Mar 2023 12:29
 Operator : CG/JU
 Sample : SST02043
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SST020626

Quant Time: Mar 29 00:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 00:54:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	254105	20.000	ng/u1	0.01
20) Naphthalene-d8	10.857	136	991696	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.687	164	627013	20.000	ng/u1	0.01
64) Phenanthrene-d10	17.445	188	1392151	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1500892	20.000	ng/u1	0.01
88) Perylene-d12	24.057	264	1760997	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.399	96	31080	4.743	ng/uL	0.00
4) Pyridine-d5	3.834	84	178743	10.728	ng/u1	0.00
7) Phenol-d5	7.193	99	253189	10.804	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.358	67	162085	10.780	ng/u1	0.01
11) 2-Chlorophenol-d4	7.558	132	186306	10.999	ng/u1	0.00
15) 4-Methylphenol-d8	8.746	113	194046	10.265	ng/u1	0.00
21) Nitrobenzene-d5	9.210	128	92240	11.522	ng/u1	0.01
24) 2-Nitrophenol-d4	9.934	143	100580	10.972	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.475	165	190258	11.396	ng/u1	0.00
31) 4-Chloroaniline-d4	10.999	131	235036	10.688	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	562323	11.061	ng/u1	0.00
49) Acenaphthylene-d8	14.375	160	627331	11.121	ng/u1	0.00
54) 4-Nitrophenol-d4	14.892	143	90517	11.785	ng/u1	0.00
60) Fluorene-d10	15.681	176	475532	11.216	ng/u1	0.01
65) 4,6-Dinitro-2-methylph...	15.804	200	106500	10.397	ng/u1	0.00
73) Anthracene-d10	17.545	188	732172	10.867	ng/u1	0.00
81) Pyrene-d10	19.775	212	932888	9.254	ng/u1	0.01
92) Benzo(a)pyrene-d12	23.892	264	1022894	10.933	ng/u1	0.01
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.434	88	33576	4.663	ng/uL	97
5) Pyridine	3.852	79	189547	10.596	ng/u1	98
6) Benzaldehyde	7.169	77	155496	13.515	ng/u1	97
8) Phenol	7.216	94	265299	10.913	ng/u1	99
10) Bis(2-Chloroethyl)ether	7.452	93	207720	10.633	ng/u1	100
12) 2-Chlorophenol	7.593	128	193620	10.983	ng/u1	98
13) 2-Methylphenol	8.481	108	190666	10.517	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.563	45	274402	10.699	ng/u1	99
16) Acetophenone	8.869	105	324291	10.389	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.846	70	174927	10.373	ng/u1	97
18) 4-Methylphenol	8.810	108	209626	10.528	ng/u1	95
19) Hexachloroethane	9.116	117	87841	11.404	ng/u1	94
22) Nitrobenzene	9.252	77	264509	11.501	ng/u1	99
23) Isophorone	9.775	82	447472	10.555	ng/u1	98
25) 2-Nitrophenol	9.969	139	109621	11.329	ng/u1	97
26) 2,4-Dimethylphenol	10.022	107	236435	10.969	ng/u1	97
27) Bis(2-Chloroethoxy)met...	10.257	93	275491	10.839	ng/u1	99
29) 2,4-Dichlorophenol	10.504	162	187719	11.425	ng/u1	90
30) Naphthalene	10.904	128	618043	11.189	ng/u1	98
32) 4-Chloroaniline	11.028	127	242539	10.889	ng/u1	99
33) Hexachlorobutadiene	11.181	225	147987	11.369	ng/u1	95
34) Caprolactam	11.816	113	18339	3.865	ng/u1	96
35) 4-Chloro-3-methylphenol	12.146	107	221838	10.977	ng/u1	98
36) 2-Methylnaphthalene	12.510	142	405516	10.832	ng/u1	100

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032823\
 Data File : BP014339.D
 Acq On : 28 Mar 2023 12:29
 Operator : CG/JU
 Sample : SSTD02043
 Misc :
 ALS Vial : 4 Sample Multiplier: 1


Instrument :
 BNA_P
 ClientSampleId :
 SSTD020626


Quant Time: Mar 29 00:59:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 29 00:54:55 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.728	142	404499	10.895	ng/ul	94
39) 1,2,4,5-Tetrachloroben...	12.875	216	252463	11.293	ng/ul	98
40) Hexachlorocyclopentadiene	12.845	237	138815	9.589	ng/ul	99
41) 2,4,6-Trichlorophenol	13.122	196	153411	11.102	ng/ul	99
42) 2,4,5-Trichlorophenol	13.198	196	166679	11.318	ng/ul	98
43) 1,1'-Biphenyl	13.516	154	557650	11.008	ng/ul	99
44) 2-Chloronaphthalene	13.557	162	447101	11.163	ng/ul	100
45) 2-Nitroaniline	13.775	65	138342	11.214	ng/ul	98
47) Dimethylphthalate	14.134	163	561949	11.055	ng/ul	99
48) 2,6-Dinitrotoluene	14.263	165	109427	11.019	ng/ul	96
50) Acenaphthylene	14.404	152	675498	11.244	ng/ul	100
51) 3-Nitroaniline	14.598	138	105905	11.903	ng/ul	99
52) Acenaphthene	14.745	153	469805	11.066	ng/ul	99
53) 2,4-Dinitrophenol	14.810	184	66455	10.333	ng/ul	99
55) 4-Nitrophenol	14.910	109	90378	11.923	ng/ul	95
56) Dibenzofuran	15.081	168	660529	11.068	ng/ul	99
57) 2,4-Dinitrotoluene	15.051	165	163316	11.593	ng/ul	98
58) 2,3,4,6-Tetrachlorophenol	15.310	232	147325	11.130	ng/ul	95
59) Diethylphthalate	15.498	149	564545	11.176	ng/ul	99
61) Fluorene	15.734	166	543262	11.231	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.722	204	283856	10.922	ng/ul	99
63) 4-Nitroaniline	15.769	138	94703	13.686	ng/ul	96
66) 4,6-Dinitro-2-methylph...	15.816	198	107459	10.825	ng/ul	99
67) N-Nitrosodiphenylamine	15.939	169	457308	10.558	ng/ul	98
68) 4-Bromophenyl-phenylether	16.622	248	180862	10.440	ng/ul	99
69) Hexachlorobenzene	16.739	284	210736	10.591	ng/ul	98
70) Atrazine	16.898	200	179640	11.393	ng/ul	98
71) Pentachlorophenol	17.092	266	122382	10.616	ng/ul	98
72) Phenanthrene	17.486	178	877457	11.329	ng/ul	99
74) Anthracene	17.581	178	868275	11.123	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.481	216	249812	10.194	ng/uL	97
76) Pentachlorobenzene	14.998	250	251866	10.301	ng/uL	99
77) Carbazole	17.851	167	787573	12.056	ng/ul	99
78) Di-n-butylphthalate	18.380	149	972053	11.834	ng/ul	100
80) Fluoranthene	19.445	202	1075475	9.022	ng/ul	100
82) Pyrene	19.798	202	1138463	9.148	ng/ul	100
83) Butylbenzylphthalate	20.657	149	457242	10.667	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.445	252	403575	12.158	ng/ul	99
85) Benzo(a)anthracene	21.516	228	1187594	11.166	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.410	149	663642	11.321	ng/ul	99
87) Chrysene	21.569	228	1130562	11.258	ng/ul	99
89) Di-n-octyl phthalate	22.374	149	1159146	10.143	ng/ul	100
90) Benzo(b)fluoranthene	23.280	252	1248525	10.498	ng/ul	98
91) Benzo(k)fluoranthene	23.333	252	1246355	10.790	ng/ul	99
93) Benzo(a)pyrene	23.945	252	1132321	11.061	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.709	276	1519663	10.790	ng/ul	99
95) Dibenzo(a,h)anthracene	26.727	278	1273193	10.797	ng/ul	99
96) Benzo(g,h,i)perylene	27.539	276	1226644	10.685	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Mar 29 00:59:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 29 00:54:55 2023
Response via : Initial Calibration




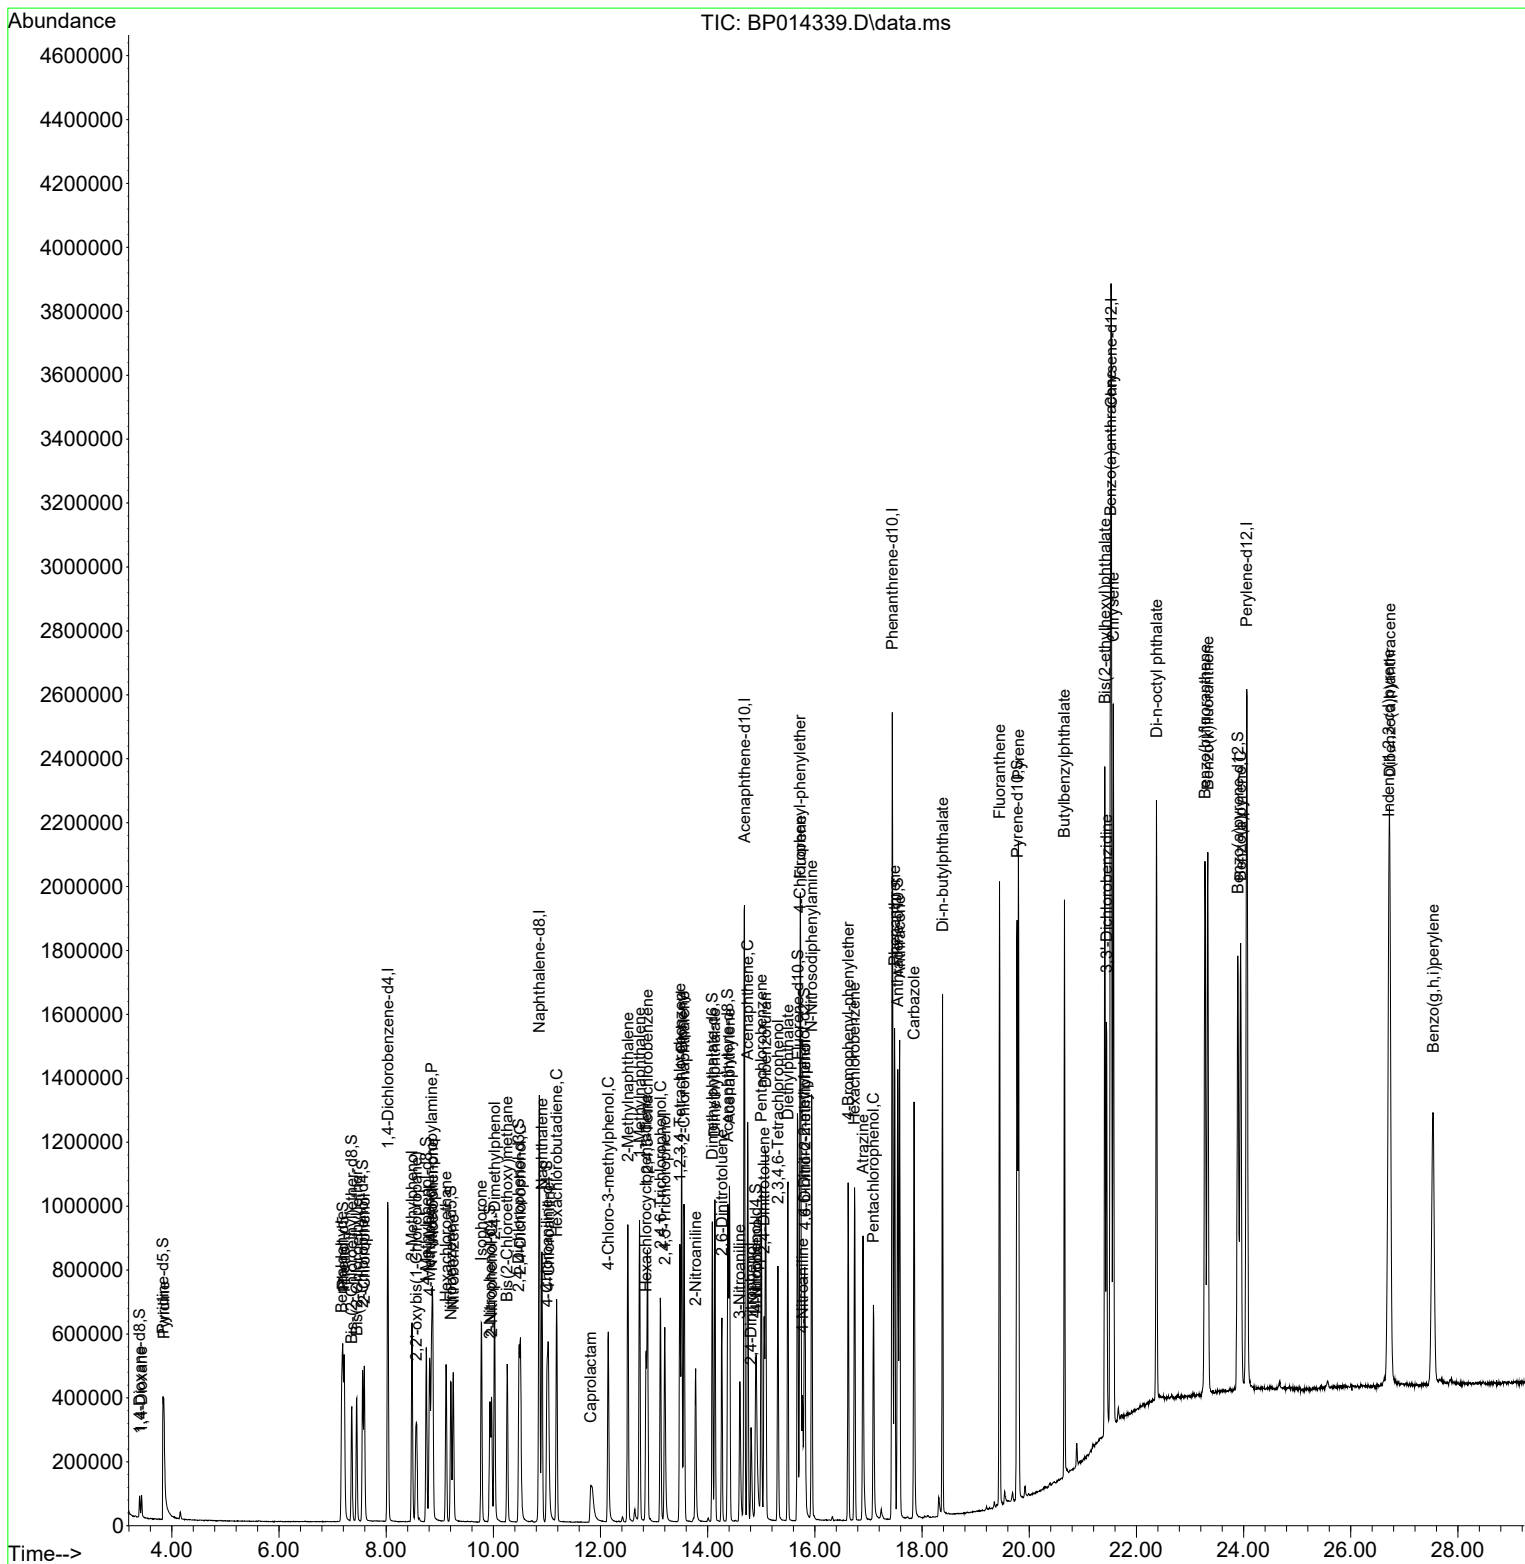


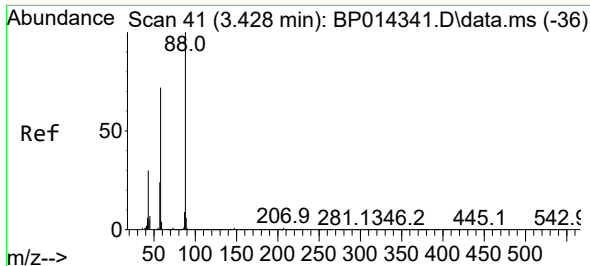

#2
1,4-Dioxane
Concen: 4.663 ng/uL
RT: 3.434 min Scan# 41
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion: 88 Resp: 33576
Ion Ratio Lower Upper
88 100
43 31.7 24.4 36.6
58 74.4 57.4 86.0

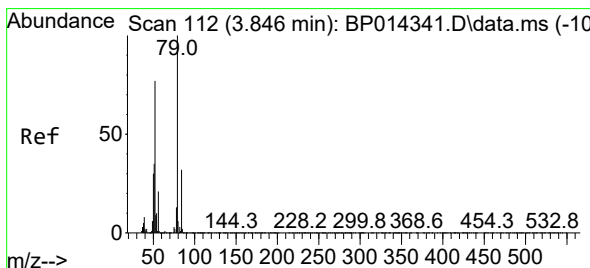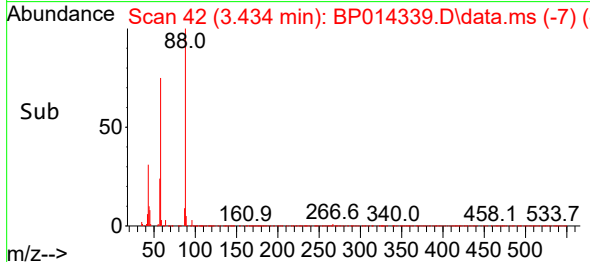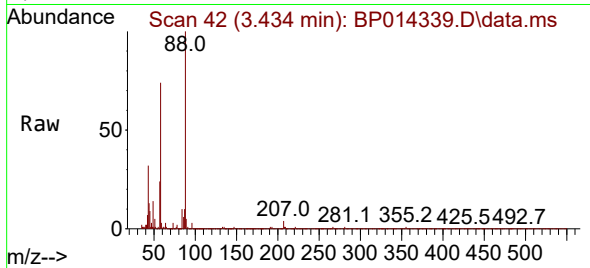

#5
Pyridine
Concen: 10.596 ng/uL
RT: 3.852 min Scan# 113
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion: 79 Resp: 189547
Ion Ratio Lower Upper
79 100
52 74.7 61.4 92.2
51 35.2 28.5 42.7


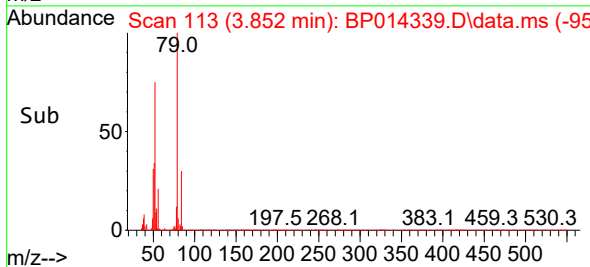

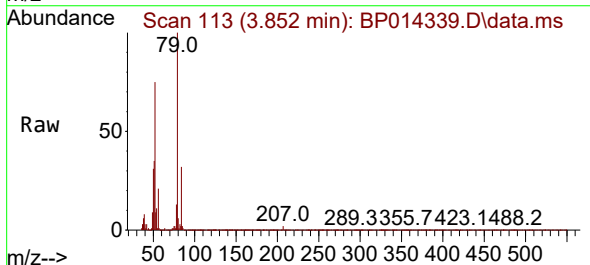




#6
Benzaldehyde
Concen: 13.515 ng/ul
RT: 7.169 min Scan# 61
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion: 77 Resp: 155496
Ion Ratio Lower Upper
77 100
105 91.1 70.6 105.8
106 86.0 66.5 99.7



#8
Phenol
Concen: 10.913 ng/ul
RT: 7.216 min Scan# 685
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion: 94 Resp: 265299
Ion Ratio Lower Upper
94 100
65 31.5 25.2 37.8
66 44.2 36.2 54.4









#10
Bis(2-Chloroethyl)ether
Concen: 10.633 ng/ul
RT: 7.452 min Scan# 71
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion: 93 Resp: 207720
Ion Ratio Lower Upper
93 100
63 78.7 63.2 94.8
95 32.8 26.0 39.0

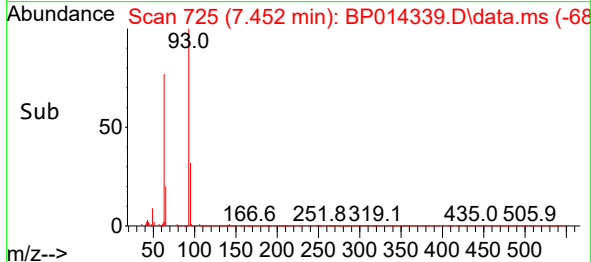

#12
2-Chlorophenol
Concen: 10.983 ng/ul
RT: 7.593 min Scan# 749
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:128 Resp: 193620
Ion Ratio Lower Upper
128 100
64 52.7 41.4 62.0
130 31.9 24.1 36.1

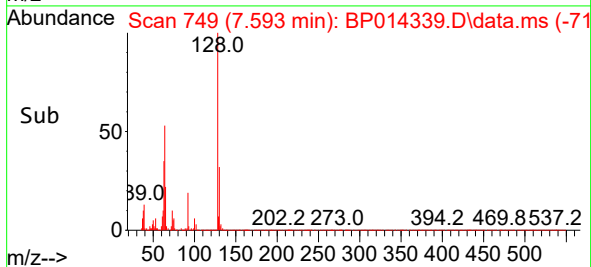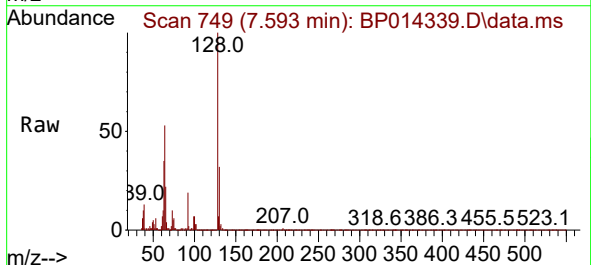



#13

2-Methylphenol

Concen: 10.517 ng/ul

RT: 8.481 min Scan# 900

Delta R.T. 0.012 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :





SSTD020626

Tgt Ion:108 Resp: 190666

Ion Ratio Lower Upper

108 100

107 90.1 71.2 106.8



#14

2,2'-oxybis(1-Chloropropane)

Concen: 10.699 ng/ul

RT: 8.563 min Scan# 914

Delta R.T. 0.018 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion: 45 Resp: 274402


Ion Ratio Lower Upper

45 100

77 15.6 12.8 19.2

79 12.9 9.6 14.4


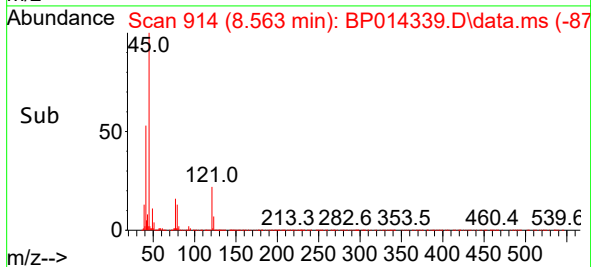

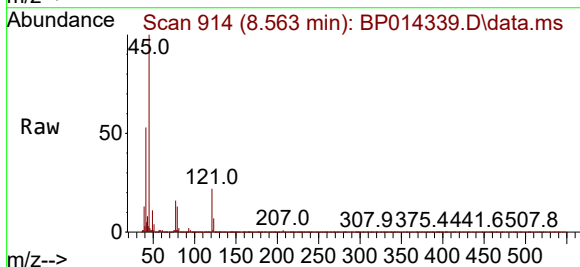




#16
Acetophenone
Concen: 10.389 ng/ul
RT: 8.869 min Scan# 90
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:105 Resp: 324291
Ion Ratio Lower Upper
105 100
77 85.1 67.3 100.9
51 28.4 23.0 34.4



#17
N-Nitroso-di-n-propylamine
Concen: 10.373 ng/ul
RT: 8.846 min Scan# 962
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion: 70 Resp: 174927
Ion Ratio Lower Upper
70 100
42 54.3 41.1 61.7
101 9.0 7.0 10.6
130 17.2 14.6 21.8



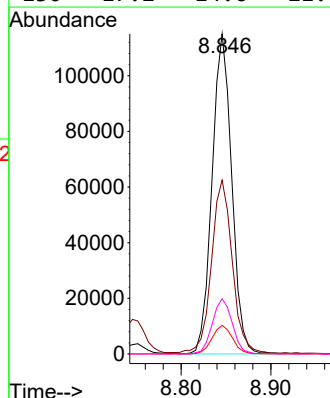





#18
4-Methylphenol
Concen: 10.528 ng/ul
RT: 8.810 min Scan# 91
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:108 Resp: 209626
Ion Ratio Lower Upper
108 100
107 116.5 89.0 133.6



#19
Hexachloroethane
Concen: 11.404 ng/ul
RT: 9.116 min Scan# 1008
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:117 Resp: 87841
Ion Ratio Lower Upper
117 100
201 102.8 90.2 135.4
199 66.4 54.2 81.2









#22
Nitrobenzene
Concen: 11.501 ng/ul
RT: 9.252 min Scan# 110
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion: 77 Resp: 264509
Ion Ratio Lower Upper
77 100
123 38.2 30.3 45.5
65 14.0 11.0 16.4



#23
Isophorone
Concen: 10.555 ng/ul
RT: 9.775 min Scan# 1120
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion: 82 Resp: 447472
Ion Ratio Lower Upper
82 100
95 8.0 6.3 9.5
138 14.2 12.2 18.2



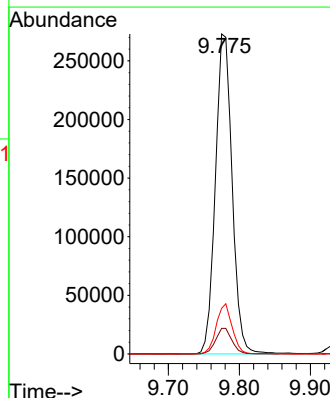





#25
2-Nitrophenol
Concen: 11.329 ng/ul
RT: 9.969 min Scan# 1151
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:139 Resp: 109621
Ion Ratio Lower Upper
139 100
65 62.9 49.7 74.5
109 42.0 31.1 46.7



#26
2,4-Dimethylphenol
Concen: 10.969 ng/ul
RT: 10.022 min Scan# 1162
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:107 Resp: 236435
Ion Ratio Lower Upper
107 100
121 45.7 37.0 55.6
122 78.5 59.8 89.6









#27
 Bis(2-Chloroethoxy)methane
 Concen: 10.839 ng/ul
 RT: 10.257 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BP014339.D
 Acq: 28 Mar 2023 12:29




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020626


Tgt Ion: 93 Resp: 275491
 Ion Ratio Lower Upper
 93 100
 95 31.9 25.8 38.8
 123 10.1 8.5 12.7

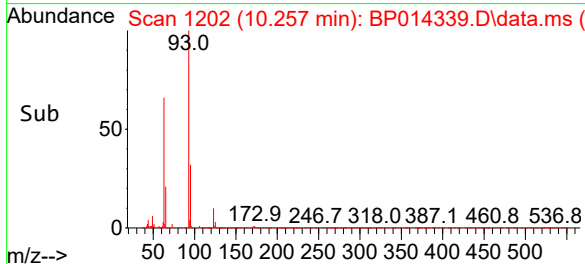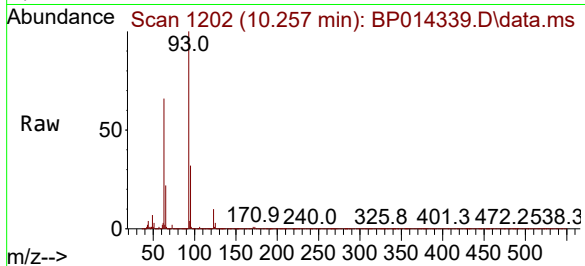

#29
 2,4-Dichlorophenol
 Concen: 11.425 ng/ul
 RT: 10.504 min Scan# 1244
 Delta R.T. 0.006 min
 Lab File: BP014339.D
 Acq: 28 Mar 2023 12:29

Tgt Ion: 162 Resp: 187719
 Ion Ratio Lower Upper
 162 100
 164 70.3 50.1 75.1
 98 43.8 30.6 45.8


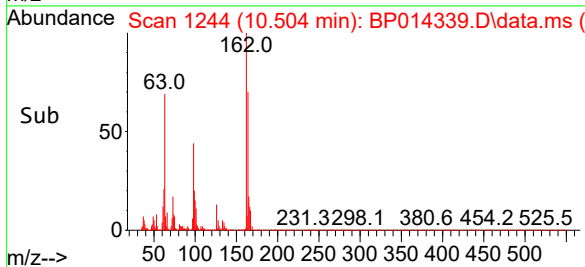

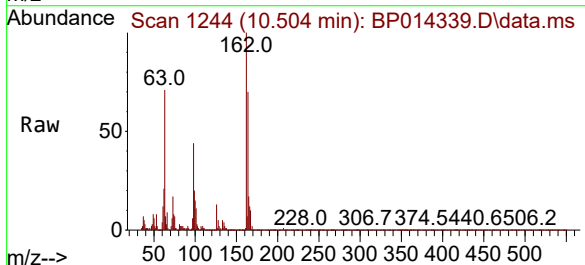




#30
Naphthalene
Concen: 11.189 ng/ul
RT: 10.904 min Scan# 1312
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:128 Resp: 618043
Ion Ratio Lower Upper
128 100
129 10.9 8.9 13.3
127 12.7 11.0 16.6

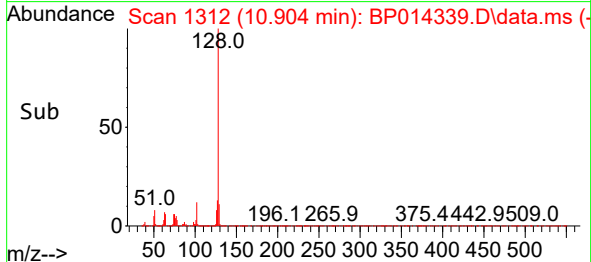

#32
4-Chloroaniline
Concen: 10.889 ng/ul
RT: 11.028 min Scan# 1333
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:127 Resp: 242539
Ion Ratio Lower Upper
127 100
129 32.4 25.4 38.0





#33

Hexachlorobutadiene

Concen: 11.369 ng/ul

RT: 11.181 min Scan# 11

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:225 Resp: 147987

Ion Ratio Lower Upper

225 100

223 65.0 49.3 73.9

227 66.9 49.6 74.4



#34

Caprolactam

Concen: 3.865 ng/ul

RT: 11.816 min Scan# 1467

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:113 Resp: 18339


Ion Ratio Lower Upper

113 100

55 169.2 131.2 196.8

56 130.8 101.1 151.7









#35
4-Chloro-3-methylphenol
Concen: 10.977 ng/ul
RT: 12.146 min Scan# 1521
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:107 Resp: 221838
Ion Ratio Lower Upper
107 100
144 23.0 17.3 25.9
142 70.0 54.6 81.8



#36
2-Methylnaphthalene
Concen: 10.832 ng/ul
RT: 12.510 min Scan# 1585
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:142 Resp: 405516
Ion Ratio Lower Upper
142 100
141 89.9 71.6 107.4


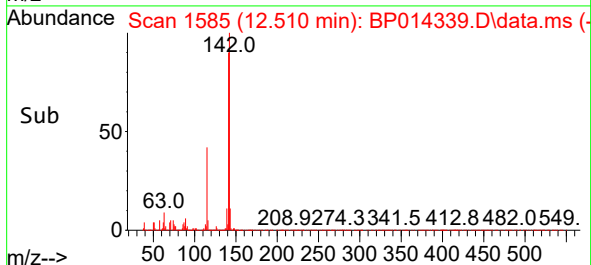
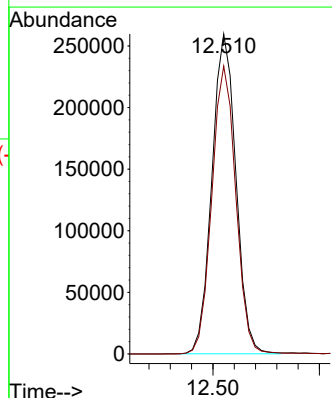
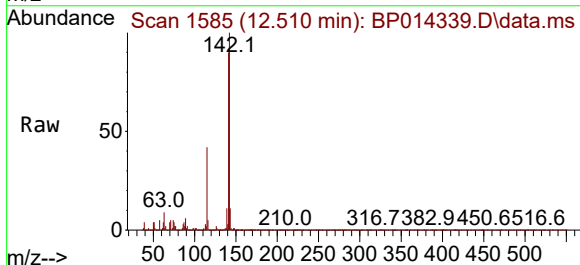




#37
1-Methylnaphthalene
Concen: 10.895 ng/ul
RT: 12.728 min Scan# 1621
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:142 Resp: 404499
Ion Ratio Lower Upper
142 100
141 89.3 76.6 114.8
116 4.7 3.6 5.4



#39
1,2,4,5-Tetrachlorobenzene
Concen: 11.293 ng/ul
RT: 12.875 min Scan# 1647
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:216 Resp: 252463
Ion Ratio Lower Upper
216 100
214 78.0 61.0 91.6
179 21.5 16.6 24.8
108 18.4 13.8 20.6



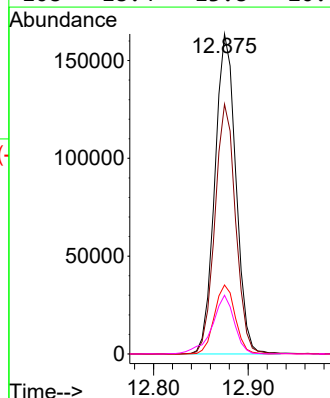





#40
Hexachlorocyclopentadiene
Concen: 9.589 ng/ul
RT: 12.845 min Scan# 1641
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:237 Resp: 138815
Ion Ratio Lower Upper
237 100
235 63.2 51.0 76.4
272 12.6 10.3 15.5



#41
2,4,6-Trichlorophenol
Concen: 11.102 ng/ul
RT: 13.122 min Scan# 1689
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:196 Resp: 153411
Ion Ratio Lower Upper
196 100
198 95.6 76.6 114.8
200 30.4 25.4 38.2









#42
2,4,5-Trichlorophenol
Concen: 11.318 ng/ul
RT: 13.198 min Scan# 1701
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:196 Resp: 166679
Ion Ratio Lower Upper
196 100
198 97.8 79.8 119.8
200 31.6 25.6 38.4



#43
1,1'-Biphenyl
Concen: 11.008 ng/ul
RT: 13.516 min Scan# 1756
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:154 Resp: 557650
Ion Ratio Lower Upper
154 100
153 40.1 32.4 48.6
76 13.4 10.7 16.1





#44

2-Chloronaphthalene

Concen: 11.163 ng/ul

RT: 13.557 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:162 Resp: 447101

Ion Ratio Lower Upper

162 100

164 33.1 26.1 39.1

127 42.1 33.7 50.5



#45

2-Nitroaniline

Concen: 11.214 ng/ul

RT: 13.775 min Scan# 1800

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion: 65 Resp: 138342


Ion Ratio Lower Upper

65 100

92 68.0 53.7 80.5

138 91.7 71.7 107.5



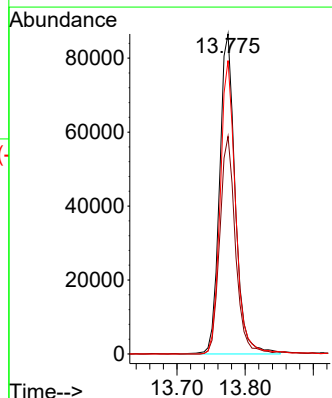





#47
Dimethylphthalate
Concen: 11.055 ng/ul
RT: 14.134 min Scan# 1861
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:163 Resp: 561949
Ion Ratio Lower Upper
163 100
194 4.2 3.1 4.7
164 10.3 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 11.019 ng/ul
RT: 14.263 min Scan# 1883
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:165 Resp: 109427
Ion Ratio Lower Upper
165 100
89 69.7 52.7 79.1
121 24.1 17.9 26.9





#50

Acenaphthylene

Concen: 11.244 ng/ul

RT: 14.404 min Scan# 1907

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:152 Resp: 675498

Ion Ratio Lower Upper

152 100

151 20.4 16.2 24.4

153 12.8 10.2 15.4

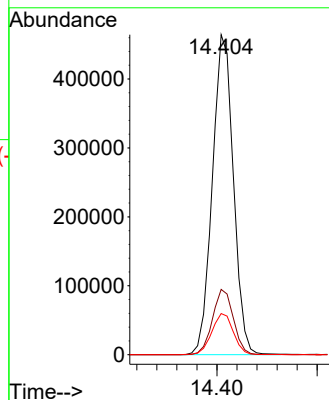

#51

3-Nitroaniline

Concen: 11.903 ng/ul

RT: 14.598 min Scan# 1940

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:138 Resp: 105905


Ion Ratio Lower Upper

138 100

108 11.7 9.9 14.9

92 135.7 107.6 161.4



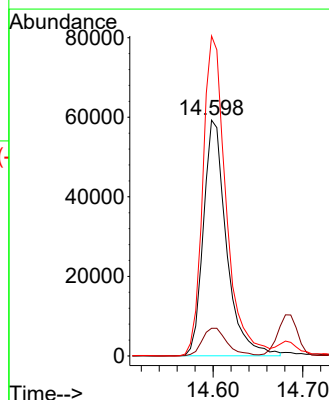





#52
Acenaphthene
Concen: 11.066 ng/ul
RT: 14.745 min Scan# 1965
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:153 Resp: 469805
Ion Ratio Lower Upper
153 100
152 46.9 38.2 57.4
154 86.5 70.2 105.2



#53
2,4-Dinitrophenol
Concen: 10.333 ng/ul
RT: 14.810 min Scan# 1976
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:184 Resp: 66455
Ion Ratio Lower Upper
184 100
63 70.5 57.1 85.7
154 69.3 55.3 82.9



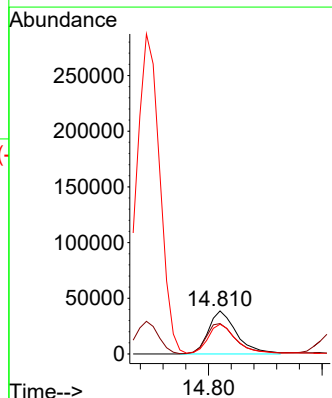





#55
4-Nitrophenol
Concen: 11.923 ng/ul
RT: 14.910 min Scan# 1993
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:109 Resp: 90378
Ion Ratio Lower Upper
109 100
139 104.2 77.4 116.2
65 125.5 97.3 145.9



#56
Dibenzofuran
Concen: 11.068 ng/ul
RT: 15.081 min Scan# 2022
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:168 Resp: 660529
Ion Ratio Lower Upper
168 100
139 40.7 32.1 48.1





#57

2,4-Dinitrotoluene

Concen: 11.593 ng/ul

RT: 15.051 min Scan# 2016

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:165 Resp: 163316

Ion Ratio Lower Upper

165 100

63 53.3 41.6 62.4

182 2.7 2.4 3.6

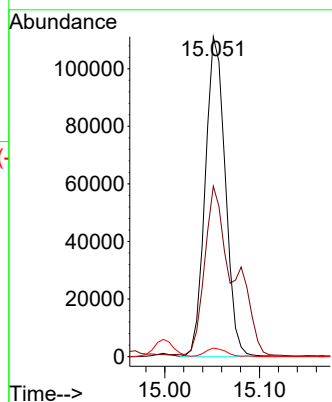

#58

2,3,4,6-Tetrachlorophenol

Concen: 11.130 ng/ul

RT: 15.310 min Scan# 2061

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Tgt Ion:232 Resp: 147325




Ion Ratio Lower Upper


232 100

131 46.1 35.0 52.4

130 2.7 1.9 2.9

166 33.5 24.1 36.1









#59
Diethylphthalate
Concen: 11.176 ng/ul
RT: 15.498 min Scan# 2092
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:149 Resp: 564545
Ion Ratio Lower Upper
149 100
177 22.1 18.2 27.2
150 12.4 9.8 14.8



#61
Fluorene
Concen: 11.231 ng/ul
RT: 15.734 min Scan# 2133
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:166 Resp: 543262
Ion Ratio Lower Upper
166 100
165 100.0 79.2 118.8
167 13.7 11.0 16.4







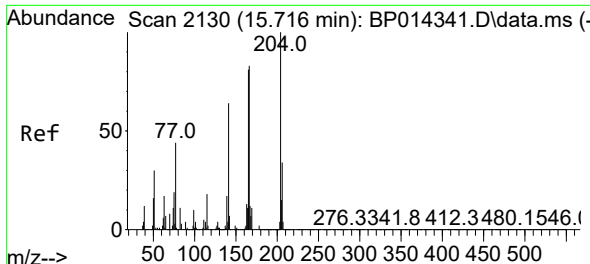

#62
4-Chlorophenyl-phenylether
Concen: 10.922 ng/ul
RT: 15.722 min Scan# 2131
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:204 Resp: 283856
Ion Ratio Lower Upper
204 100
206 32.8 26.9 40.3
141 63.2 51.3 76.9

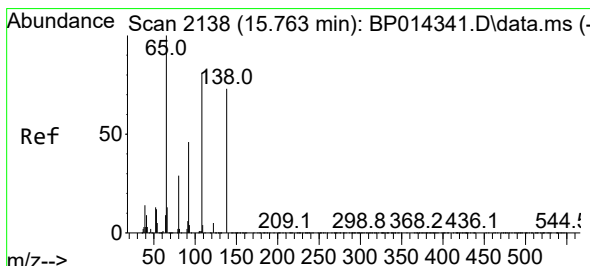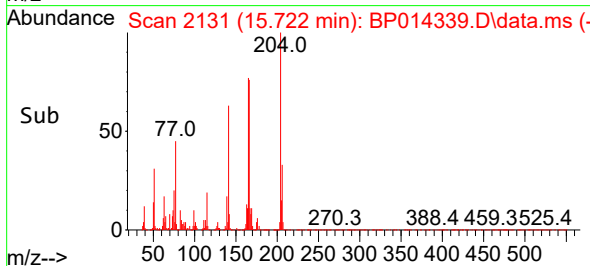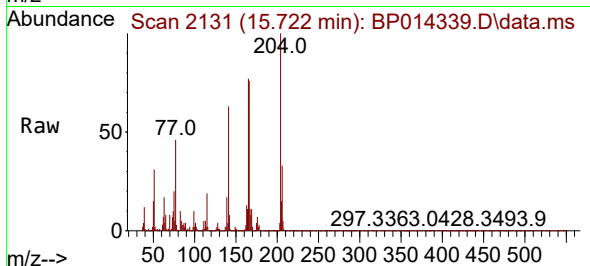

#63
4-Nitroaniline
Concen: 13.686 ng/ul
RT: 15.769 min Scan# 2139
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:138 Resp: 94703
Ion Ratio Lower Upper
138 100
92 62.2 47.8 71.6
108 107.3 82.3 123.5


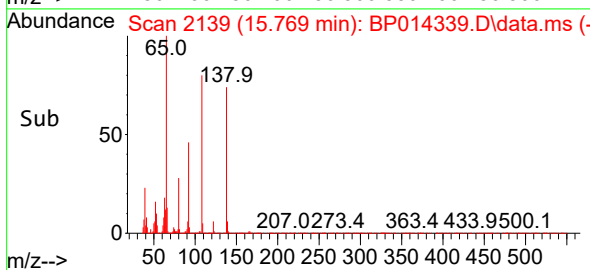

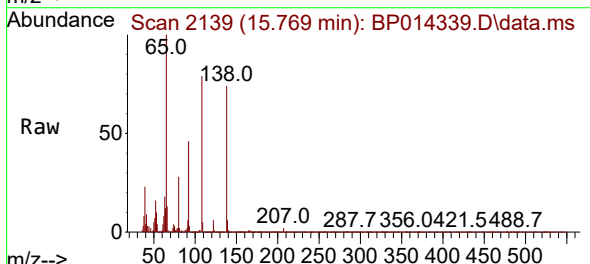




#66
4,6-Dinitro-2-methylphenol
Concen: 10.825 ng/ul
RT: 15.816 min Scan# 2146
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:198 Resp: 107459
Ion Ratio Lower Upper
198 100
182 5.2 3.5 5.3
77 29.9 24.4 36.6



#67
N-Nitrosodiphenylamine
Concen: 10.558 ng/ul
RT: 15.939 min Scan# 2168
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:169 Resp: 457308
Ion Ratio Lower Upper
169 100
168 68.4 54.2 81.2
167 35.1 29.4 44.2



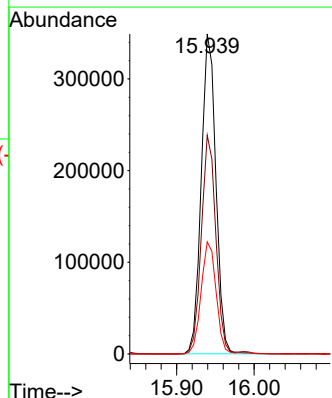



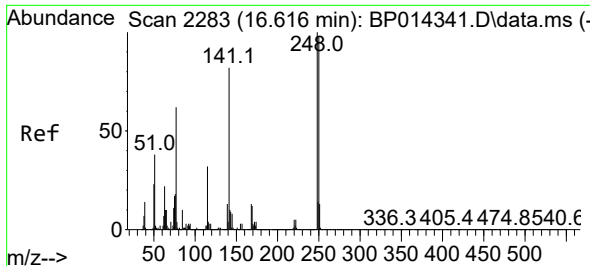

#68
4-Bromophenyl-phenylether
Concen: 10.440 ng/ul
RT: 16.622 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:248 Resp: 180862
Ion Ratio Lower Upper
248 100
250 96.1 78.1 117.1
141 81.8 66.0 99.0

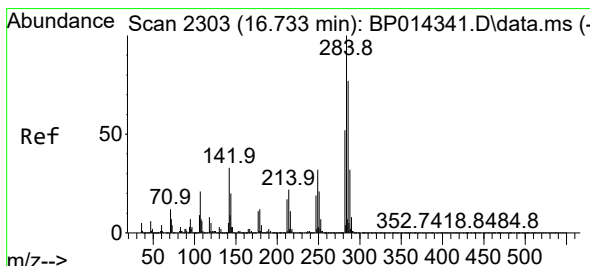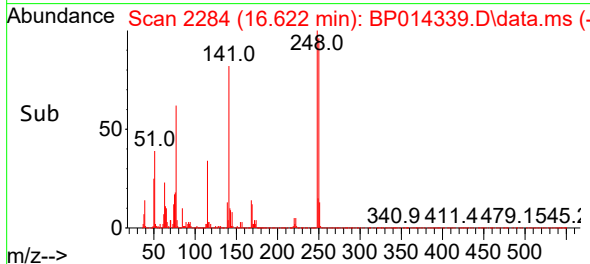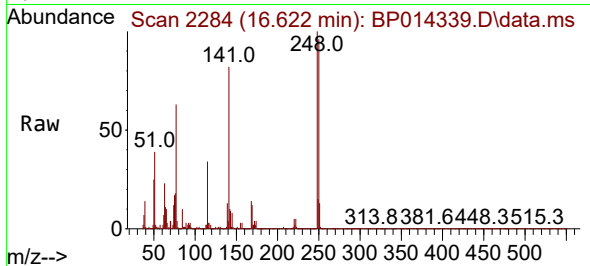

#69
Hexachlorobenzene
Concen: 10.591 ng/ul
RT: 16.739 min Scan# 2304
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:284 Resp: 210736
Ion Ratio Lower Upper
284 100
142 35.5 26.6 39.8
249 32.3 25.7 38.5

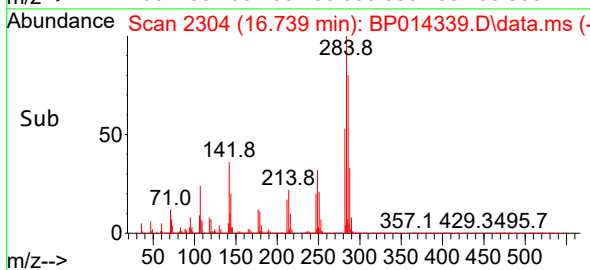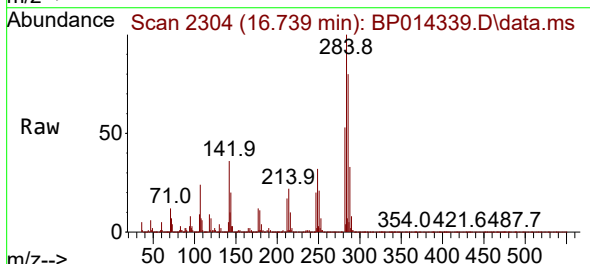



#70

Atrazine

Concen: 11.393 ng/ul

RT: 16.898 min Scan# 21

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:200 Resp: 179640

Ion Ratio Lower Upper

200 100

173 24.5 20.6 30.8

215 47.8 37.2 55.8



#71

Pentachlorophenol

Concen: 10.616 ng/ul

RT: 17.092 min Scan# 2364

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:266 Resp: 122382


Ion Ratio Lower Upper

266 100

264 66.6 51.0 76.4

268 65.2 51.4 77.2





#72

Phenanthrene

Concen: 11.329 ng/ul

RT: 17.486 min Scan# 2430

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:178 Resp: 877457

Ion Ratio Lower Upper

178 100

179 15.7 12.2 18.4

176 18.9 15.3 22.9

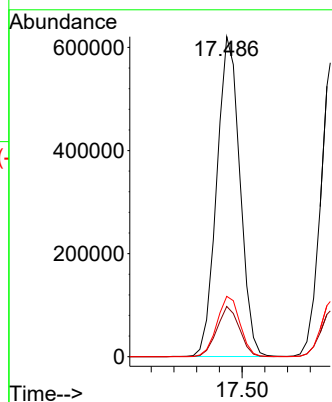

#74

Anthracene

Concen: 11.123 ng/ul

RT: 17.581 min Scan# 2447

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:178 Resp: 868275


Ion Ratio Lower Upper

178 100

179 15.5 12.2 18.4

176 18.7 14.9 22.3





#75

1,2,3,4-Tetrachlorobenzene

Concen: 10.194 ng/uL

RT: 13.481 min Scan# 1

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:216 Resp: 249812

Ion Ratio Lower Upper

216 100

214 80.4 61.0 91.6

218 49.4 38.7 58.1

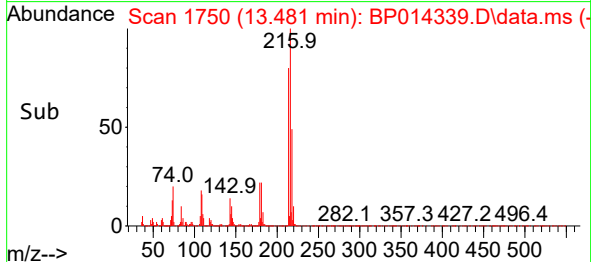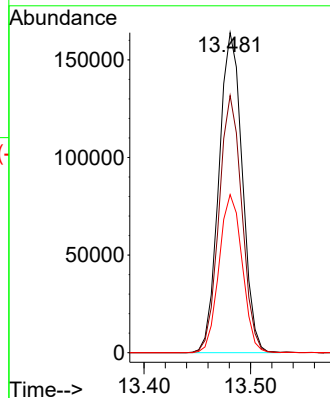

#76

Pentachlorobenzene

Concen: 10.301 ng/uL

RT: 14.998 min Scan# 2008

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:250 Resp: 251866


Ion Ratio Lower Upper

250 100

248 61.4 49.0 73.6

252 62.2 50.7 76.1


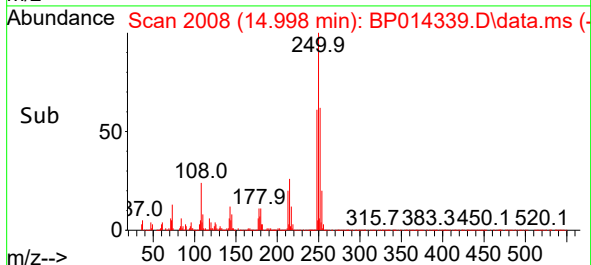
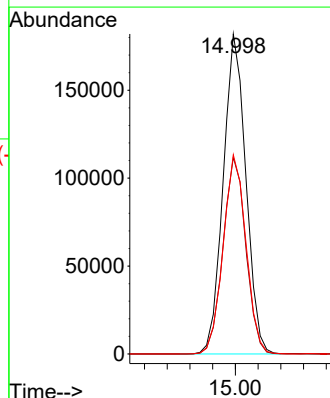
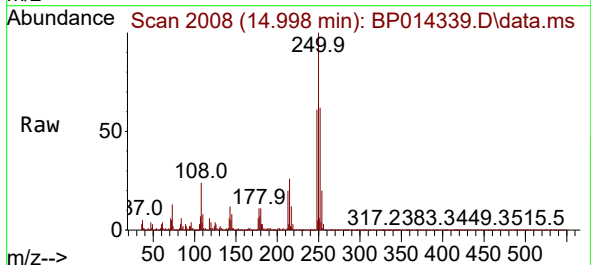




#77
Carbazole
Concen: 12.056 ng/ul
RT: 17.851 min Scan# 2492
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:167 Resp: 787573
Ion Ratio Lower Upper
167 100
166 22.1 17.4 26.2
139 13.5 11.3 16.9



#78
Di-n-butylphthalate
Concen: 11.834 ng/ul
RT: 18.380 min Scan# 2583
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:149 Resp: 972053
Ion Ratio Lower Upper
149 100
150 9.3 7.4 11.0
104 5.8 4.8 7.2



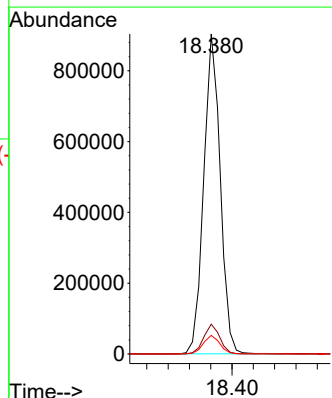





#80
Fluoranthene
Concen: 9.022 ng/ul
RT: 19.445 min Scan# 21
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:202 Resp: 1075475
Ion Ratio Lower Upper
202 100
101 10.1 8.2 12.2
100 8.1 6.4 9.6



#82
Pyrene
Concen: 9.148 ng/ul
RT: 19.798 min Scan# 2824
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:202 Resp: 1138463
Ion Ratio Lower Upper
202 100
101 12.2 9.7 14.5
100 10.2 8.0 12.0





#83

Butylbenzylphthalate

Concen: 10.667 ng/ul

RT: 20.657 min Scan# 2969

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:149 Resp: 457242

Ion Ratio Lower Upper

149 100

91 77.6 61.8 92.8

206 21.8 17.8 26.6



#84

3,3'-Dichlorobenzidine

Concen: 12.158 ng/ul

RT: 21.445 min Scan# 3104

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:252 Resp: 403575


Ion Ratio Lower Upper

252 100

254 63.6 51.4 77.0

126 9.2 7.8 11.6









#85
Benzo(a)anthracene
Concen: 11.166 ng/ul
RT: 21.516 min Scan# 3116
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:228 Resp: 1187594
Ion Ratio Lower Upper
228 100
229 20.0 15.6 23.4
226 27.0 21.8 32.6



#86
Bis(2-ethylhexyl)phthalate
Concen: 11.321 ng/ul
RT: 21.410 min Scan# 3098
Delta R.T. 0.006 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:149 Resp: 663642
Ion Ratio Lower Upper
149 100
167 27.7 21.9 32.9
279 4.7 3.7 5.5





#87

Chrysene

Concen: 11.258 ng/ul

RT: 21.569 min Scan# 3124

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:228 Resp: 1130562

Ion Ratio Lower Upper

228 100

226 30.1 23.8 35.8

229 19.7 16.1 24.1



#89

Di-n-octyl phthalate

Concen: 10.143 ng/ul




RT: 22.374 min Scan# 3262


Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Tgt Ion:149 Resp: 1159146









#90
Benzo(b)fluoranthene
Concen: 10.498 ng/ul
RT: 23.280 min Scan# 3414
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29




Instrument :
BNA_P
ClientSampleId :
SSTD020626


Tgt Ion:252 Resp: 1248525
Ion Ratio Lower Upper
252 100
253 21.7 18.0 27.0
125 7.9 6.8 10.2

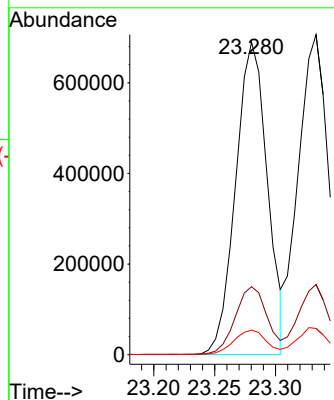

#91
Benzo(k)fluoranthene
Concen: 10.790 ng/ul
RT: 23.333 min Scan# 3425
Delta R.T. 0.012 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:252 Resp: 1246355
Ion Ratio Lower Upper
252 100
253 22.0 17.3 25.9
125 8.2 6.9 10.3

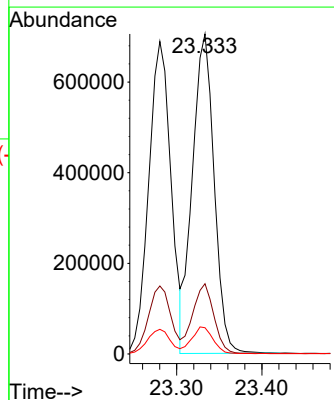



#93

Benzo(a)pyrene

Concen: 11.061 ng/ul

RT: 23.945 min Scan# 3

Delta R.T. 0.006 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29

Instrument :

BNA_P

ClientSampleId :

SSTD020626





Tgt Ion:252 Resp: 1132321

Ion Ratio Lower Upper

252 100

253 22.2 16.9 25.3

125 9.3 6.8 10.2

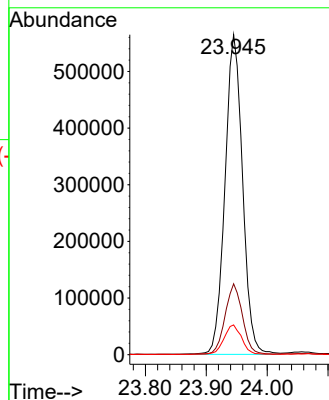

#94

Indeno(1,2,3-cd)pyrene

Concen: 10.790 ng/ul

RT: 26.709 min Scan# 3999

Delta R.T. 0.018 min

Lab File: BP014339.D

Acq: 28 Mar 2023 12:29




Tgt Ion:276 Resp: 1519663


Ion Ratio Lower Upper

276 100

138 19.2 14.9 22.3

277 25.8 20.3 30.5



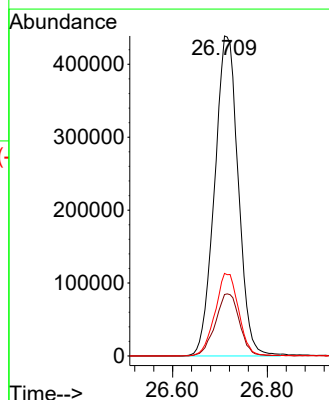





#95
Dibenzo(a,h)anthracene
Concen: 10.797 ng/ul
RT: 26.727 min Scan# 4002
Delta R.T. 0.018 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Instrument :
BNA_P
ClientSampleId :
SSTD020626

Tgt Ion:278 Resp: 1273193
Ion Ratio Lower Upper
278 100
139 12.1 10.4 15.6
279 23.2 18.9 28.3



#96
Benzo(g,h,i)perylene
Concen: 10.685 ng/ul
RT: 27.539 min Scan# 4140
Delta R.T. 0.024 min
Lab File: BP014339.D
Acq: 28 Mar 2023 12:29

Tgt Ion:276 Resp: 1226644
Ion Ratio Lower Upper
276 100
138 16.6 13.0 19.4
277 23.6 18.4 27.6

