




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020012.D
Acq On : 28 Mar 2024 14:51
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 28 15:42:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :Jagrut Upadhyay 03/29/2024

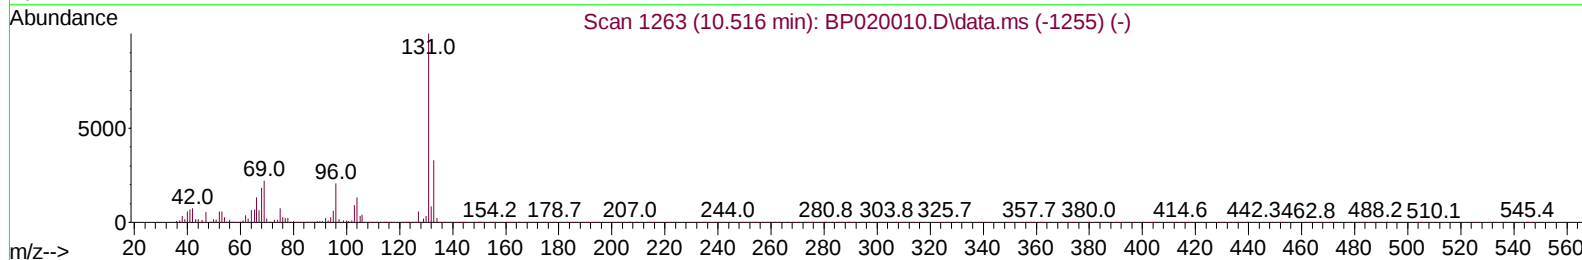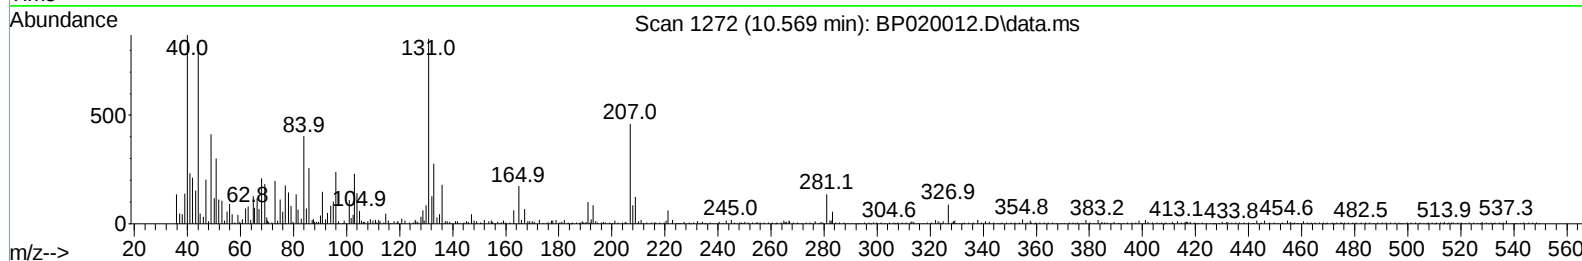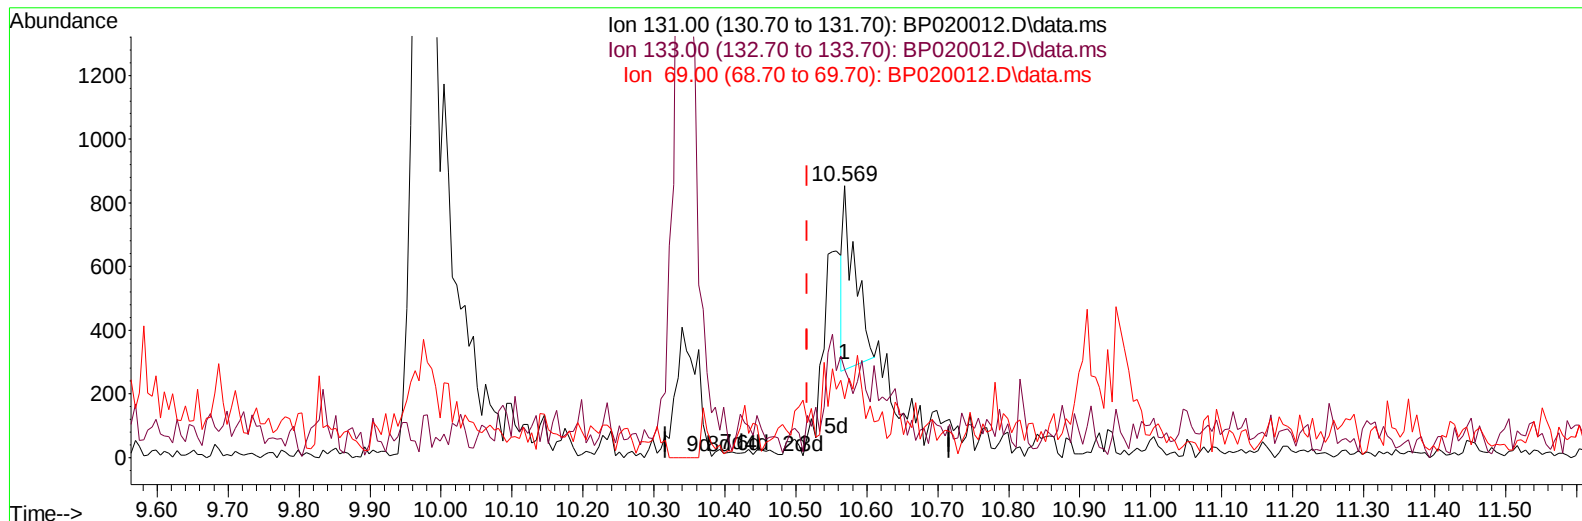

TIC: BP020012.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.569min (+ 0.053) 0.06 ng/u1

response 661

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	32.47
69.00	22.40	21.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020012.D
Acq On : 28 Mar 2024 14:51
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 28 15:42:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :Jagrut Upadhyay 03/29/2024

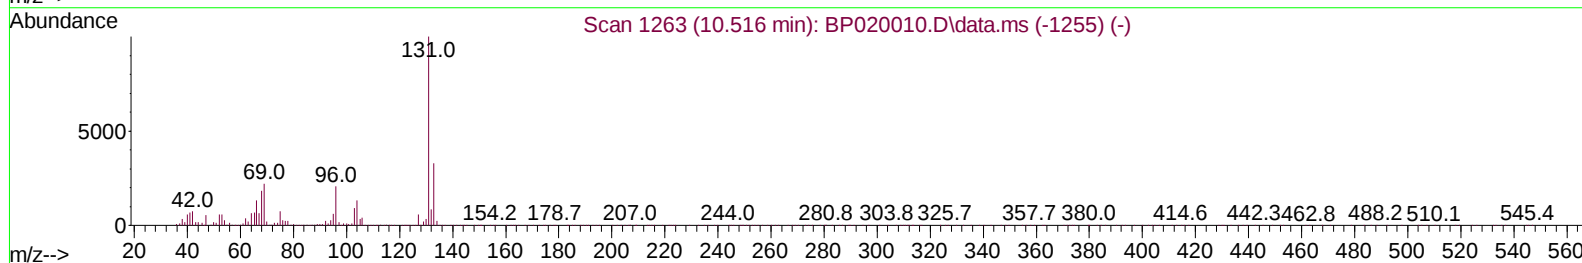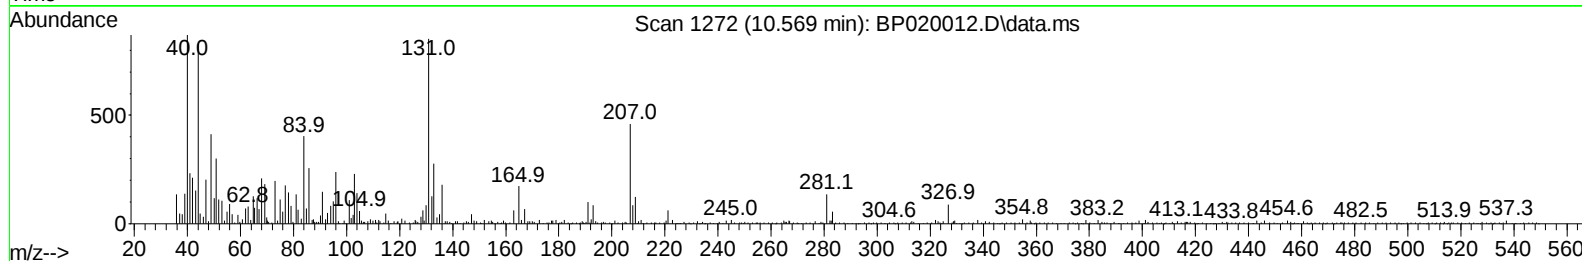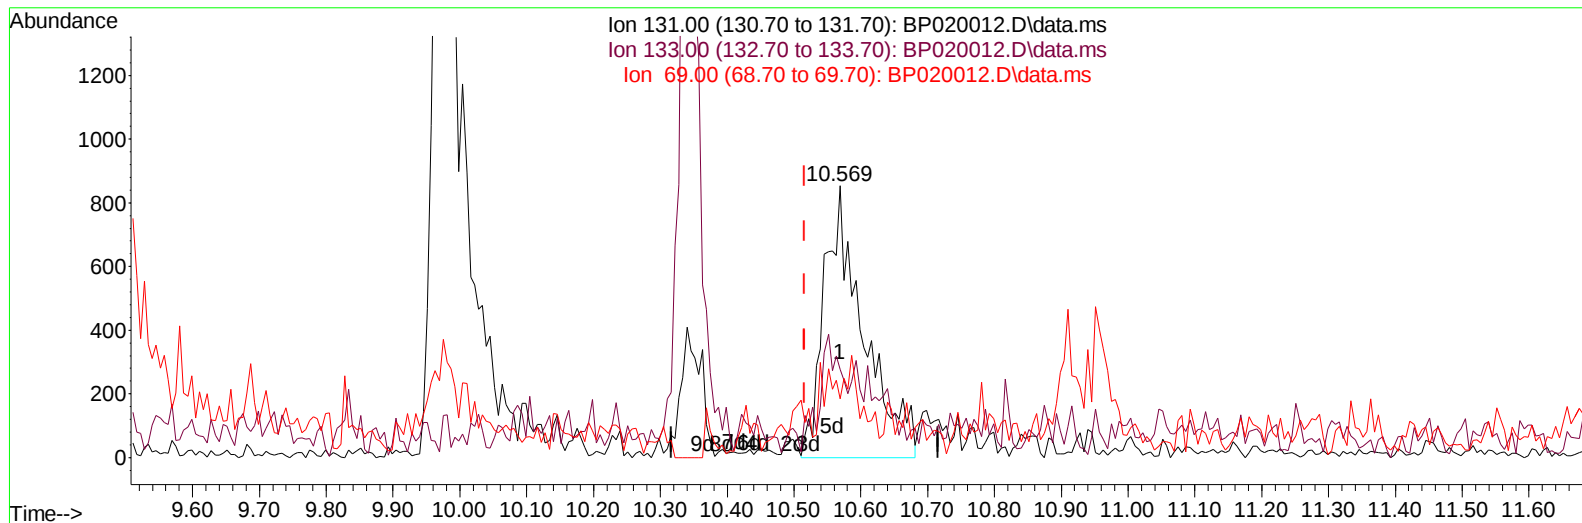

TIC: BP020012.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.569min (+ 0.053) 0.33 ng/ul m

response 3460

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	32.47
69.00	22.40	21.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020012.D
Acq On : 28 Mar 2024 14:51
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 28 15:42:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :Jagrut Upadhyay 03/29/2024

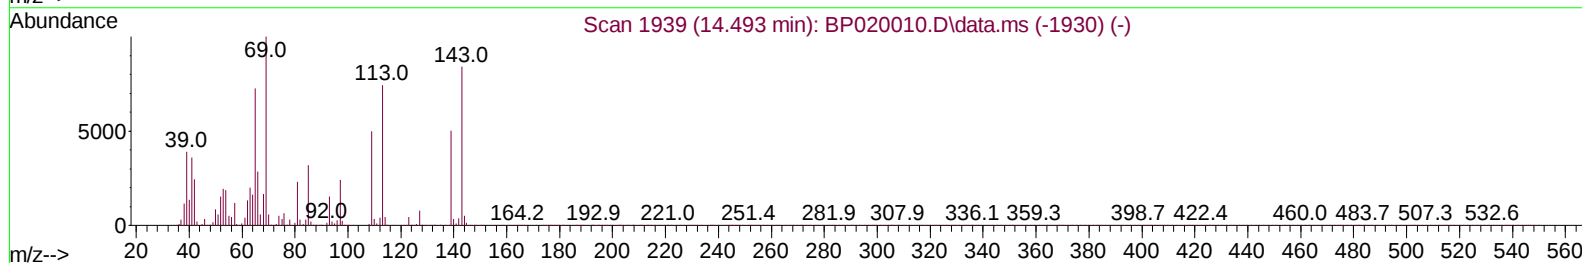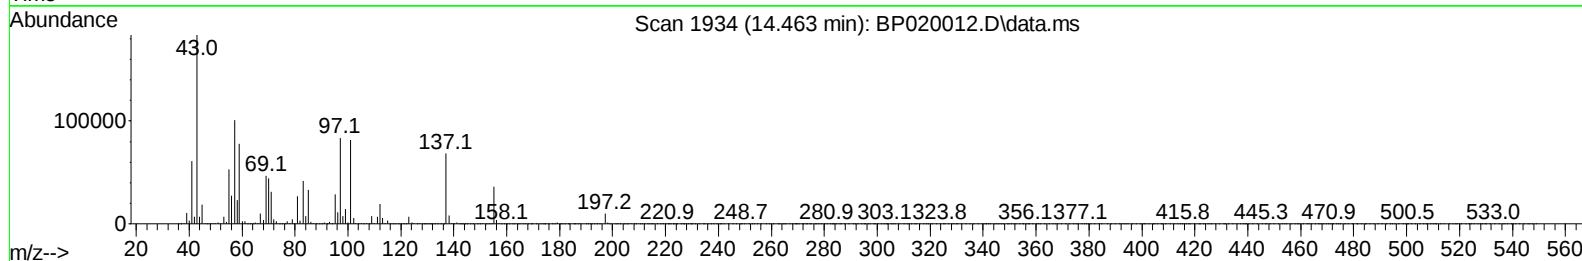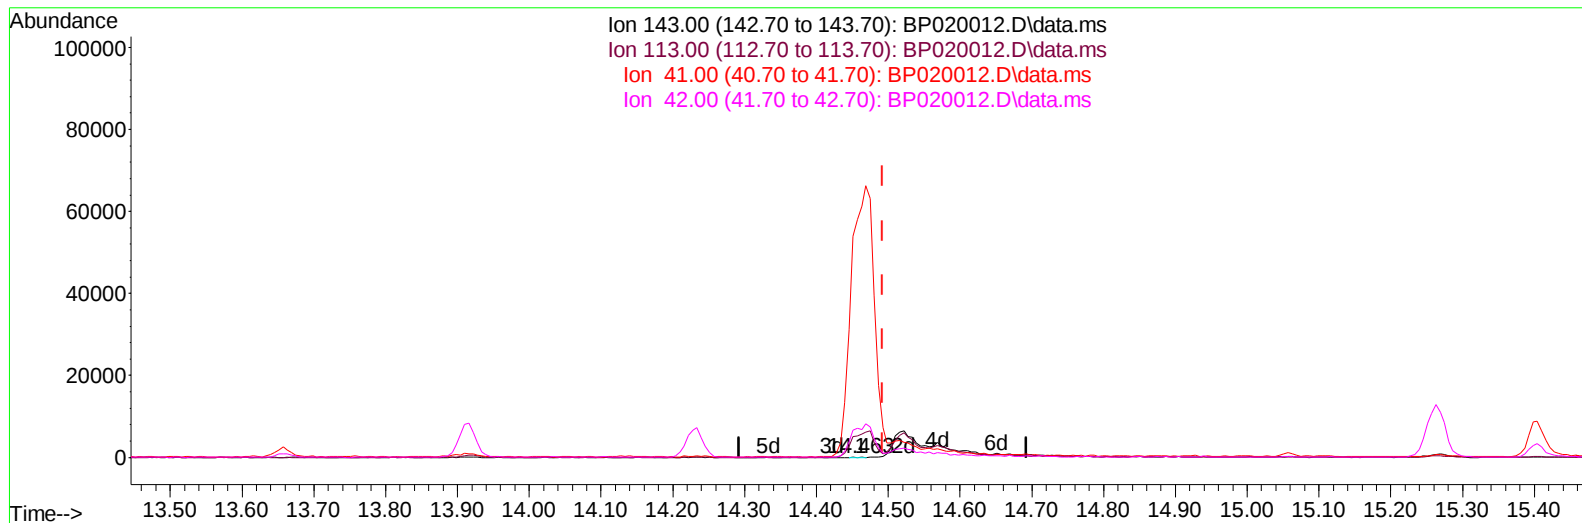

TIC: BP020012.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.463min (-0.030) 0.01 ng/u1

response 29

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	17551.52#
41.00	40.90	185842.42#
42.00	28.50	20569.70#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020012.D
Acq On : 28 Mar 2024 14:51
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 28 15:42:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :Jagrut Upadhyay 03/29/2024

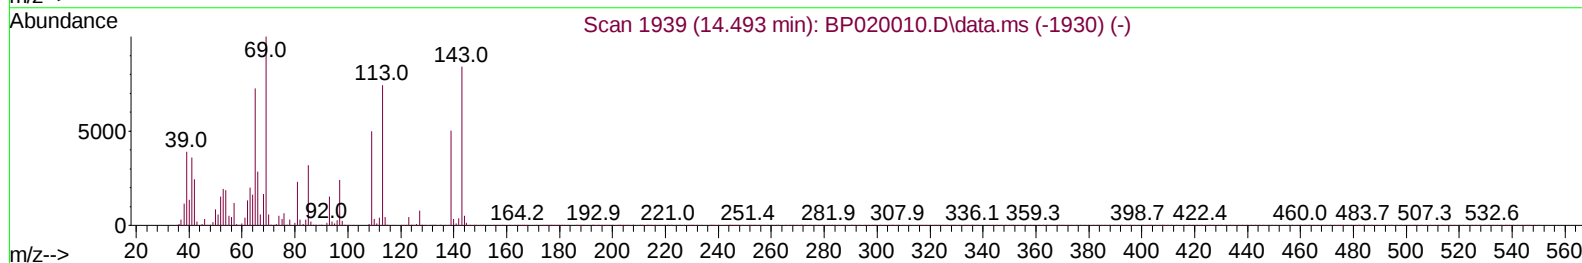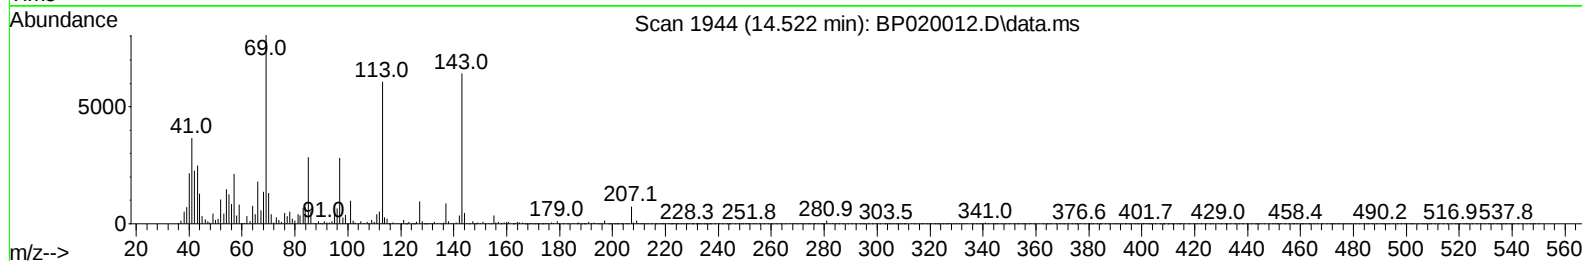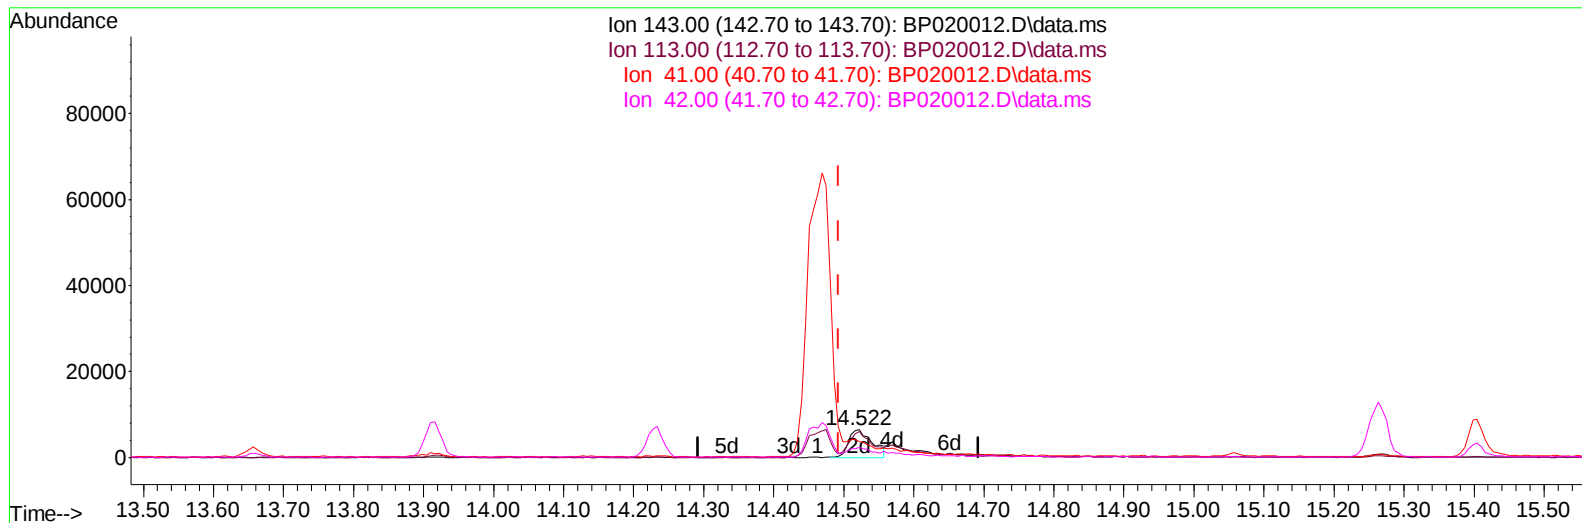

TIC: BP020012.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.522min (+ 0.029) 3.93 ng/ul m

response 15251

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	94.30
41.00	40.90	57.22#
42.00	28.50	35.30#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
 Data File : BP020012.D
 Acq On : 28 Mar 2024 14:51
 Operator : MA/JU
 Sample : P1866-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AL3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/29/2024
 Supervised By :Jagrut Upadhyay 03/29/2024

Quant Time: Mar 28 23:32:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 28 14:08:48 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.575	152	118837	20.000	ng/ul	-0.04
20) Naphthalene-d8	10.340	136	511125	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.234	164	351985	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.069	188	738724	20.000	ng/ul	0.00
79) Chrysene-d12	21.551	240	541074	20.000	ng/ul	0.01
88) Perylene-d12	24.845	264	560091	20.000	ng/ul	0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.228	96	14796	5.455	ng/uL	-0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	6.769	99	65134	6.499	ng/ul	-0.04
9) Bis-(2-Chloroethyl)eth...	6.946	67	242385	37.120	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.116	132	187746	26.084	ng/ul	-0.04
15) 4-Methylphenol-d8	8.281	113	127571	16.452	ng/ul	-0.03
21) Nitrobenzene-d5	8.728	128	135252	34.524	ng/ul	-0.04
24) 2-Nitrophenol-d4	9.446	143	141839	32.359	ng/ul	-0.02
28) 2,4-Dichlorophenol-d3	9.975	165	223122	27.872	ng/ul	-0.02
31) 4-Chloroaniline-d4	10.569	131	3460m	0.332	ng/ul	0.05
46) Dimethylphthalate-d6	13.657	166	948833	38.448	ng/ul	0.01
49) Acenaphthylene-d8	13.916	160	1030822	35.757	ng/ul	0.00
54) 4-Nitrophenol-d4	14.522	143	15251m	3.931	ng/ul	0.03
60) Fluorene-d10	15.263	176	848015	40.338	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.404	200	164615	37.227	ng/ul	0.00
73) Anthracene-d10	17.163	188	1427737	43.661	ng/ul	0.00
81) Pyrene-d10	19.569	212	1552105	48.892	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.610	264	1208298	44.905	ng/ul	0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020012.D
Acq On : 28 Mar 2024 14:51
Operator : MA/JU
Sample : P1866-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AL3

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:32:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/29/2024
Supervised By :Jagrut Upadhyay 03/29/2024

