




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:11:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

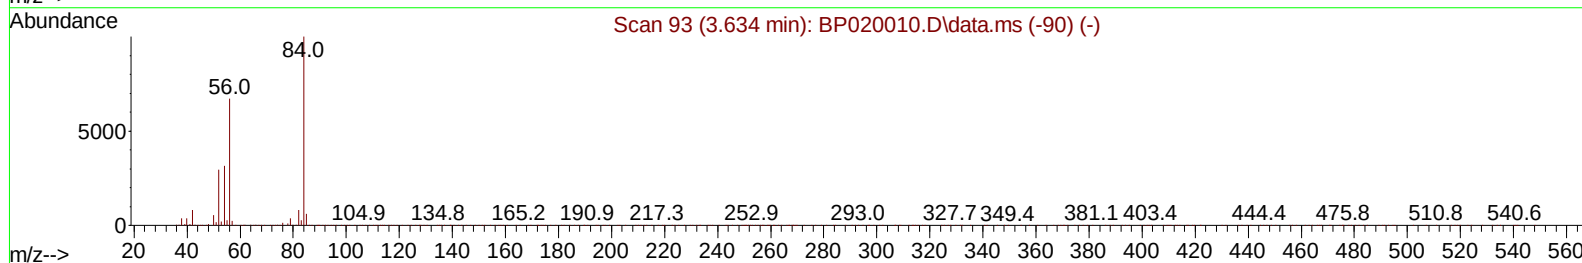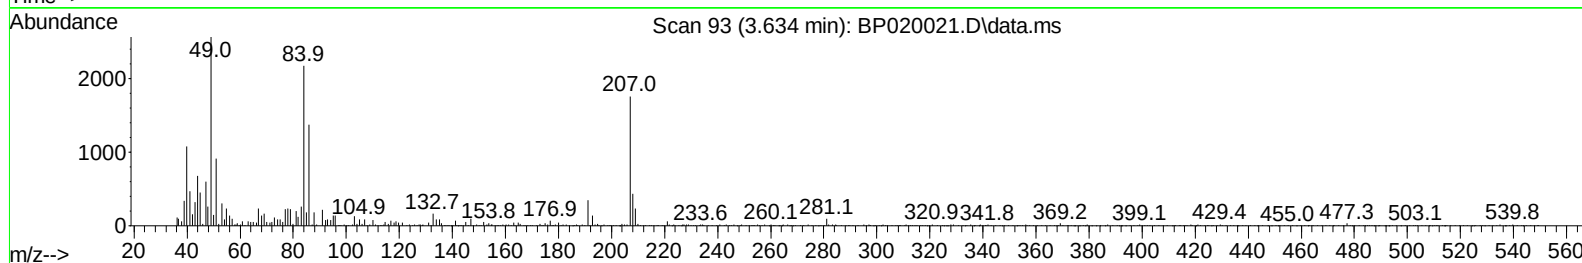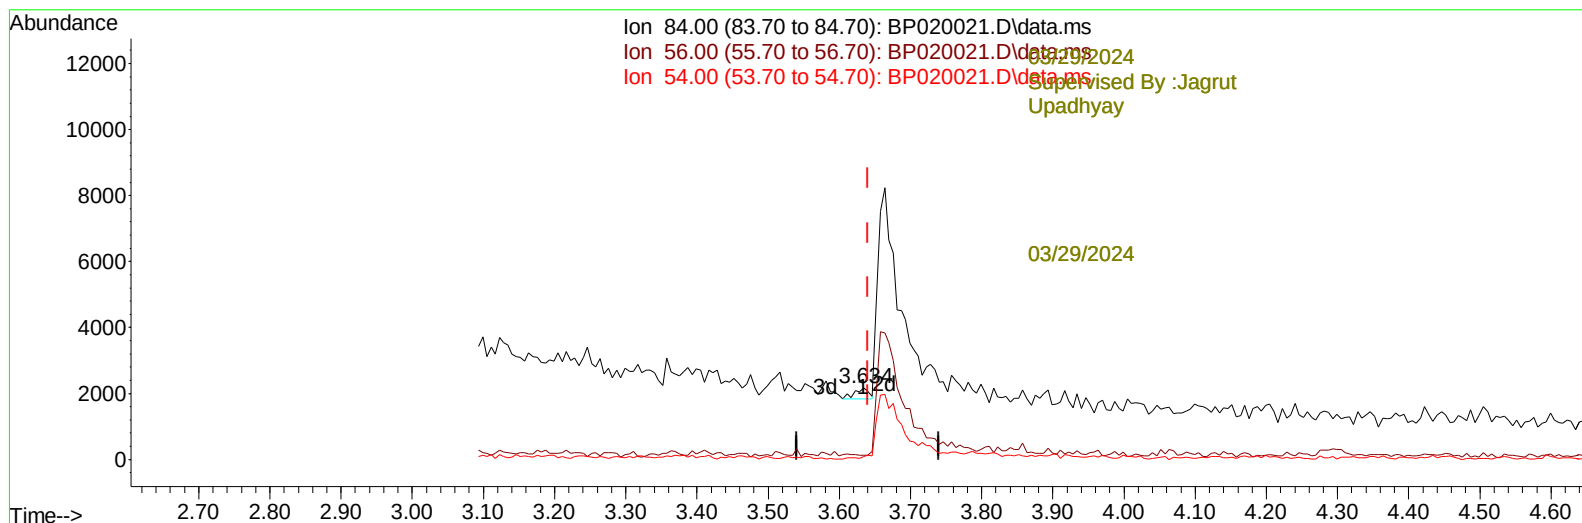

TIC: BP020021.D\data.ms

(4) Pyridine-d5 (S)

3.634min (-0.006) 0.08 ng/u1

response 478

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	63.20	6.21#
54.00	30.60	3.96#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:11:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

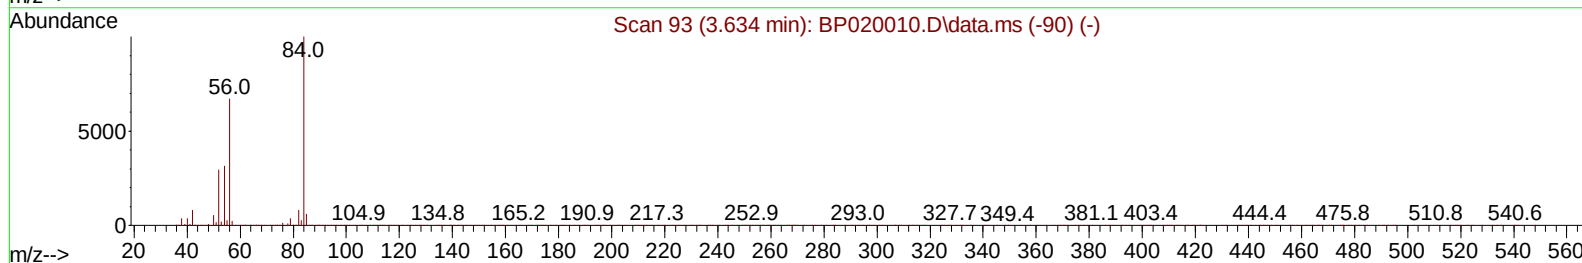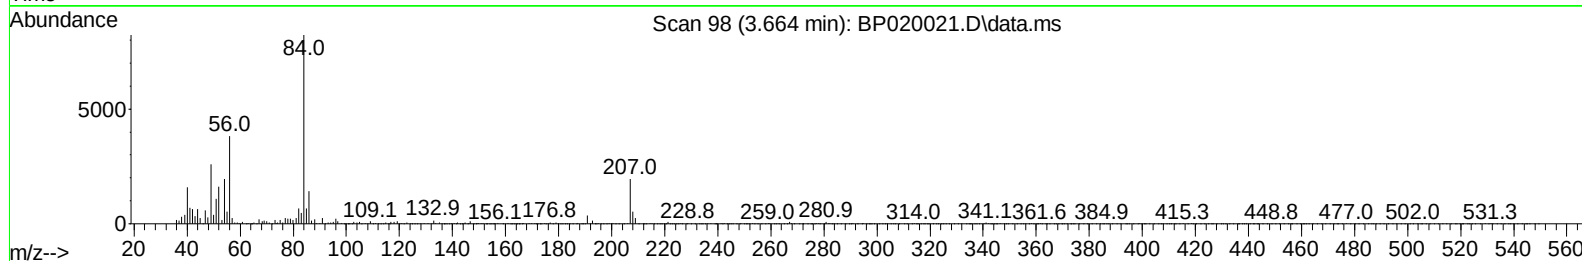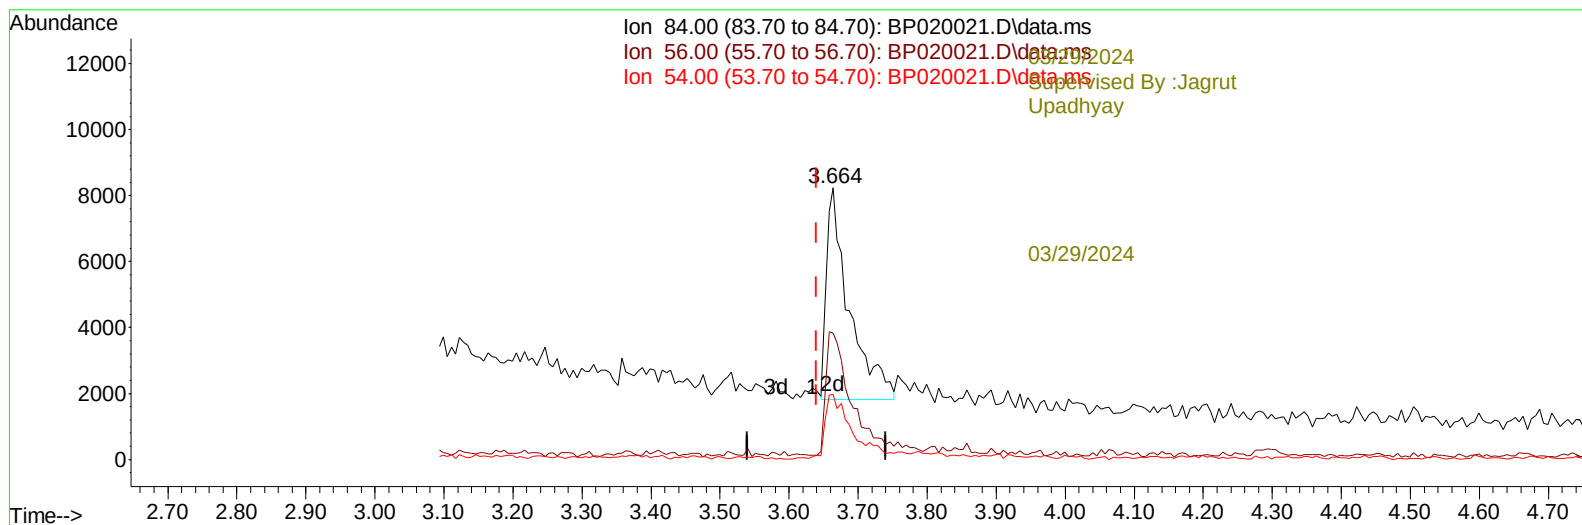

TIC: BP020021.D\data.ms

(4) Pyridine-d5 (S)

3.664min (+ 0.023) 2.37 ng/ul m

response 14693

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	63.20	46.59#
54.00	30.60	23.89#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:11:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

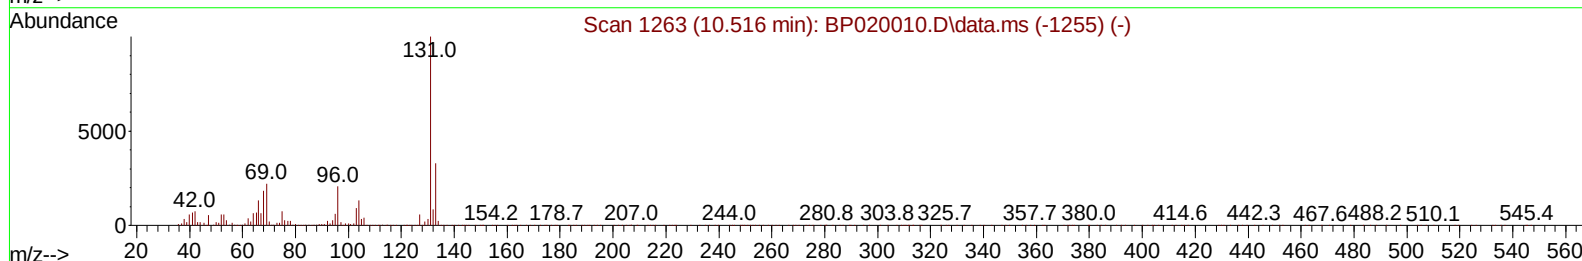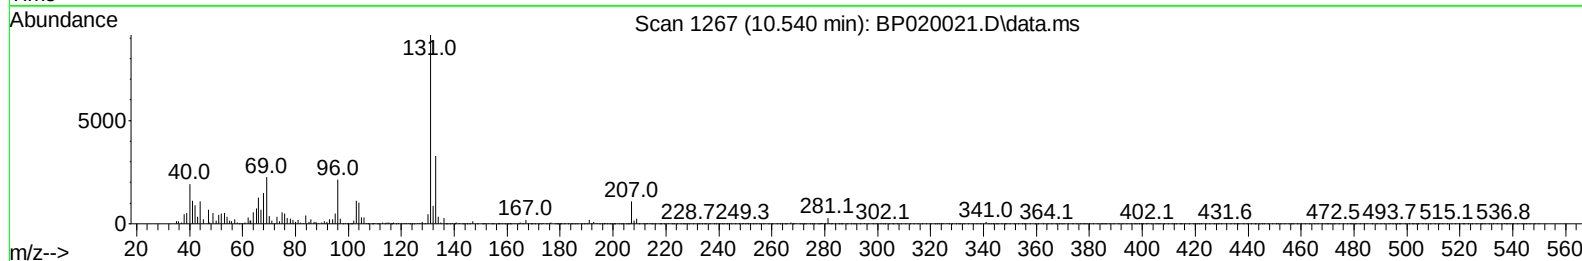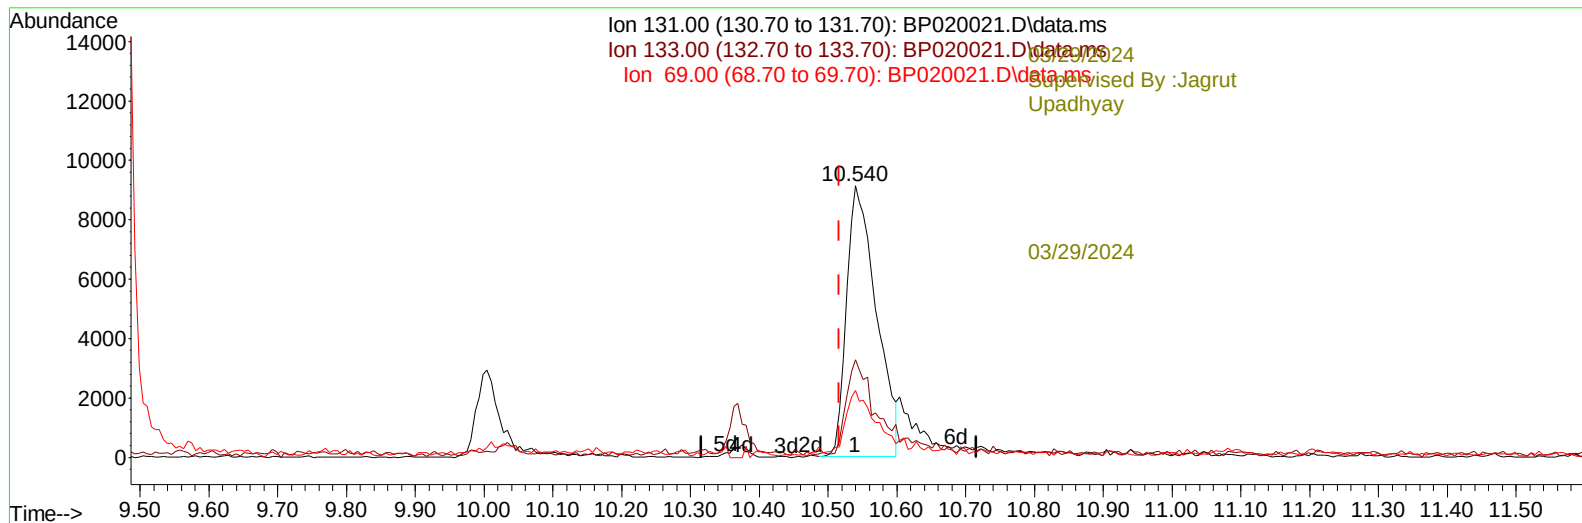

TIC: BP020021.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.540min (+ 0.023) 3.70 ng/uI

response 27486

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	35.99
69.00	22.40	24.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:11:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

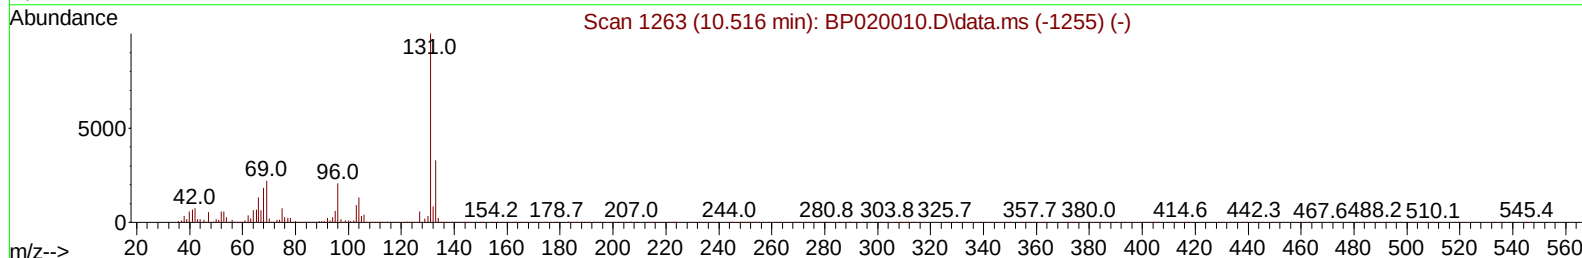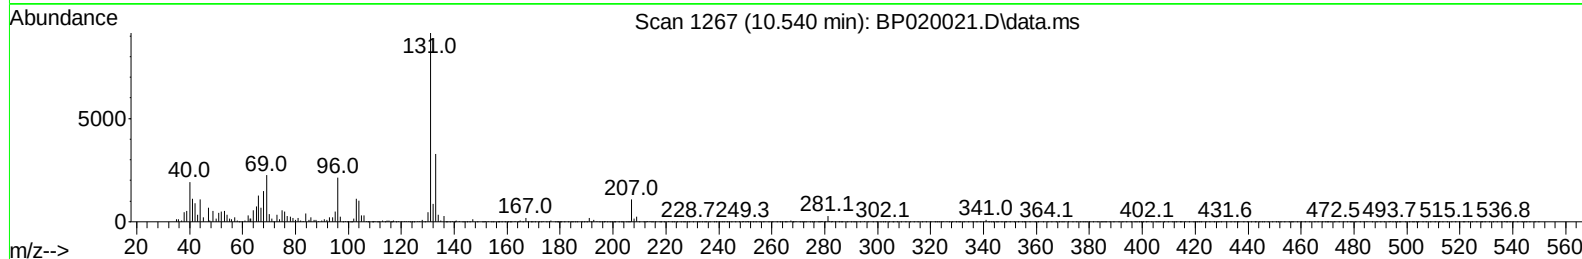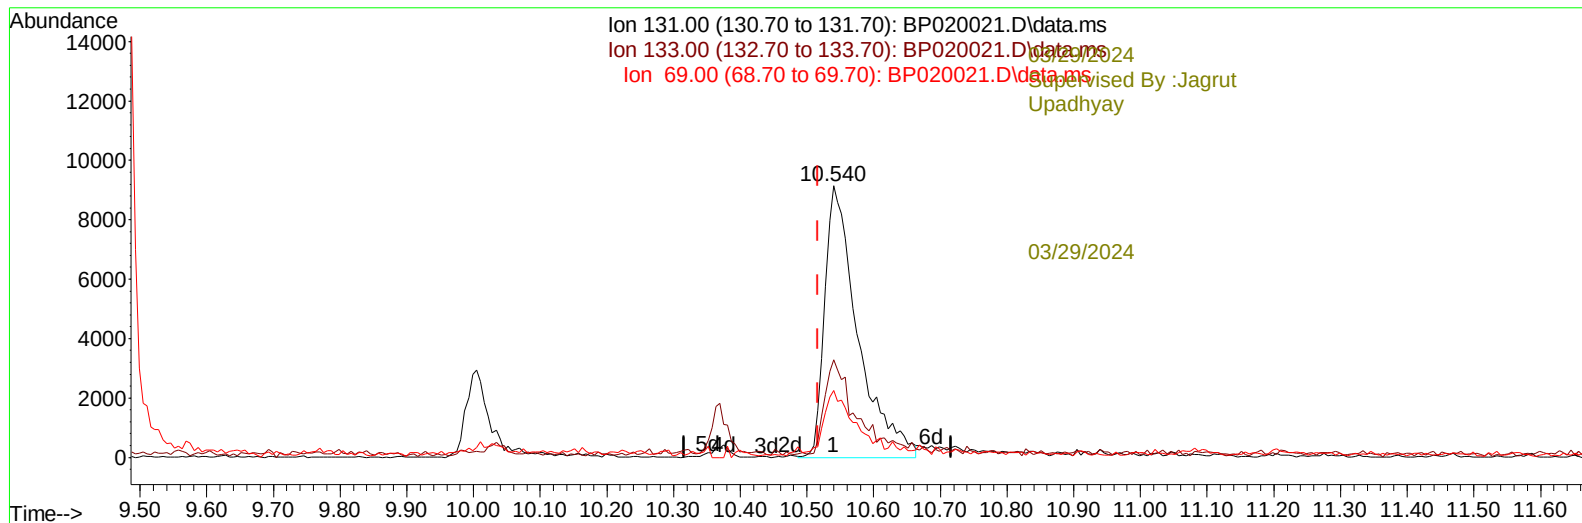

TIC: BP020021.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.540min (+ 0.023) 4.24 ng/ul m

response 31520

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.80	35.99
69.00	22.40	24.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:11:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

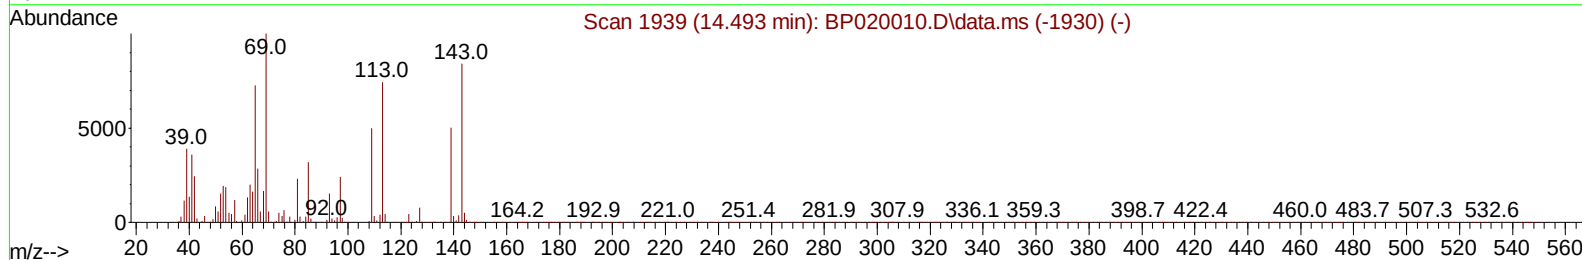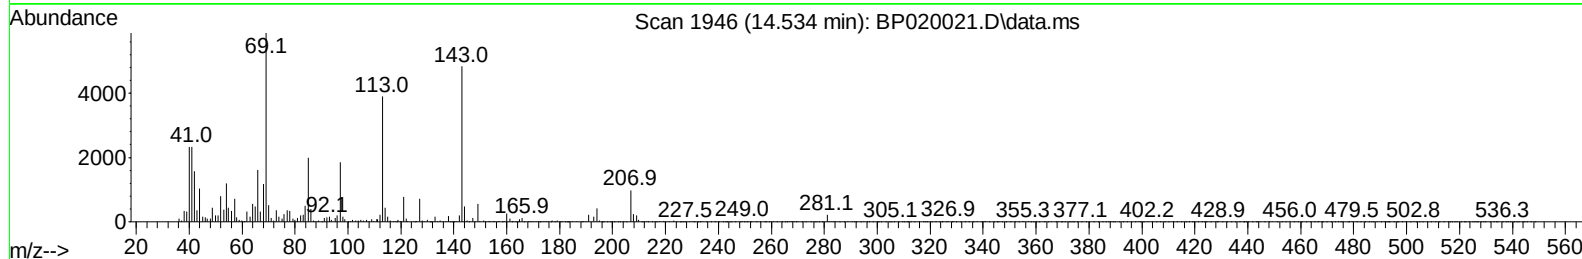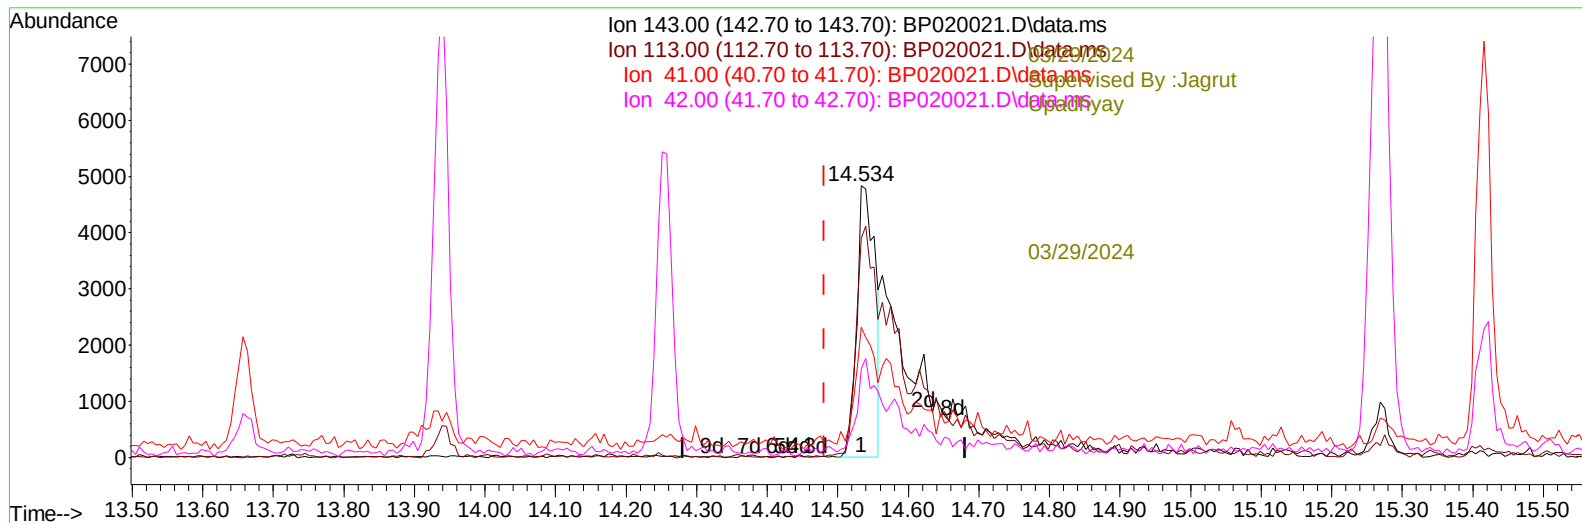

TIC: BP020021.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.534min (+ 0.053) 3.15 ng/ul

response 8776

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	80.69
41.00	40.90	48.05
42.00	28.50	32.57




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:11:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

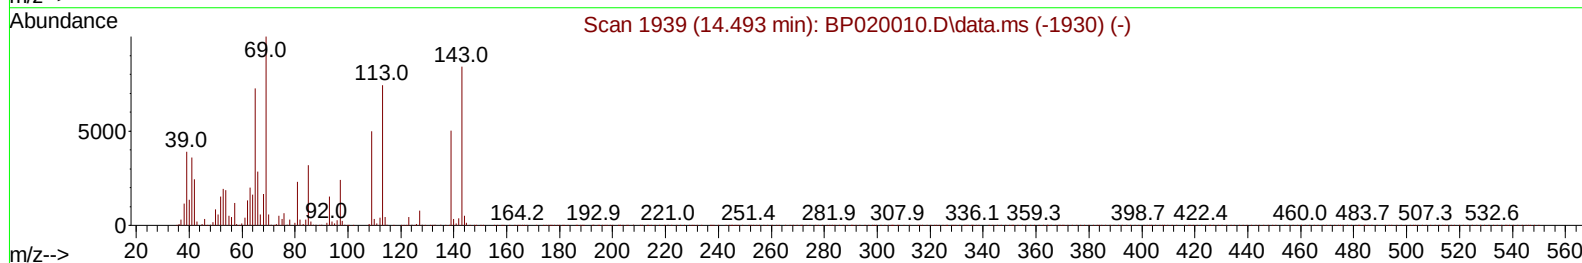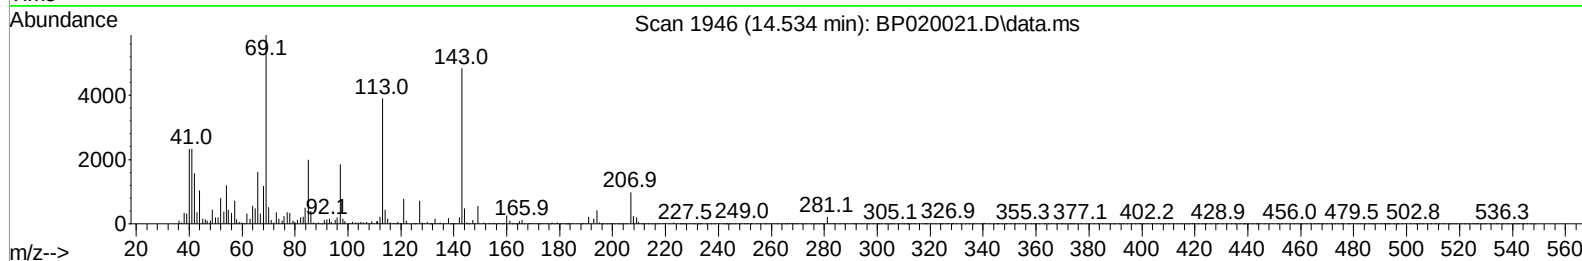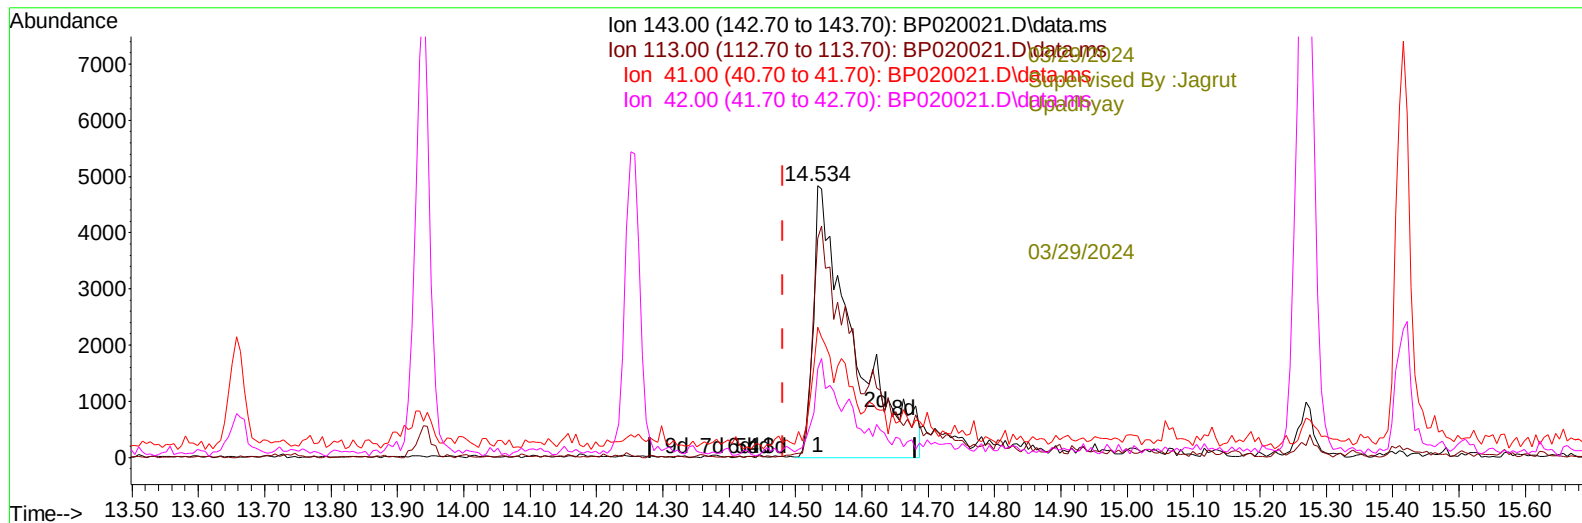

TIC: BP020021.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.534min (+ 0.053) 7.20 ng/ul m

response 20060

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	80.69
41.00	40.90	48.05
42.00	28.50	32.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
 Data File : BP020021.D
 Acq On : 28 Mar 2024 22:23
 Operator : MA/JU
 Sample : P1856-04 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:27:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 28 14:08:48 2024
 Response via : Initial Calibration

Reviewed By :Yogesh
 Patel

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----							-03/29/2024
Internal Standards							Supervised By :Jagrut
1) 1,4-Dichlorobenzene-d4	7.611	152		89980	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136		364288	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.257	164		252722	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.063	188		553378	20.000	ng/ul	-0.01
79) Chrysene-d12	21.545	240		510609	20.000	ng/ul	0.00
88) Perylene-d12	24.827	264		537034	20.000	ng/ul	0.00
System Monitoring Compounds							03/29/2024
3) 1,4-Dioxane-d8	3.240	96		6665	3.245	ng/uL	0.00
4) Pyridine-d5	3.664	84		14693m	2.369	ng/ul	0.02
7) Phenol-d5	6.811	99		60153	7.927	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.969	67		227848	46.084	ng/ul	0.00
11) 2-Chlorophenol-d4	7.152	132		171027	31.381	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113		116046	19.765	ng/ul	0.00
21) Nitrobenzene-d5	8.758	128		125296	44.874	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143		126110	40.367	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	9.999	165		200110	35.073	ng/ul	0.00
31) 4-Chloroaniline-d4	10.540	131		31520m	4.238	ng/ul	0.02
46) Dimethylphthalate-d6	13.657	166		849743	47.957	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160		935013	45.173	ng/ul	0.00
54) 4-Nitrophenol-d4	14.534	143		20060m	7.201	ng/ul	0.05
60) Fluorene-d10	15.269	176		726935	48.161	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.416	200		126177	38.092	ng/ul	0.00
73) Anthracene-d10	17.175	188		1215829	49.634	ng/ul	0.00
81) Pyrene-d10	19.569	212		1445732	48.258	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.604	264		1342282	52.026	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020021.D
Acq On : 28 Mar 2024 22:23
Operator : MA/JU
Sample : P1856-04 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LZ1

Manual IntegrationsAPPROVED

Quant Time: Mar 28 23:27:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 28 14:08:48 2024
Response via : Initial Calibration

Reviewed By :Yogesh
Patel

