

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
 Data File : BP020011.D
 Acq On : 28 Mar 2024 13:55
 Operator : MA/JU
 Sample : PB159847BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK847

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	36	rVB	41277	64194	2.31%	0.227%
2	3.646	92	95	110	rBV	106477	192679	6.94%	0.681%
3	3.934	140	144	148	rVB3	8509	11857	0.43%	0.042%
4	4.381	218	220	224	rBV5	2251	3100	0.11%	0.011%
5	6.799	624	631	652	rBV	494503	884834	31.86%	3.127%
6	6.964	653	659	673	rVV	398449	688294	24.79%	2.432%
7	7.152	684	691	705	rBV	539460	855711	30.82%	3.024%
8	7.611	761	769	782	rBV	468698	752987	27.12%	2.661%
9	8.311	881	888	908	rBV	605085	1040406	37.47%	3.677%
10	8.758	957	964	979	rBV	480677	861606	31.03%	3.045%
11	9.469	1076	1085	1098	rBV	372298	720569	25.95%	2.546%
12	10.005	1166	1176	1198	rBV	365629	1010278	36.38%	3.570%
13	10.228	1213	1214	1221	rVB7	2319	3199	0.12%	0.011%
14	10.357	1228	1236	1252	rBV	535115	1023777	36.87%	3.618%
15	10.605	1272	1278	1279	rBV6	2805	4595	0.17%	0.016%
16	11.999	1510	1515	1523	rBV5	6336	14849	0.53%	0.052%
17	13.128	1700	1707	1713	rBV6	7941	17334	0.62%	0.061%
18	13.669	1791	1799	1819	rBV	782848	1449116	52.18%	5.121%
19	13.928	1833	1843	1863	rBV	992561	1732455	62.39%	6.122%
20	14.240	1889	1896	1909	rBV	891336	1321319	47.58%	4.669%
21	14.498	1934	1940	1952	rBV	239354	536943	19.34%	1.897%
22	14.940	2013	2015	2020	rVB6	1961	3352	0.12%	0.012%
23	15.269	2063	2071	2087	rVV	1227433	2078875	74.86%	7.346%
24	15.404	2088	2094	2108	rBV	359224	649772	23.40%	2.296%
25	15.781	2154	2158	2161	rVB3	4394	5923	0.21%	0.021%
26	16.081	2203	2209	2214	rBV8	5194	9518	0.34%	0.034%
27	16.757	2320	2324	2326	rBV4	2920	3567	0.13%	0.013%
28	16.863	2340	2342	2346	rVB5	2352	2850	0.10%	0.010%
29	17.069	2369	2377	2389	rBV	764681	1478572	53.25%	5.225%
30	17.181	2389	2396	2416	rVV	1420836	2194484	79.03%	7.755%
31	17.722	2483	2488	2489	rBV5	1882	2959	0.11%	0.010%
32	17.810	2500	2503	2506	rBV4	2603	2994	0.11%	0.011%
33	19.116	2721	2725	2732	rBV5	14829	24794	0.89%	0.088%
34	19.198	2735	2739	2745	rVB4	11107	20125	0.72%	0.071%
35	19.569	2796	2802	2815	rBV	1695231	2526748	90.99%	8.929%
36	21.533	3130	3136	3151	rBV	930181	1631443	58.75%	5.765%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020011.D
Acq On : 28 Mar 2024 13:55
Operator : MA/JU
Sample : PB159847BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	24.586	3646	3655	3670	rBV2	1150550	2776900	100.00%	9.813%
38	24.821	3685	3695	3709	rVB2	474263	1694734	61.03%	5.989%




Sum of corrected areas: 28297712

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020011.D
Acq On : 28 Mar 2024 13:55
Operator : MA/JU
Sample : PB159847BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

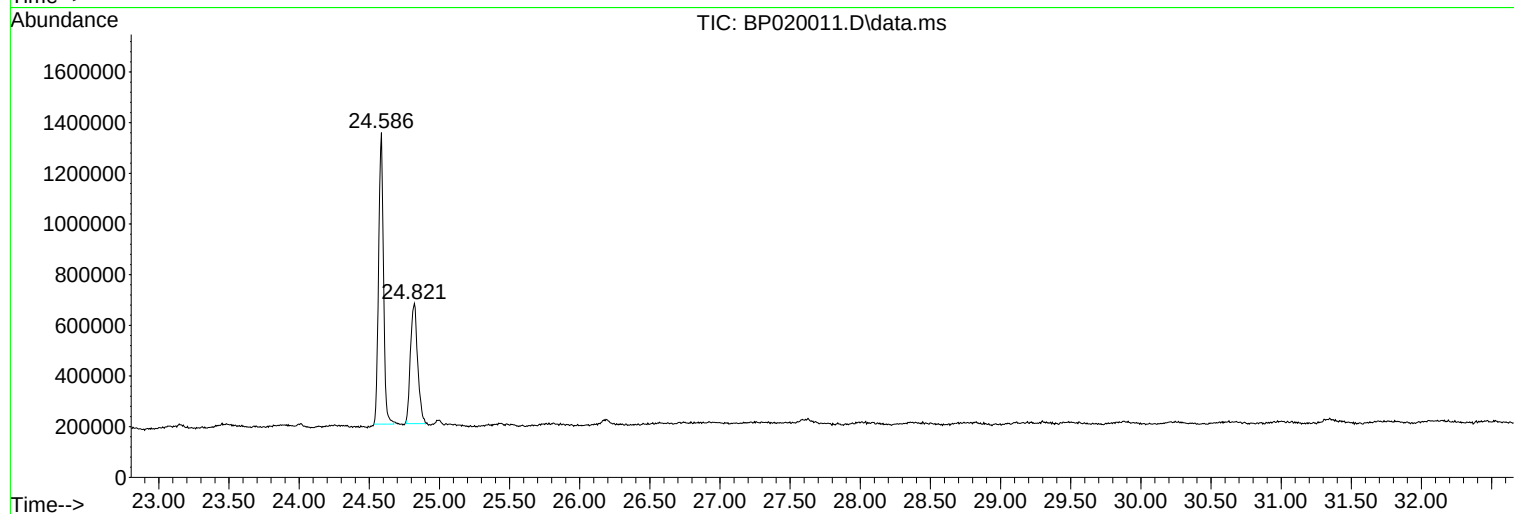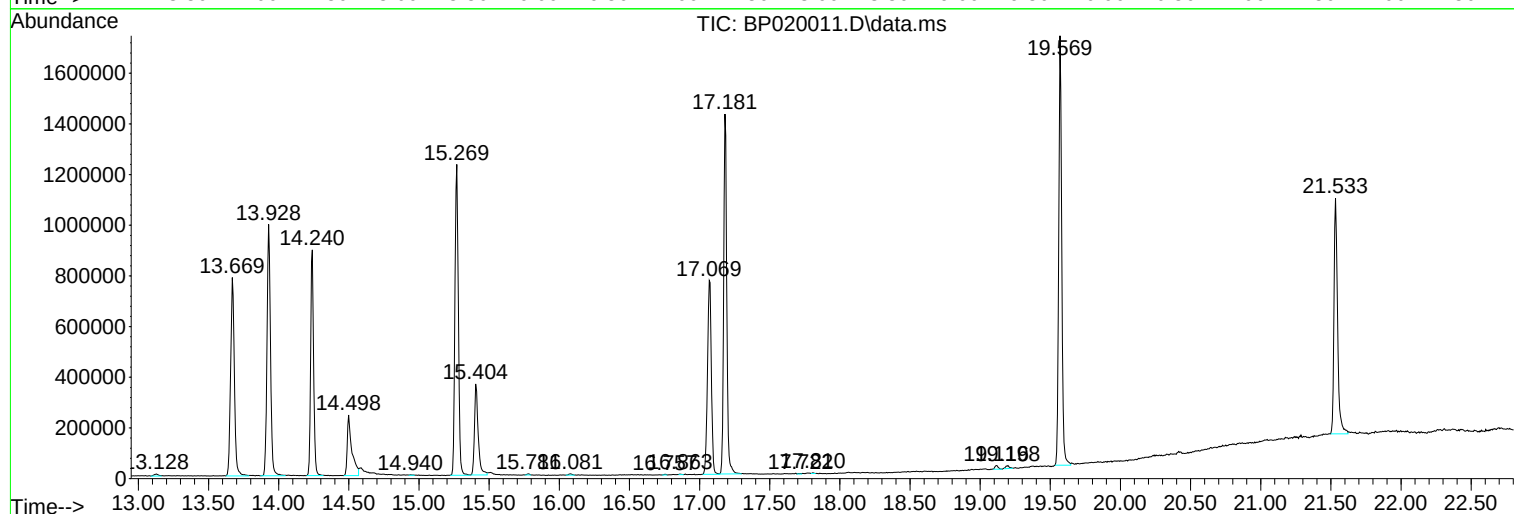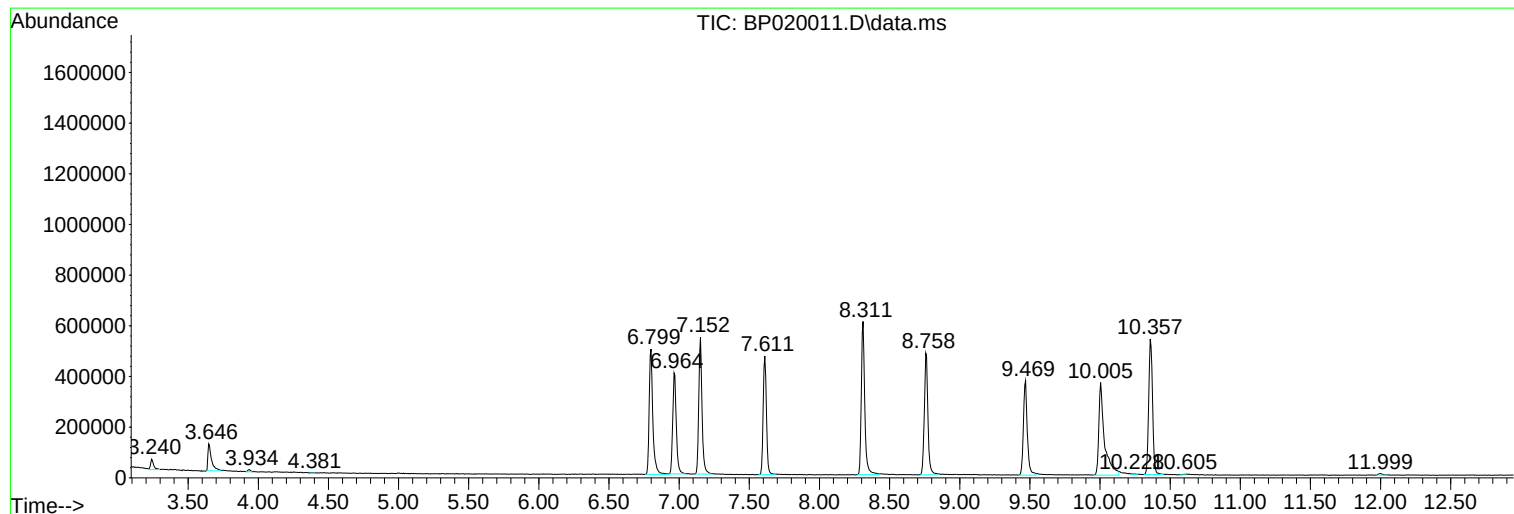

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020011.D
Acq On : 28 Mar 2024 13:55
Operator : MA/JU
Sample : PB159847BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020011.D
Acq On : 28 Mar 2024 13:55
Operator : MA/JU
Sample : PB159847BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK847

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------