

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
 Data File : BP020026.D
 Acq On : 29 Mar 2024 01:57
 Operator : MA/JU
 Sample : PB159808TB 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB808

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	22	26	34	rVB	52071	70473	1.98%	0.181%
2	3.640	90	94	109	rBV	406046	642763	18.10%	1.652%
3	3.934	141	144	148	rVB	7735	8563	0.24%	0.022%
4	4.340	208	213	218	rVB8	4573	10370	0.29%	0.027%
5	5.616	428	430	438	rVB9	2117	3655	0.10%	0.009%
6	6.804	625	632	653	rBV2	631448	1220259	34.36%	3.137%
7	6.969	653	660	672	rVV	569038	927263	26.11%	2.384%
8	7.157	683	692	704	rBV	611151	1149647	32.37%	2.956%
9	7.616	762	770	783	rBV	522661	877637	24.71%	2.256%
10	8.310	881	888	908	rBV	736533	1496817	42.15%	3.848%
11	8.469	913	915	923	rVB9	2492	4834	0.14%	0.012%
12	8.757	954	964	980	rBV	662389	1224822	34.49%	3.149%
13	9.469	1076	1085	1104	rBV	599782	1050633	29.58%	2.701%
14	9.998	1168	1175	1190	rBV	561382	1437415	40.48%	3.695%
15	10.357	1227	1236	1248	rVB	729211	1285597	36.20%	3.305%
16	10.569	1263	1272	1285	rBV3	17152	53246	1.50%	0.137%
17	11.228	1380	1384	1388	rVB7	2933	4666	0.13%	0.012%
18	11.604	1441	1448	1451	rBV9	2523	5468	0.15%	0.014%
19	11.992	1509	1514	1527	rVB4	9074	21373	0.60%	0.055%
20	13.663	1789	1798	1814	rBV	1306174	2372677	66.81%	6.100%
21	13.934	1836	1844	1858	rBV	1755031	2642366	74.41%	6.793%
22	14.245	1890	1897	1917	rVB	1320685	1816901	51.16%	4.671%
23	14.398	1920	1923	1926	rBV5	2353	3740	0.11%	0.010%
24	14.492	1932	1939	1954	rBV	346980	881197	24.81%	2.265%
25	15.275	2065	2072	2086	rVB	2333399	3267659	92.01%	8.401%
26	15.404	2086	2094	2106	rBV	551158	1102745	31.05%	2.835%
27	15.780	2153	2158	2166	rVB	23959	39369	1.11%	0.101%
28	16.080	2204	2209	2212	rVB4	8529	12532	0.35%	0.032%
29	16.751	2318	2323	2327	rBV7	4909	9275	0.26%	0.024%
30	16.857	2338	2341	2345	rBV3	3441	4647	0.13%	0.012%
31	17.075	2370	2378	2389	rBV	1196884	2077803	58.51%	5.342%
32	17.180	2389	2396	2412	rVB	2217155	3383823	95.28%	8.699%
33	17.539	2450	2457	2460	rBV9	2765	7086	0.20%	0.018%
34	17.798	2497	2501	2508	rVB3	9575	17100	0.48%	0.044%
35	18.051	2542	2544	2549	rVB5	3756	4548	0.13%	0.012%
36	19.121	2722	2726	2731	rBV2	26445	34369	0.97%	0.088%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020026.D
Acq On : 29 Mar 2024 01:57
Operator : MA/JU
Sample : PB159808TB 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB808

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	19.198	2732	2739	2744	rBV2	24507	53719	1.51%	0.138%
38	19.574	2797	2803	2815	rBV	2510692	3551315	100.00%	9.130%
39	21.533	3130	3136	3152	rBV	924646	1772016	49.90%	4.556%
40	24.609	3649	3659	3677	rVB	913503	2708509	76.27%	6.963%
41	24.845	3690	3699	3713	rVB	529653	1638635	46.14%	4.213%




Sum of corrected areas: 38897532

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020026.D
Acq On : 29 Mar 2024 01:57
Operator : MA/JU
Sample : PB159808TB 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB808

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

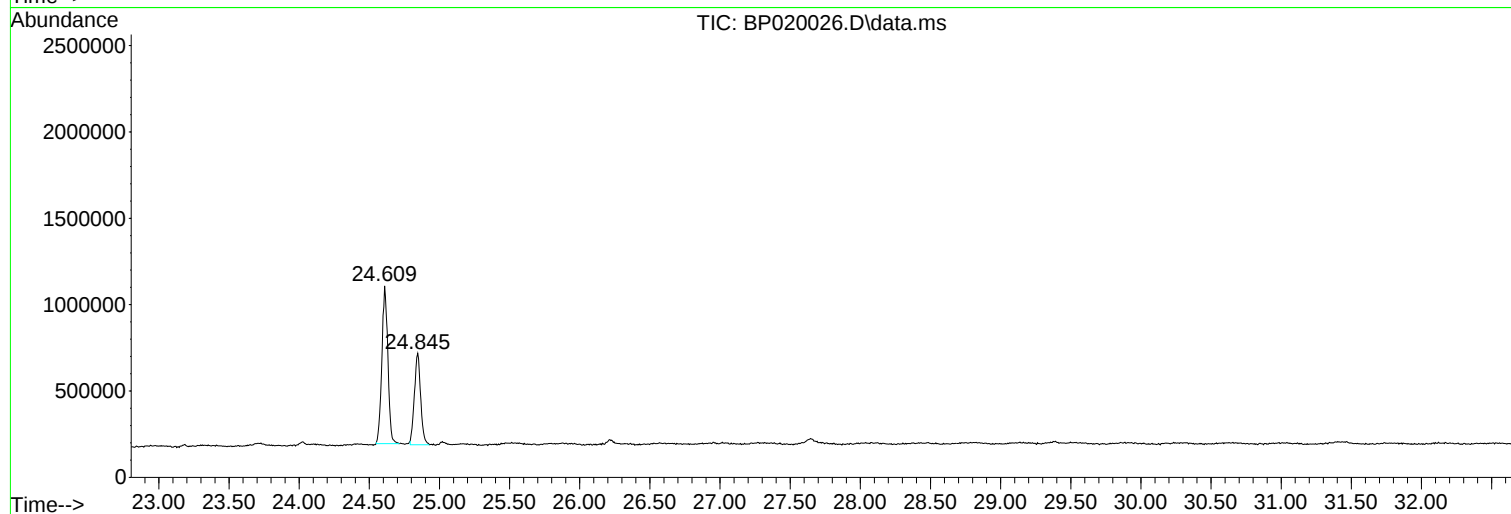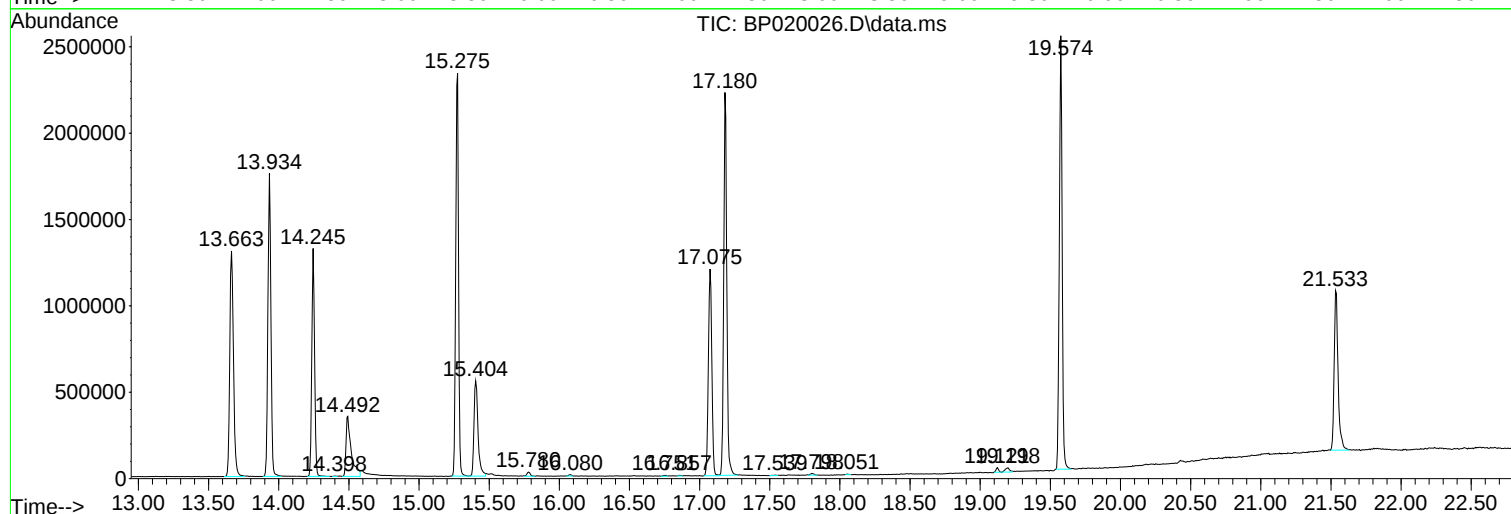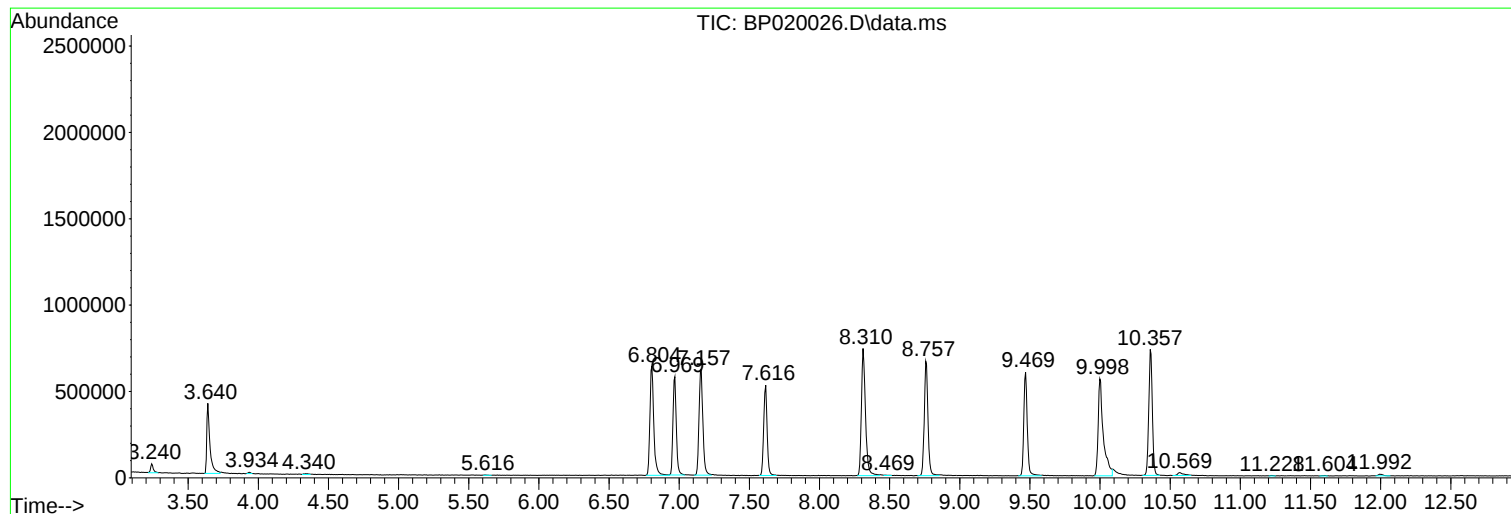

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020026.D
Acq On : 29 Mar 2024 01:57
Operator : MA/JU
Sample : PB159808TB 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB808

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020026.D
Acq On : 29 Mar 2024 01:57
Operator : MA/JU
Sample : PB159808TB 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB808

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc