

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
 Data File : BP020027.D
 Acq On : 29 Mar 2024 02:40
 Operator : MA/JU
 Sample : PB159810TB 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SLEB810

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020027.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	34	rVB	44187	60027	1.97%	0.180%
2	3.640	91	94	111	rBV	314767	537816	17.65%	1.616%
3	3.934	141	144	150	rVB3	9021	13119	0.43%	0.039%
4	4.352	210	215	218	rBV6	3401	5736	0.19%	0.017%
5	6.793	623	630	644	rBV	594173	1095250	35.94%	3.291%
6	6.969	652	660	676	rBV	477256	843277	27.67%	2.534%
7	7.152	684	691	708	rVB	629373	1053954	34.59%	3.167%
8	7.605	761	768	779	rBV	417975	741161	24.32%	2.227%
9	8.305	880	887	901	rBV	800719	1346593	44.19%	4.046%
10	8.758	956	964	985	rBV	633712	1111611	36.48%	3.340%
11	9.463	1076	1084	1097	rBV	488428	946431	31.06%	2.844%
12	9.999	1166	1175	1201	rBV	515552	1376457	45.17%	4.136%
13	10.316	1225	1229	1230	rBV4	3133	4242	0.14%	0.013%
14	10.363	1230	1237	1250	rVB	558302	1077610	35.36%	3.238%
15	10.552	1261	1269	1282	rBV3	20919	75775	2.49%	0.228%
16	11.999	1508	1515	1521	rBV4	8690	19485	0.64%	0.059%
17	13.669	1790	1799	1816	rBV	1265311	2082674	68.35%	6.258%
18	13.934	1835	1844	1859	rBV	1300914	2327089	76.37%	6.993%
19	14.240	1887	1896	1912	rBV	860972	1509280	49.53%	4.535%
20	14.493	1932	1939	1953	rBV	249790	716482	23.51%	2.153%
21	15.263	2062	2070	2082	rBV	1746897	2882419	94.59%	8.662%
22	15.416	2087	2096	2110	rBV	454549	942409	30.93%	2.832%
23	15.563	2119	2121	2125	rVB5	3193	3422	0.11%	0.010%
24	15.787	2153	2159	2167	rBV2	19972	33873	1.11%	0.102%
25	16.069	2203	2207	2212	rVB5	7905	12871	0.42%	0.039%
26	16.751	2319	2323	2328	rBV7	3699	5991	0.20%	0.018%
27	16.851	2336	2340	2347	rVB8	3891	8298	0.27%	0.025%
28	17.087	2369	2380	2389	rBV	1102946	1667693	54.73%	5.011%
29	17.175	2390	2395	2415	rVB	2122637	2942547	96.57%	8.842%
30	17.522	2451	2454	2457	rBV5	2048	3479	0.11%	0.010%
31	17.810	2497	2503	2512	rVB4	10153	24697	0.81%	0.074%
32	18.481	2615	2617	2620	rBV4	3664	3744	0.12%	0.011%
33	19.128	2722	2727	2732	rBV4	22157	37706	1.24%	0.113%
34	19.192	2733	2738	2742	rBV3	21719	40191	1.32%	0.121%
35	19.575	2797	2803	2816	rBV	2163525	3047189	100.00%	9.157%
36	21.545	3132	3138	3153	rBV2	639587	1459476	47.90%	4.386%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020027.D
Acq On : 29 Mar 2024 02:40
Operator : MA/JU
Sample : PB159810TB 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB810

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	24.604	3649	3658	3671	rBV2	943712	2569110	84.31%	7.720%
38	24.839	3691	3698	3699	rBV	414765	649232	21.31%	1.951%




Sum of corrected areas: 33278416

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020027.D
Acq On : 29 Mar 2024 02:40
Operator : MA/JU
Sample : PB159810TB 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

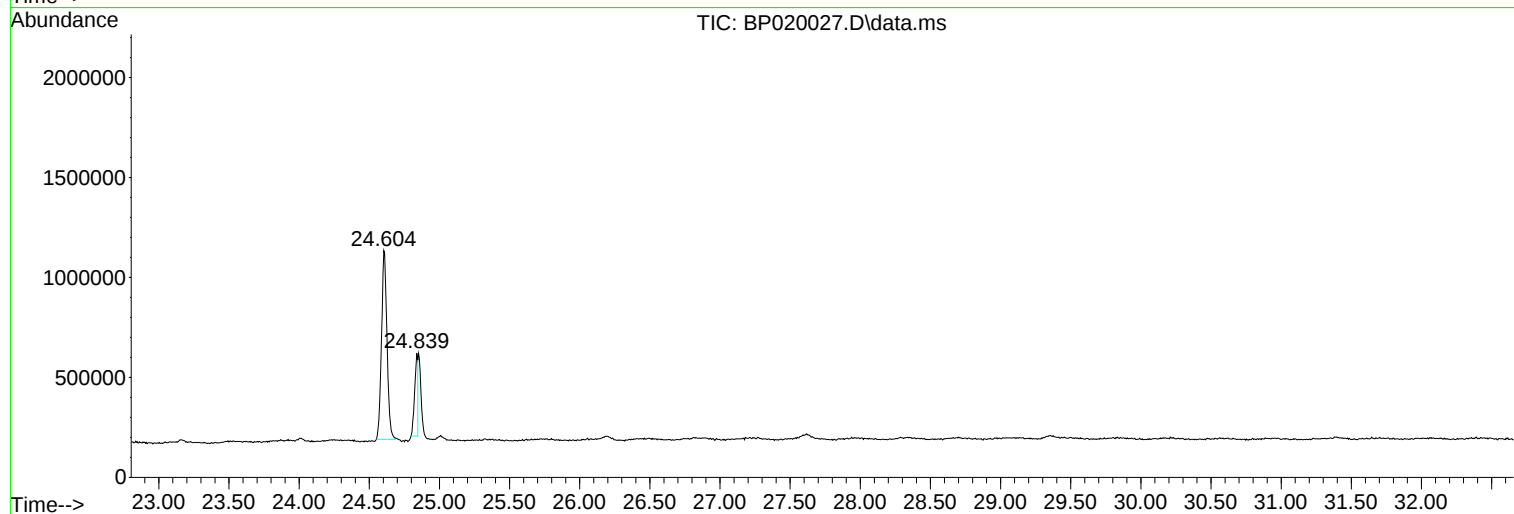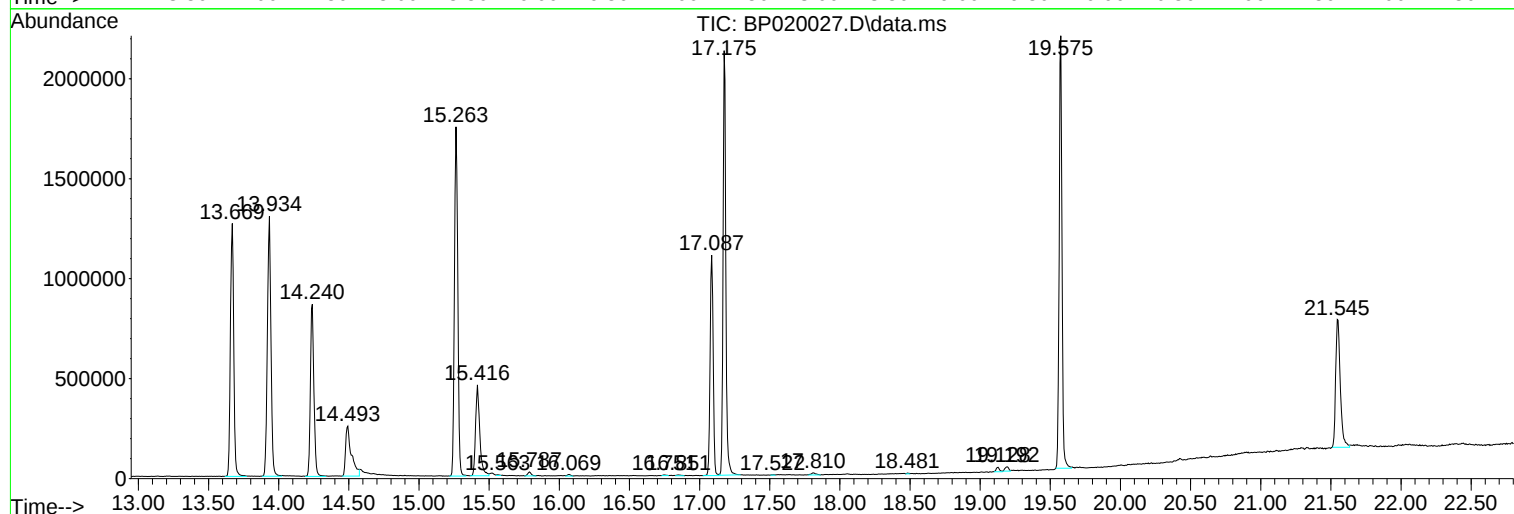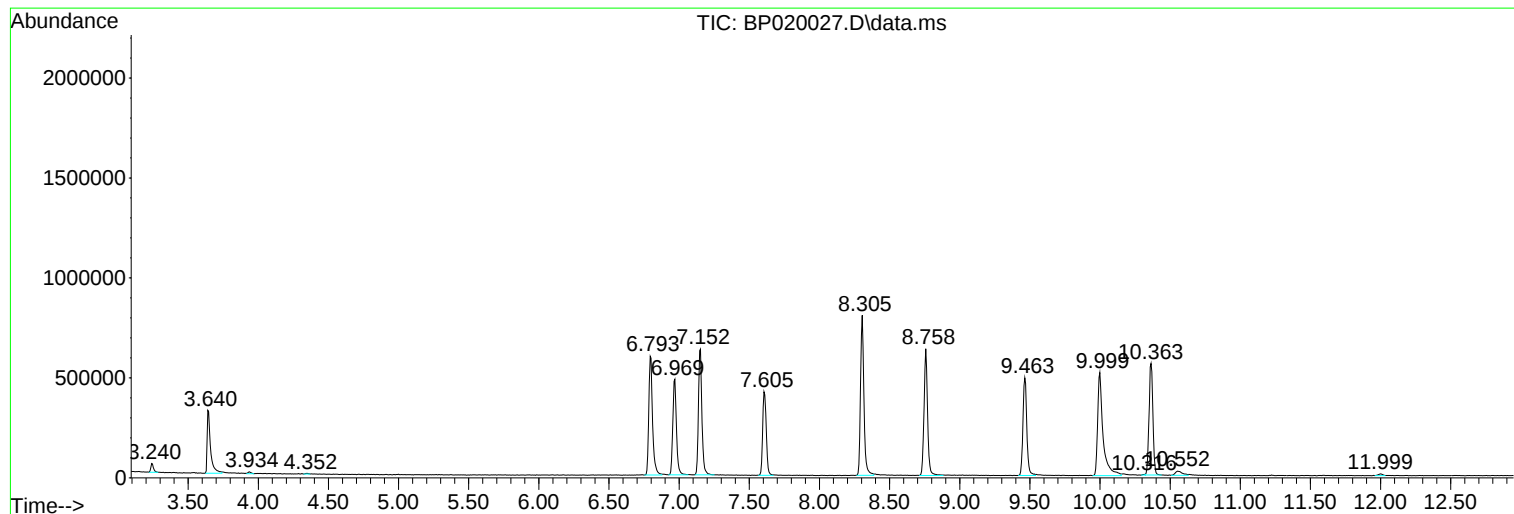

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020027.D
Acq On : 29 Mar 2024 02:40
Operator : MA/JU
Sample : PB159810TB 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032824\
Data File : BP020027.D
Acq On : 29 Mar 2024 02:40
Operator : MA/JU
Sample : PB159810TB 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SLEB810

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc