
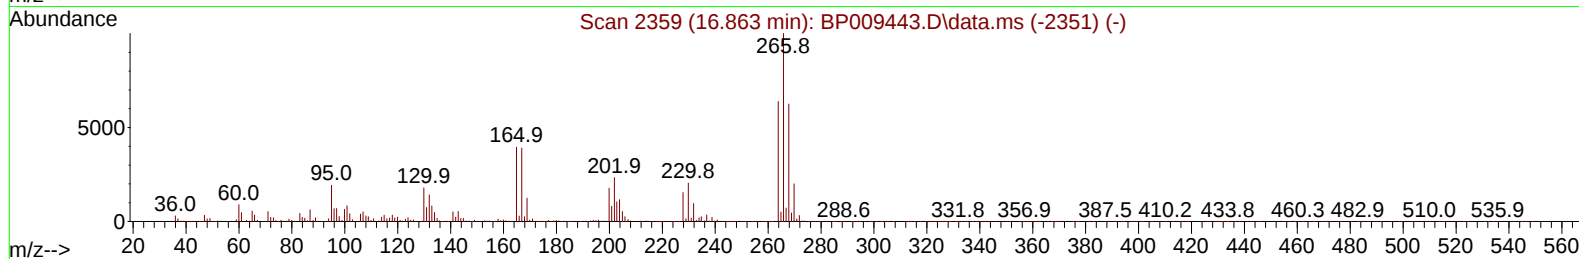
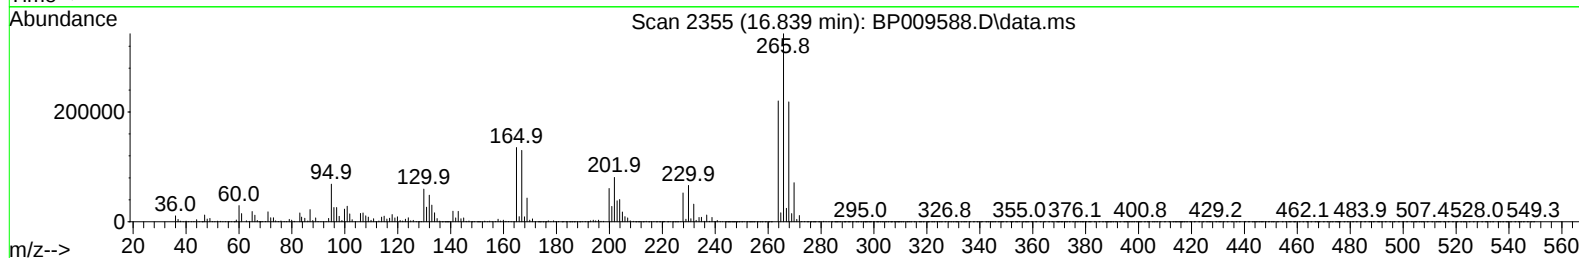


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009588.D
Acq On : 29 Mar 2022 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:16:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 04:00:13 2022
Response via : Initial Calibration

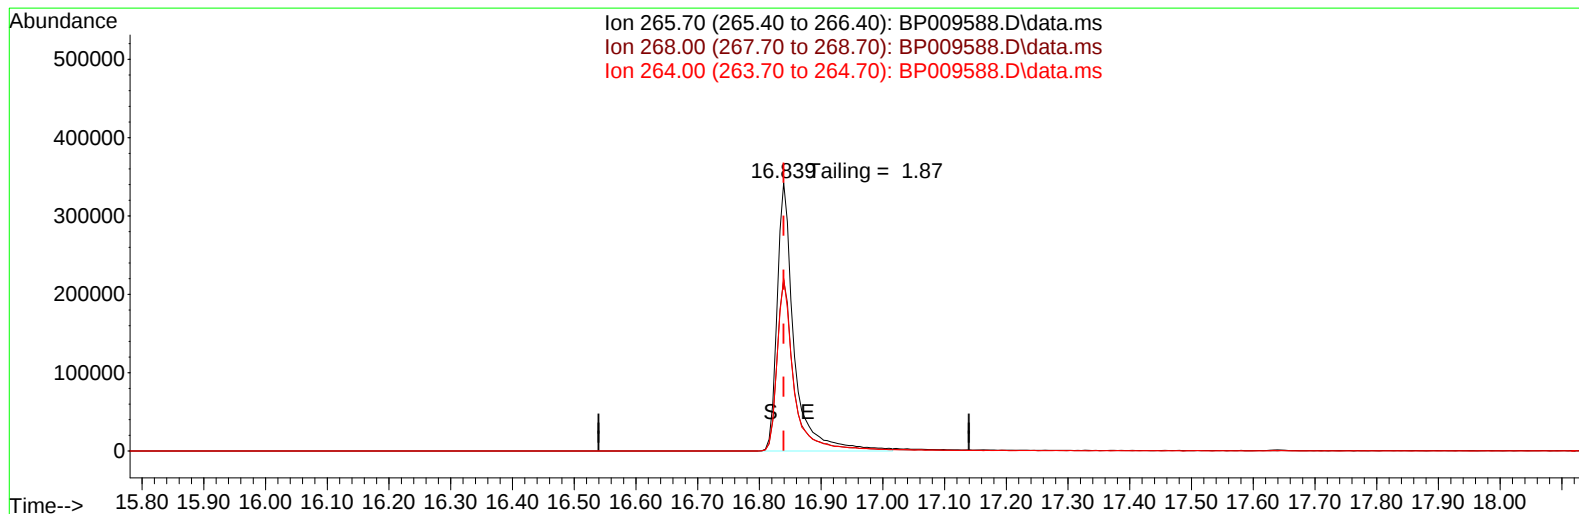

TIC: BP009588.D\data.ms

(70) Pentachlorophenol (C)




16.839min (+ 0.000) 160956.73 ng

response 671292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.76
264.00	63.60	64.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009588.D
 Acq On : 29 Mar 2022 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 30 08:16:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 30 04:00:13 2022
 Response via : Initial Calibration

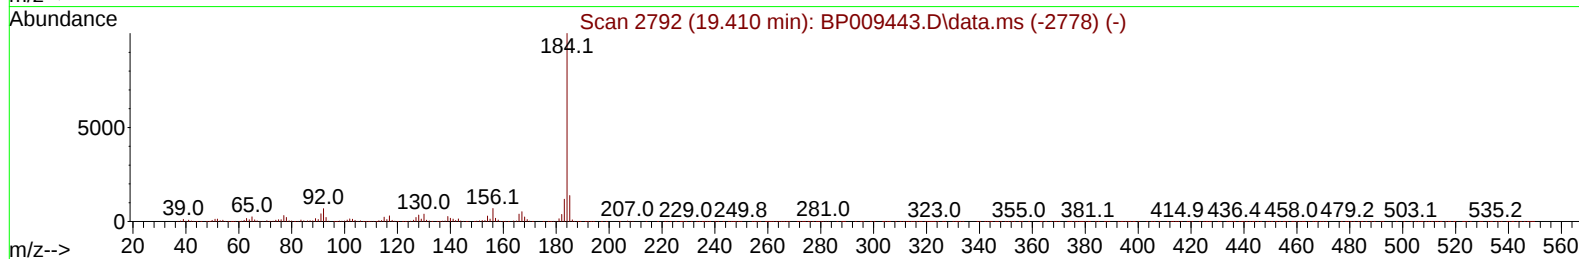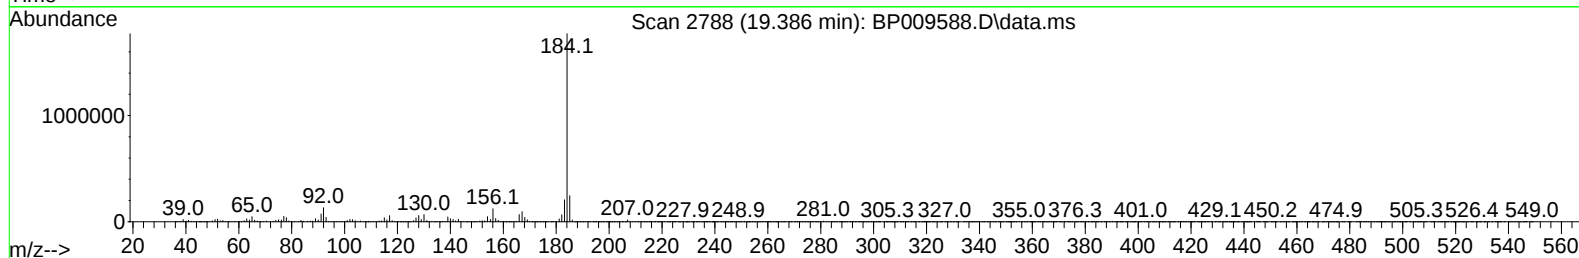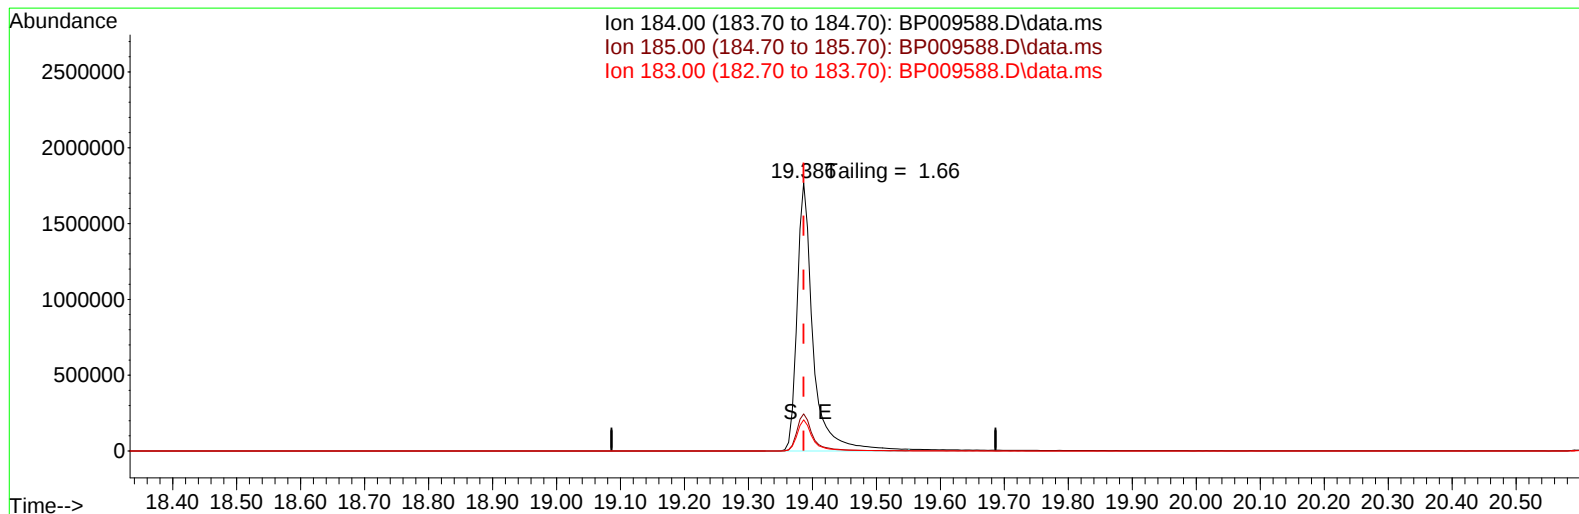

TIC: BP009588.D\data.ms

(77) Benzidine**19.386min (+ 0.000) 48238.76 ng****response 3113248**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.84
183.00	11.70	11.66
0.00	0.00	0.00