

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009594.D
 Acq On : 29 Mar 2022 14:19
 Operator : CG/JU
 Sample : PB143663BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143663BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.370	398	405	439	rBV	3761155	6734257	48.68%	10.706%
2	6.952	666	674	705	rBV	3535919	6680912	48.30%	10.621%
3	7.764	804	812	827	rBV	742833	1348823	9.75%	2.144%
4	8.922	1000	1009	1037	rBV	2118240	4332499	31.32%	6.888%
5	10.558	1278	1287	1315	rBV	762062	1790464	12.94%	2.846%
6	13.028	1698	1707	1733	rBV	5871458	10057510	72.71%	15.989%
7	14.410	1935	1942	1963	rBV	1210346	2260926	16.34%	3.594%
8	15.910	2189	2197	2224	rBV	3941258	7056758	51.02%	11.219%
9	17.175	2405	2412	2434	rBV	1323515	2573144	18.60%	4.091%
10	19.751	2845	2850	2866	rBV	9812889	13832678	100.00%	21.991%
11	21.292	3107	3112	3125	rBV	1890970	2981131	21.55%	4.739%
12	23.680	3512	3518	3538	rVB2	1387124	3253618	23.52%	5.172%




Sum of corrected areas: 62902720

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009594.D
Acq On : 29 Mar 2022 14:19
Operator : CG/JU
Sample : PB143663BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143663BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

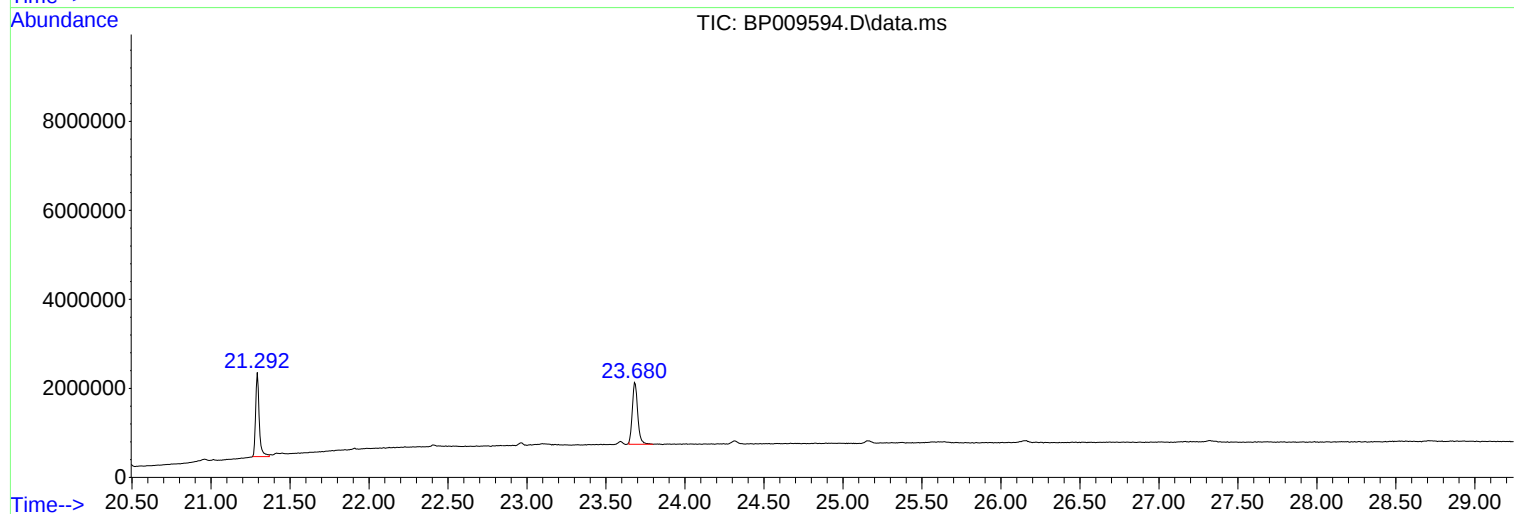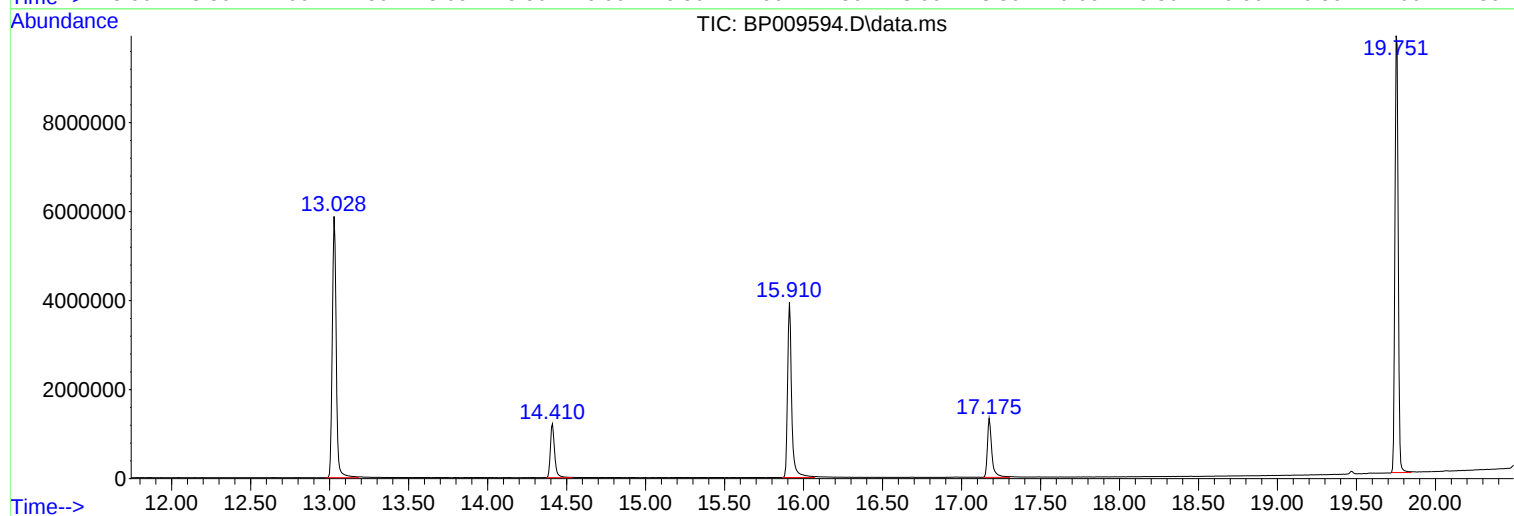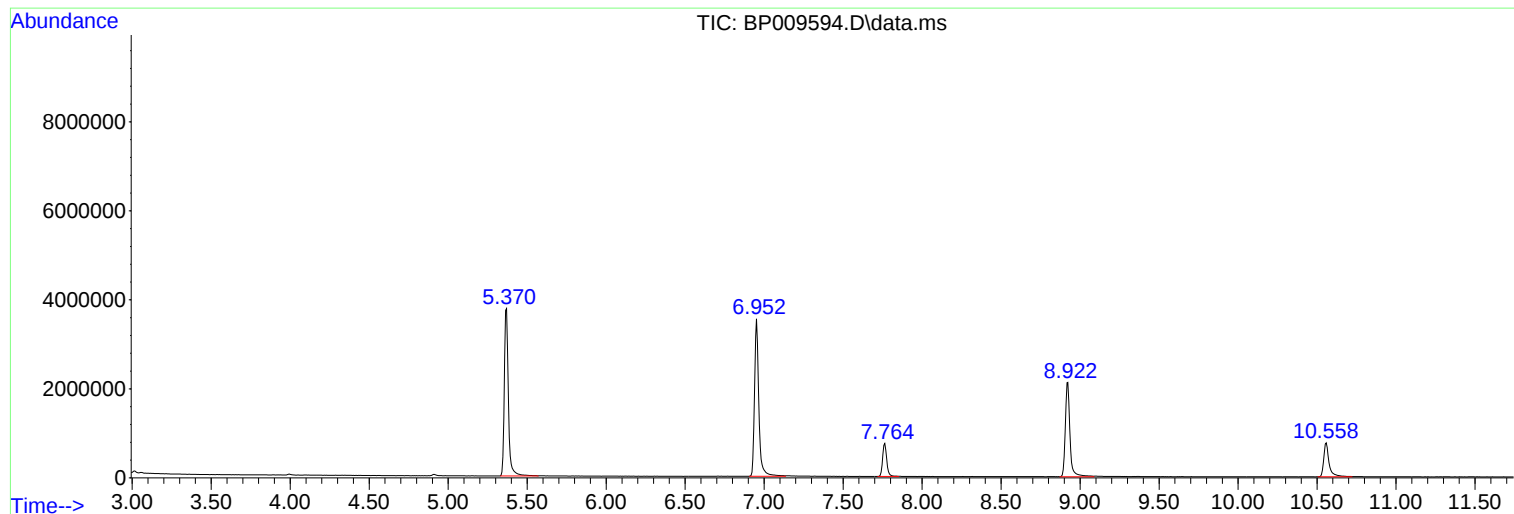

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009594.D
Acq On : 29 Mar 2022 14:19
Operator : CG/JU
Sample : PB143663BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143663BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009594.D
Acq On : 29 Mar 2022 14:19
Operator : CG/JU
Sample : PB143663BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143663BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------