

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009597.D
Acq On : 29 Mar 2022 16:35
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009597.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	398	405	439	rBV	4018175	7091444	50.74%	10.950%
2	6.951	667	674	699	rBV	3667855	6931893	49.60%	10.703%
3	7.763	805	812	826	rBV	776793	1438748	10.29%	2.221%
4	8.922	1000	1009	1039	rBV	2244296	4577453	32.75%	7.068%
5	10.557	1278	1287	1318	rBV	801818	1892408	13.54%	2.922%
6	13.027	1699	1707	1748	rBV	6149839	10549879	75.48%	16.290%
7	14.410	1933	1942	1962	rBV	1250632	2349228	16.81%	3.627%
8	15.910	2190	2197	2228	rBV	4055008	7214778	51.62%	11.140%
9	17.174	2405	2412	2446	rBV	1346322	2653973	18.99%	4.098%
10	19.757	2845	2851	2866	rBV	10350711	13976900	100.00%	21.581%
11	21.292	3107	3112	3124	rBV	1849953	2974347	21.28%	4.593%
12	23.686	3512	3519	3534	rVB2	1348622	3113801	22.28%	4.808%




Sum of corrected areas: 64764852

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009597.D
Acq On : 29 Mar 2022 16:35
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

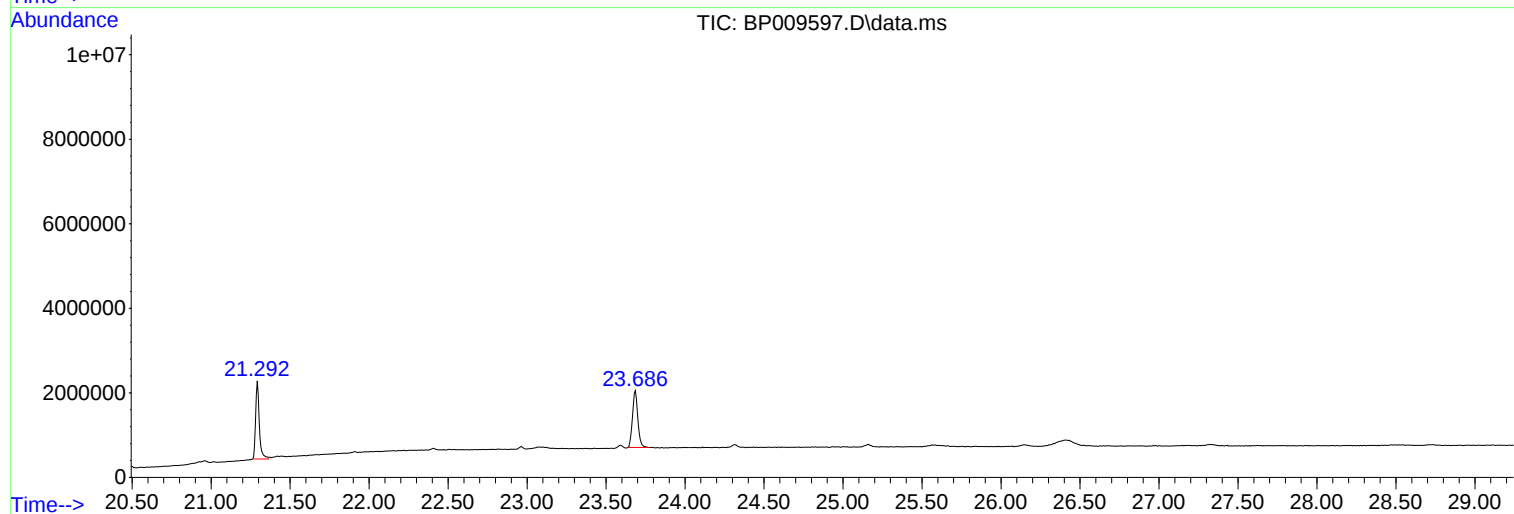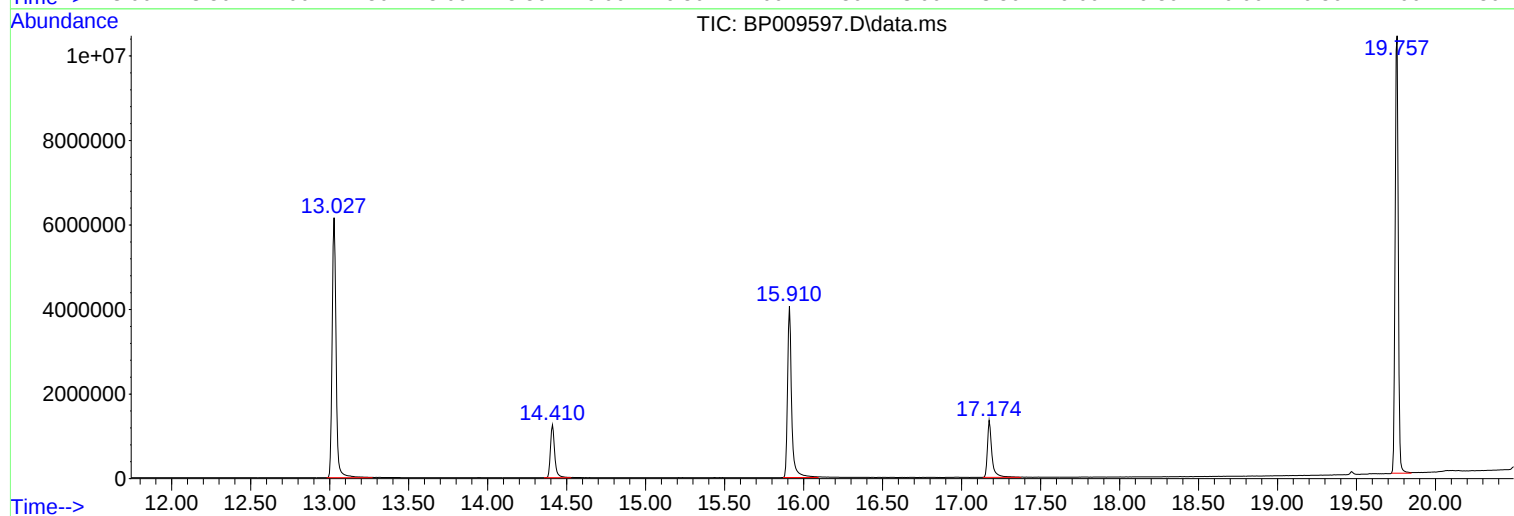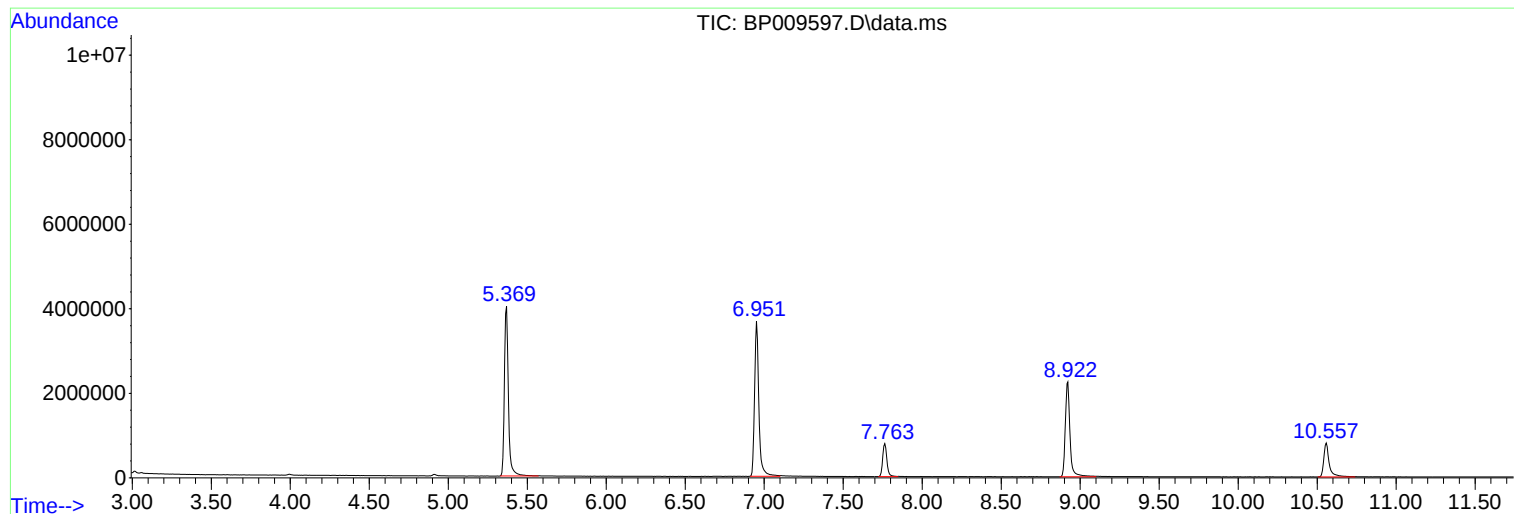

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009597.D
Acq On : 29 Mar 2022 16:35
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009597.D
Acq On : 29 Mar 2022 16:35
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------