

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009610.D
 Acq On : 30 Mar 2022 00:07
 Operator : CG/JU
 Sample : N2095-01 2X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-01-5.0-6.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009610.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.369	398	405	427	rBV	1497412	2748413	15.99%	4.513%
2	6.951	666	674	689	rBV	1337958	2783390	16.19%	4.570%
3	7.763	805	812	824	rBV	1054137	1854950	10.79%	3.046%
4	8.922	996	1009	1033	rBV	857309	1865896	10.85%	3.064%
5	10.557	1276	1287	1302	rBV	1303870	2619555	15.24%	4.301%
6	13.028	1700	1707	1722	rBV	2765683	4630340	26.93%	7.603%
7	14.410	1935	1942	1950	rBV	2157775	3482723	20.26%	5.718%
8	15.910	2191	2197	2215	rBV	2087201	3474042	20.21%	5.704%
9	17.174	2406	2412	2423	rBV	2632424	4053449	23.58%	6.655%
10	18.086	2563	2567	2579	rBV3	193662	353826	2.06%	0.581%
11	19.751	2845	2850	2856	rBV	4886745	6402222	37.24%	10.512%
12	21.292	3107	3112	3121	rBV	3183860	4677063	27.20%	7.679%
13	21.410	3127	3132	3148	rBV	11743019	17193683	100.00%	28.231%
14	23.686	3513	3519	3527	rVB2	2260545	4764320	27.71%	7.823%




Sum of corrected areas: 60903872

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009610.D
Acq On : 30 Mar 2022 00:07
Operator : CG/JU
Sample : N2095-01 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-01-5.0-6.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

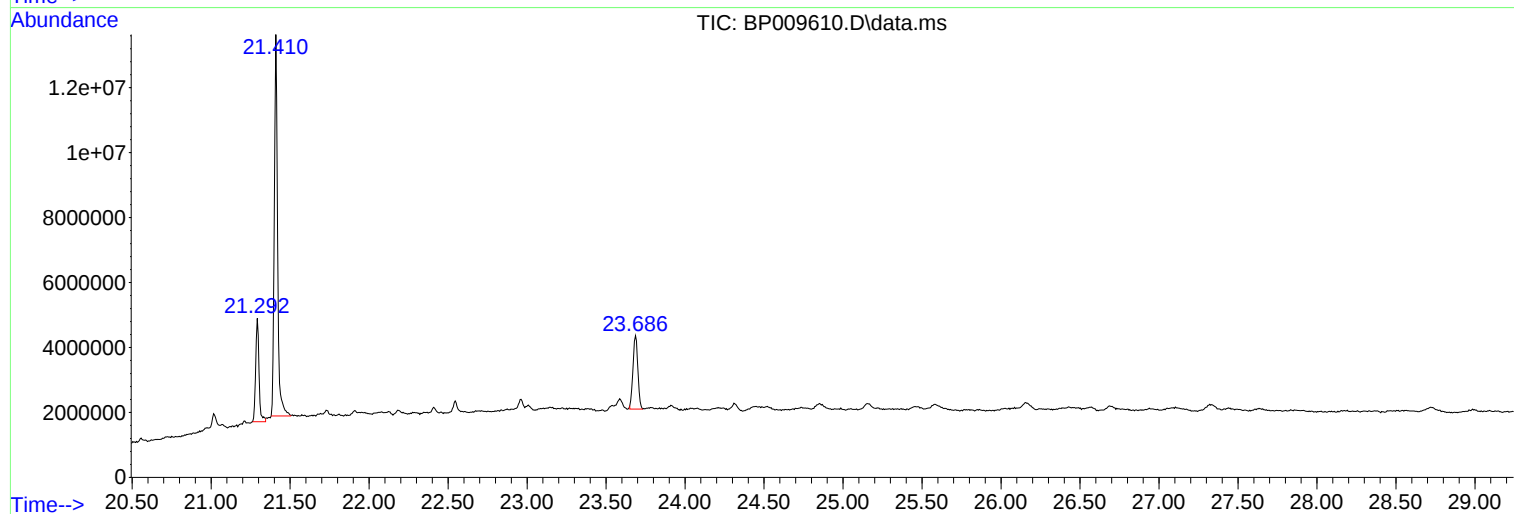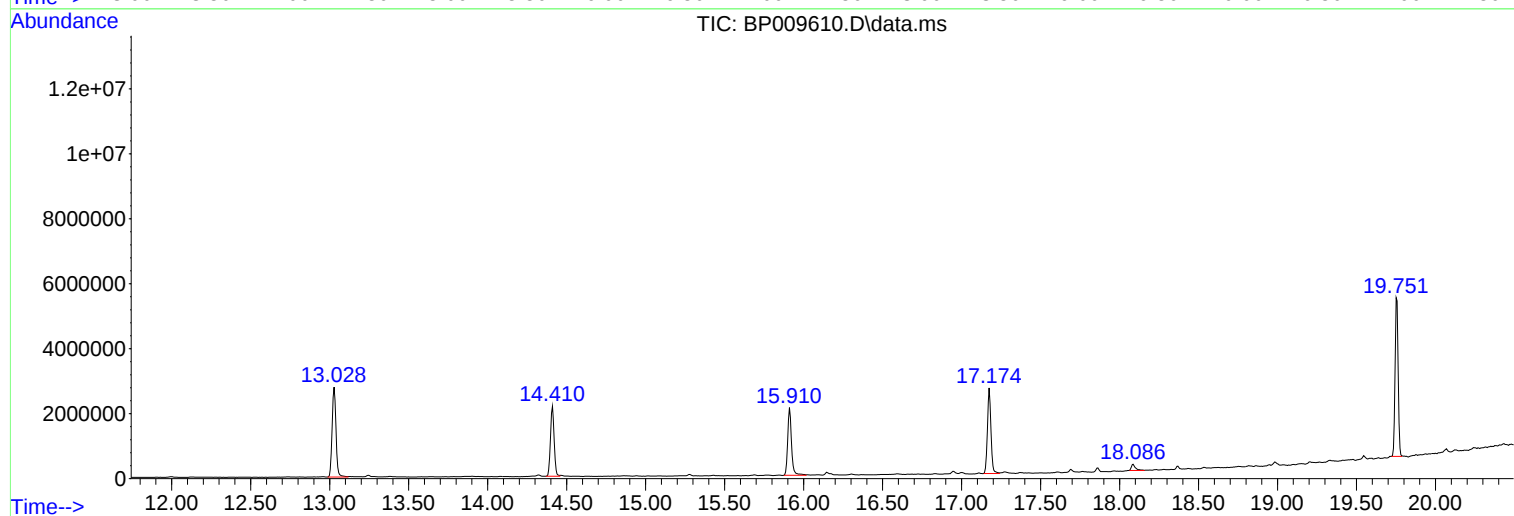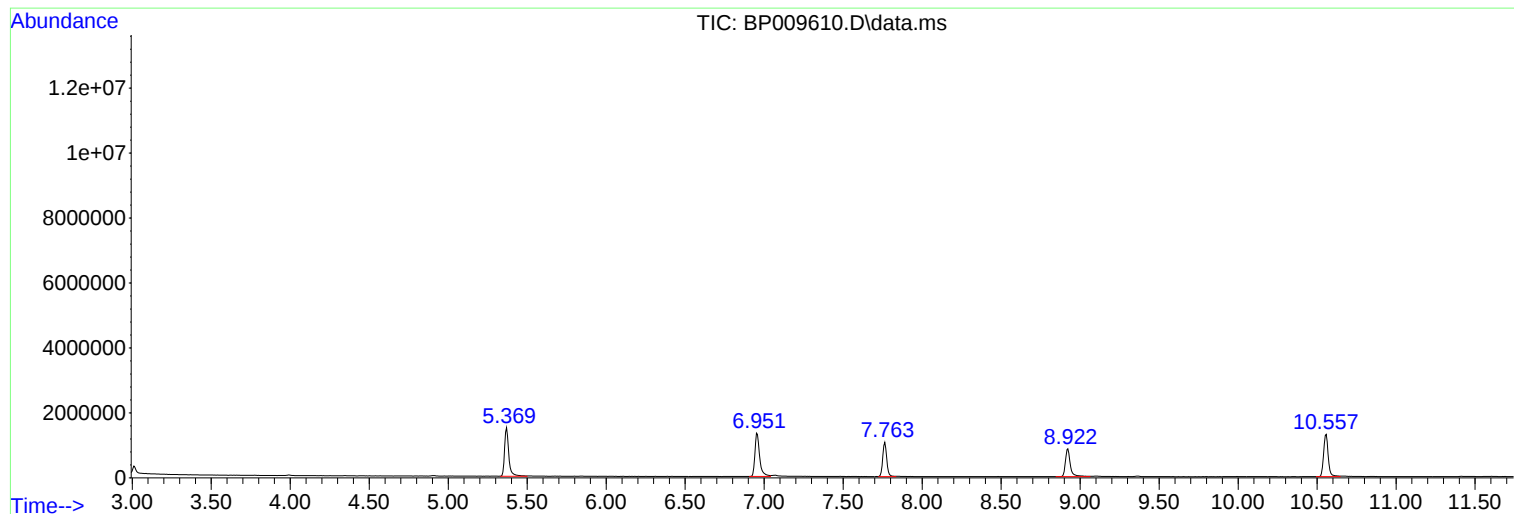

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009610.D
Acq On : 30 Mar 2022 00:07
Operator : CG/JU
Sample : N2095-01 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-01-5.0-6.0










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (E)-7-Benzylidene-1-azabicyclo... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.410	73.52 ng	17193700	Chrysene-d12	21.292

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	(E)-7-Benzylidene-1-azabicyclo[3... 293	C15H19NO3S	1000483-83-4	91			
2	Triphenylphosphine oxide	278	C18H15OP	000791-28-6	72		
3	Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	37		
4	5-Methyl-8-phenylfuro[3',2':5,6]...	277	C16H11N3O2	1000460-07-9	25		
5	[1,2,4]Triazolo[1,5-a]pyrimidine...	278	C15H14N6	1000350-69-0	9		

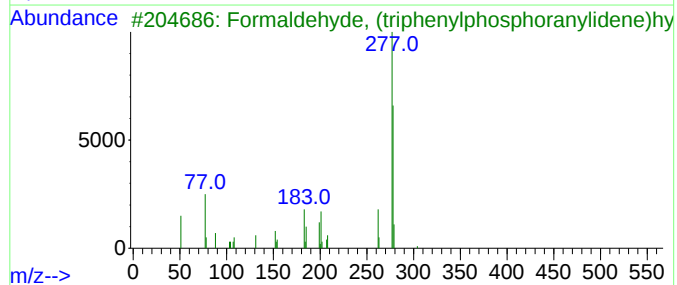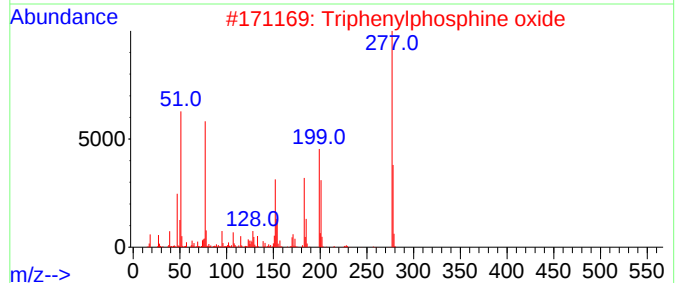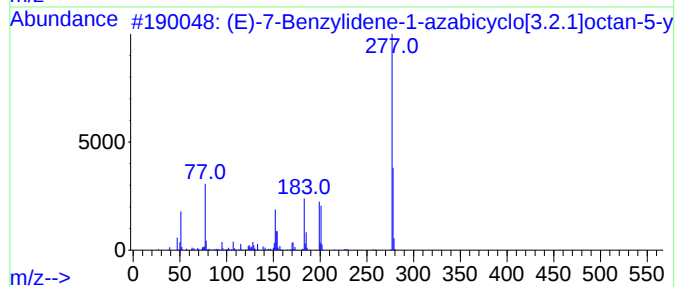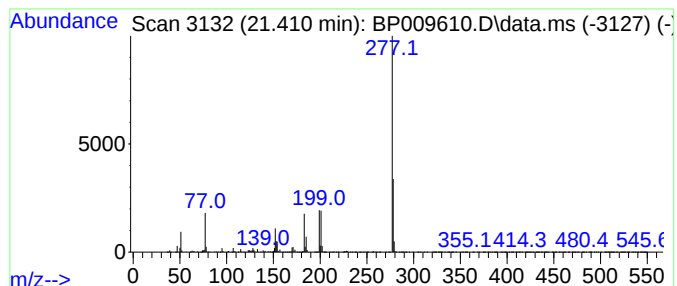

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009610.D
Acq On : 30 Mar 2022 00:07
Operator : CG/JU
Sample : N2095-01 2X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-01-5.0-6.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(E)-7-Benzylide...	21.410	73.5	ng	17193700	5	21.292	4677060	20.0