
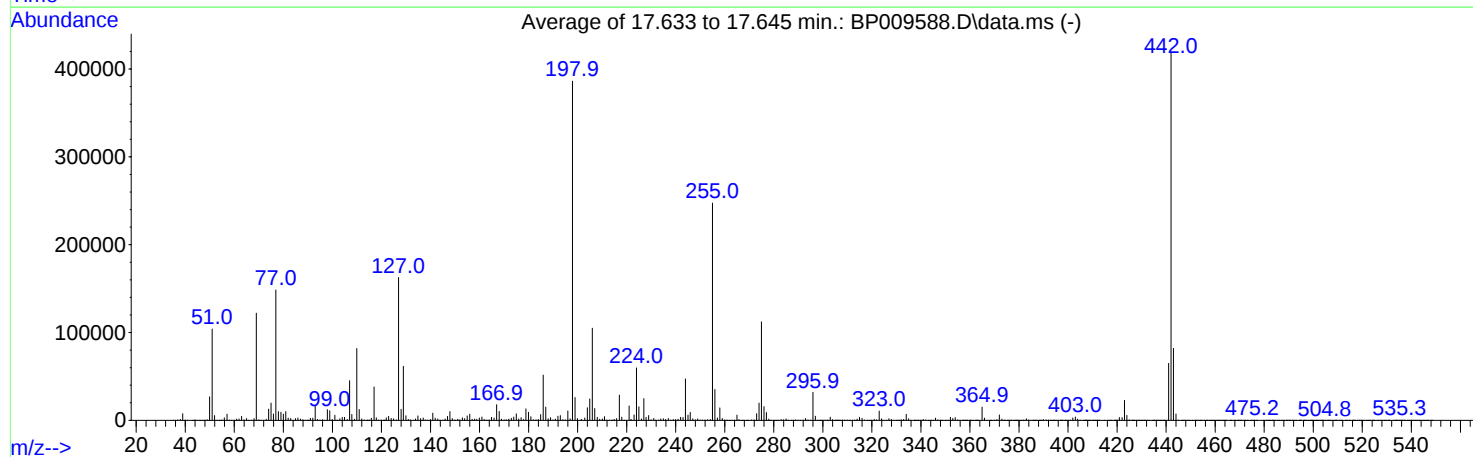


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009588.D
 Acq On : 29 Mar 2022 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 04:00:13 2022

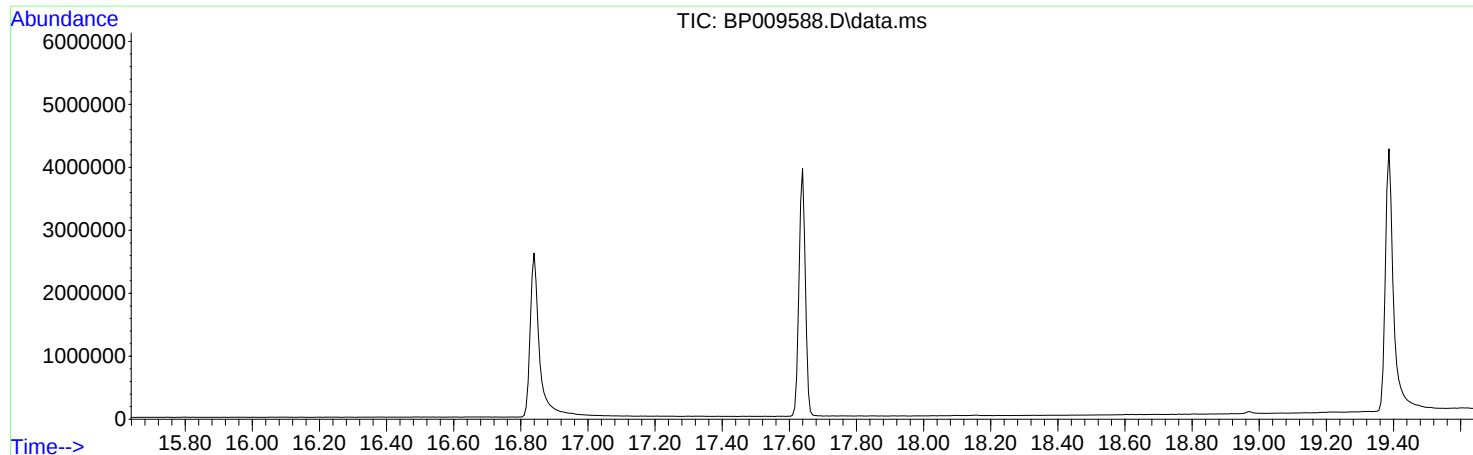




AutoFind: Scans 2490, 2491, 2492; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.9	103942	PASS
68	69	0.00	2	1.7	2104	PASS
69	198	0.00	100	31.6	121970	PASS
70	69	0.00	2	0.6	729	PASS
127	198	10	80	42.1	162770	PASS
197	198	0.00	2	0.5	1832	PASS
198	198	100	100	100.0	386185	PASS
199	198	5	9	6.7	26022	PASS
275	198	10	60	29.1	112315	PASS
365	198	1	100	3.9	15168	PASS
441	198	0.01	100	16.8	64939	PASS
442	442	100	100	100.0	418815	PASS
443	442	15	24	19.6	81949	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009588.D
Acq On : 29 Mar 2022 10:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 30 08:16:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 04:00:13 2022
Response via : Initial Calibration

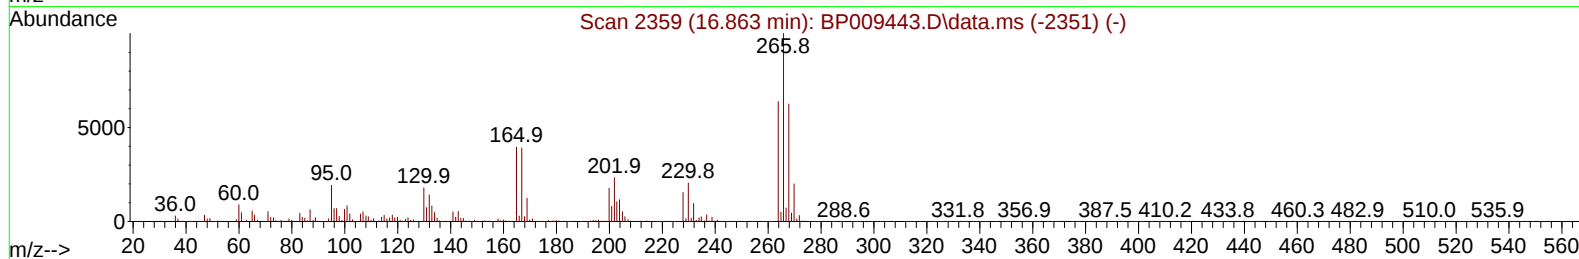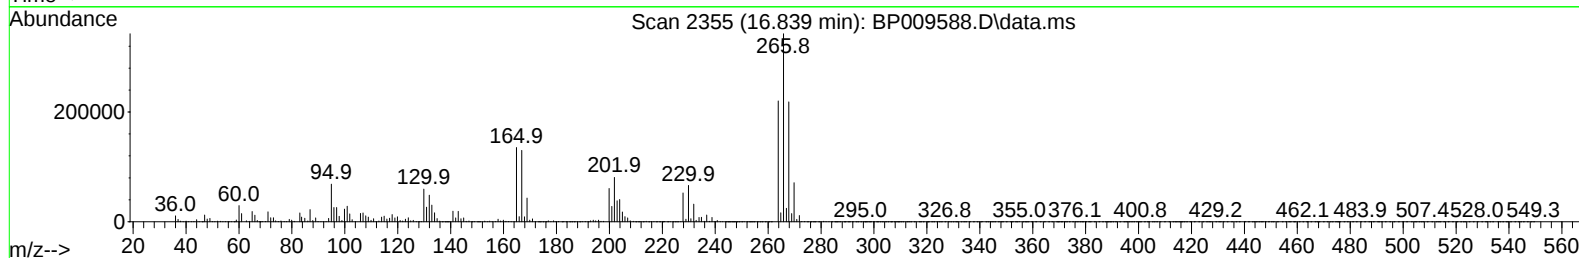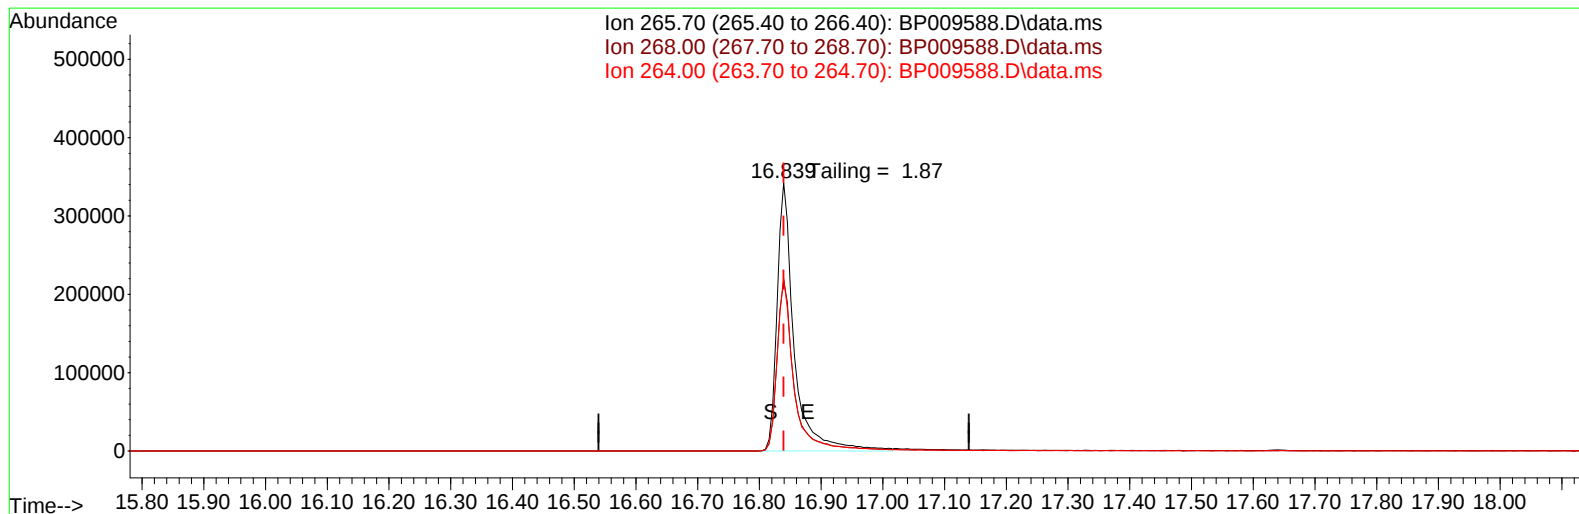

TIC: BP009588.D\data.ms

(70) Pentachlorophenol (C)

16.839min (+ 0.000) 160956.73 ng




response 671292

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	63.76
264.00	63.60	64.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009588.D
 Acq On : 29 Mar 2022 10:10
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 30 08:16:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 30 04:00:13 2022
 Response via : Initial Calibration

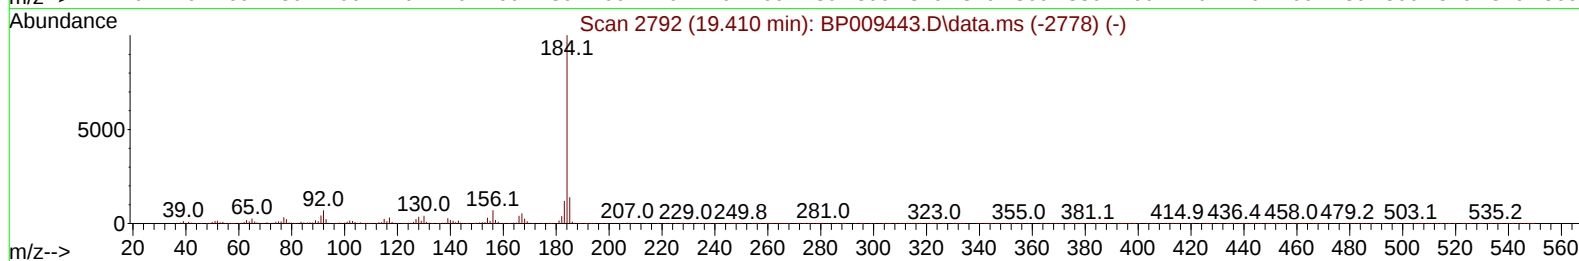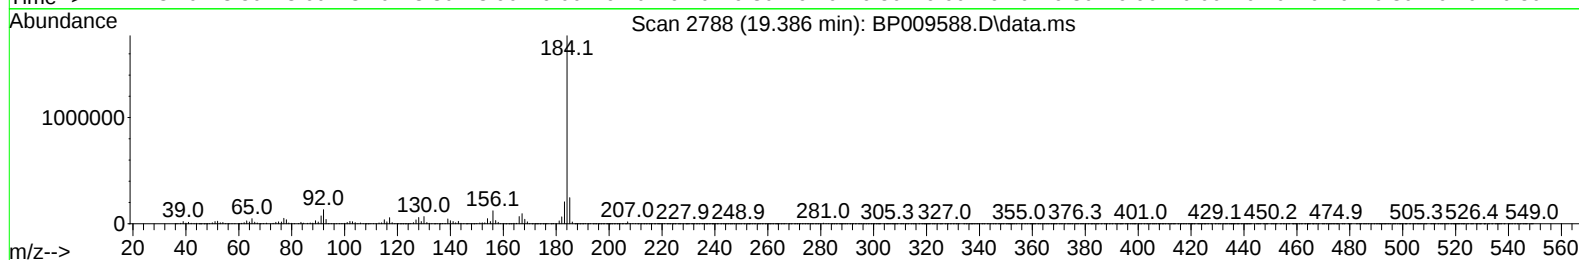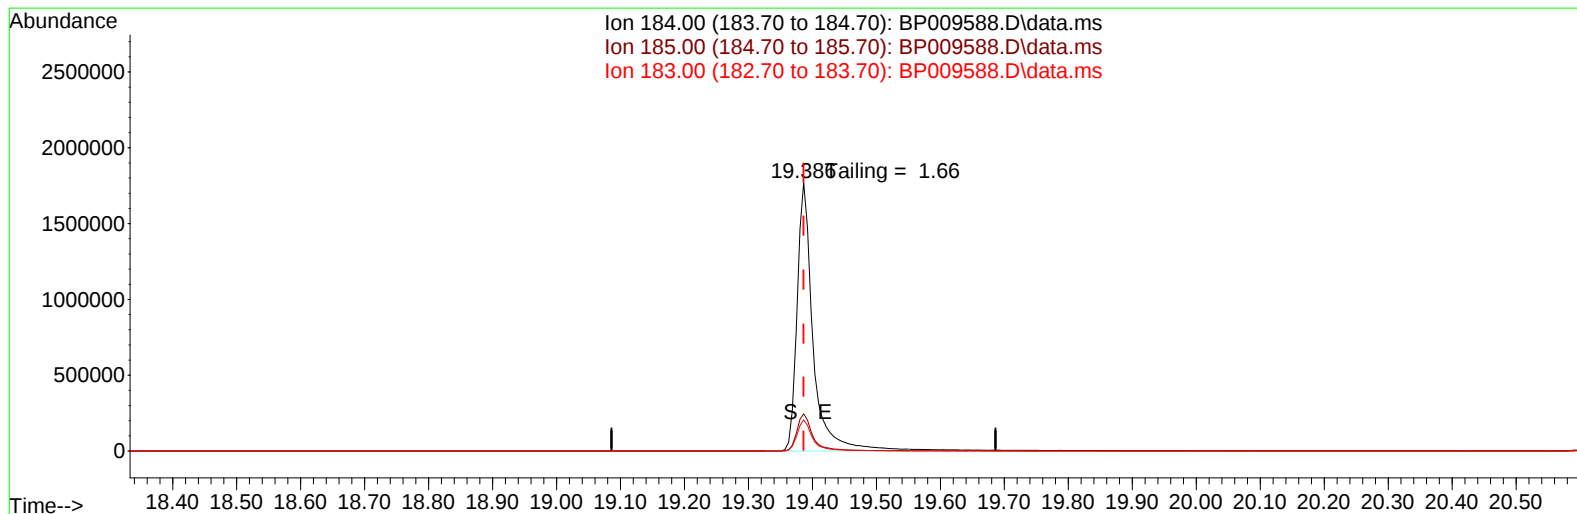

TIC: BP009588.D\data.ms

(77) Benzidine

19.386min (+ 0.000) 48238.76 ng

response 3113248

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.84
183.00	11.70	11.66
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/29/2022	BNA_P	<u>BP009588.D</u>
Compound Name	Response	Retention Time
DDT	1506402	20.598
DDD	25169	20.169
DDE	3271	19.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
28440	1534842	1.85

Instrument :
BNA_P
ClientSampleId :
DFTPP