
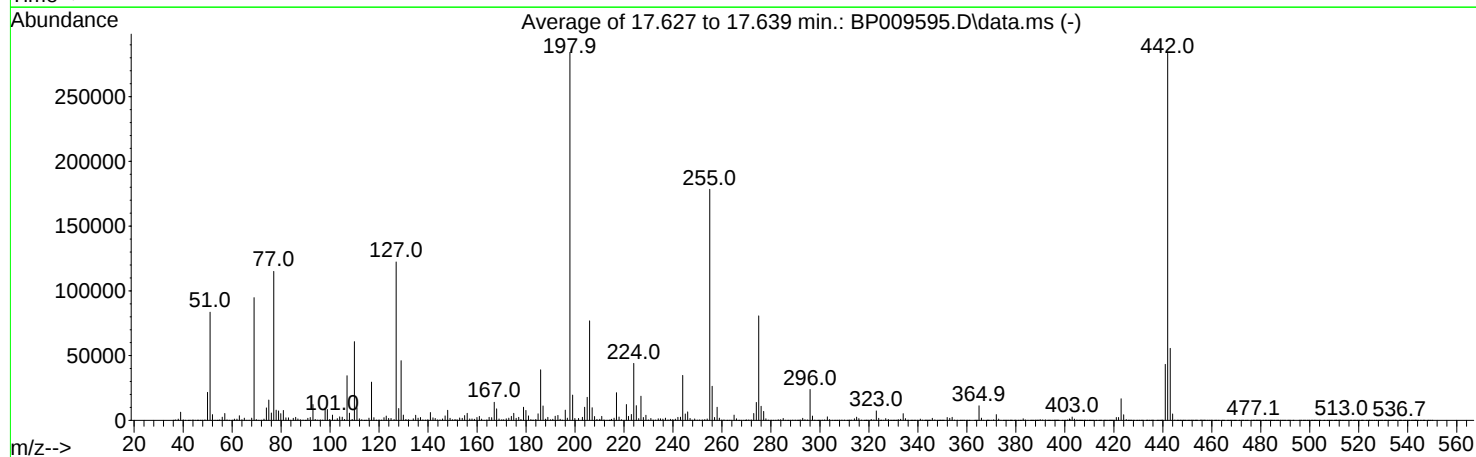


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009595.D
 Acq On : 29 Mar 2022 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 30 04:00:13 2022

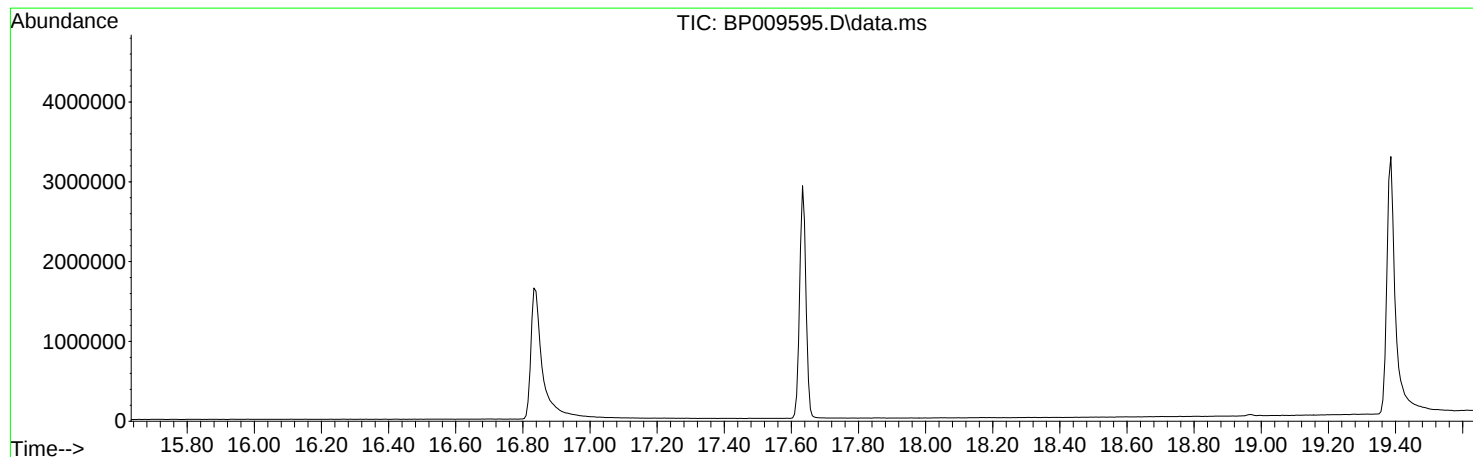

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.4	83591	PASS
68	69	0.00	2	1.8	1744	PASS
69	198	0.00	100	33.4	94838	PASS
70	69	0.00	2	0.6	602	PASS
127	198	10	80	43.0	122280	PASS
197	198	0.00	2	0.6	1722	PASS
198	198	100	100	100.0	284077	PASS
199	198	5	9	6.9	19507	PASS
275	198	10	60	28.4	80725	PASS
365	198	1	100	4.0	11260	PASS
441	198	0.01	100	15.2	43248	PASS
442	442	100	100	100.0	283499	PASS
443	442	15	24	19.6	55552	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/29/2022	BNA_P	<u>BP009595.D</u>
Compound Name	Response	Retention Time
DDT	1164830	20.592
DDD	23036	20.168
DDE	3351	19.668
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26387	1191217	2.22

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
Data File : BP009595.D
Acq On : 29 Mar 2022 15:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 30 05:34:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 30 04:00:13 2022
Response via : Initial Calibration

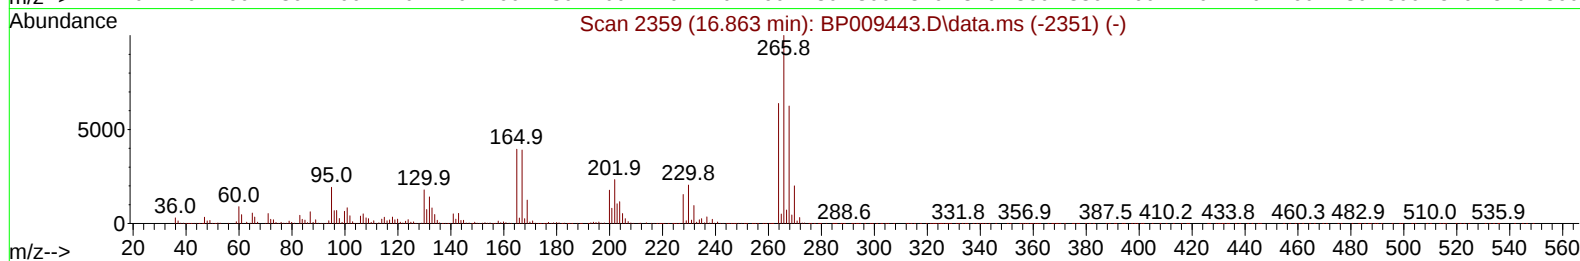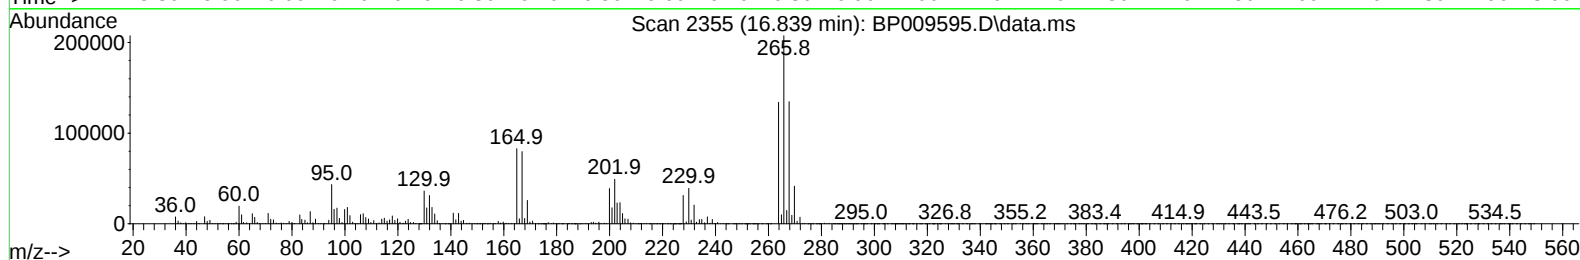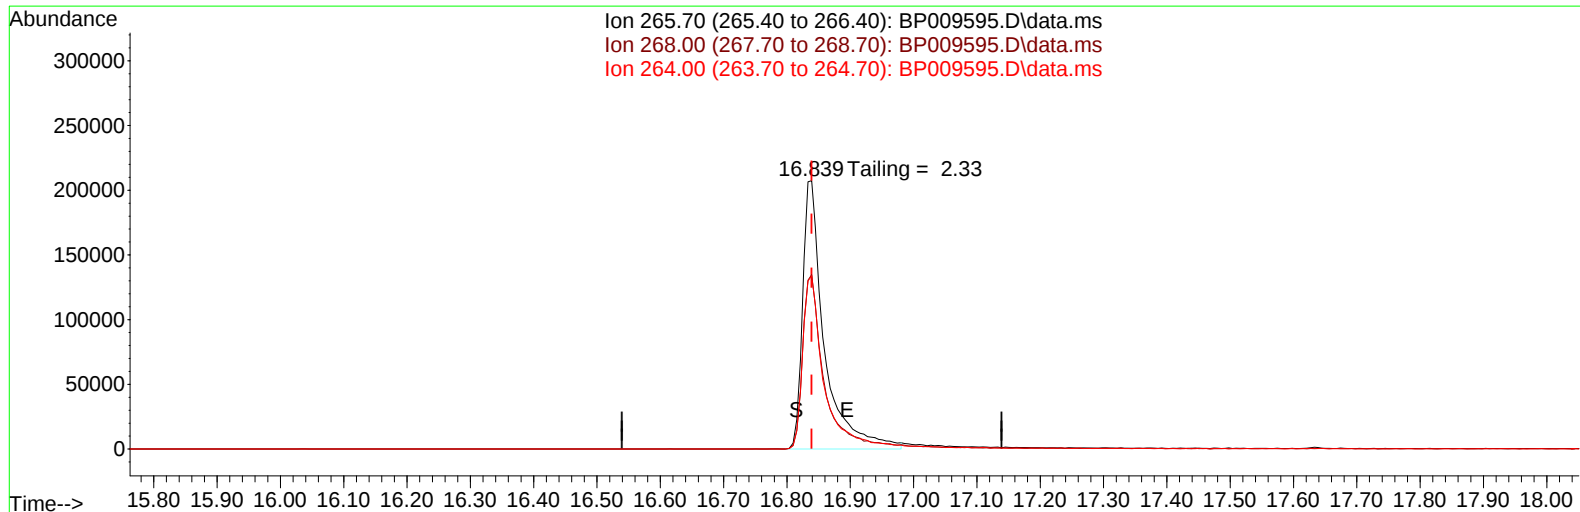

TIC: BP009595.D\data.ms

(70) Pentachlorophenol (C)

16.839min (-0.000) 1355373.98 ng




response 510178

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.95
264.00	63.60	64.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032922\
 Data File : BP009595.D
 Acq On : 29 Mar 2022 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 30 05:34:41 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 30 04:00:13 2022
 Response via : Initial Calibration

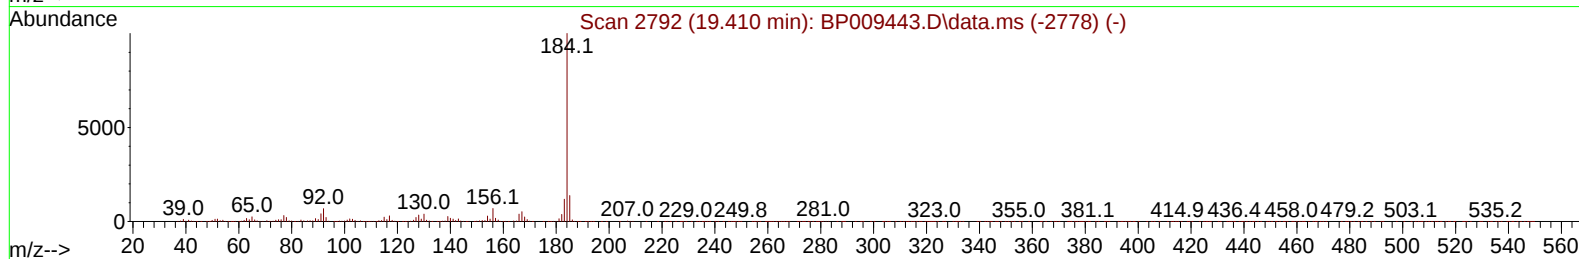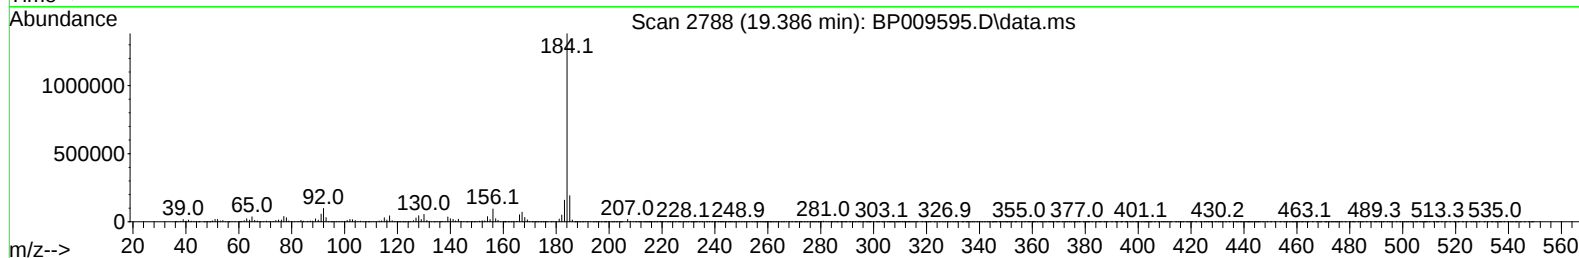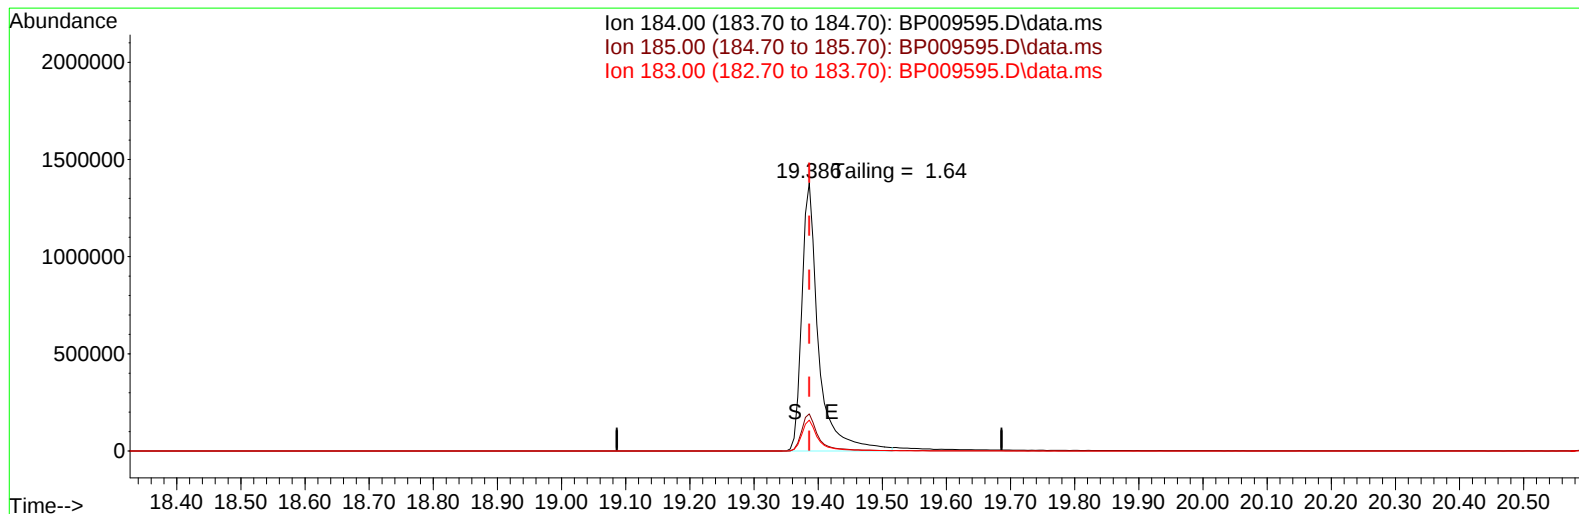

TIC: BP009595.D\data.ms

(77) Benzidine

19.386min (-0.000) 431758.17 ng

response 2550494

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.83
183.00	11.70	11.50
0.00	0.00	0.00