
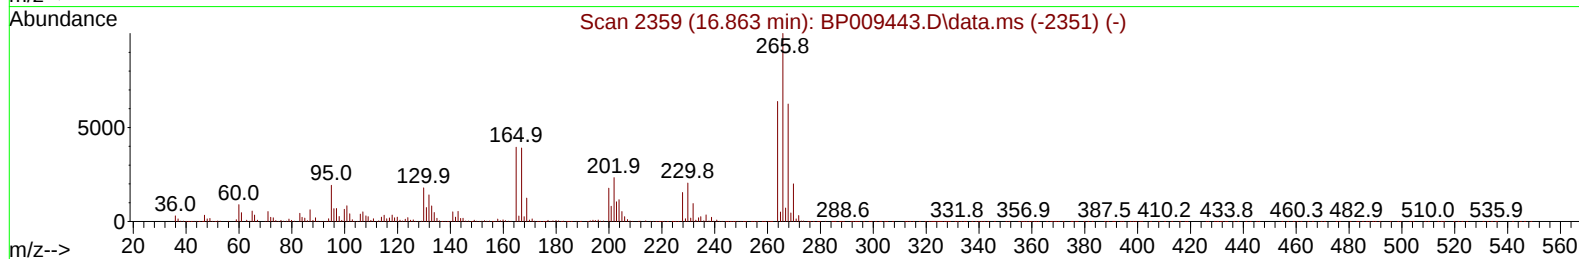
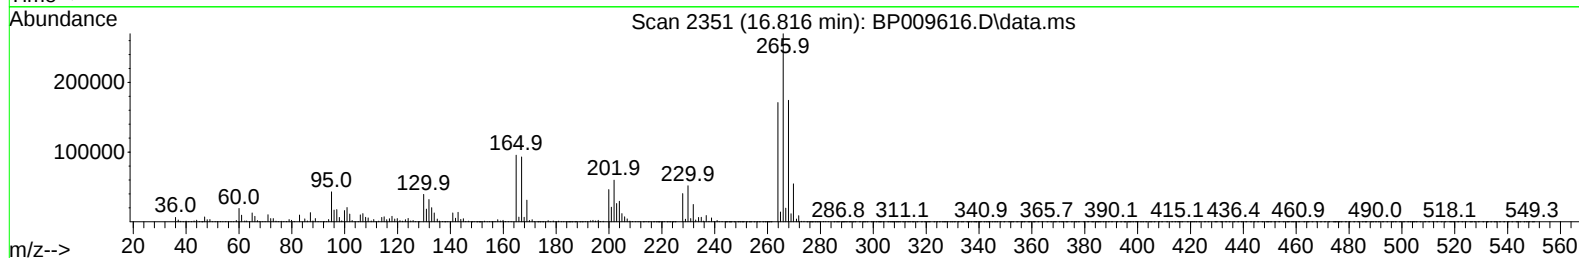


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033022\
Data File : BP009616.D
Acq On : 30 Mar 2022 12:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 05:51:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 31 04:36:51 2022
Response via : Initial Calibration

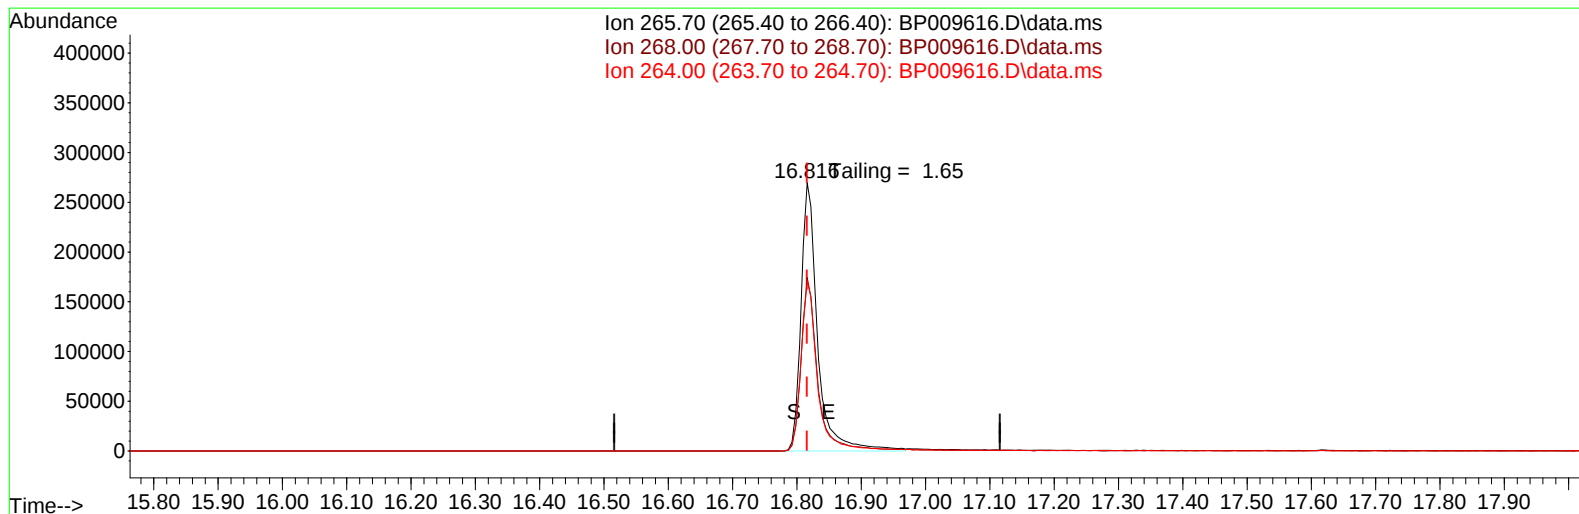

TIC: BP009616.D\data.ms

(70) Pentachlorophenol (C)




16.816min (+ 0.000) 3263319.14 ng

response 491340

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.58
264.00	63.60	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033022\
 Data File : BP009616.D
 Acq On : 30 Mar 2022 12:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 31 05:51:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 31 04:36:51 2022
 Response via : Initial Calibration

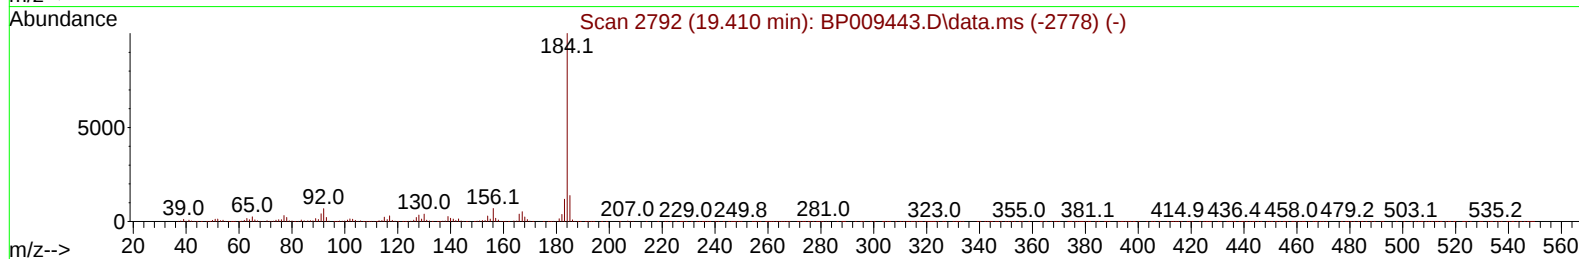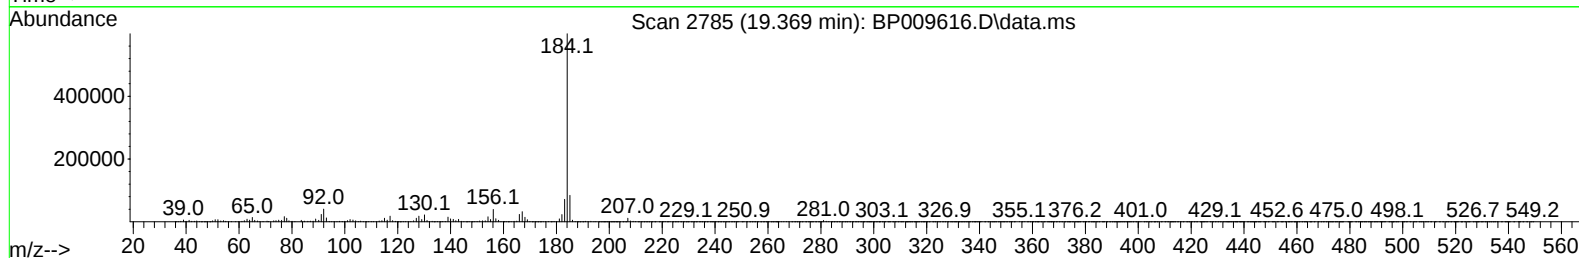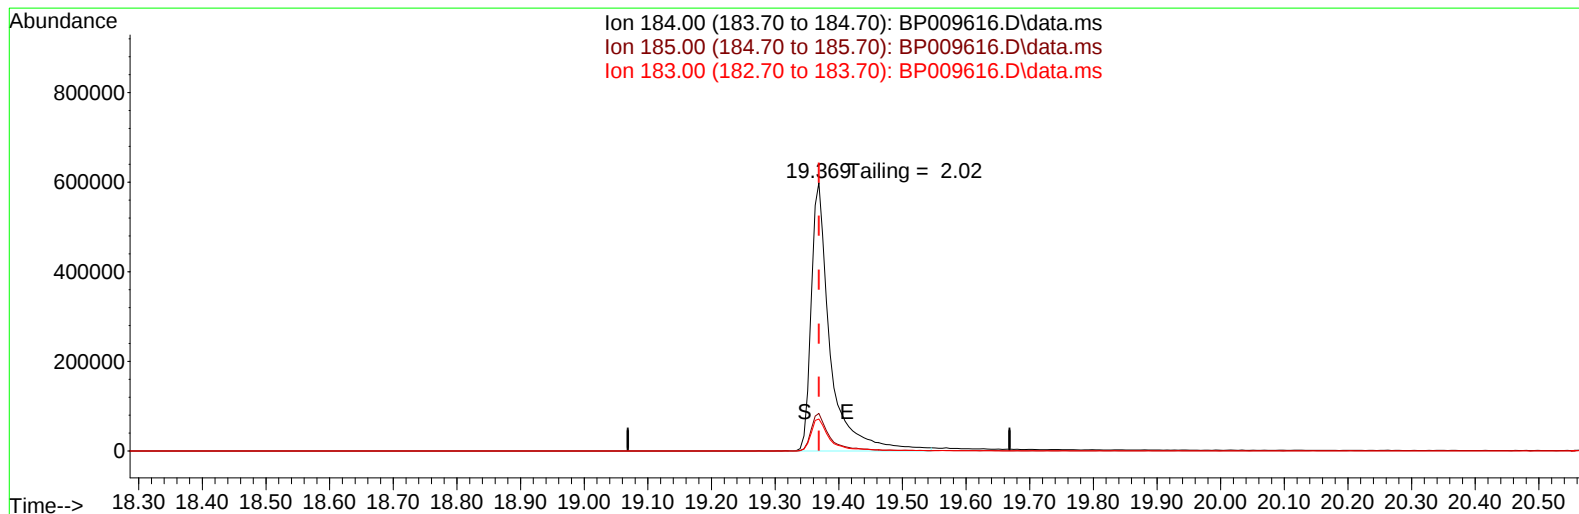

TIC: BP009616.D\data.ms

(77) Benzidine**19.369min (+ 0.000) 107110.57 ng****response 1252326**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.02
183.00	11.70	11.92
0.00	0.00	0.00