

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033022\
Data File : BP009618.D
Acq On : 30 Mar 2022 14:43
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009618.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.340	394	400	419	rBV	2971516	5101514	42.36%	9.882%
2	6.928	663	670	692	rBV	2946941	5471122	45.43%	10.598%
3	7.740	800	808	819	rBV	570617	1045402	8.68%	2.025%
4	8.893	996	1004	1035	rBV	1653887	3327815	27.63%	6.446%
5	10.528	1274	1282	1300	rBV	638471	1366307	11.35%	2.647%
6	13.004	1694	1703	1732	rBV	4910422	8383249	69.61%	16.239%
7	14.387	1929	1938	1955	rBV	965514	1626630	13.51%	3.151%
8	15.892	2186	2194	2223	rBV	3532599	5981747	49.67%	11.587%
9	17.151	2401	2408	2424	rBV	1200108	2021751	16.79%	3.916%
10	19.733	2841	2847	2859	rBV	8957892	12042684	100.00%	23.328%
11	21.269	3103	3108	3122	rBV	1744494	2597312	21.57%	5.031%
12	23.651	3506	3513	3526	rVB2	1224224	2658673	22.08%	5.150%




Sum of corrected areas: 51624206

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033022\
Data File : BP009618.D
Acq On : 30 Mar 2022 14:43
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

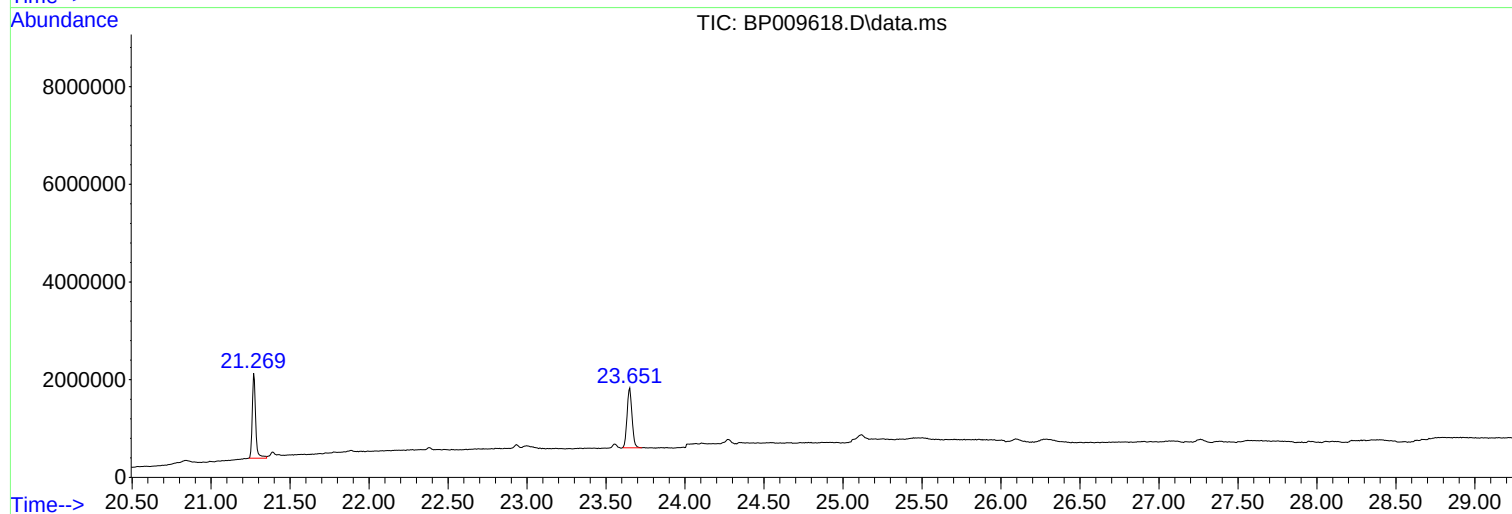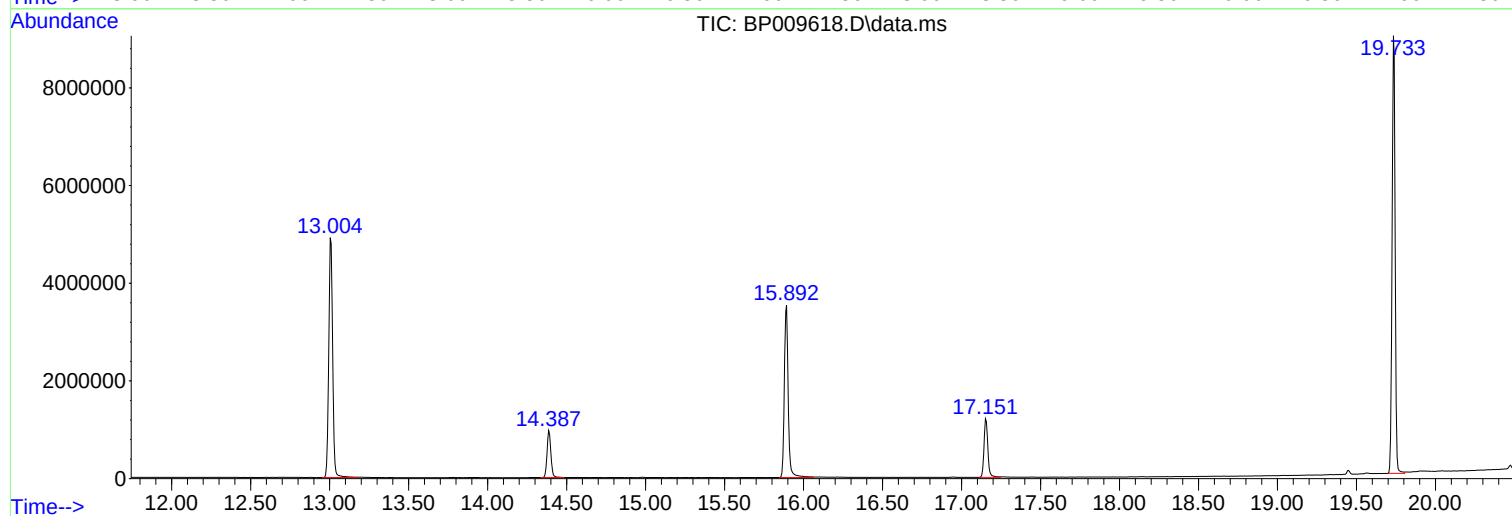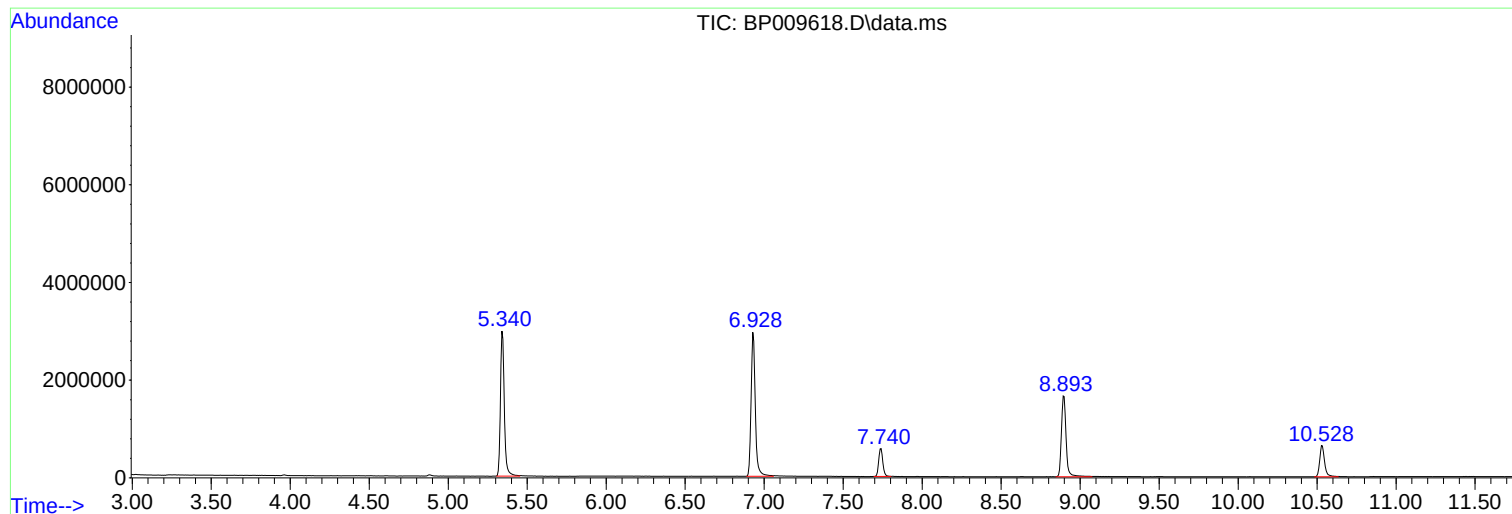

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033022\
Data File : BP009618.D
Acq On : 30 Mar 2022 14:43
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033022\
Data File : BP009618.D
Acq On : 30 Mar 2022 14:43
Operator : CG/JU
Sample : PB143709BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143709BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------