

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014405.D
 Acq On : 30 Mar 2023 17:00
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020799

Quant Time: Mar 30 22:41:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	160974	20.000	ng/u1	0.00
20) Naphthalene-d8	10.840	136	726450	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.669	164	500646	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.433	188	1112954	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	930349	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	819402	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	34938	8.417	ng/uL	0.00
4) Pyridine-d5	3.822	84	232407	21.848	ng/u1	0.00
7) Phenol-d5	7.175	99	312259	21.034	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	208686	21.909	ng/u1	0.00
11) 2-Chlorophenol-d4	7.546	132	232834	21.699	ng/u1	0.00
15) 4-Methylphenol-d8	8.734	113	262686	21.936	ng/u1	0.00
21) Nitrobenzene-d5	9.193	128	124430	21.217	ng/u1	0.00
24) 2-Nitrophenol-d4	9.916	143	144451	21.511	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	262070	21.429	ng/u1	0.00
31) 4-Chloroaniline-d4	10.987	131	347356	21.563	ng/u1	0.00
46) Dimethylphthalate-d6	14.075	166	873036	21.507	ng/u1	0.00
49) Acenaphthylene-d8	14.363	160	958005	21.269	ng/u1	0.00
54) 4-Nitrophenol-d4	14.881	143	130186	21.229	ng/u1	0.00
60) Fluorene-d10	15.669	176	722632	21.347	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	163000	19.904	ng/u1	0.00
73) Anthracene-d10	17.533	188	1132510	21.026	ng/u1	0.00
81) Pyrene-d10	19.763	212	1280276	20.487	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.874	264	933972	21.454	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	36702	8.046	ng/uL	97
5) Pyridine	3.840	79	242788	21.810	ng/u1	99
6) Benzaldehyde	7.152	77	192795	26.127	ng/u1	99
8) Phenol	7.205	94	332278	21.576	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.434	93	268869	21.725	ng/u1	99
12) 2-Chlorophenol	7.575	128	242782	21.739	ng/u1	94
13) 2-Methylphenol	8.463	108	243734	21.222	ng/u1	96
14) 2,2'-oxybis(1-Chloropr...	8.540	45	370922	22.827	ng/u1	99
16) Acetophenone	8.852	105	438881	22.194	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.828	70	246026	23.030	ng/u1	94
18) 4-Methylphenol	8.799	108	272793	21.627	ng/u1	97
19) Hexachloroethane	9.099	117	108405	22.216	ng/u1	92
22) Nitrobenzene	9.234	77	357349	21.211	ng/u1	98
23) Isophorone	9.763	82	672416	21.652	ng/u1	100
25) 2-Nitrophenol	9.951	139	152568	21.525	ng/u1	97
26) 2,4-Dimethylphenol	10.004	107	335095	21.122	ng/u1	99
27) Bis(2-Chloroethoxy)met...	10.246	93	395967	21.267	ng/u1	99
29) 2,4-Dichlorophenol	10.487	162	256941	21.348	ng/u1	95
30) Naphthalene	10.893	128	847372	20.941	ng/u1	100
32) 4-Chloroaniline	11.010	127	358505	21.972	ng/u1	99
33) Hexachlorobutadiene	11.163	225	196878	20.648	ng/u1	98
34) Caprolactam	11.798	113	81360	22.882	ng/u1	91
35) 4-Chloro-3-methylphenol	12.128	107	324765	21.938	ng/u1	99
36) 2-Methylnaphthalene	12.498	142	589609	21.501	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014405.D
 Acq On : 30 Mar 2023 17:00
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020799

Quant Time: Mar 30 22:41:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.716	142	593276	21.814	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.863	216	358583	20.089	ng/ul	98
40) Hexachlorocyclopentadiene	12.834	237	215571	18.649	ng/ul	97
41) 2,4,6-Trichlorophenol	13.104	196	228426	20.680	ng/ul	98
42) 2,4,5-Trichlorophenol	13.181	196	248040	21.093	ng/ul	97
43) 1,1'-Biphenyl	13.504	154	825815	20.417	ng/ul	99
44) 2-Chloronaphthalene	13.545	162	651142	20.360	ng/ul	100
45) 2-Nitroaniline	13.763	65	221657	22.380	ng/ul	99
47) Dimethylphthalate	14.122	163	870868	21.457	ng/ul	99
48) 2,6-Dinitrotoluene	14.251	165	174978	22.066	ng/ul	99
50) Acenaphthylene	14.392	152	1014670	21.152	ng/ul	100
51) 3-Nitroaniline	14.587	138	161169	22.687	ng/ul	98
52) Acenaphthene	14.734	153	709402	20.928	ng/ul	99
53) 2,4-Dinitrophenol	14.798	184	100219	19.517	ng/ul	99
55) 4-Nitrophenol	14.898	109	130220	21.516	ng/ul	95
56) Dibenzofuran	15.069	168	998678	20.958	ng/ul	100
57) 2,4-Dinitrotoluene	15.045	165	257421	22.886	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.298	232	229473	21.712	ng/ul	96
59) Diethylphthalate	15.486	149	891302	22.099	ng/ul	98
61) Fluorene	15.722	166	825848	21.382	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.710	204	440942	21.249	ng/ul	99
63) 4-Nitroaniline	15.757	138	138888	24.062	ng/ul	99
66) 4,6-Dinitro-2-methylph...	15.810	198	157505	19.846	ng/ul	96
67) N-Nitrosodiphenylamine	15.928	169	704209	20.336	ng/ul	100
68) 4-Bromophenyl-phenylether	16.610	248	279190	20.159	ng/ul	97
69) Hexachlorobenzene	16.728	284	319313	20.073	ng/ul	100
70) Atrazine	16.886	200	272862	21.646	ng/ul	97
71) Pentachlorophenol	17.081	266	179235	19.449	ng/ul	97
72) Phenanthrene	17.475	178	1299078	20.981	ng/ul	100
74) Anthracene	17.569	178	1322541	21.193	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.469	216	371348	18.955	ng/uL	98
76) Pentachlorobenzene	14.986	250	378898	19.383	ng/uL	98
77) Carbazole	17.839	167	1144600	21.917	ng/ul	99
78) Di-n-butylphthalate	18.369	149	1498972	22.827	ng/ul	100
80) Fluoranthene	19.433	202	1510169	20.439	ng/ul	97
82) Pyrene	19.792	202	1556700	20.180	ng/ul	99
83) Butylbenzylphthalate	20.645	149	628514	23.654	ng/ul	97
84) 3,3'-Dichlorobenzidine	21.433	252	433068	21.048	ng/ul	100
85) Benzo(a)anthracene	21.504	228	1384352	20.998	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.398	149	865512	23.820	ng/ul	100
87) Chrysene	21.563	228	1313661	21.103	ng/ul	99
89) Di-n-octyl phthalate	22.363	149	1315519	24.740	ng/ul	100
90) Benzo(b)fluoranthene	23.268	252	1218219	22.013	ng/ul	99
91) Benzo(k)fluoranthene	23.315	252	1188742	22.117	ng/ul	100
93) Benzo(a)pyrene	23.927	252	1028698	21.595	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.686	276	1257231	19.184	ng/ul	98
95) Dibenzo(a,h)anthracene	26.704	278	1054577	19.220	ng/ul	98
96) Benzo(g,h,i)perylene	27.503	276	1003195	18.780	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014405.D
 Acq On : 30 Mar 2023 17:00
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SSTD020799

Quant Time: Mar 30 22:41:24 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration




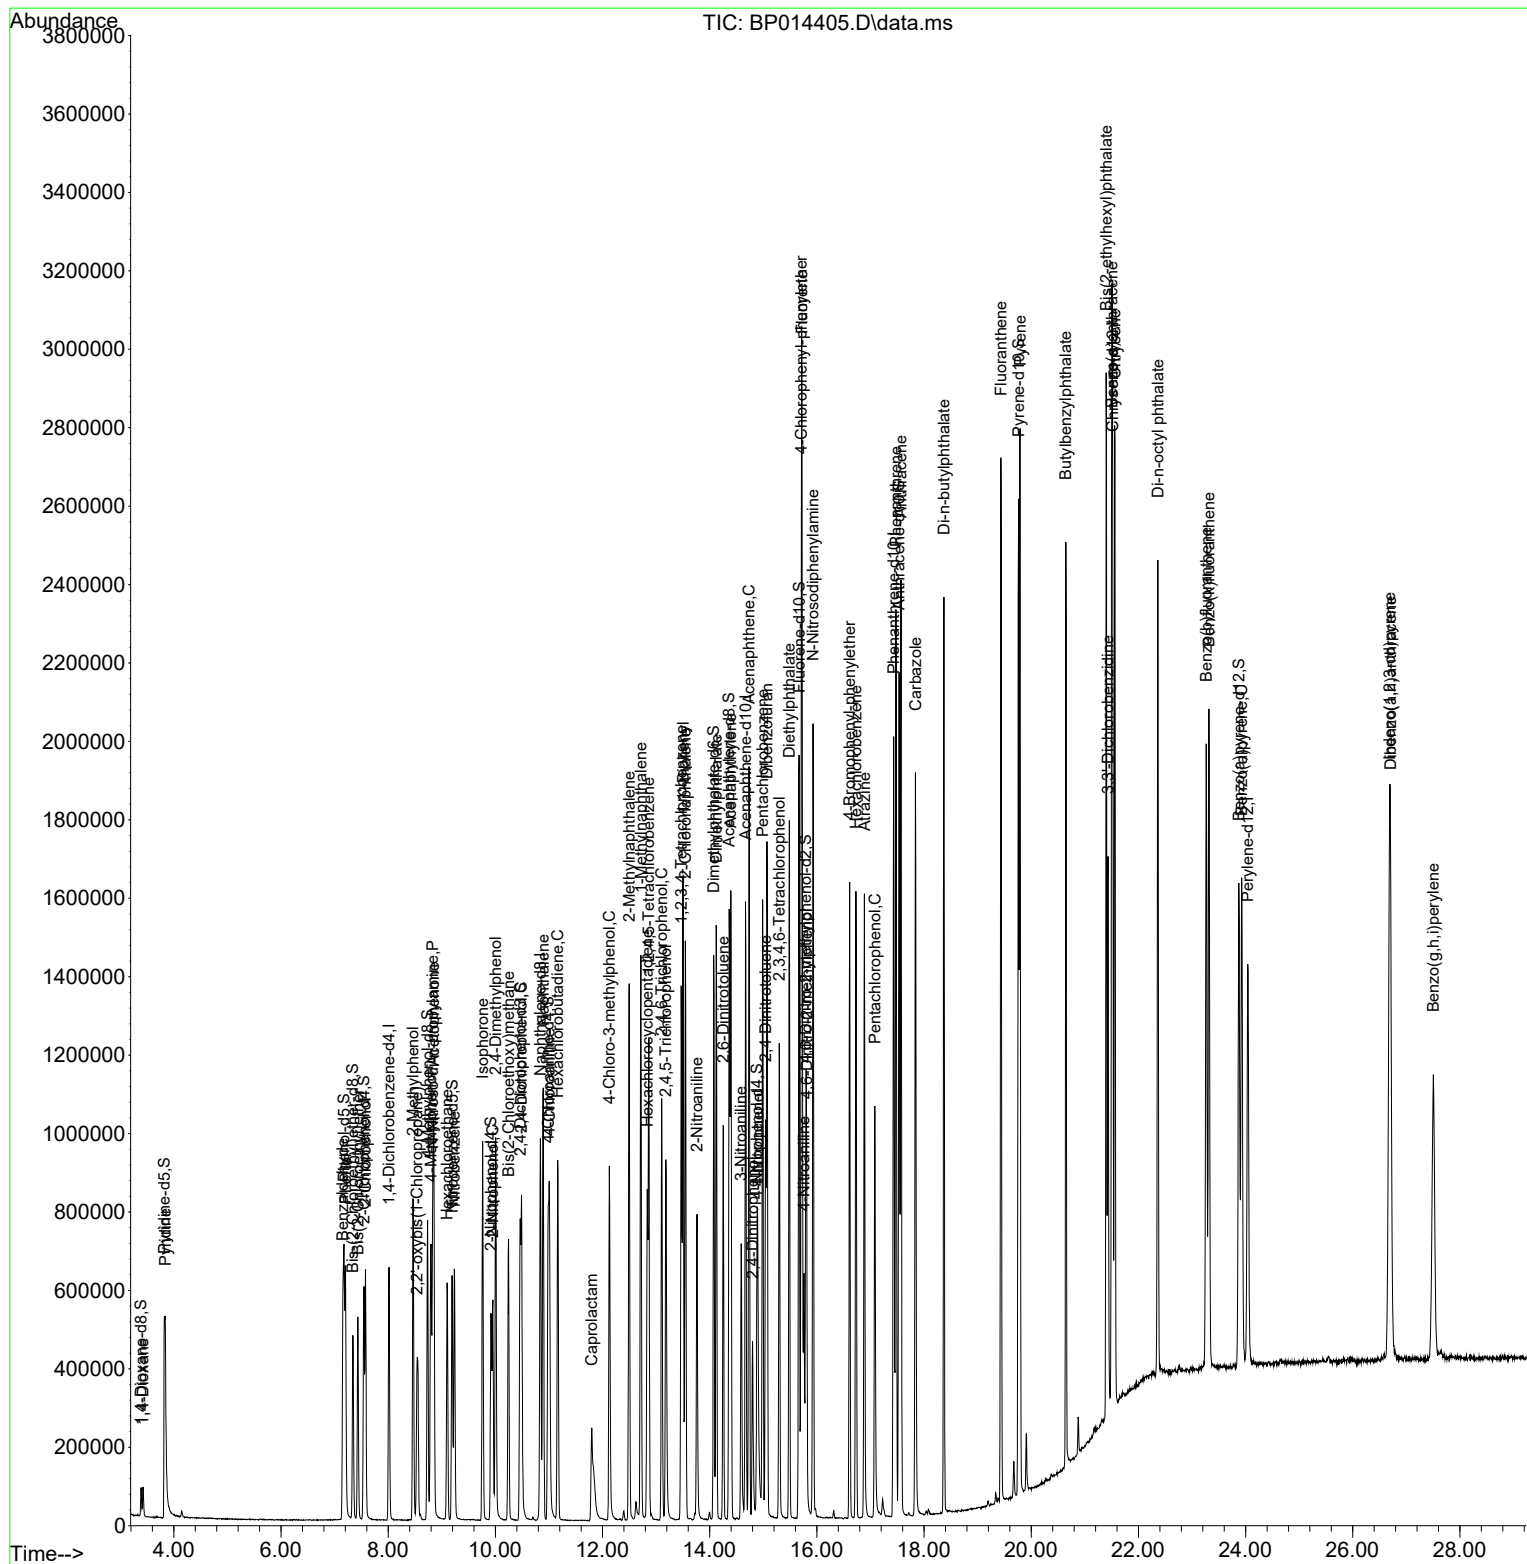


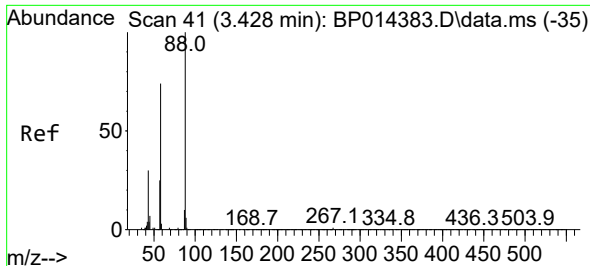

#2
1,4-Dioxane
Concen: 8.046 ng/uL
RT: 3.422 min Scan# 40
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion: 88 Resp: 36702
Ion Ratio Lower Upper
88 100
43 29.7 24.4 36.6
58 74.5 57.4 86.0

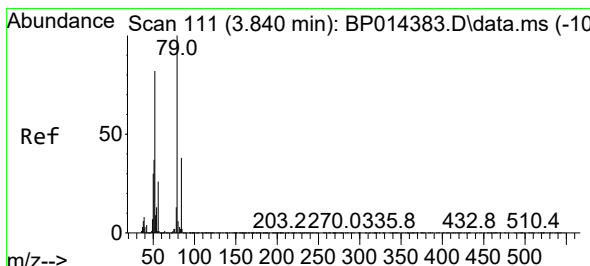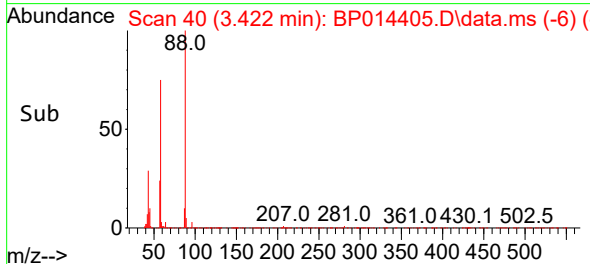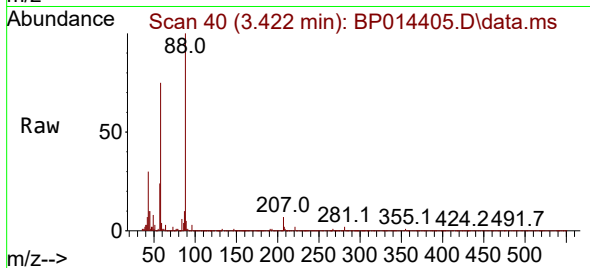

#5
Pyridine
Concen: 21.810 ng/uL
RT: 3.840 min Scan# 111
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion: 79 Resp: 242788
Ion Ratio Lower Upper
79 100
52 77.7 61.4 92.2
51 36.7 28.5 42.7


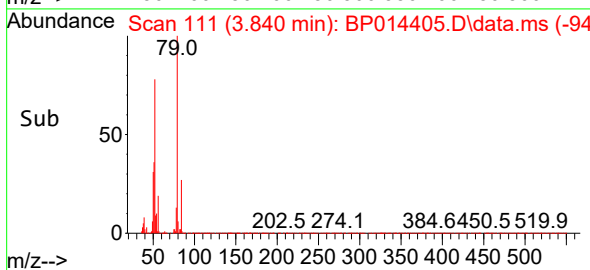

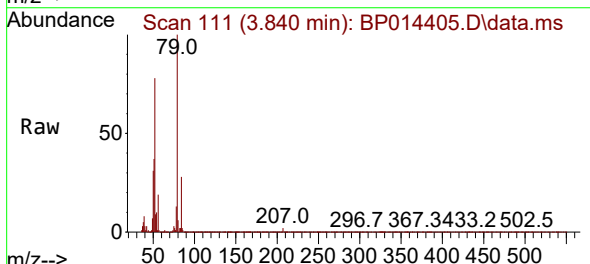




#6
Benzaldehyde
Concen: 26.127 ng/ul
RT: 7.152 min Scan# 61
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion: 77 Resp: 192795
Ion Ratio Lower Upper
77 100
105 89.1 70.6 105.8
106 82.4 66.5 99.7

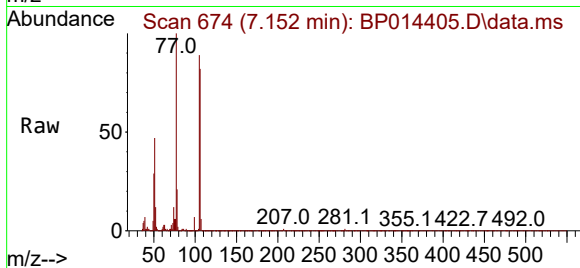

#8
Phenol
Concen: 21.576 ng/ul
RT: 7.205 min Scan# 683
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion: 94 Resp: 332278
Ion Ratio Lower Upper
94 100
65 30.9 25.2 37.8
66 43.9 36.2 54.4


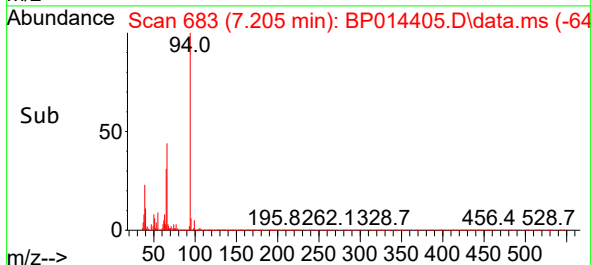

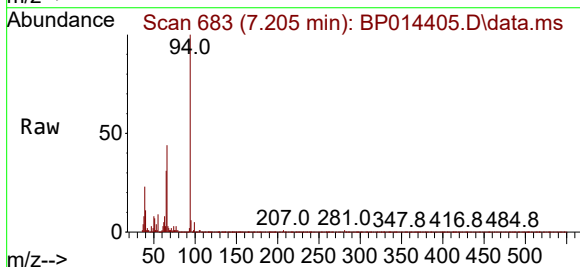




#10
Bis(2-Chloroethyl)ether
Concen: 21.725 ng/ul
RT: 7.434 min Scan# 71
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion: 93 Resp: 268869
Ion Ratio Lower Upper
93 100
63 80.0 63.2 94.8
95 31.5 26.0 39.0



#12
2-Chlorophenol
Concen: 21.739 ng/ul
RT: 7.575 min Scan# 746
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:128 Resp: 242782
Ion Ratio Lower Upper
128 100
64 56.6 41.4 62.0
130 32.2 24.1 36.1

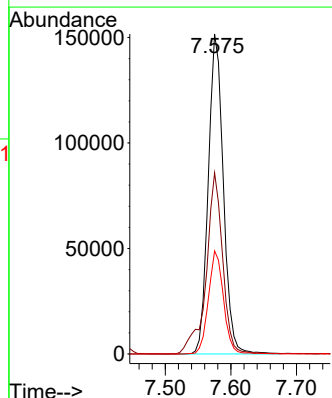



#13

2-Methylphenol

Concen: 21.222 ng/ul

RT: 8.463 min Scan# 89

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :





SSTD020799

Tgt Ion:108 Resp: 243734

Ion Ratio Lower Upper

108 100

107 92.7 71.2 106.8



#14

2,2'-oxybis(1-Chloropropane)

Concen: 22.827 ng/ul

RT: 8.540 min Scan# 910

Delta R.T. -0.012 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion: 45 Resp: 370922


Ion Ratio Lower Upper

45 100

77 16.4 12.8 19.2

79 11.5 9.6 14.4









#16
Acetophenone
Concen: 22.194 ng/ul
RT: 8.852 min Scan# 90
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:105 Resp: 438881
Ion Ratio Lower Upper
105 100
77 85.3 67.3 100.9
51 29.4 23.0 34.4



#17
N-Nitroso-di-n-propylamine
Concen: 23.030 ng/ul
RT: 8.828 min Scan# 959
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion: 70 Resp: 246026
Ion Ratio Lower Upper
70 100
42 56.4 41.1 61.7
101 9.9 7.0 10.6
130 17.3 14.6 21.8



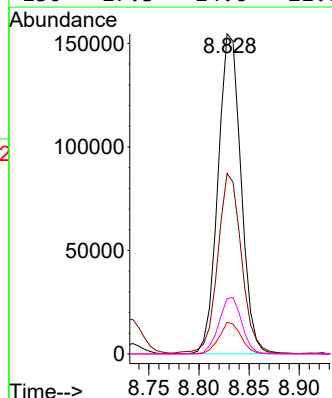





#18
4-Methylphenol
Concen: 21.627 ng/ul
RT: 8.799 min Scan# 91
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:108 Resp: 272793
Ion Ratio Lower Upper
108 100
107 114.0 89.0 133.6



#19
Hexachloroethane
Concen: 22.216 ng/ul
RT: 9.099 min Scan# 1005
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:117 Resp: 108405
Ion Ratio Lower Upper
117 100
201 102.1 90.2 135.4
199 63.1 54.2 81.2



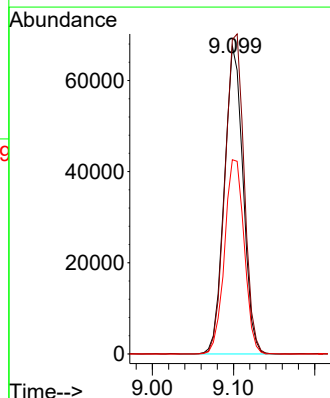





#22
Nitrobenzene
Concen: 21.211 ng/ul
RT: 9.234 min Scan# 1028
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion: 77 Resp: 357349
Ion Ratio Lower Upper
77 100
123 39.0 30.3 45.5
65 14.1 11.0 16.4



#23
Isophorone
Concen: 21.652 ng/ul
RT: 9.763 min Scan# 1118
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion: 82 Resp: 672416
Ion Ratio Lower Upper
82 100
95 7.6 6.3 9.5
138 15.2 12.2 18.2









#25
2-Nitrophenol
Concen: 21.525 ng/ul
RT: 9.951 min Scan# 1150
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:139 Resp: 152568
Ion Ratio Lower Upper
139 100
65 63.7 49.7 74.5
109 42.1 31.1 46.7



#26
2,4-Dimethylphenol
Concen: 21.122 ng/ul
RT: 10.004 min Scan# 1159
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:107 Resp: 335095
Ion Ratio Lower Upper
107 100
121 46.1 37.0 55.6
122 75.9 59.8 89.6



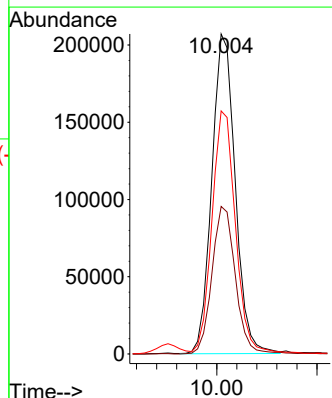





#27
 Bis(2-Chloroethoxy)methane
 Concen: 21.267 ng/ul
 RT: 10.246 min Scan# 1200
 Delta R.T. -0.000 min
 Lab File: BP014405.D
 Acq: 30 Mar 2023 17:00




Instrument :
 BNA_P
 ClientSampleId :
 SST020799


Tgt Ion: 93 Resp: 395967
 Ion Ratio Lower Upper
 93 100
 95 32.9 25.8 38.8
 123 10.1 8.5 12.7



#29
 2,4-Dichlorophenol
 Concen: 21.348 ng/ul
 RT: 10.487 min Scan# 1241
 Delta R.T. -0.006 min
 Lab File: BP014405.D
 Acq: 30 Mar 2023 17:00

Tgt Ion: 162 Resp: 256941
 Ion Ratio Lower Upper
 162 100
 164 66.5 50.1 75.1
 98 41.8 30.6 45.8




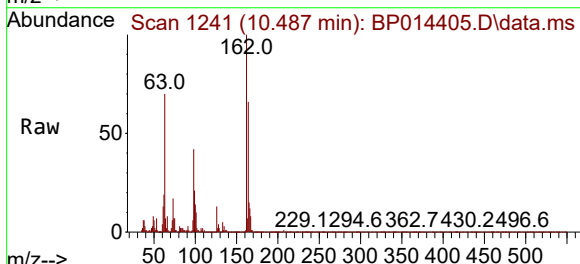




#30
Naphthalene
Concen: 20.941 ng/ul
RT: 10.893 min Scan# 1310
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:128 Resp: 847372
Ion Ratio Lower Upper
128 100
129 10.8 8.9 13.3
127 13.8 11.0 16.6

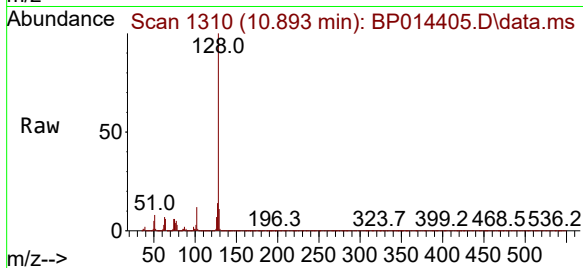

#32
4-Chloroaniline
Concen: 21.972 ng/ul
RT: 11.010 min Scan# 1330
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:127 Resp: 358505
Ion Ratio Lower Upper
127 100
129 32.5 25.4 38.0

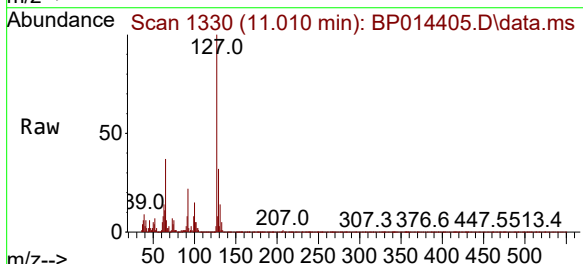



#33

Hexachlorobutadiene

Concen: 20.648 ng/ul

RT: 11.163 min Scan# 11

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:225 Resp: 196878

Ion Ratio Lower Upper

225 100

223 59.5 49.3 73.9

227 63.0 49.6 74.4

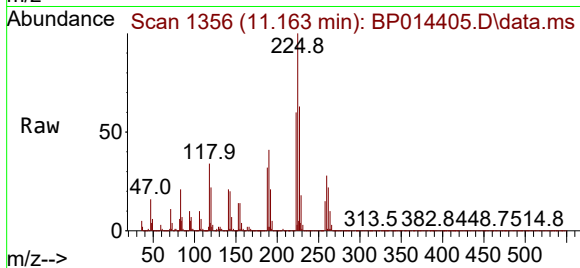

#34

Caprolactam

Concen: 22.882 ng/ul

RT: 11.798 min Scan# 1464

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:113 Resp: 81360


Ion Ratio Lower Upper

113 100

55 175.6 131.2 196.8

56 138.3 101.1 151.7









#35
4-Chloro-3-methylphenol
Concen: 21.938 ng/ul
RT: 12.128 min Scan# 1520
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:107 Resp: 324765
Ion Ratio Lower Upper
107 100
144 22.7 17.3 25.9
142 68.1 54.6 81.8

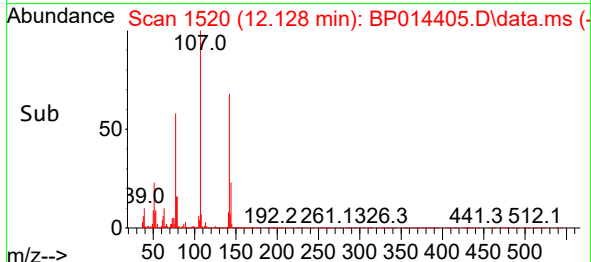

#36
2-Methylnaphthalene
Concen: 21.501 ng/ul
RT: 12.498 min Scan# 1583
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:142 Resp: 589609
Ion Ratio Lower Upper
142 100
141 90.5 71.6 107.4









#37
1-Methylnaphthalene
Concen: 21.814 ng/ul
RT: 12.716 min Scan# 1620
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:142 Resp: 593276
Ion Ratio Lower Upper
142 100
141 93.5 76.6 114.8
116 4.8 3.6 5.4



#39
1,2,4,5-Tetrachlorobenzene
Concen: 20.089 ng/ul
RT: 12.863 min Scan# 1645
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:216 Resp: 358583
Ion Ratio Lower Upper
216 100
214 77.9 61.0 91.6
179 21.2 16.6 24.8
108 16.8 13.8 20.6

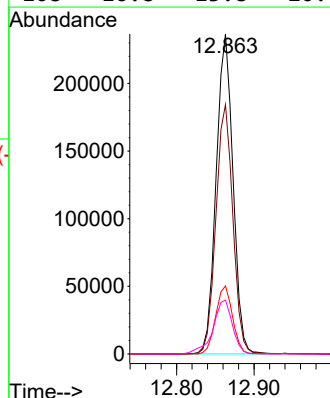



#40

Hexachlorocyclopentadiene

Concen: 18.649 ng/ul

RT: 12.834 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:237 Resp: 215571

Ion Ratio Lower Upper

237 100

235 60.8 51.0 76.4

272 12.2 10.3 15.5



#41

2,4,6-Trichlorophenol

Concen: 20.680 ng/ul

RT: 13.104 min Scan# 1686

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:196 Resp: 228426


Ion Ratio Lower Upper

196 100

198 97.6 76.6 114.8

200 30.5 25.4 38.2





#42

2,4,5-Trichlorophenol

Concen: 21.093 ng/ul

RT: 13.181 min Scan# 1

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:196 Resp: 248040

Ion Ratio Lower Upper

196 100

198 95.5 79.8 119.8

200 32.1 25.6 38.4



#43

1,1'-Biphenyl

Concen: 20.417 ng/ul

RT: 13.504 min Scan# 1754

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:154 Resp: 825815


Ion Ratio Lower Upper

154 100

153 40.8 32.4 48.6

76 14.2 10.7 16.1

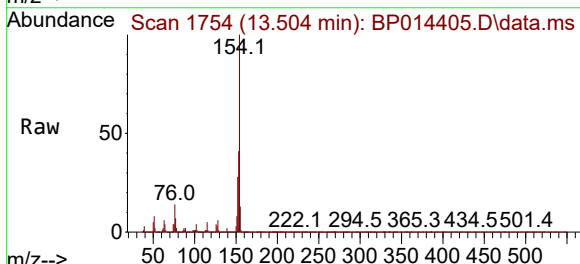



#44

2-Chloronaphthalene

Concen: 20.360 ng/ul

RT: 13.545 min Scan# 1762

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:162 Resp: 651142

Ion Ratio Lower Upper

162 100

164 32.7 26.1 39.1

127 42.4 33.7 50.5

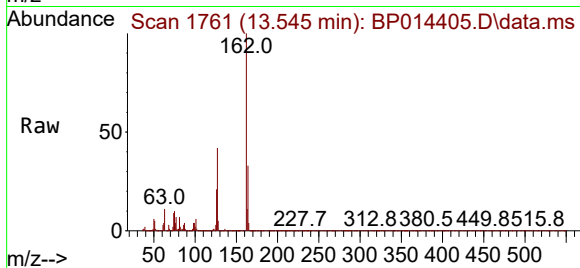

#45

2-Nitroaniline

Concen: 22.380 ng/ul

RT: 13.763 min Scan# 1798

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion: 65 Resp: 221657


Ion Ratio Lower Upper

65 100

92 66.3 53.7 80.5

138 88.6 71.7 107.5


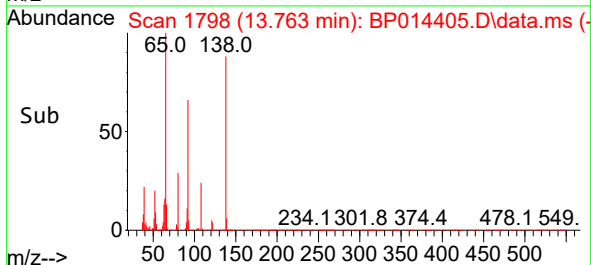
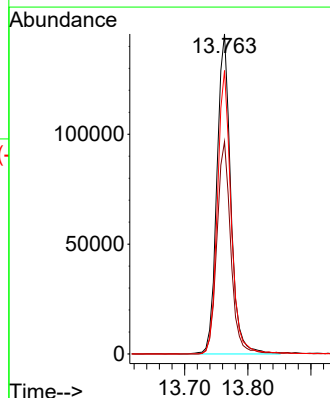
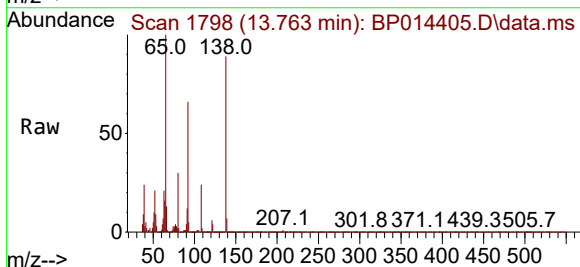




#47
Dimethylphthalate
Concen: 21.457 ng/ul
RT: 14.122 min Scan# 1859
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:163 Resp: 870868
Ion Ratio Lower Upper
163 100
194 3.9 3.1 4.7
164 10.1 7.8 11.8



#48
2,6-Dinitrotoluene
Concen: 22.066 ng/ul
RT: 14.251 min Scan# 1881
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:165 Resp: 174978
Ion Ratio Lower Upper
165 100
89 67.4 52.7 79.1
121 22.3 17.9 26.9




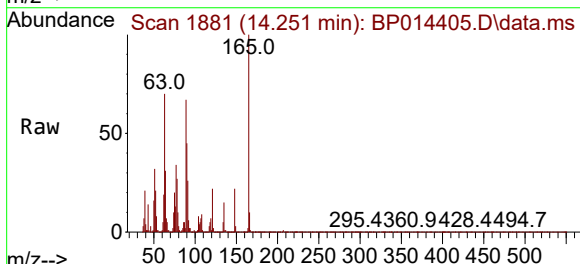




#50
Acenaphthylene
Concen: 21.152 ng/ul
RT: 14.392 min Scan# 1905
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:152 Resp: 1014670
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.4
153 13.0 10.2 15.4



#51
3-Nitroaniline
Concen: 22.687 ng/ul
RT: 14.587 min Scan# 1938
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:138 Resp: 161169
Ion Ratio Lower Upper
138 100
108 12.3 9.9 14.9
92 131.8 107.6 161.4









#52
Acenaphthene
Concen: 20.928 ng/ul
RT: 14.734 min Scan# 1964
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:153 Resp: 709402
Ion Ratio Lower Upper
153 100
152 46.6 38.2 57.4
154 87.5 70.2 105.2



#53
2,4-Dinitrophenol
Concen: 19.517 ng/ul
RT: 14.798 min Scan# 1974
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:184 Resp: 100219
Ion Ratio Lower Upper
184 100
63 71.3 57.1 85.7
154 70.2 55.3 82.9



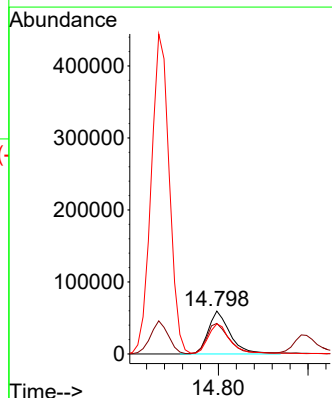
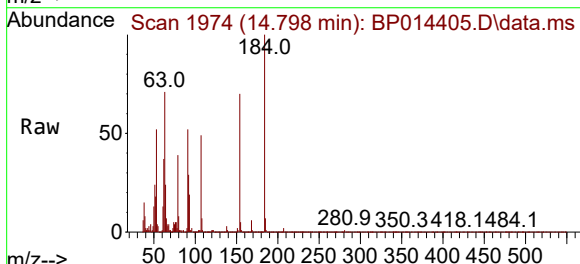




#55
4-Nitrophenol
Concen: 21.516 ng/ul
RT: 14.898 min Scan# 1991
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:109 Resp: 130220
Ion Ratio Lower Upper
109 100
139 105.6 77.4 116.2
65 123.6 97.3 145.9

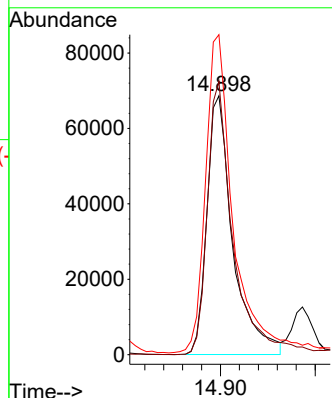

#56
Dibenzofuran
Concen: 20.958 ng/ul
RT: 15.069 min Scan# 2020
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:168 Resp: 998678
Ion Ratio Lower Upper
168 100
139 40.3 32.1 48.1



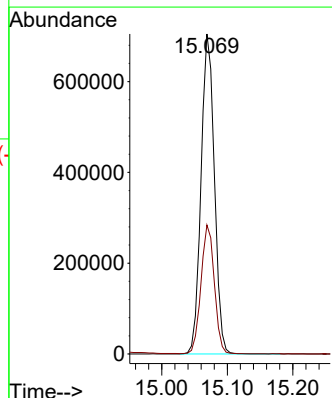
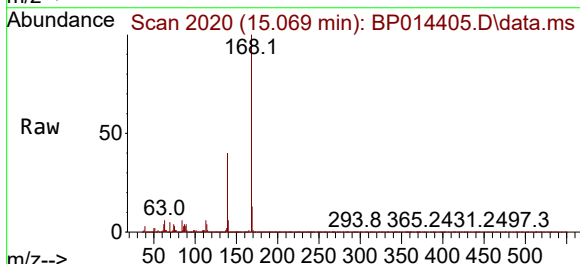




#57
2,4-Dinitrotoluene
Concen: 22.886 ng/ul
RT: 15.045 min Scan# 2016
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:165 Resp: 257421
Ion Ratio Lower Upper
165 100
63 49.6 41.6 62.4
182 2.8 2.4 3.6



#58
2,3,4,6-Tetrachlorophenol
Concen: 21.712 ng/ul
RT: 15.298 min Scan# 2059
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:232 Resp: 229473
Ion Ratio Lower Upper
232 100
131 46.4 35.0 52.4
130 2.9 1.9 2.9
166 32.5 24.1 36.1




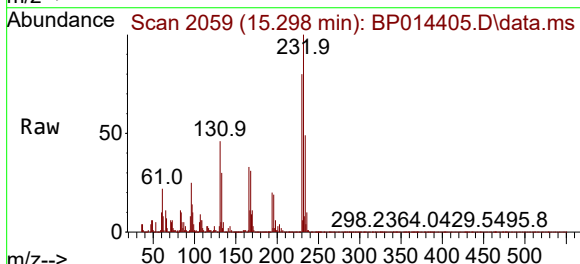




#59
Diethylphthalate
Concen: 22.099 ng/ul
RT: 15.486 min Scan# 2091
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:149 Resp: 891302
Ion Ratio Lower Upper
149 100
177 21.8 18.2 27.2
150 13.1 9.8 14.8



#61
Fluorene
Concen: 21.382 ng/ul
RT: 15.722 min Scan# 2131
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:166 Resp: 825848
Ion Ratio Lower Upper
166 100
165 99.4 79.2 118.8
167 13.1 11.0 16.4




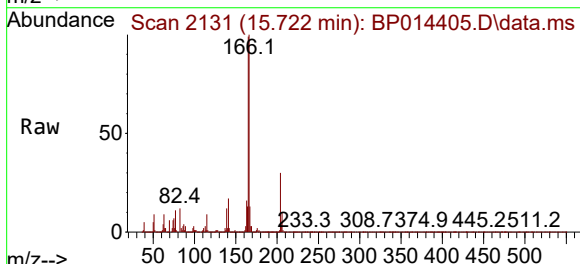


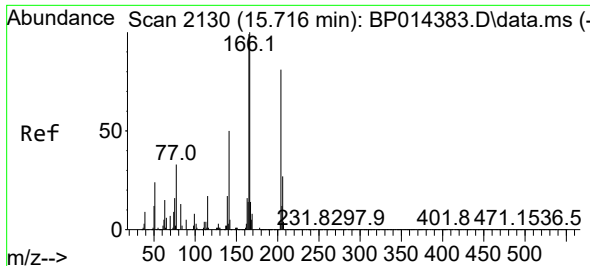

#62
4-Chlorophenyl-phenylether
Concen: 21.249 ng/ul
RT: 15.710 min Scan# 2110
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:204 Resp: 440942
Ion Ratio Lower Upper
204 100
206 32.5 26.9 40.3
141 63.3 51.3 76.9

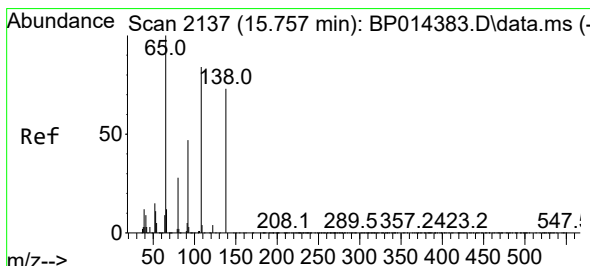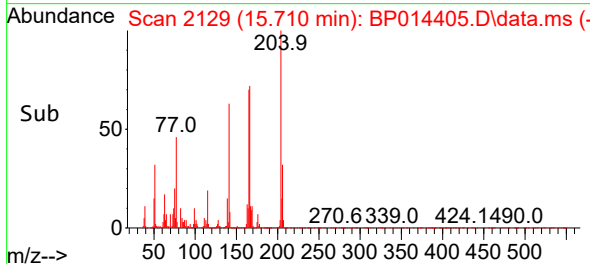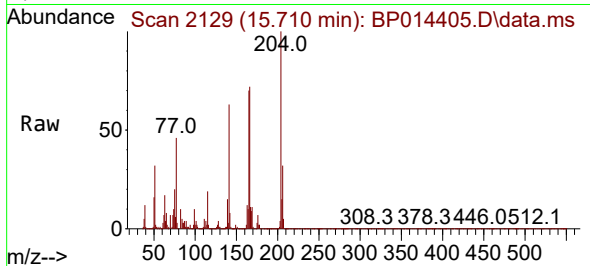

#63
4-Nitroaniline
Concen: 24.062 ng/ul
RT: 15.757 min Scan# 2137
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:138 Resp: 138888
Ion Ratio Lower Upper
138 100
92 59.6 47.8 71.6
108 101.5 82.3 123.5


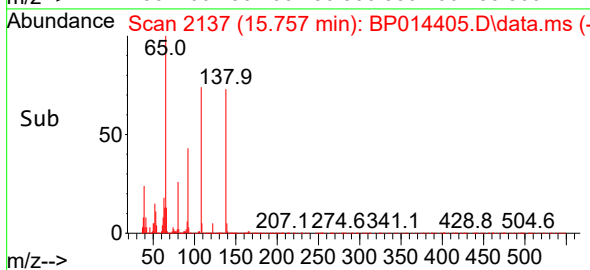

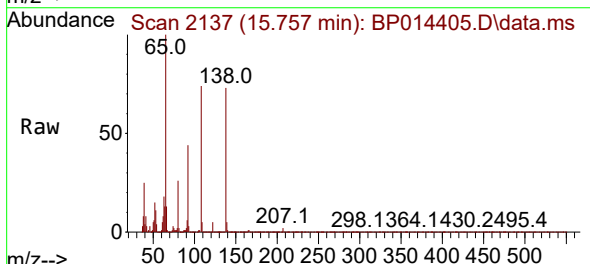




#66
 4,6-Dinitro-2-methylphenol
 Concen: 19.846 ng/ul
 RT: 15.810 min Scan# 2146
 Delta R.T. -0.000 min
 Lab File: BP014405.D
 Acq: 30 Mar 2023 17:00




Instrument :
 BNA_P
 ClientSampleId :
 SSTD020799


Tgt Ion:198 Resp: 157505
 Ion Ratio Lower Upper
 198 100
 182 3.8 3.5 5.3
 77 28.3 24.4 36.6

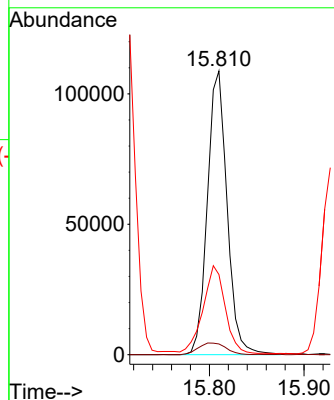

#67
 N-Nitrosodiphenylamine
 Concen: 20.336 ng/ul
 RT: 15.928 min Scan# 2166
 Delta R.T. -0.006 min
 Lab File: BP014405.D
 Acq: 30 Mar 2023 17:00

Tgt Ion:169 Resp: 704209
 Ion Ratio Lower Upper
 169 100
 168 67.4 54.2 81.2
 167 36.5 29.4 44.2



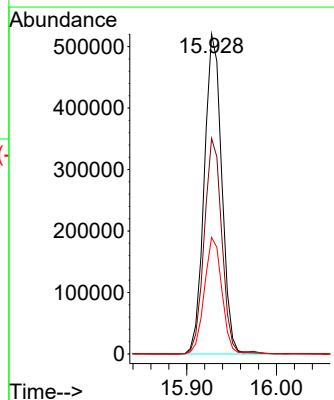
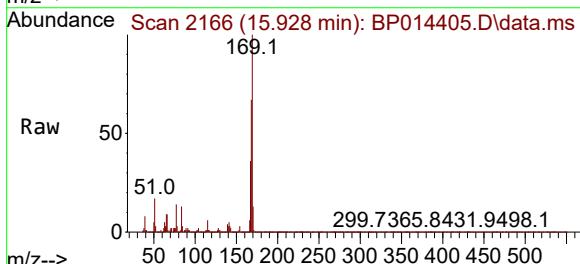




#68
4-Bromophenyl-phenylether
Concen: 20.159 ng/ul
RT: 16.610 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:248 Resp: 279190
Ion Ratio Lower Upper
248 100
250 95.1 78.1 117.1
141 79.2 66.0 99.0

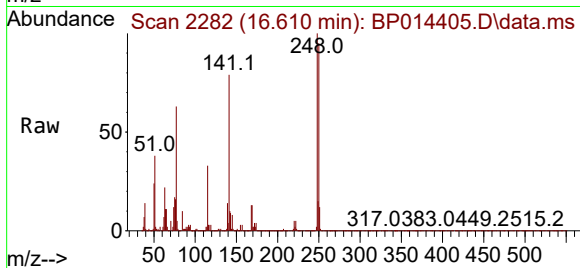

#69
Hexachlorobenzene
Concen: 20.073 ng/ul
RT: 16.728 min Scan# 2302
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:284 Resp: 319313
Ion Ratio Lower Upper
284 100
142 33.1 26.6 39.8
249 31.8 25.7 38.5





#70

Atrazine

Concen: 21.646 ng/ul

RT: 16.886 min Scan# 2329

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:200 Resp: 272862

Ion Ratio Lower Upper

200 100

173 25.1 20.6 30.8

215 48.7 37.2 55.8

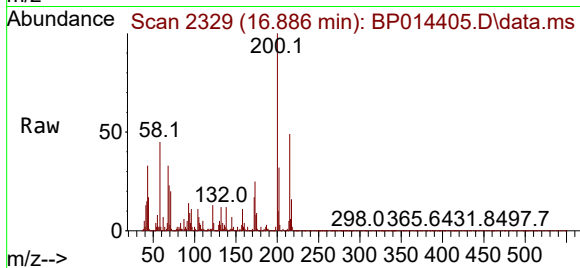

#71

Pentachlorophenol

Concen: 19.449 ng/ul

RT: 17.081 min Scan# 2362

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:266 Resp: 179235


Ion Ratio Lower Upper

266 100

264 61.0 51.0 76.4

268 62.7 51.4 77.2




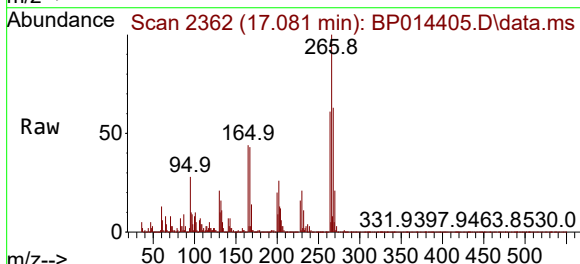




#72
Phenanthrene
Concen: 20.981 ng/ul
RT: 17.475 min Scan# 2430
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:178 Resp: 1299078
Ion Ratio Lower Upper
178 100
179 15.4 12.2 18.4
176 19.2 15.3 22.9



#74
Anthracene
Concen: 21.193 ng/ul
RT: 17.569 min Scan# 2445
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:178 Resp: 1322541
Ion Ratio Lower Upper
178 100
179 15.3 12.2 18.4
176 18.6 14.9 22.3





#75

1,2,3,4-Tetrachlorobenzene

Concen: 18.955 ng/uL

RT: 13.469 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:216 Resp: 371348

Ion Ratio Lower Upper

216 100

214 78.6 61.0 91.6

218 47.8 38.7 58.1

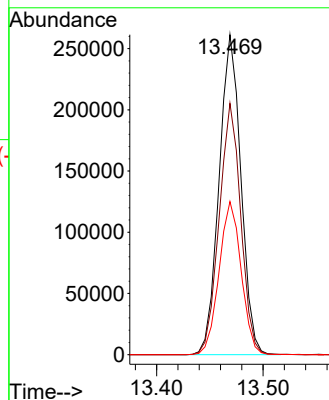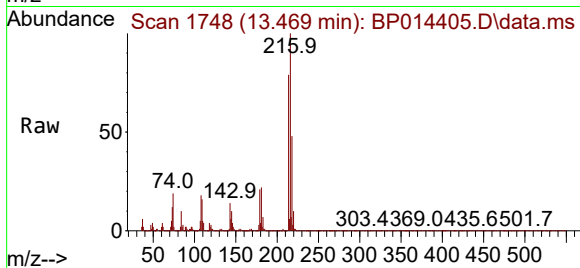

#76

Pentachlorobenzene

Concen: 19.383 ng/uL

RT: 14.986 min Scan# 2006

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:250 Resp: 378898


Ion Ratio Lower Upper

250 100

248 63.1 49.0 73.6

252 61.8 50.7 76.1

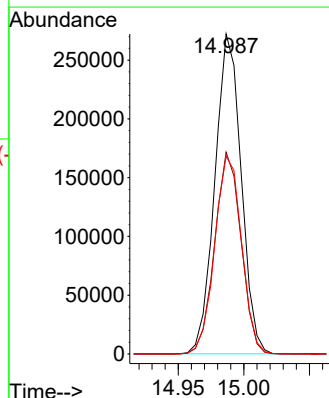



#77

Carbazole

Concen: 21.917 ng/ul

RT: 17.839 min Scan# 2491

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:167 Resp: 1144600

Ion Ratio Lower Upper

167 100

166 21.7 17.4 26.2

139 13.5 11.3 16.9

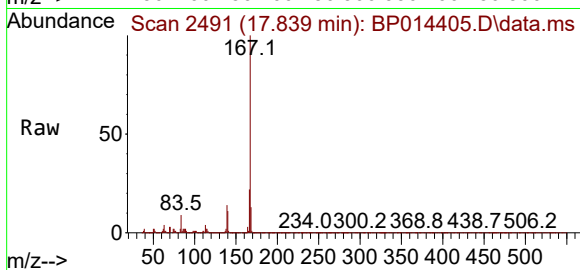

#78

Di-n-butylphthalate

Concen: 22.827 ng/ul

RT: 18.369 min Scan# 2581

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:149 Resp: 1498972


Ion Ratio Lower Upper

149 100

150 9.1 7.4 11.0

104 6.1 4.8 7.2









#80
Fluoranthene
Concen: 20.439 ng/ul
RT: 19.433 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00




Instrument :
BNA_P
ClientSampleId :
SSTD020799


Tgt Ion:202 Resp: 1510169
Ion Ratio Lower Upper
202 100
101 11.4 8.2 12.2
100 8.7 6.4 9.6

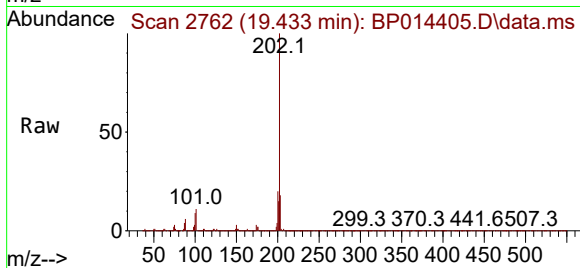

#82
Pyrene
Concen: 20.180 ng/ul
RT: 19.792 min Scan# 2823
Delta R.T. -0.000 min
Lab File: BP014405.D
Acq: 30 Mar 2023 17:00

Tgt Ion:202 Resp: 1556700
Ion Ratio Lower Upper
202 100
101 11.7 9.7 14.5
100 9.7 8.0 12.0

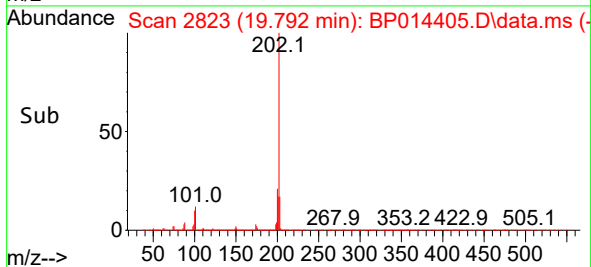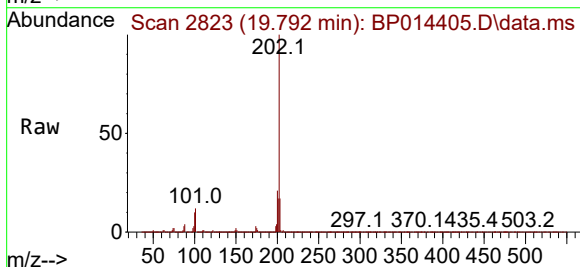



#83

Butylbenzylphthalate

Concen: 23.654 ng/ul

RT: 20.645 min Scan# 2968

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:149 Resp: 628514

Ion Ratio Lower Upper

149 100

91 80.2 61.8 92.8

206 21.0 17.8 26.6



#84

3,3'-Dichlorobenzidine

Concen: 21.048 ng/ul

RT: 21.433 min Scan# 3102

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:252 Resp: 433068


Ion Ratio Lower Upper

252 100

254 64.0 51.4 77.0

126 10.1 7.8 11.6





#85

Benzo(a)anthracene

Concen: 20.998 ng/ul

RT: 21.504 min Scan# 3114

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:228 Resp: 1384352

Ion Ratio Lower Upper

228 100

229 19.8 15.6 23.4

226 27.6 21.8 32.6

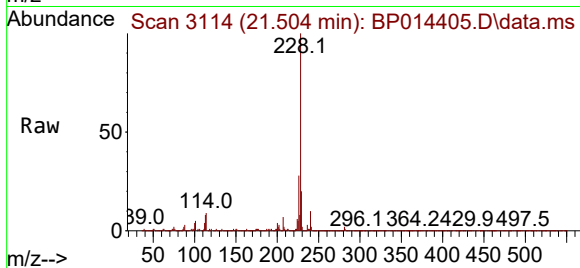

#86

Bis(2-ethylhexyl)phthalate

Concen: 23.820 ng/ul

RT: 21.398 min Scan# 3096

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:149 Resp: 865512


Ion Ratio Lower Upper

149 100

167 27.2 21.9 32.9

279 4.2 3.7 5.5





#87

Chrysene

Concen: 21.103 ng/ul

RT: 21.563 min Scan# 3124

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:228 Resp: 1313661

Ion Ratio Lower Upper

228 100

226 29.9 23.8 35.8

229 19.6 16.1 24.1



#89

Di-n-octyl phthalate

Concen: 24.740 ng/ul




RT: 22.363 min Scan# 3260


Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Tgt Ion:149 Resp: 1315519





#90

Benzo(b)fluoranthene

Concen: 22.013 ng/ul

RT: 23.268 min Scan# 3414

Delta R.T. -0.000 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:252 Resp: 1218219

Ion Ratio Lower Upper

252 100

253 21.9 18.0 27.0

125 8.4 6.8 10.2



#91

Benzo(k)fluoranthene

Concen: 22.117 ng/ul

RT: 23.315 min Scan# 3422

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:252 Resp: 1188742


Ion Ratio Lower Upper

252 100

253 21.9 17.3 25.9

125 8.6 6.9 10.3





#93

Benzo(a)pyrene

Concen: 21.595 ng/ul

RT: 23.927 min Scan# 3

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:252 Resp: 1028698

Ion Ratio Lower Upper

252 100

253 21.9 16.9 25.3

125 9.2 6.8 10.2



#94

Indeno(1,2,3-cd)pyrene

Concen: 19.184 ng/ul

RT: 26.686 min Scan# 3995

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00




Tgt Ion:276 Resp: 1257231


Ion Ratio Lower Upper

276 100

138 19.7 14.9 22.3

277 25.9 20.3 30.5

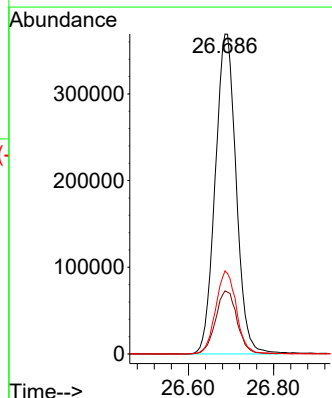



#95

Dibenzo(a,h)anthracene

Concen: 19.220 ng/ul

RT: 26.704 min Scan# 3998

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Instrument :

BNA_P

ClientSampleId :

SSTD020799





Tgt Ion:278 Resp: 1054577

Ion Ratio Lower Upper

278 100

139 12.9 10.4 15.6

279 24.7 18.9 28.3



#96

Benzo(g,h,i)perylene

Concen: 18.780 ng/ul

RT: 27.503 min Scan# 4134

Delta R.T. -0.006 min

Lab File: BP014405.D

Acq: 30 Mar 2023 17:00

Tgt Ion:276 Resp: 1003195

Ion Ratio Lower Upper

276 100

138 18.1 13.0 19.4

277 24.0 18.4 27.6

