

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014410.D
 Acq On : 30 Mar 2023 19:48
 Operator : CG/JU
 Sample : PB151800BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK800

Quant Time: Mar 30 22:43:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	145862	20.000	ng/ul	0.00
20) Naphthalene-d8	10.840	136	647988	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	445979	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.434	188	989758	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	765864	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	726053	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	22292	5.927	ng/uL	0.00
4) Pyridine-d5	3.817	84	310704	32.234	ng/ul	0.00
7) Phenol-d5	7.175	99	400529	29.774	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	273873	31.732	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	300670	30.924	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	329641	30.379	ng/ul	0.00
21) Nitrobenzene-d5	9.193	128	157502	30.109	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	183548	30.642	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	302684	27.747	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	422186	29.381	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1184155	32.747	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1237335	30.838	ng/ul	0.00
54) 4-Nitrophenol-d4	14.887	143	133095	24.363	ng/ul	0.00
60) Fluorene-d10	15.663	176	965476	32.017	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	196829	27.027	ng/ul	0.00
73) Anthracene-d10	17.534	188	1531897	31.981	ng/ul	0.00
81) Pyrene-d10	19.763	212	1683752	32.731	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1280519	33.196	ng/ul	0.00


Target Compounds					Qvalue	
5) Pyridine	3.846	79	10396	1.031	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014410.D
Acq On : 30 Mar 2023 19:48
Operator : CG/JU
Sample : PB151800BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK800

Quant Time: Mar 30 22:43:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 12:32:14 2023
Response via : Initial Calibration

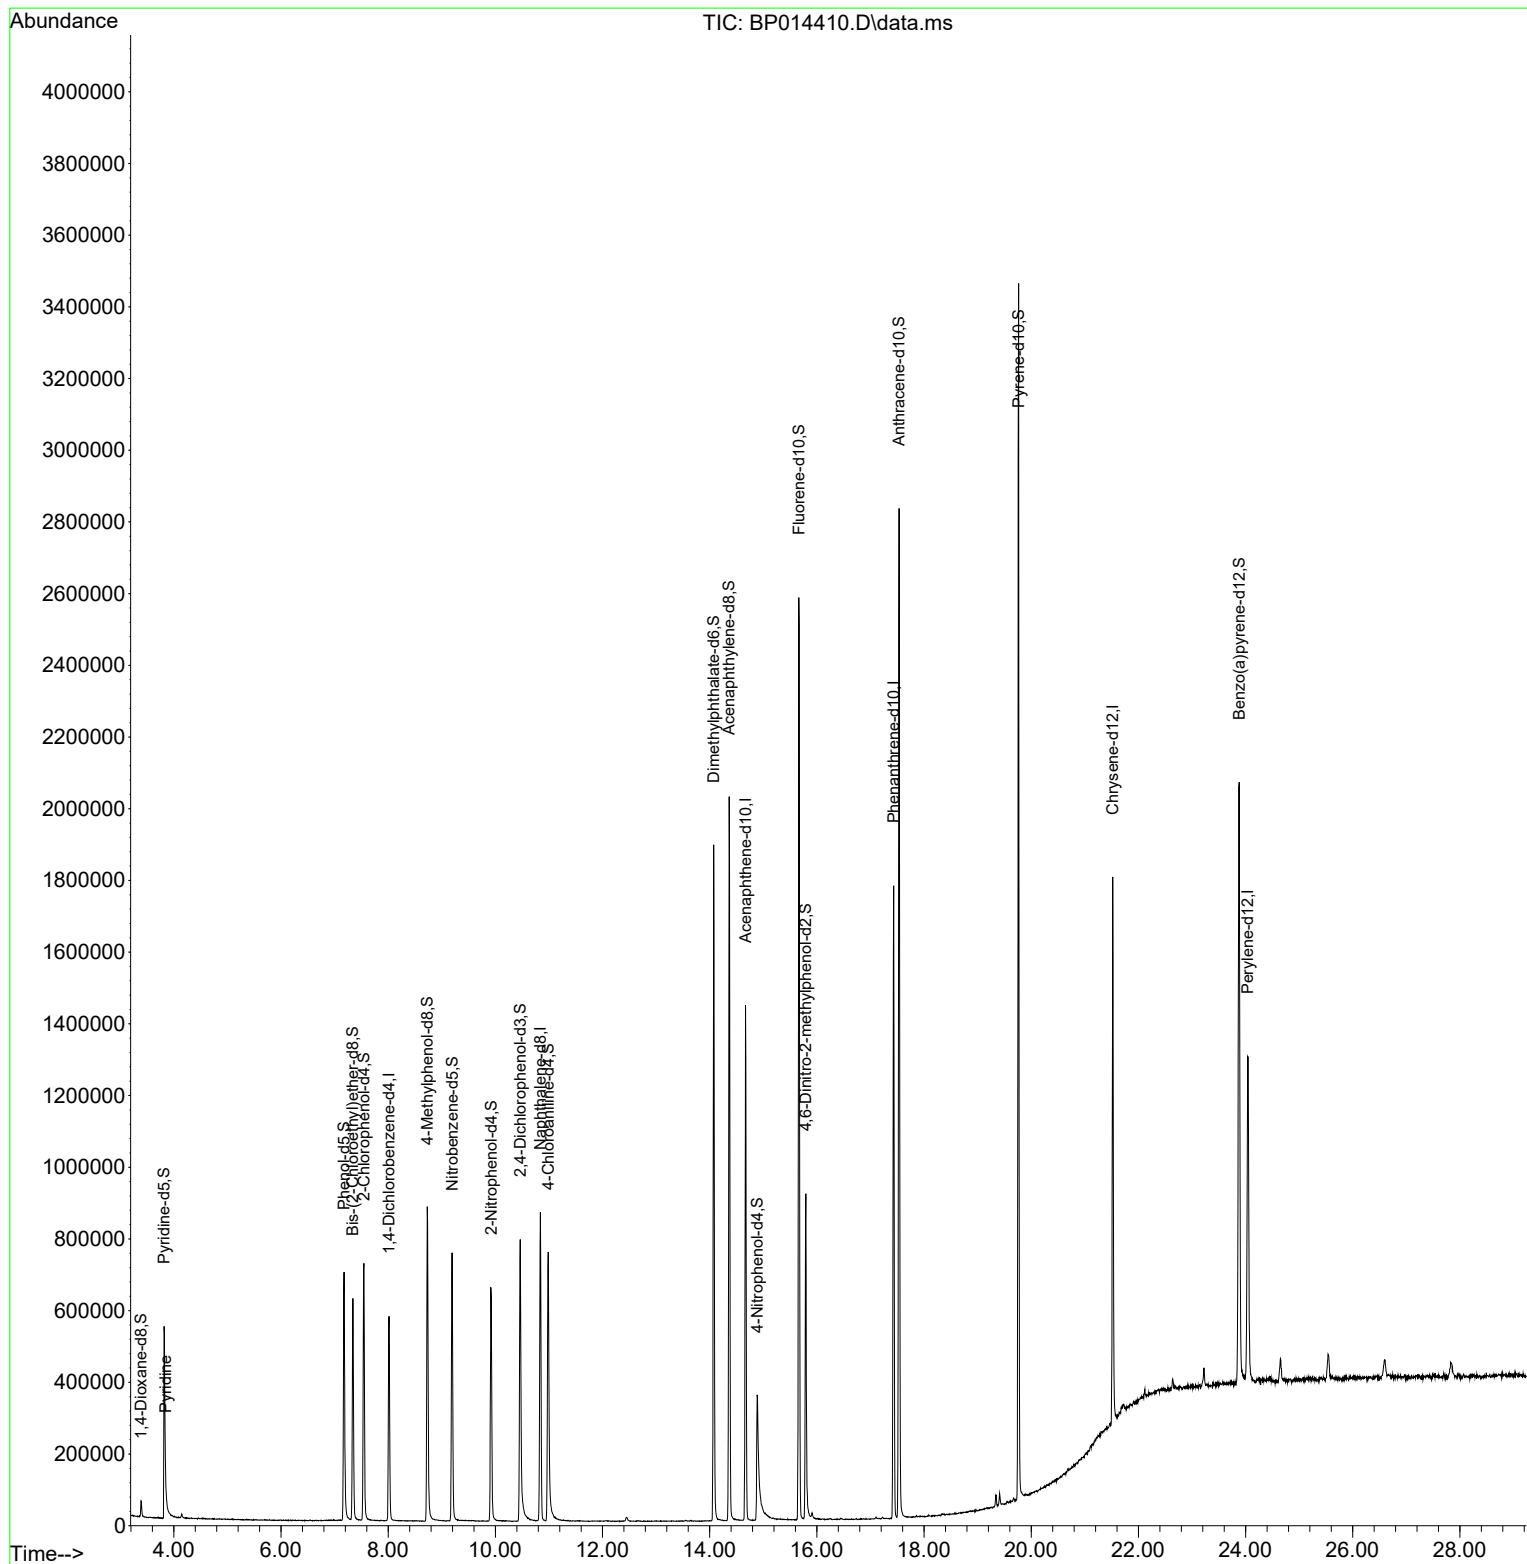

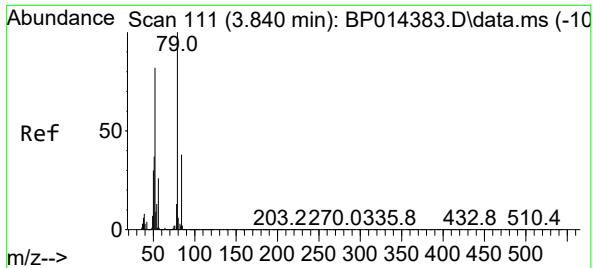

Pyridine
 Concen: 1.031 ng/ul
 RT: 3.846 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: BP014410.D
 Acq: 30 Mar 2023 19:48

Instrument :
 BNA_P
 ClientSampleId :
 SBLK800

Tgt Ion: 79 Resp: 10396
 Ion Ratio Lower Upper
 79 100
 52 322.2 61.4 92.2#
 51 49.4 28.5 42.7#

