

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014449.D
 Acq On : 31 Mar 2023 18:14
 Operator : CG/JU
 Sample : 02093-02
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Mar 31 22:55:17 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	149060	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	678510	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	469454	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	998128	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	686536	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	681340	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	19114	4.973	ng/uL	0.00
4) Pyridine-d5	3.828	84	72939	7.405	ng/ul	0.01
7) Phenol-d5	7.175	99	117398	8.540	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	353270	40.053	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	307738	30.972	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	230666	20.802	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	211078	38.535	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	240083	38.278	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	403946	35.363	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	90878	6.040	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1583571	41.603	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1657731	39.249	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	31749	5.521	ng/ul	0.03
60) Fluorene-d10	15.663	176	1284087	40.453	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	232348	31.636	ng/ul	0.00
73) Anthracene-d10	17.528	188	2034962	42.127	ng/ul	0.00
81) Pyrene-d10	19.757	212	2137892	46.361	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1575319	43.518	ng/ul	0.00


Target Compounds					Qvalue	
19) Hexachloroethane	9.122	117	5678	1.257	ng/ul#	3


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014449.D
Acq On : 31 Mar 2023 18:14
Operator : CG/JU
Sample : 02093-02
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :


Quant Time: Mar 31 22:55:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

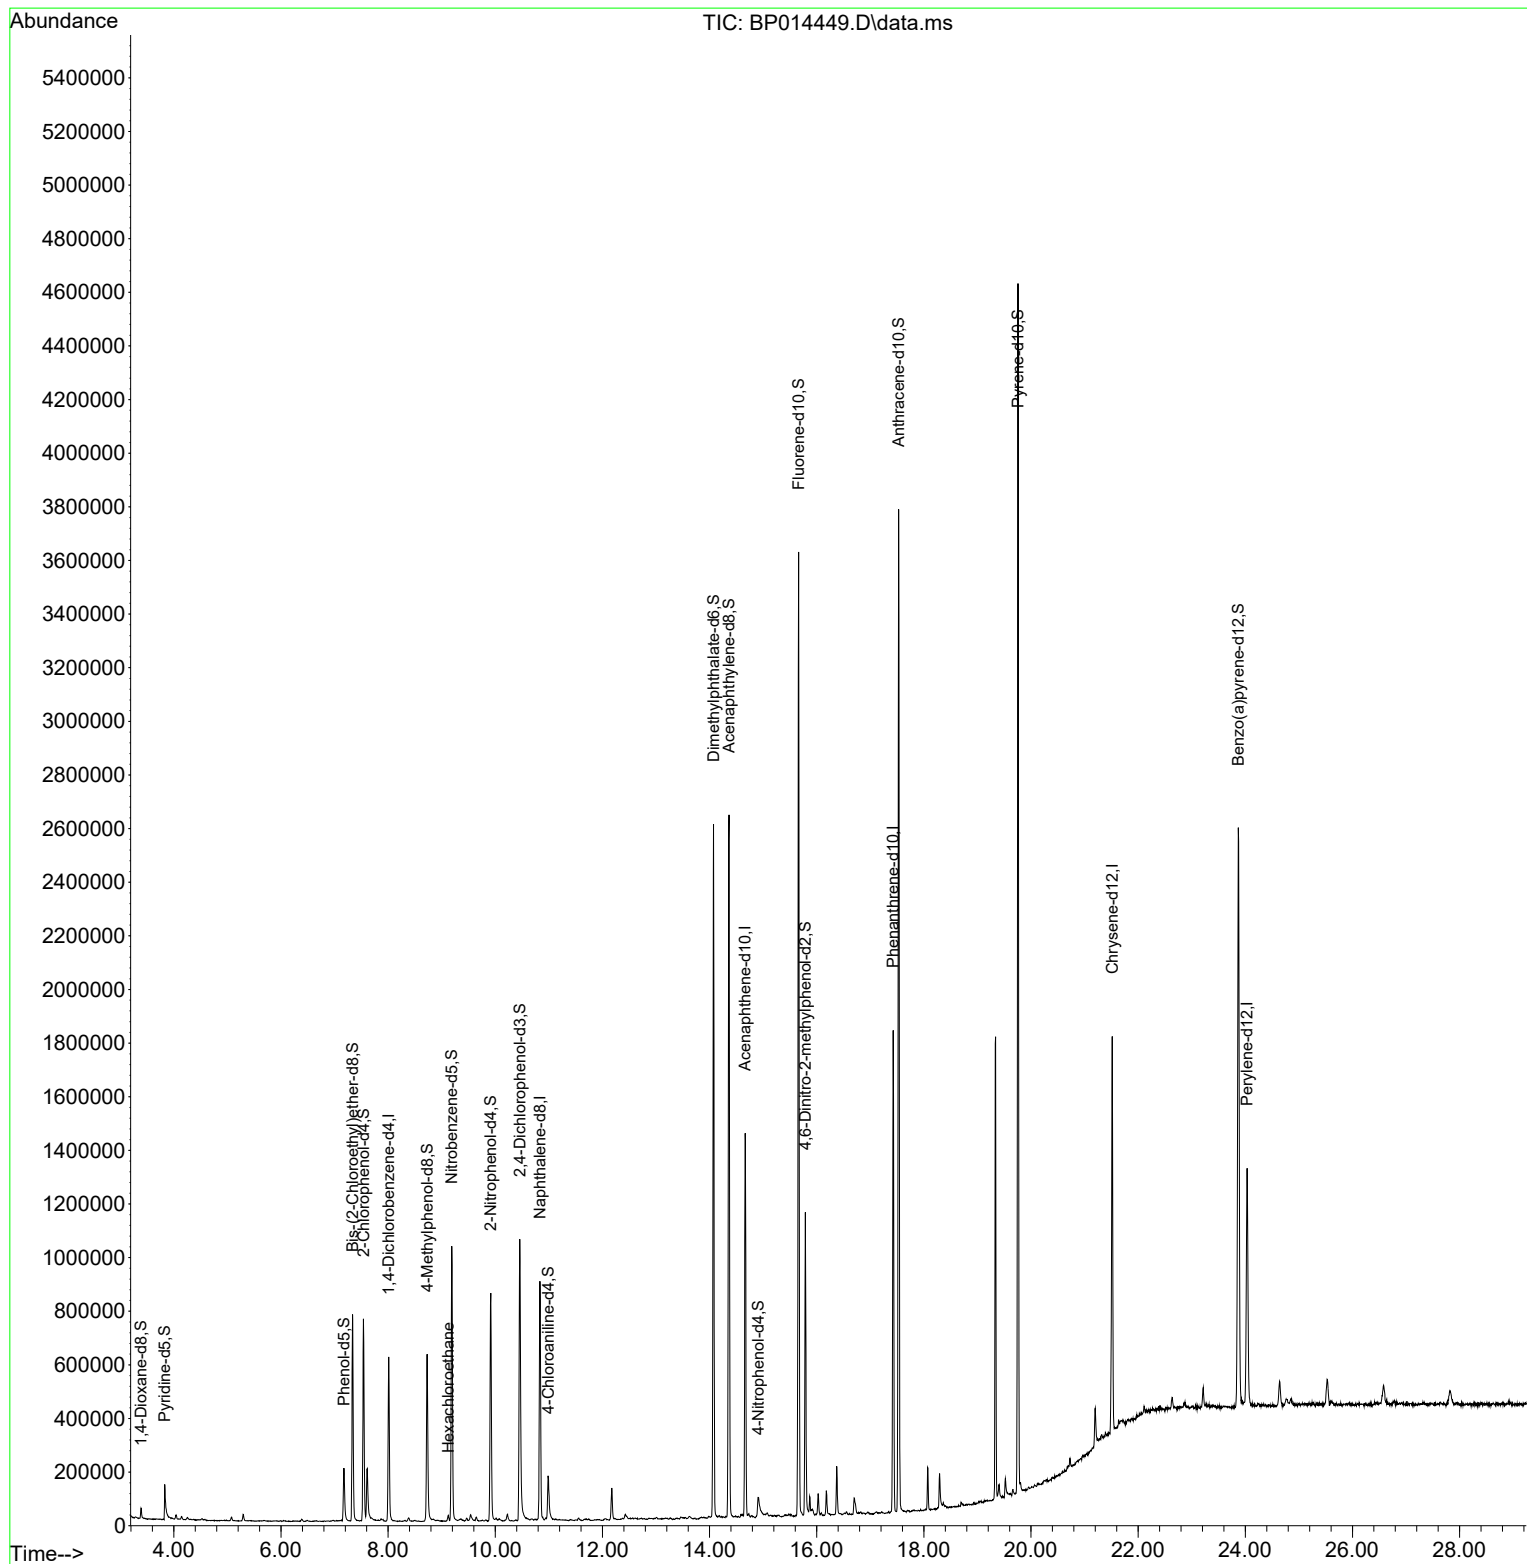

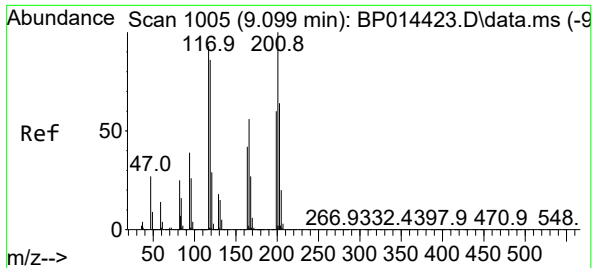

#19
 Hexachloroethane
 Concen: 1.257 ng/ul
 RT: 9.122 min Scan# 10
 Delta R.T. 0.023 min
 Lab File: BP014449.D
 Acq: 31 Mar 2023 18:14

Instrument :
 BNA_P
 ClientSampleId :

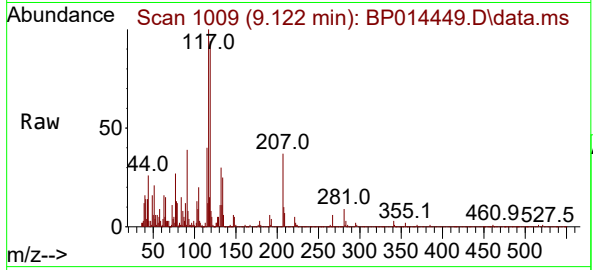

Tgt Ion:117 Resp: 5678
 Ion Ratio Lower Upper
 117 100
 201 0.5 90.2 135.4#
 199 0.0 54.2 81.2#

