




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014394.D
 Acq On : 30 Mar 2023 10:38
 Operator : CG/JU
 Sample : PB151777BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK777

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:49:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

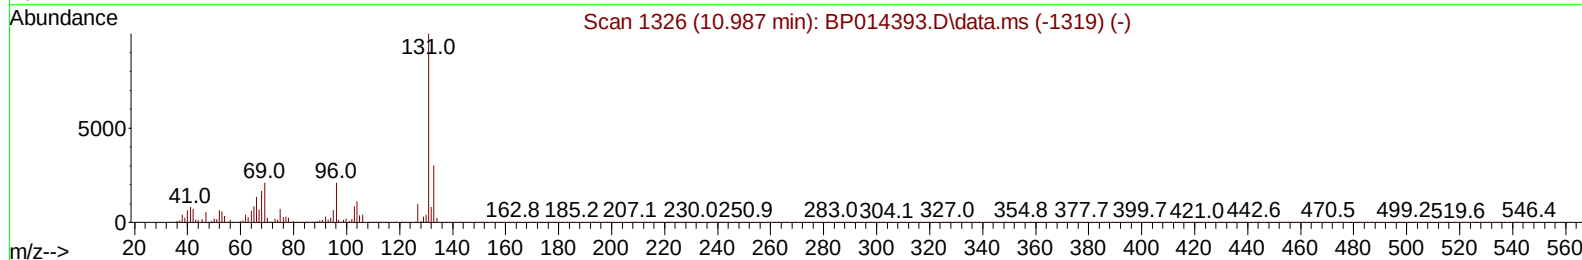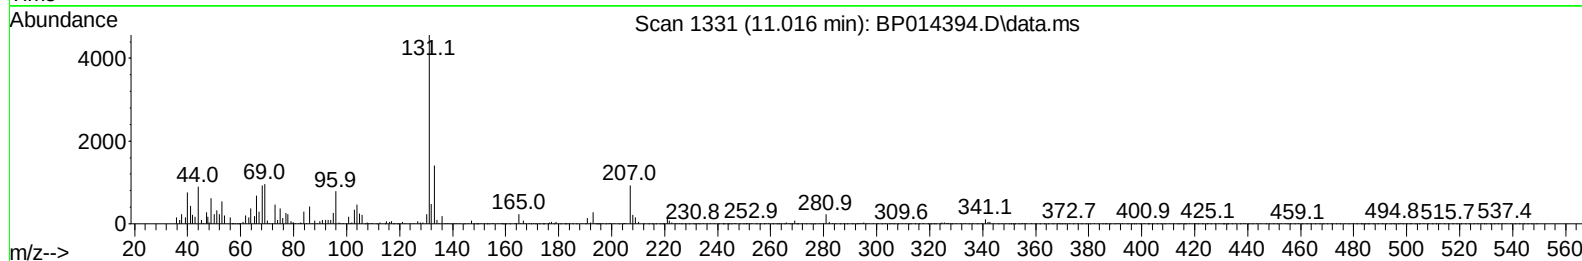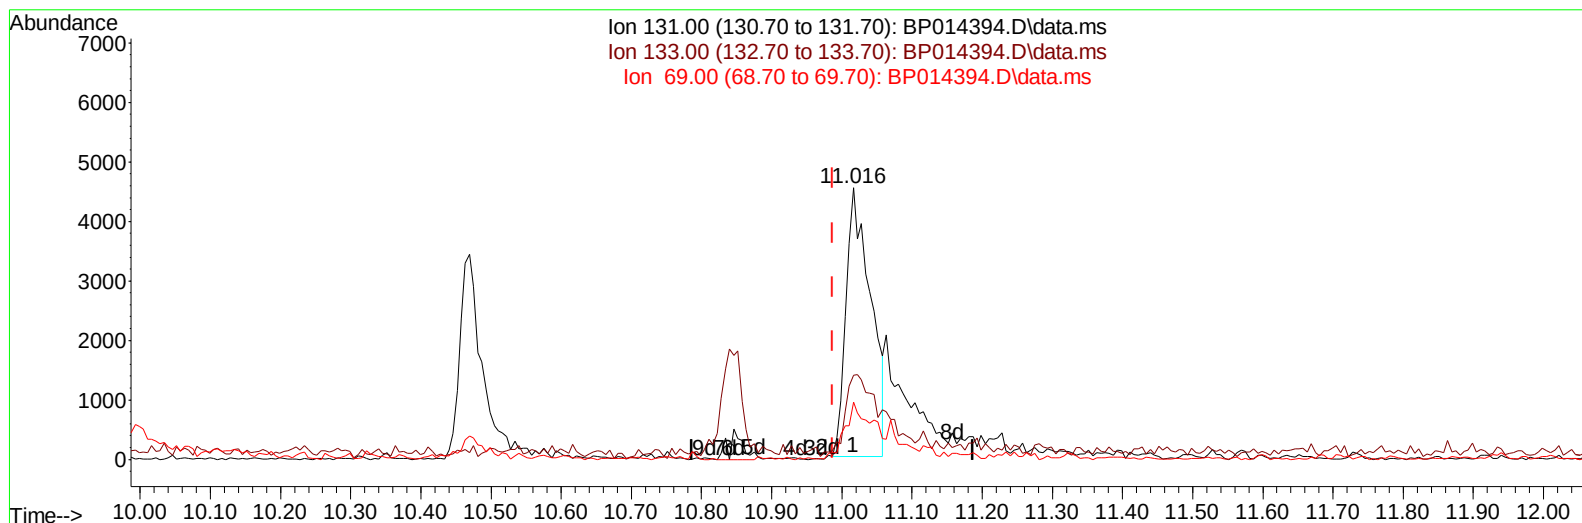

TIC: BP014394.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.016min (+ 0.029) 1.16 ng/uI

response 11037

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.92
69.00	21.30	21.04
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014394.D
 Acq On : 30 Mar 2023 10:38
 Operator : CG/JU
 Sample : PB151777BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK777

Manual IntegrationsAPPROVED

Quant Time: Mar 30 22:49:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

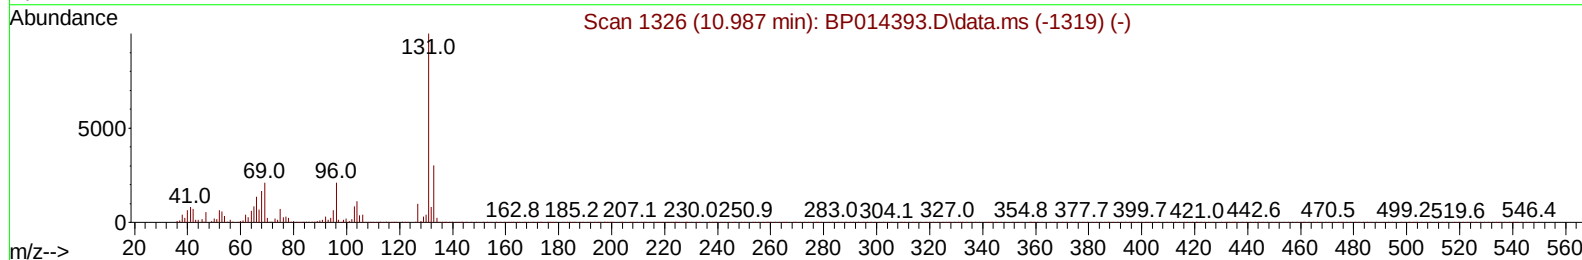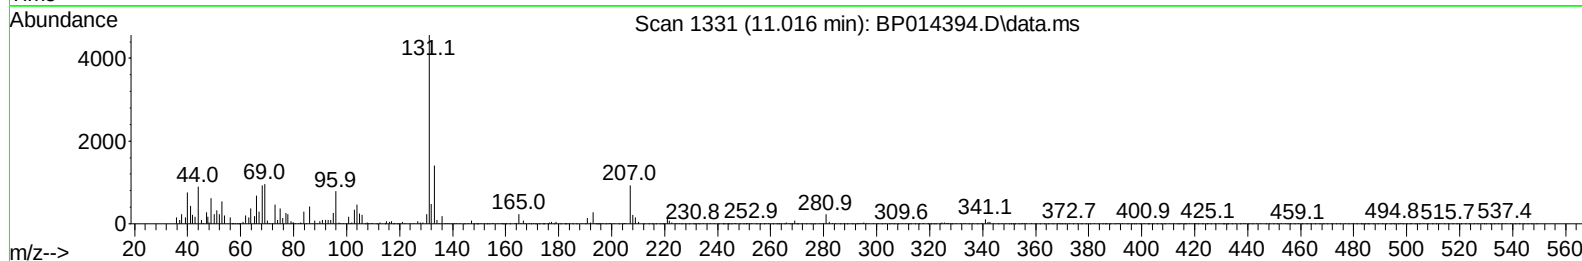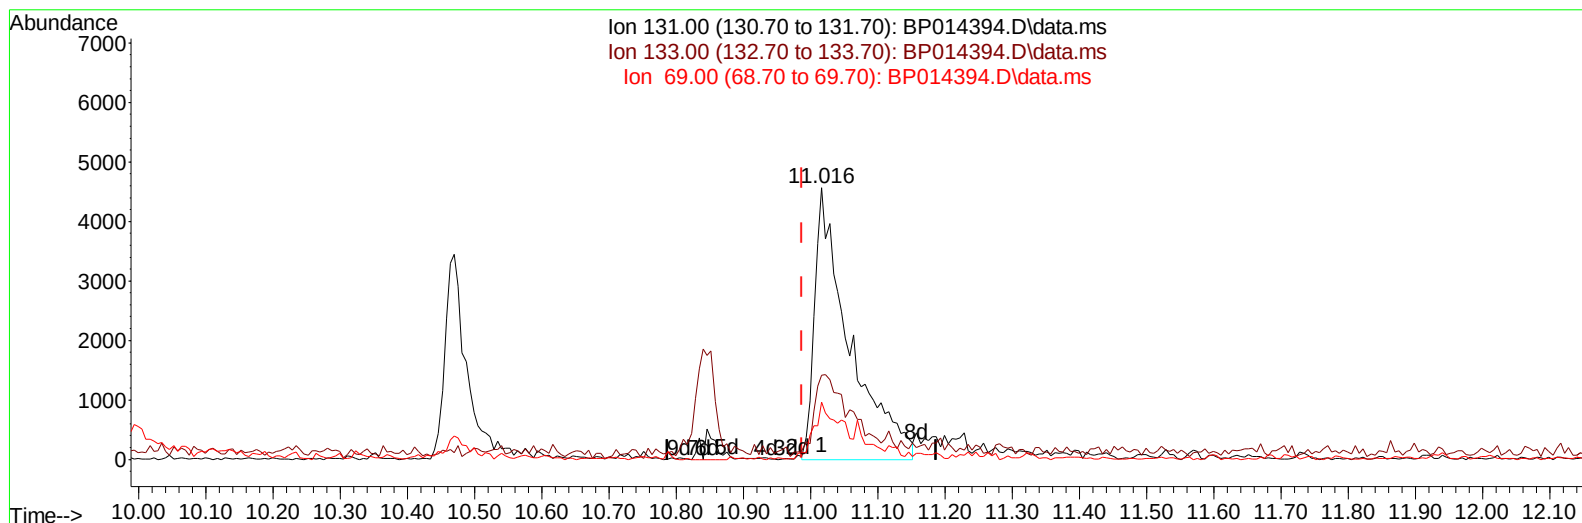

TIC: BP014394.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.016min (+ 0.029) 1.71 ng/ul m

response 16241

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	30.92
69.00	21.30	21.04
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014394.D
 Acq On : 30 Mar 2023 10:38
 Operator : CG/JU
 Sample : PB151777BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK777

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:49:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	100539	20.000	ng/ul	0.00
20) Naphthalene-d8	10.840	136	428365	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	296319	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.434	188	709204	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	718739	20.000	ng/ul	0.00
88) Perylene-d12	24.045	264	784016	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	15953	6.153	ng/uL	0.00
4) Pyridine-d5	3.828	84	91939	13.838	ng/ul	0.00
7) Phenol-d5	7.175	99	282853	30.506	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	188699	31.719	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	212259	31.673	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	232412	31.074	ng/ul	0.00
21) Nitrobenzene-d5	9.193	128	104474	30.211	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	124942	31.553	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.469	165	207413	28.761	ng/ul	0.00
31) 4-Chloroaniline-d4	11.016	131	16241m	1.710	ng/ul	0.03
46) Dimethylphthalate-d6	14.075	166	787635	32.782	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	825005	30.946	ng/ul	0.00
54) 4-Nitrophenol-d4	14.893	143	104443	28.775	ng/ul	0.01
60) Fluorene-d10	15.669	176	675416	33.710	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	129700	24.854	ng/ul	0.00
73) Anthracene-d10	17.534	188	1136969	33.126	ng/ul	0.00
81) Pyrene-d10	19.763	212	1419762	29.408	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1393034	33.443	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014394.D
Acq On : 30 Mar 2023 10:38
Operator : CG/JU
Sample : PB151777BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK777

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:49:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 12:32:14 2023
Response via : Initial Calibration

