




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014400.D
Acq On : 30 Mar 2023 14:11
Operator : CG/JU
Sample : 02092-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB986

Manual IntegrationsAPPROVED

Quant Time: Mar 30 22:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 12:32:14 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

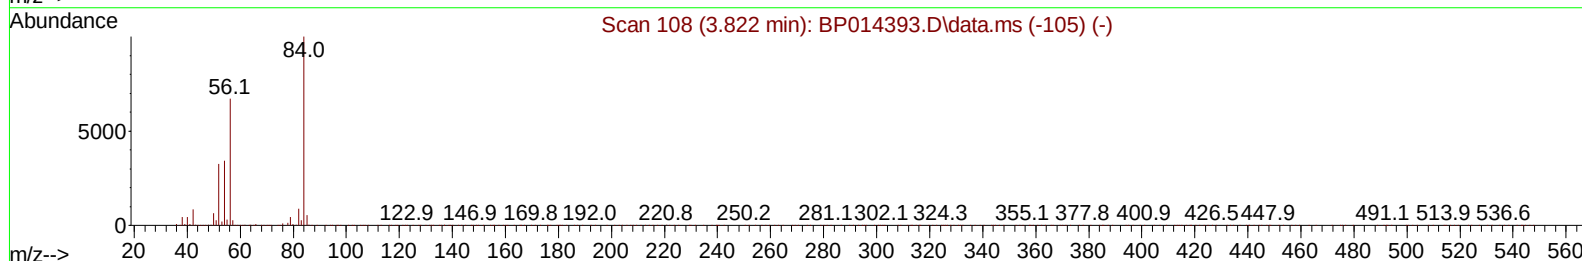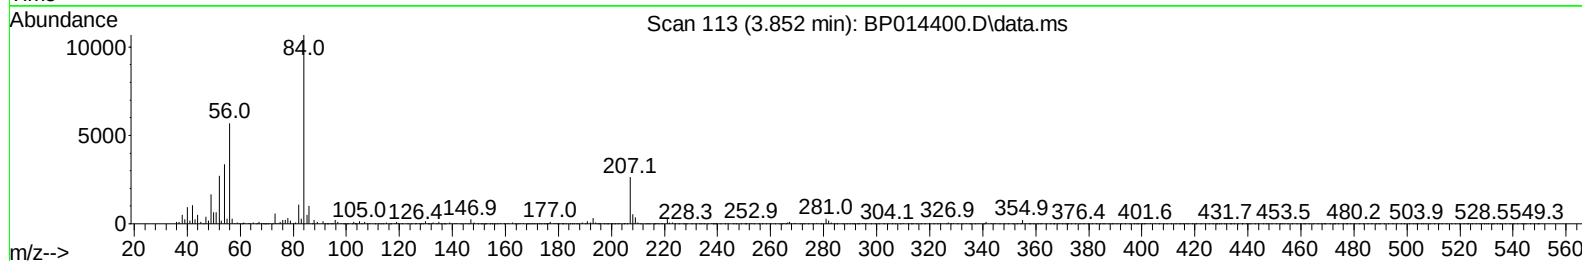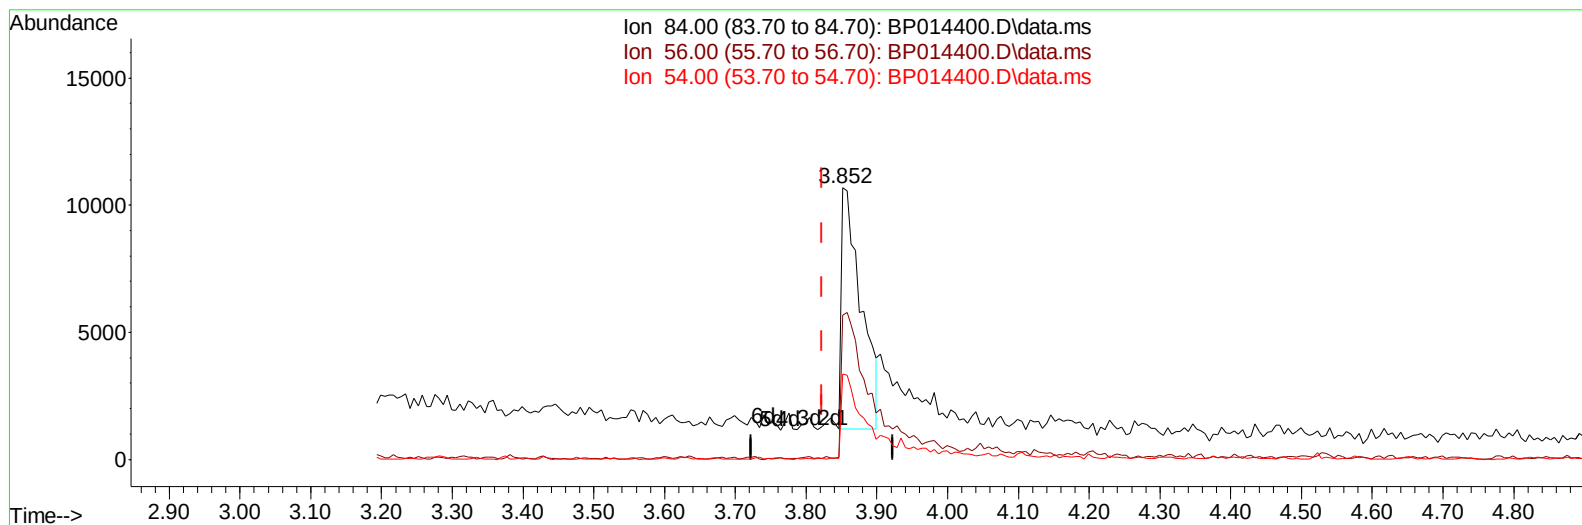

TIC: BP014400.D\data.ms

(4) Pyridine-d5 (S)

3.852min (+ 0.029) 1.90 ng/u1

response 18447

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	53.25
54.00	32.60	31.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014400.D
 Acq On : 30 Mar 2023 14:11
 Operator : CG/JU
 Sample : 02092-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB986

Manual IntegrationsAPPROVED

Quant Time: Mar 30 22:40:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

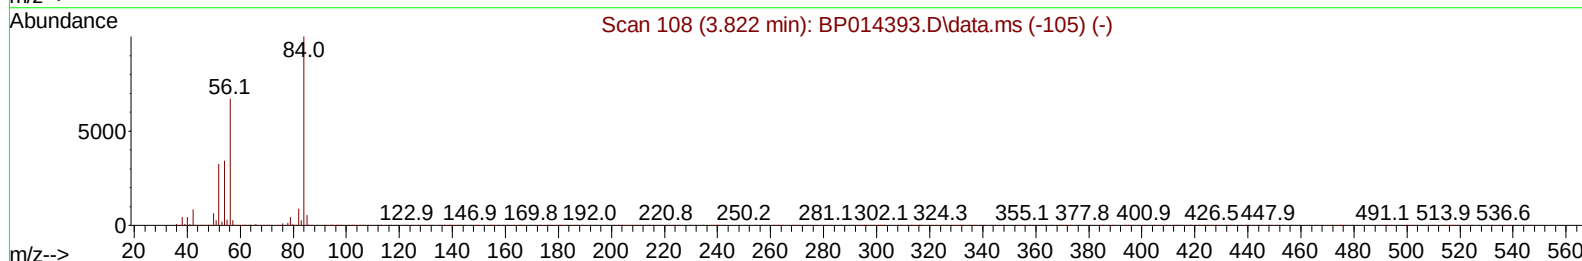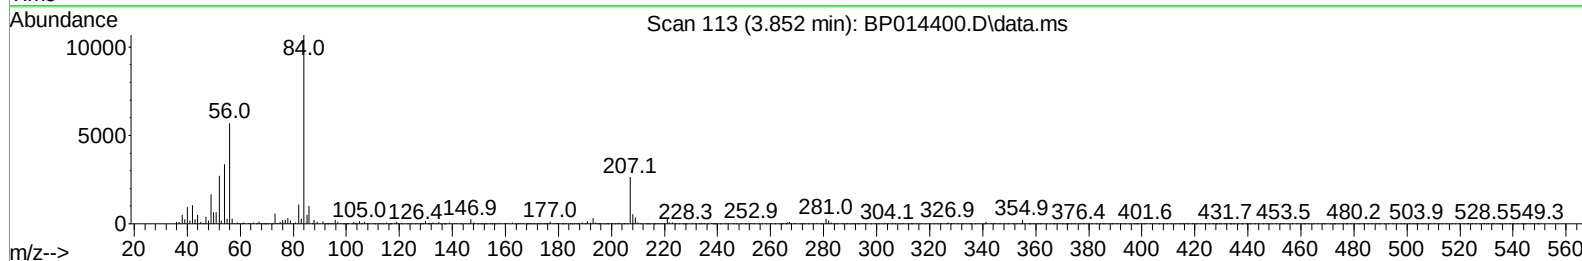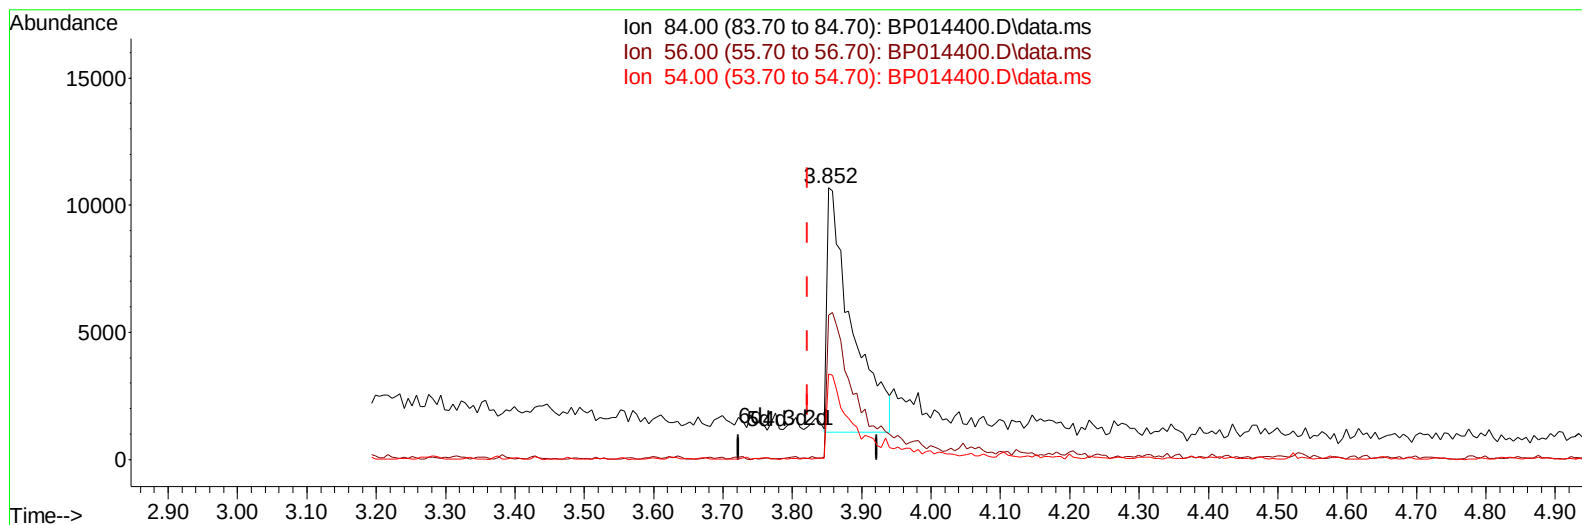

TIC: BP014400.D\data.ms

(4) Pyridine-d5 (S)

3.852min (+ 0.029) 2.47 ng/ul m

response 24061

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	53.25
54.00	32.60	31.40
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014400.D
 Acq On : 30 Mar 2023 14:11
 Operator : CG/JU
 Sample : 02092-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB986

Manual IntegrationsAPPROVED

Quant Time: Mar 30 22:40:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

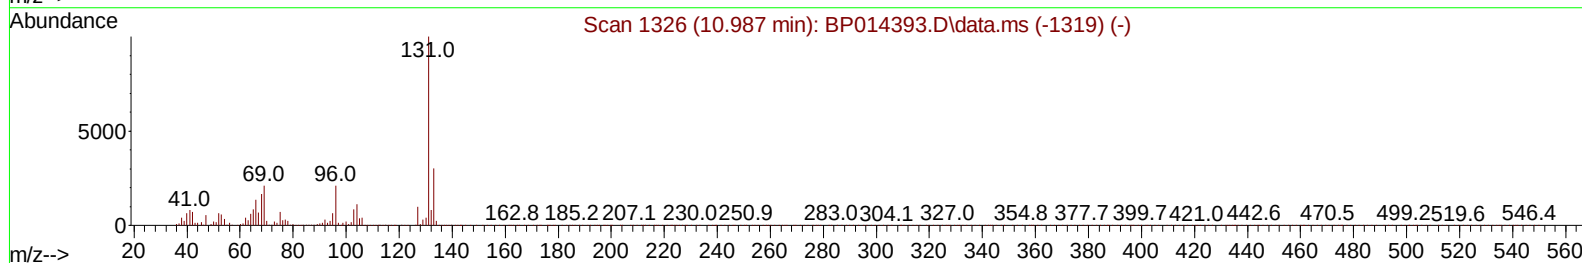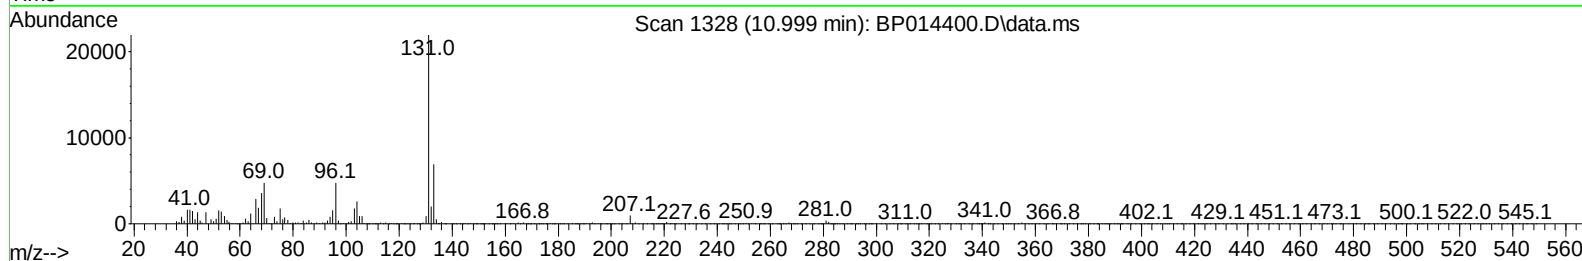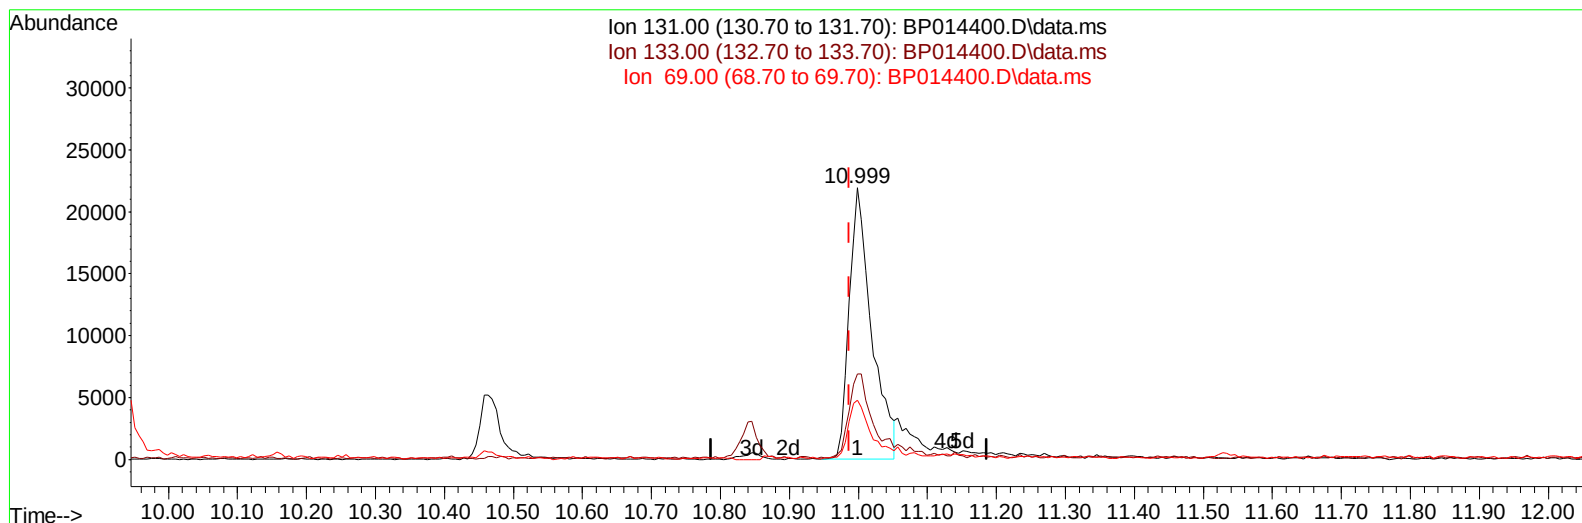

TIC: BP014400.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.999min (+ 0.012) 3.48 ng/ul

response 49666

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	31.40
69.00	21.30	21.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014400.D
 Acq On : 30 Mar 2023 14:11
 Operator : CG/JU
 Sample : 02092-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB986

Manual IntegrationsAPPROVED

Quant Time: Mar 30 22:40:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

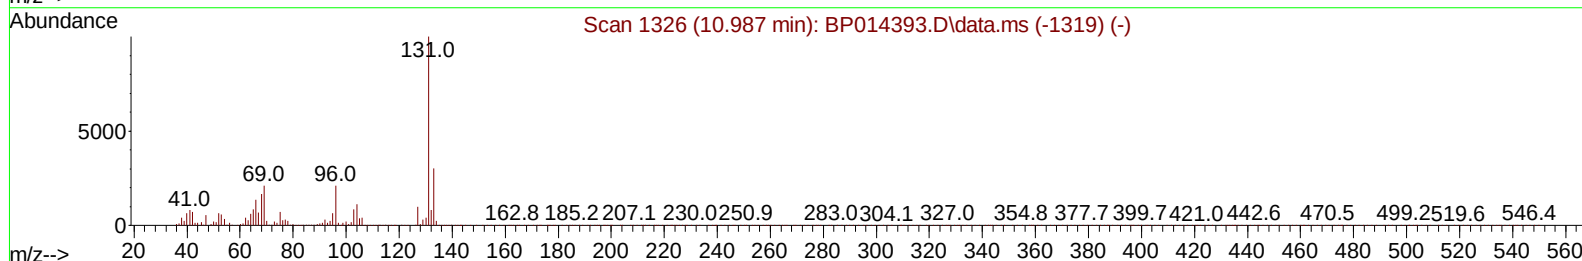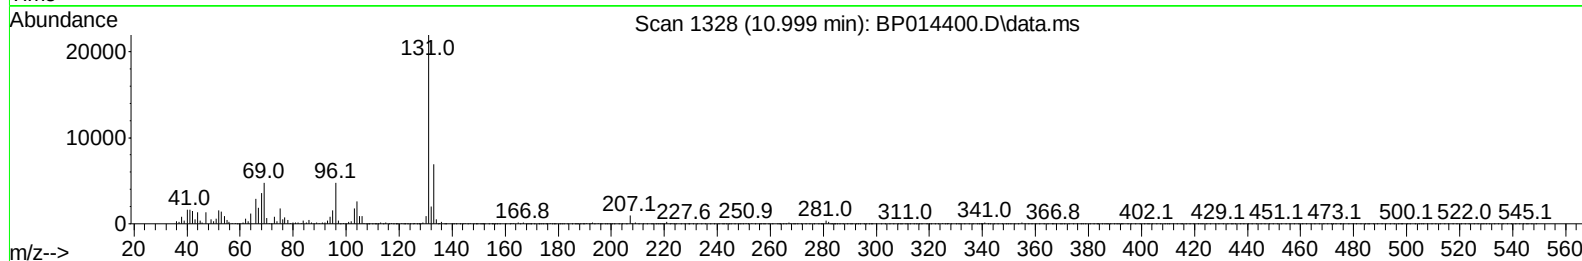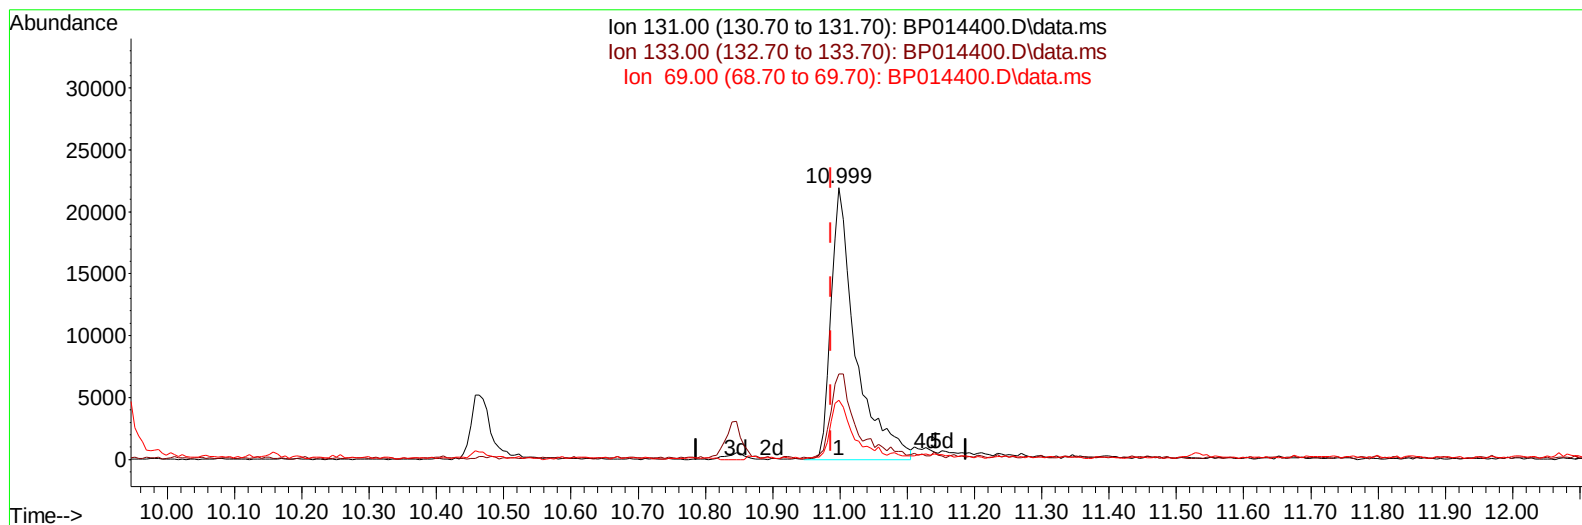

TIC: BP014400.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.999min (+ 0.012) 3.90 ng/ul m

response 55632

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	31.40
69.00	21.30	21.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014400.D
Acq On : 30 Mar 2023 14:11
Operator : CG/JU
Sample : 02092-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB986

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 12:32:14 2023
Response via : Initial Calibration

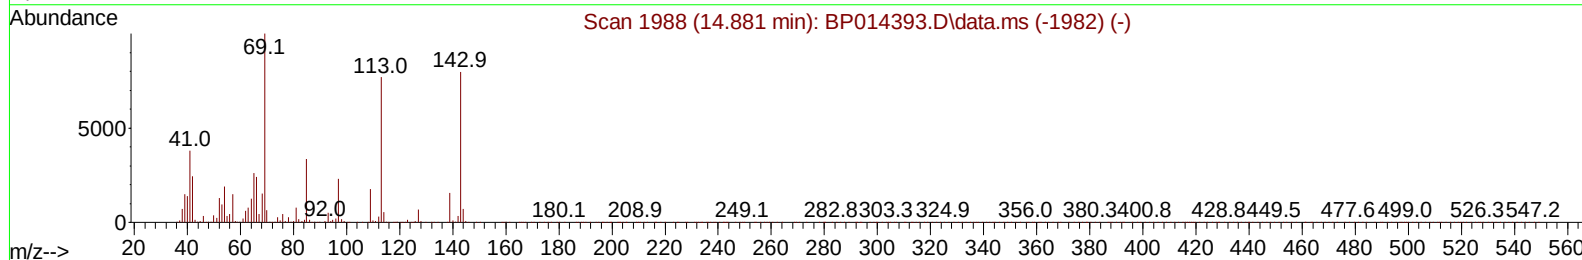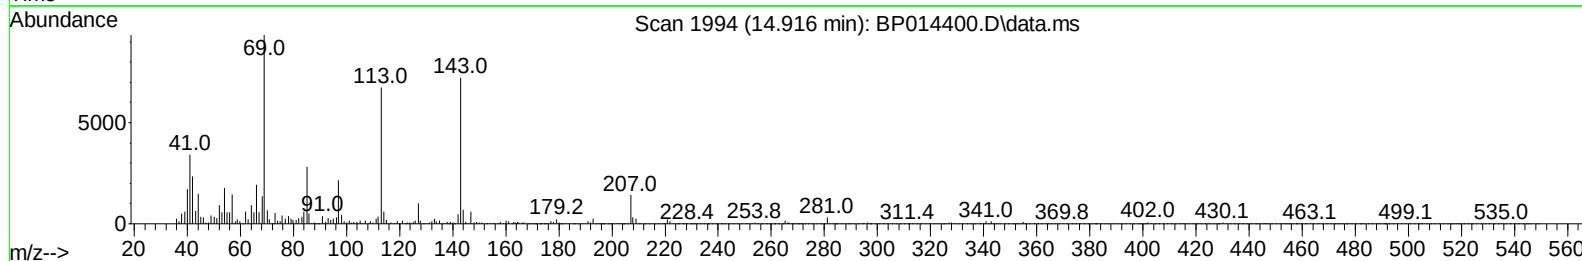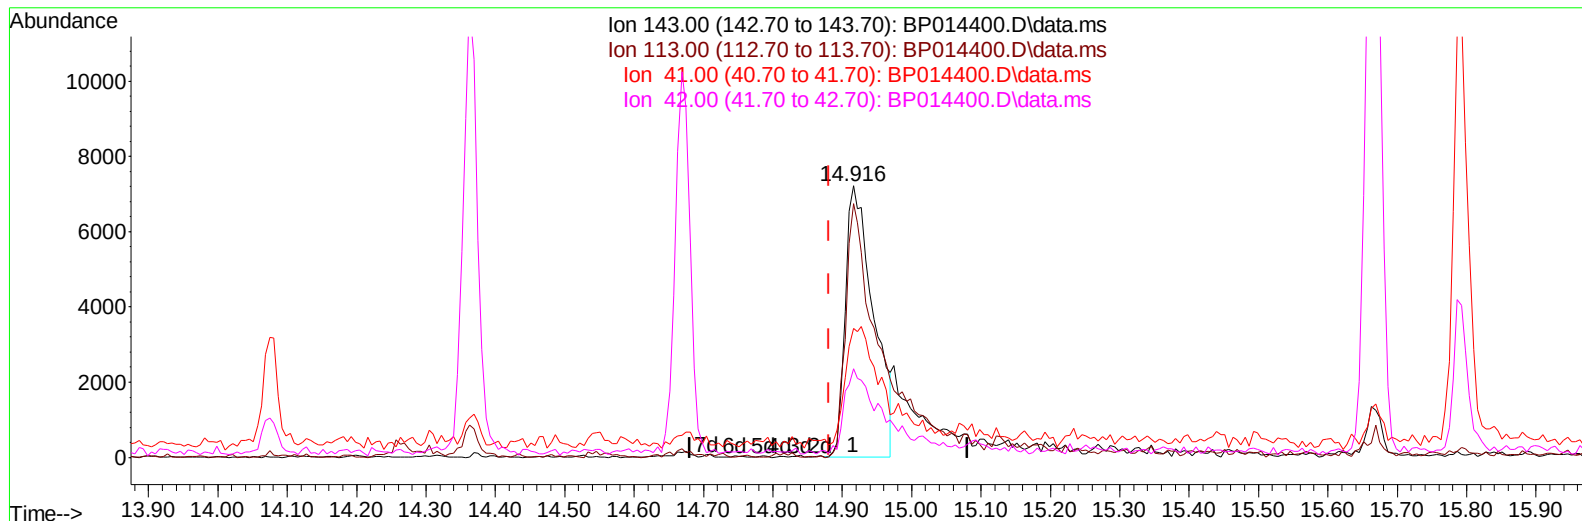

TIC: BP014400.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.035) 3.77 ng/u1

response 20131

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	93.38
41.00	44.20	47.51
42.00	31.50	32.64

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014400.D
 Acq On : 30 Mar 2023 14:11
 Operator : CG/JU
 Sample : 02092-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB986

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:40:23 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	147279	20.000	ng/ul	0.00
20) Naphthalene-d8	10.840	136	643851	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	436054	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.433	188	949943	20.000	ng/ul	0.00
79) Chrysene-d12	21.522	240	682831	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	643270	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	15553	4.095	ng/uL	0.00
4) Pyridine-d5	3.852	84	24061m	2.472	ng/ul	0.03
7) Phenol-d5	7.181	99	77516	5.707	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	254286	29.179	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	227552	23.179	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	163464	14.920	ng/ul	0.00
21) Nitrobenzene-d5	9.193	128	149260	28.717	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	169014	28.397	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	295306	27.244	ng/ul	0.00
31) 4-Chloroaniline-d4	10.999	131	55632m	3.896	ng/ul	0.01
46) Dimethylphthalate-d6	14.075	166	1230615	34.806	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1249522	31.850	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	25571m	4.787	ng/ul	0.04
60) Fluorene-d10	15.669	176	1001962	33.983	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	203139	29.062	ng/ul	0.00
73) Anthracene-d10	17.533	188	1591892	34.627	ng/ul	0.00
81) Pyrene-d10	19.763	212	1770779	38.608	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	1252103	36.636	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014400.D
Acq On : 30 Mar 2023 14:11
Operator : CG/JU
Sample : 02092-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB986

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:40:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 12:32:14 2023
Response via : Initial Calibration

