




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014425.D
Acq On : 31 Mar 2023 04:44
Operator : CG/JU
Sample : PB151687BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 31 05:13:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

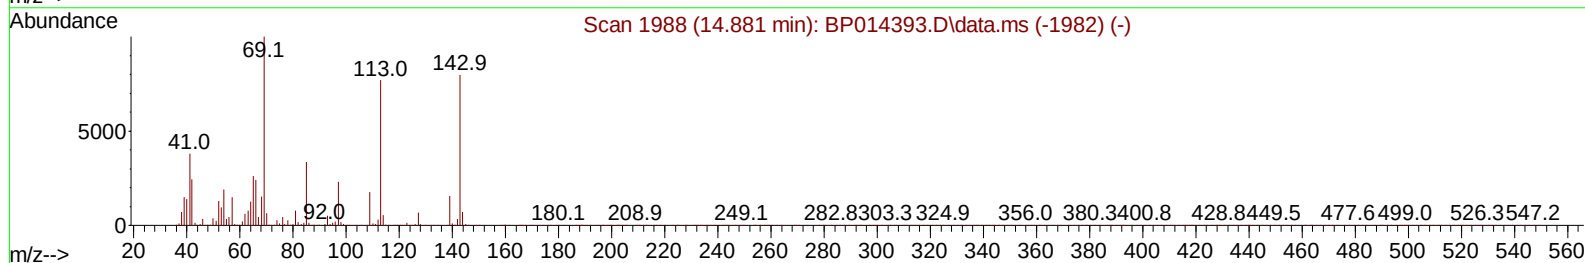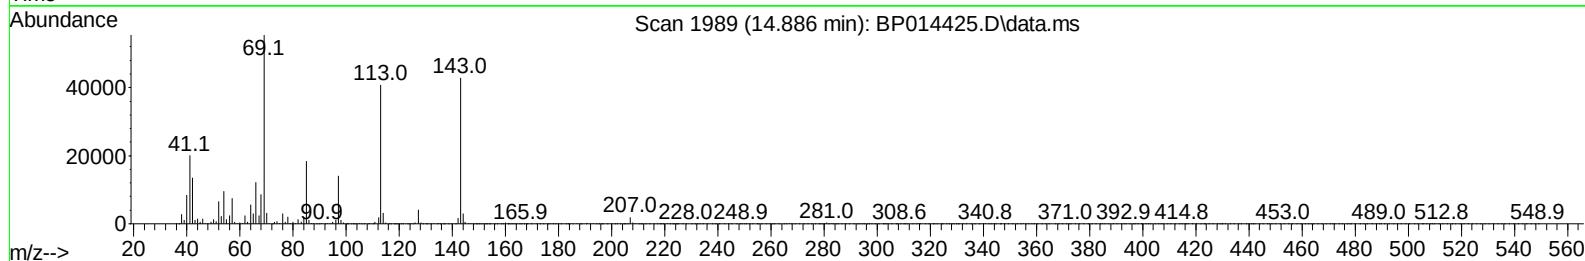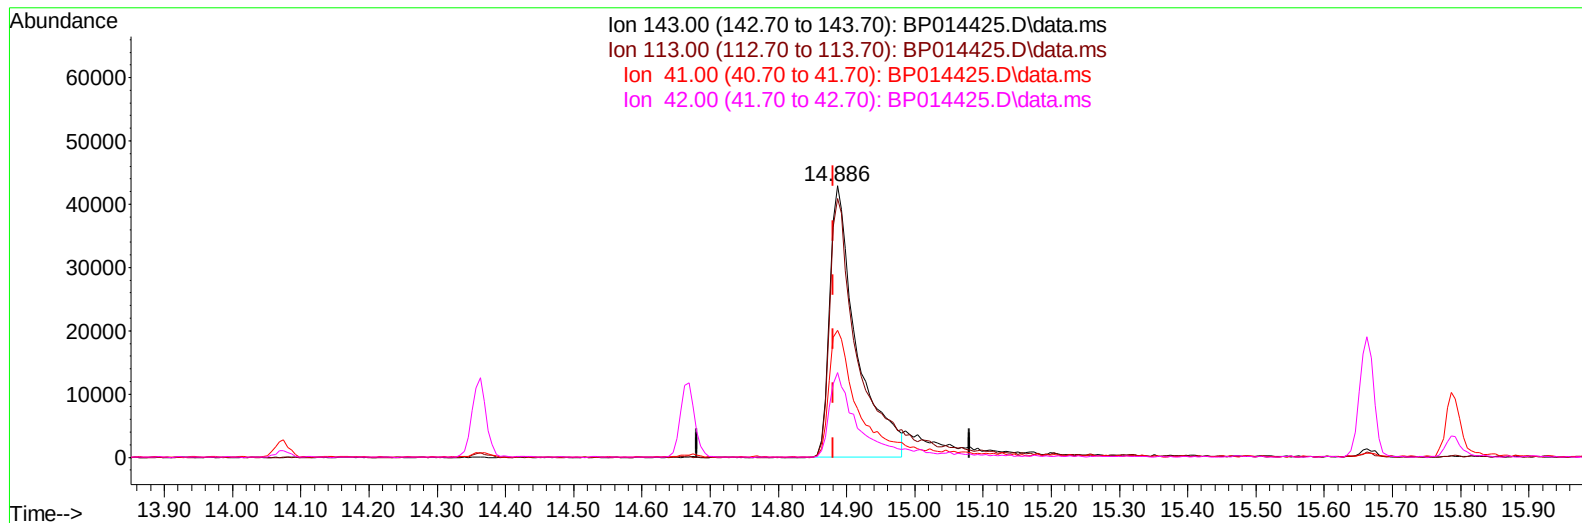

TIC: BP014425.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.886min (+ 0.006) 19.85 ng/ul****response 117450**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	95.34
41.00	44.20	46.89
42.00	31.50	31.37




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014425.D
Acq On : 31 Mar 2023 04:44
Operator : CG/JU
Sample : PB151687BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 31 05:13:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

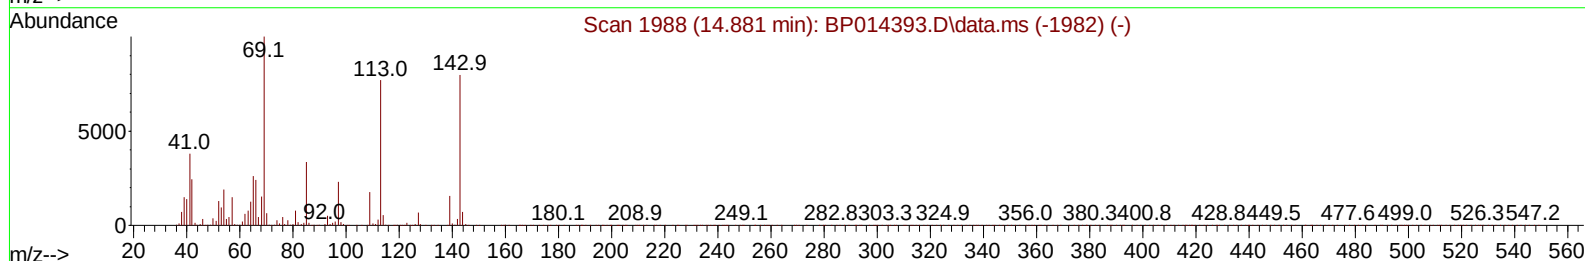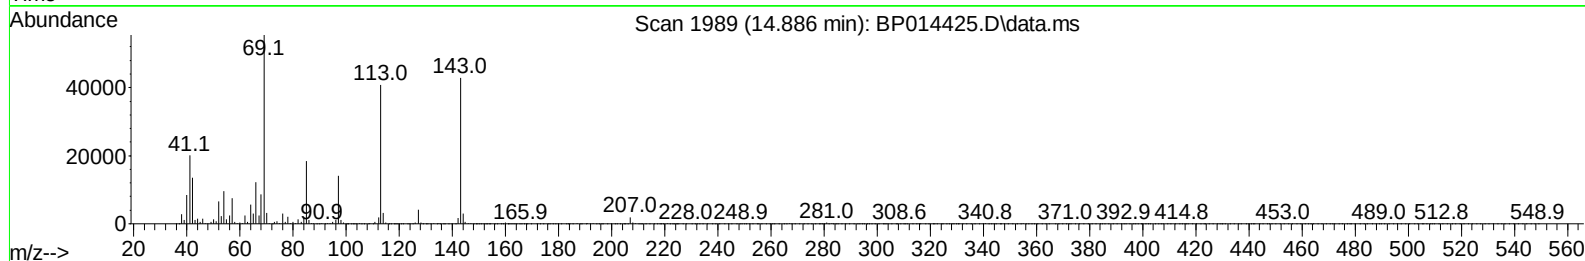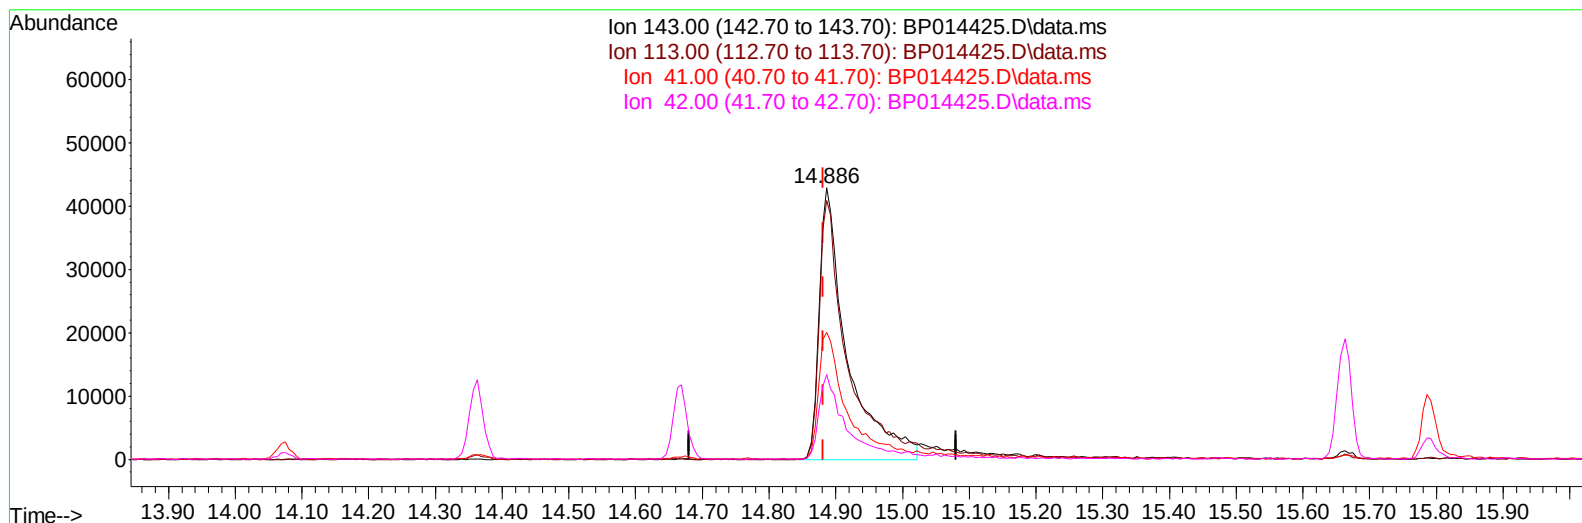

TIC: BP014425.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.886min (+ 0.006) 21.21 ng/ul m

response 125516

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	95.34
41.00	44.20	46.89
42.00	31.50	31.37

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014425.D
 Acq On : 31 Mar 2023 04:44
 Operator : CG/JU
 Sample : PB151687BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK687

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 31 05:13:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	171812	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	753297	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	483140	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.427	188	950464	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	750307	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	818201	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	24849	5.609	ng/uL	0.00
4) Pyridine-d5	3.816	84	298007	26.247	ng/ul	0.00
7) Phenol-d5	7.169	99	441853	27.885	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	299431	29.453	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	330591	28.866	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	361478	28.282	ng/ul	0.00
21) Nitrobenzene-d5	9.193	128	170749	28.078	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	201919	28.997	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	335774	26.477	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	311650	18.657	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1161436	29.648	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1244749	28.636	ng/ul	0.00
54) 4-Nitrophenol-d4	14.886	143	125516m	21.209	ng/ul	0.00
60) Fluorene-d10	15.663	176	944234	28.904	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	182922	26.155	ng/ul	0.00
73) Anthracene-d10	17.527	188	1382635	30.058	ng/ul	0.00
81) Pyrene-d10	19.757	212	1488353	29.532	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	1342133	30.875	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014425.D
Acq On : 31 Mar 2023 04:44
Operator : CG/JU
Sample : PB151687BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK687

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/31/2023
Supervised By :Jagrut Upadhyay 03/31/2023

Quant Time: Mar 31 05:13:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

