




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014434.D
Acq On : 31 Mar 2023 09:46
Operator : CG/JU
Sample : 02059-01DL2 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG0DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:51:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

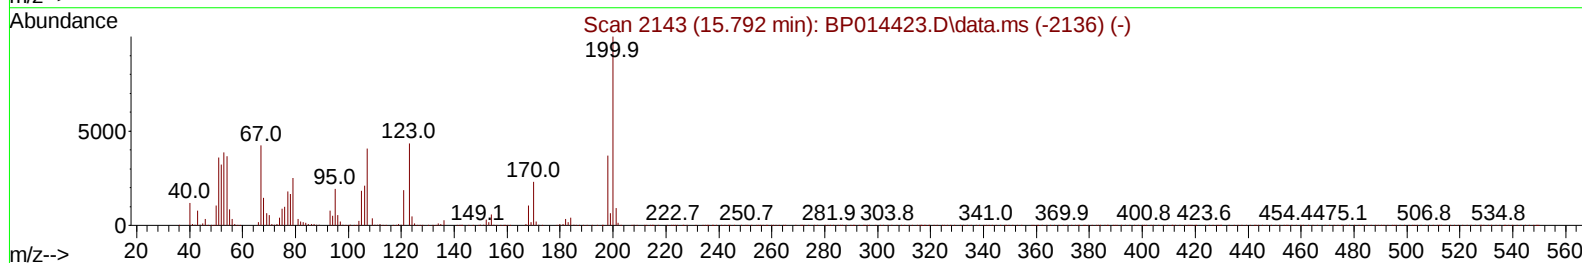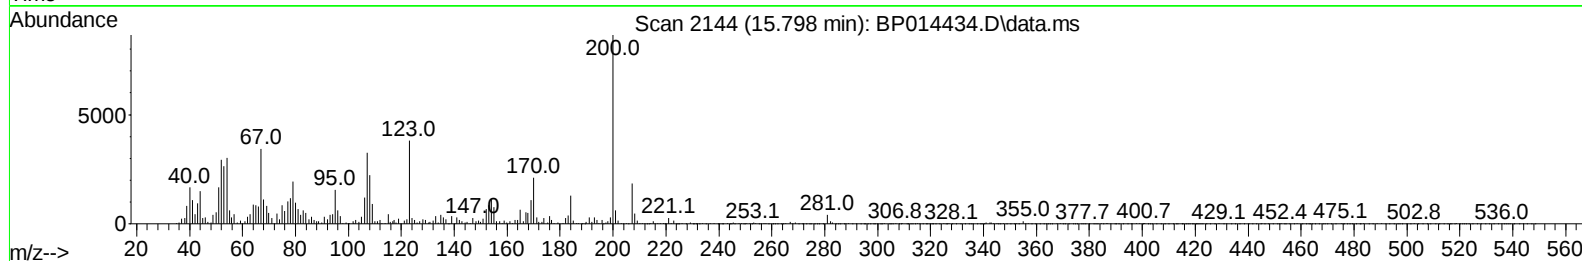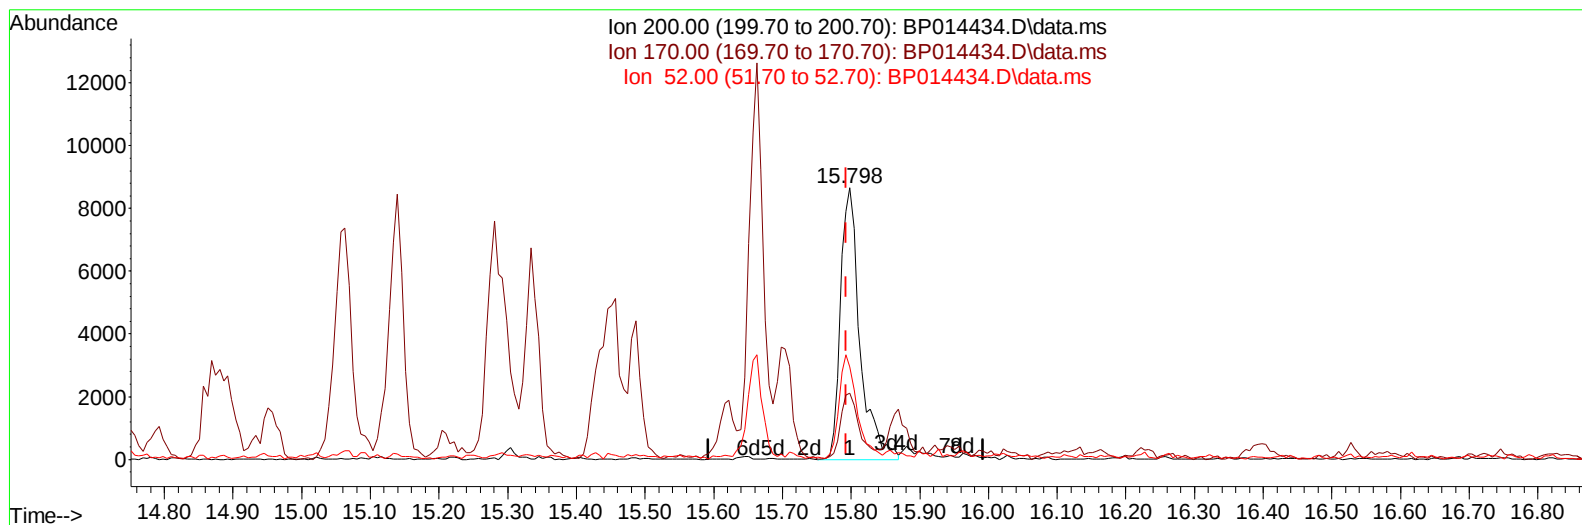

TIC: BP014434.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.798min (+ 0.006) 1.89 ng/ul m

response 16950

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	24.46
52.00	45.50	33.98#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014434.D
 Acq On : 31 Mar 2023 09:46
 Operator : CG/JU
 Sample : 02059-01DL2 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG0DL2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:51:46 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	194046	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	887040	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	583417	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1217783	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	876937	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	863721	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	2446	0.489	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.193	99	9088	0.508	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.340	67	35824	3.120	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	29692	2.296	ng/ul	0.00
15) 4-Methylphenol-d8	8.740	113	19681	1.363	ng/ul	0.01
21) Nitrobenzene-d5	9.193	128	17502	2.444	ng/ul	0.00
24) 2-Nitrophenol-d4	9.922	143	20134	2.455	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.475	165	34954	2.341	ng/ul	0.02
31) 4-Chloroaniline-d4	10.998	131	30723	1.562	ng/ul	0.02
46) Dimethylphthalate-d6	14.069	166	170602	3.606	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	164994	3.143	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.663	176	142426	3.610	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	16950m	1.892	ng/ul	0.00
73) Anthracene-d10	17.528	188	213827	3.628	ng/ul	0.00
81) Pyrene-d10	19.757	212	238903	4.056	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.863	264	167135	3.642	ng/ul	0.00
Target Compounds						
					Qvalue	
30) Naphthalene	10.887	128	740634	14.990	ng/ul	99
36) 2-Methylnaphthalene	12.493	142	89527	2.674	ng/ul	98
37) 1-Methylnaphthalene	12.710	142	72136	2.172	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	15.298	232	45121	3.664	ng/ul	94
71) Pentachlorophenol	17.081	266	822458	81.562	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014434.D
Acq On : 31 Mar 2023 09:46
Operator : CG/JU
Sample : 02059-01DL2 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG0DL2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:51:46 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

