




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

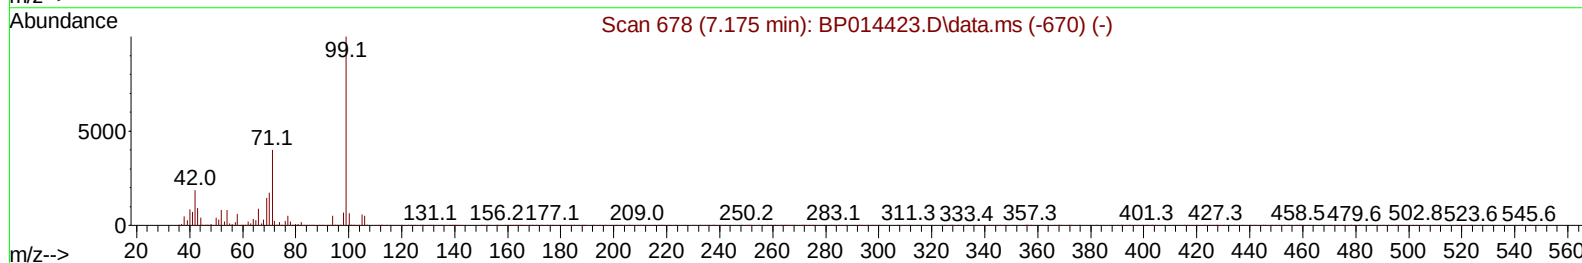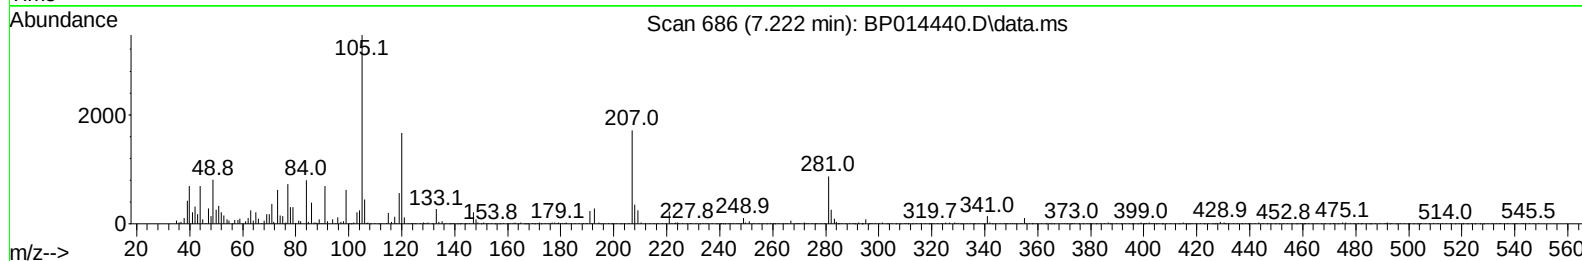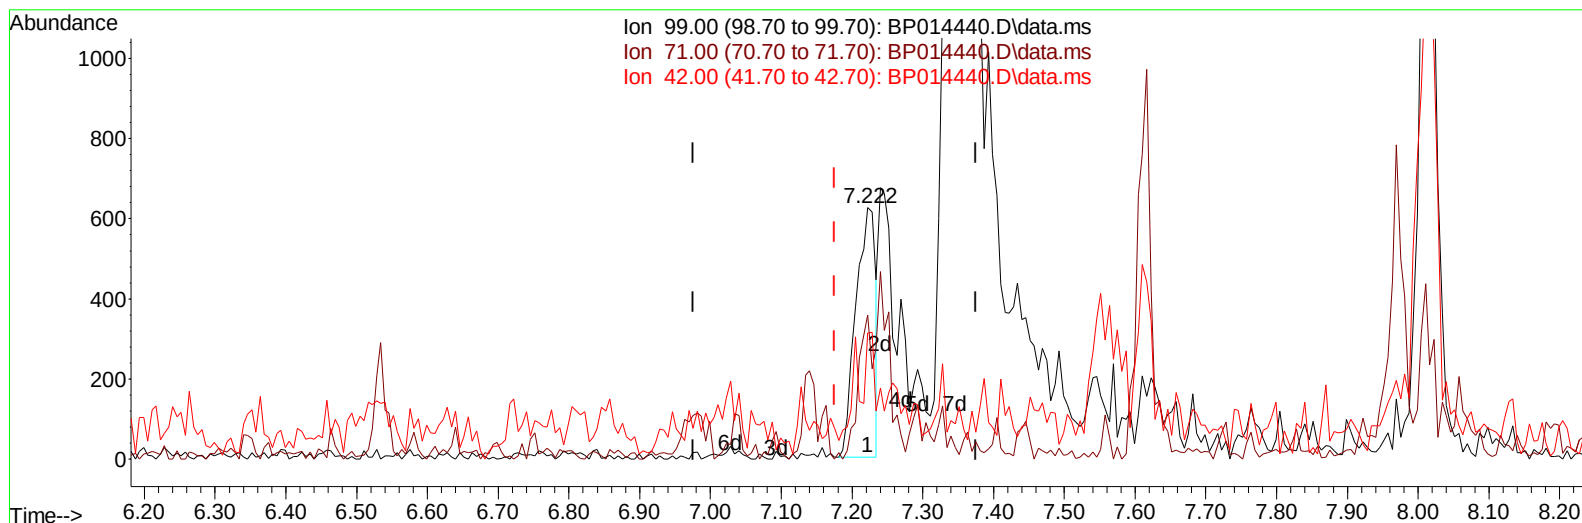

TIC: BP014440.D\data.ms

(7) Phenol-d5 (S)

7.222min (+ 0.047) 0.09 ng/ul

response 1203

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	40.30	57.42#
42.00	18.90	50.24#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

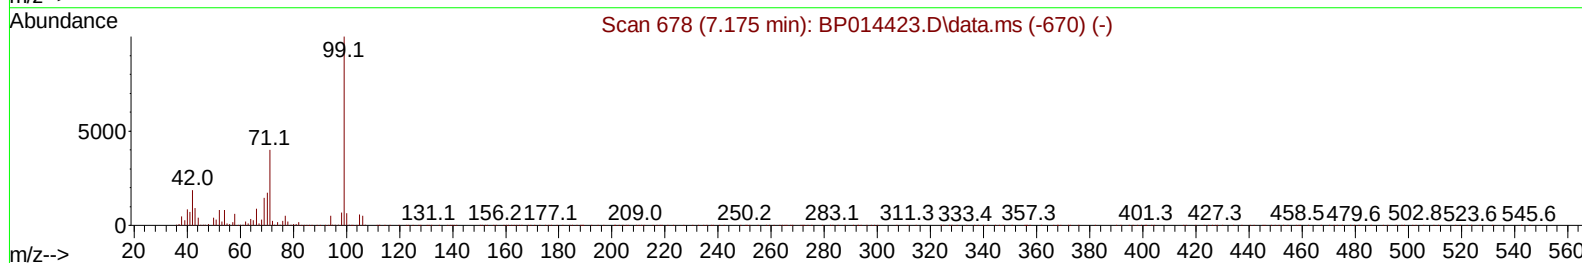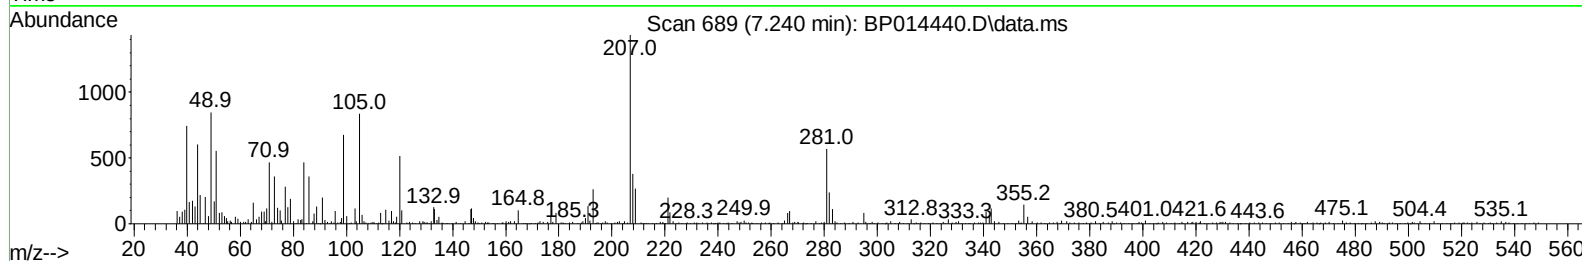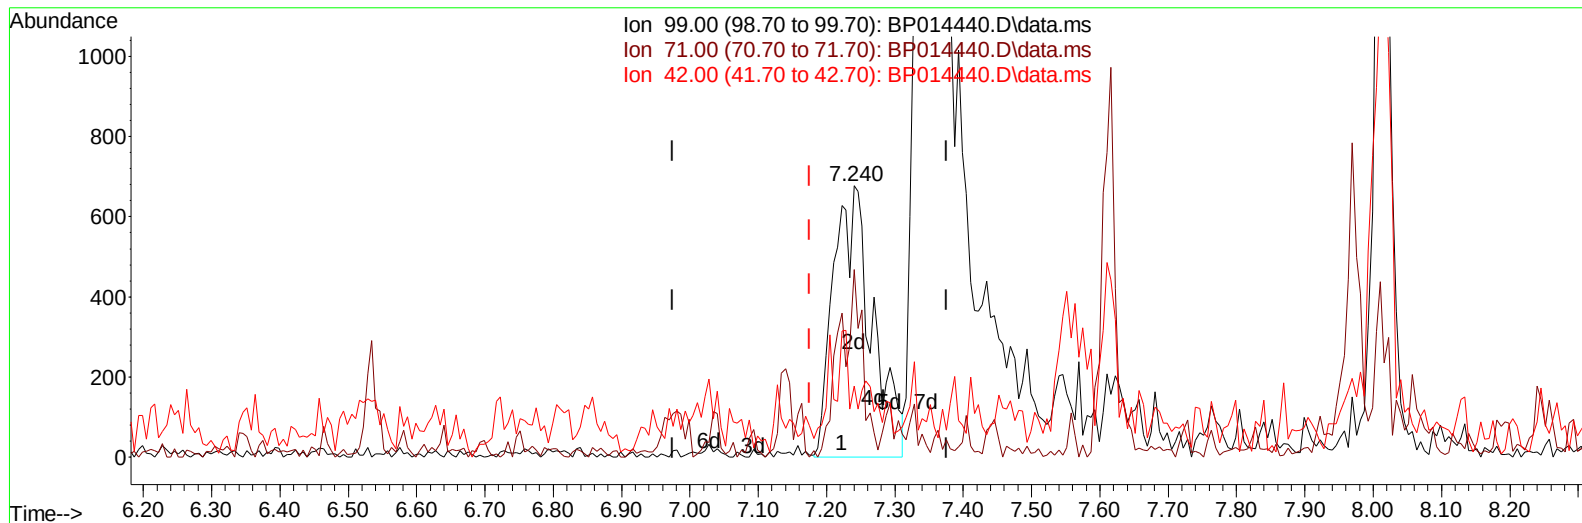

TIC: BP014440.D\data.ms

(7) Phenol-d5 (S)

7.240min (+ 0.065) 0.19 ng/ul m

response 2674

Ion	Exp%	Act%
99.00	100.00	100.00
71.00	40.30	69.13#
42.00	18.90	26.14#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

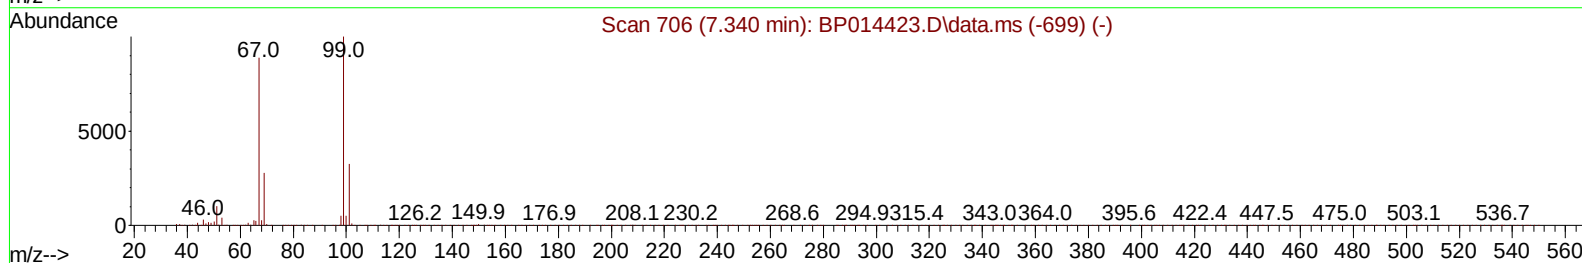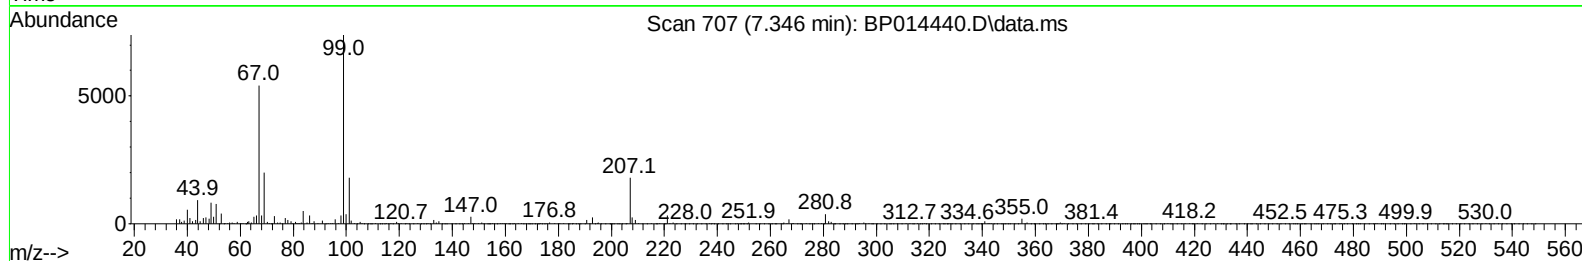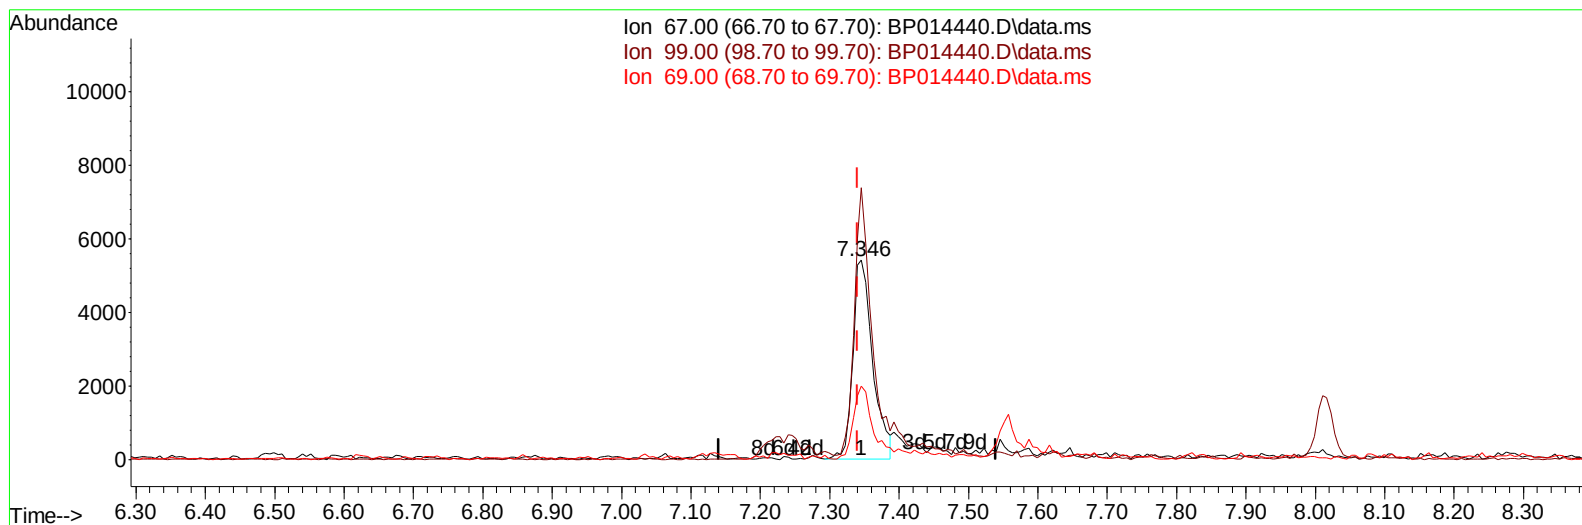

TIC: BP014440.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.346min (+ 0.006) 1.19 ng/u1

response 10755

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.40	136.33
69.00	32.60	36.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

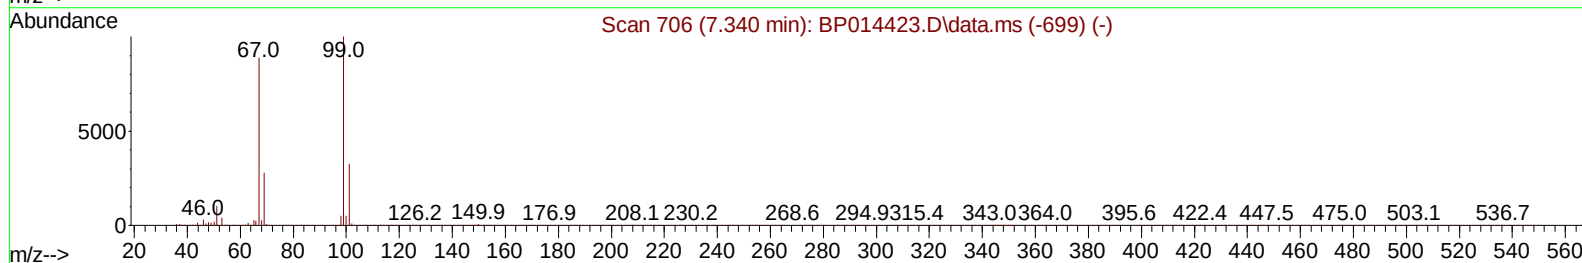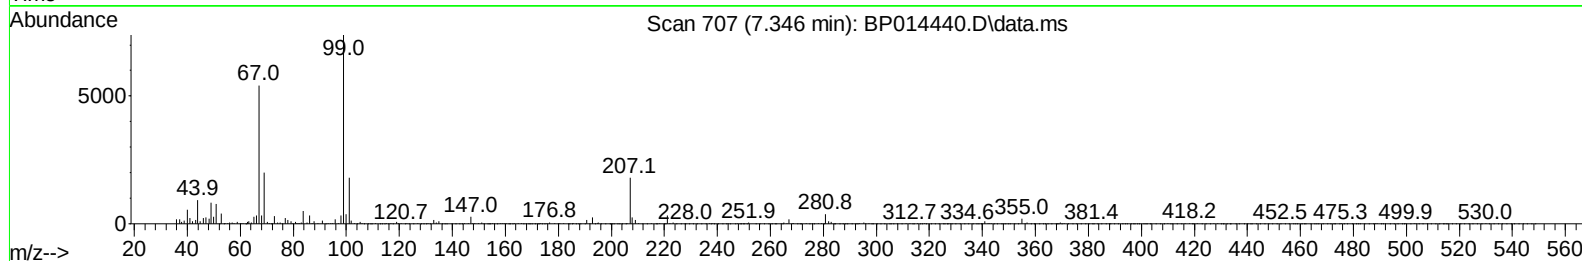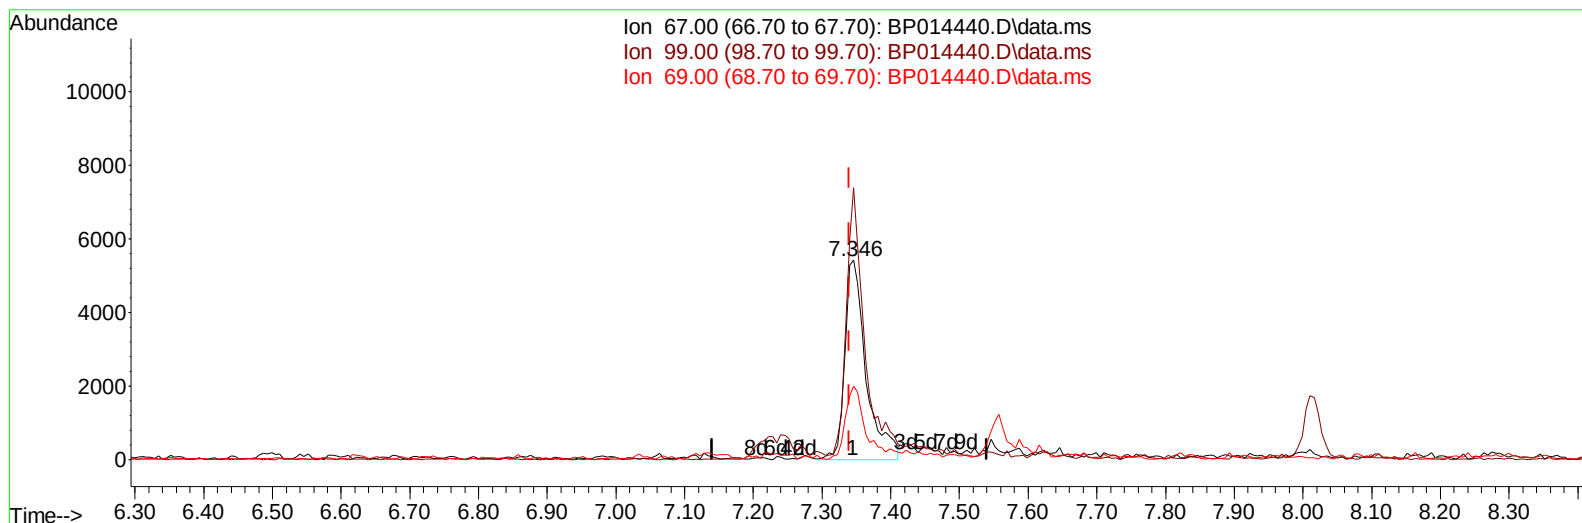

TIC: BP014440.D\data.ms

(9) Bis-(2-Chloroethyl)ether-d8 (S)

7.346min (+ 0.006) 1.28 ng/ul m

response 11578

Ion	Exp%	Act%
67.00	100.00	100.00
99.00	117.40	136.33
69.00	32.60	36.77
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

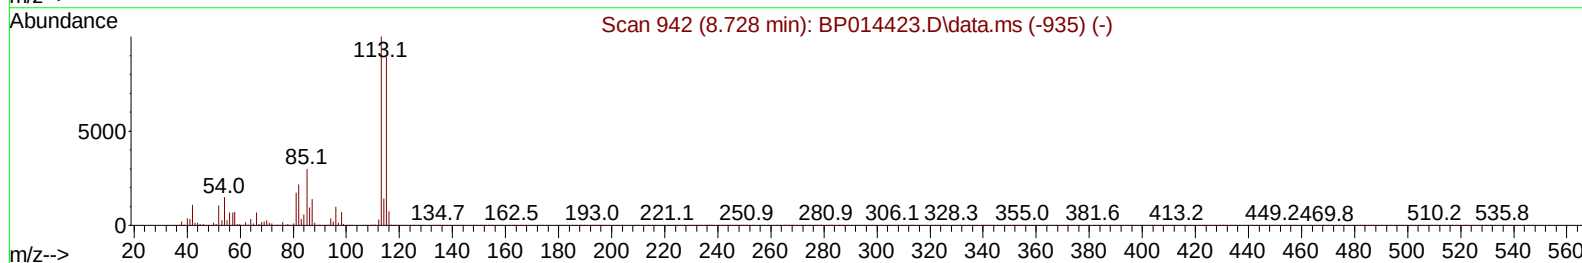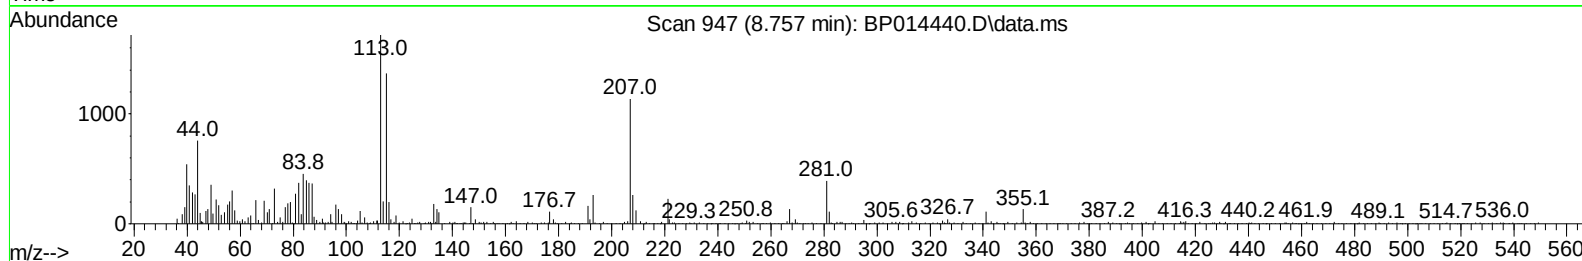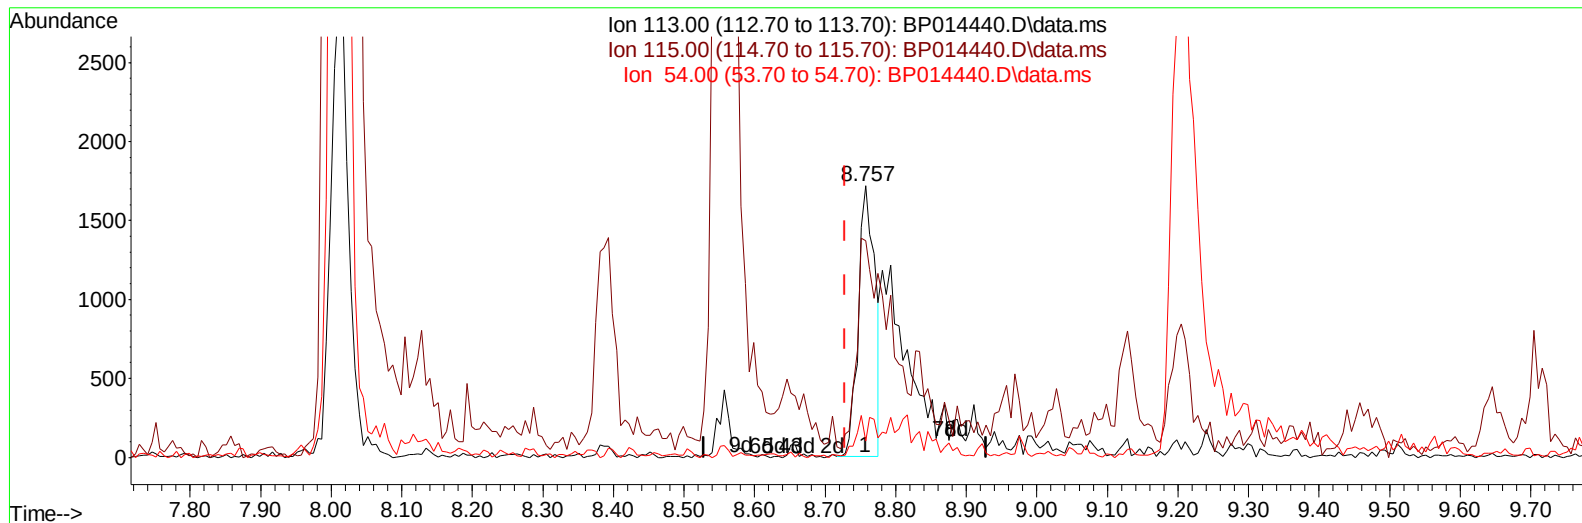

TIC: BP014440.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.757min (+ 0.029) 0.25 ng/uL

response 2819

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	79.76
54.00	15.10	6.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

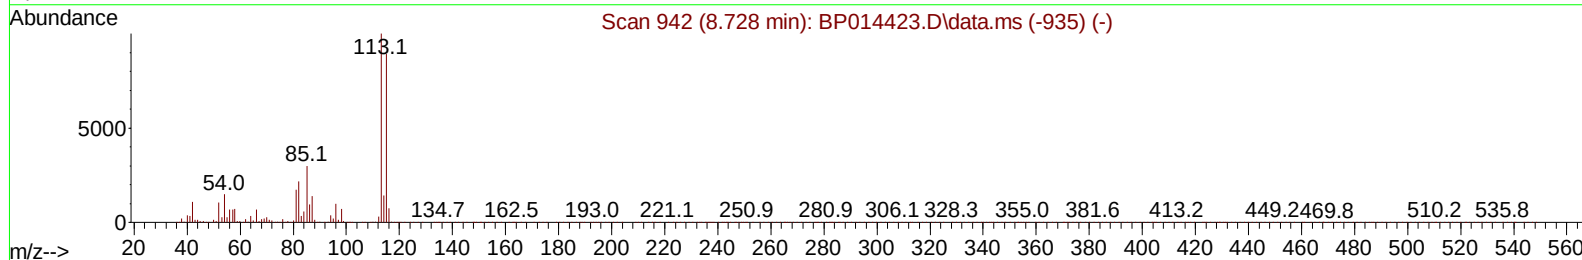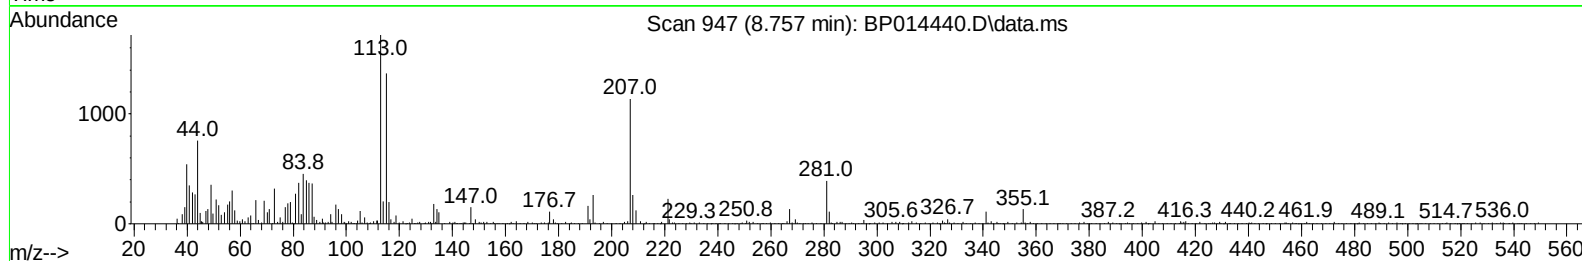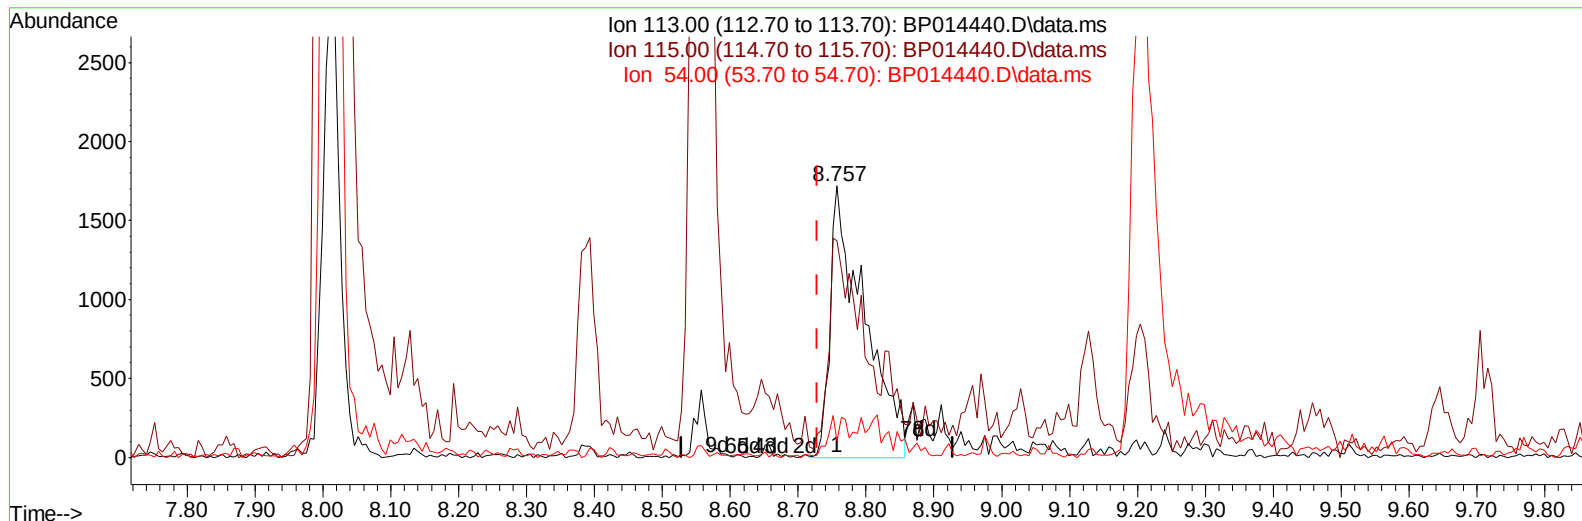

TIC: BP014440.D\data.ms

(15) 4-Methylphenol-d8 (S)

8.757min (+ 0.029) 0.53 ng/ul m

response 5984

Ion	Exp%	Act%
113.00	100.00	100.00
115.00	89.90	79.76
54.00	15.10	6.11#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

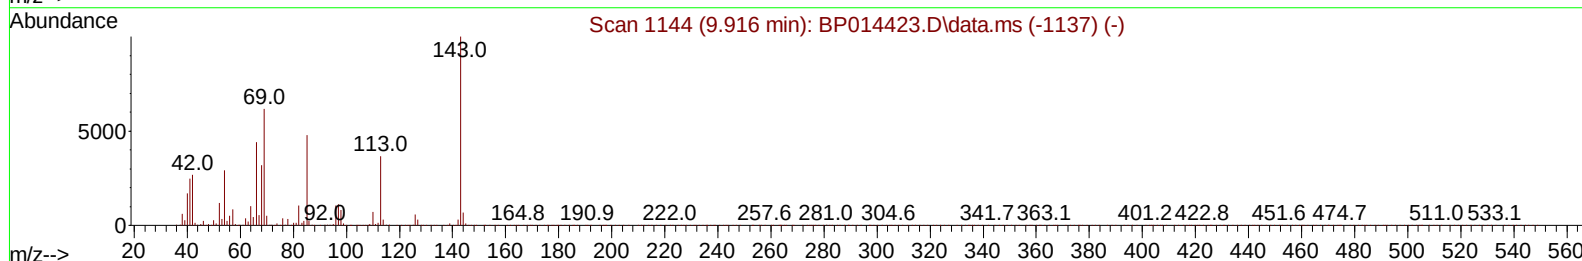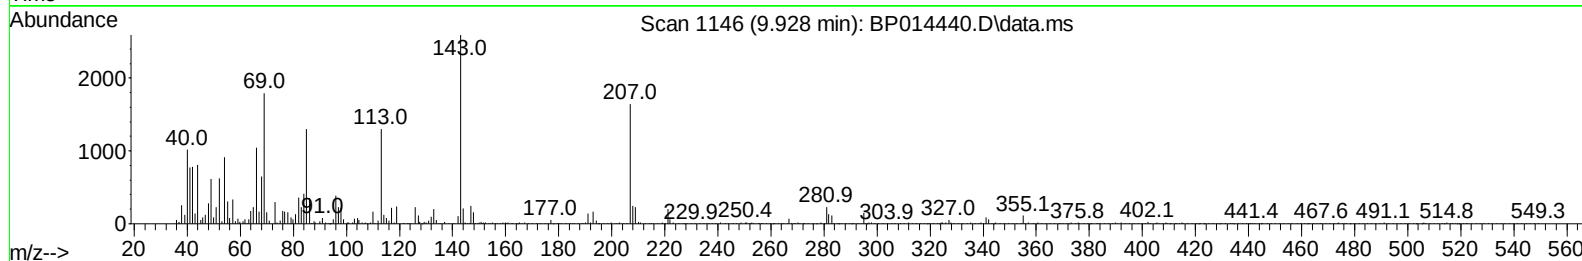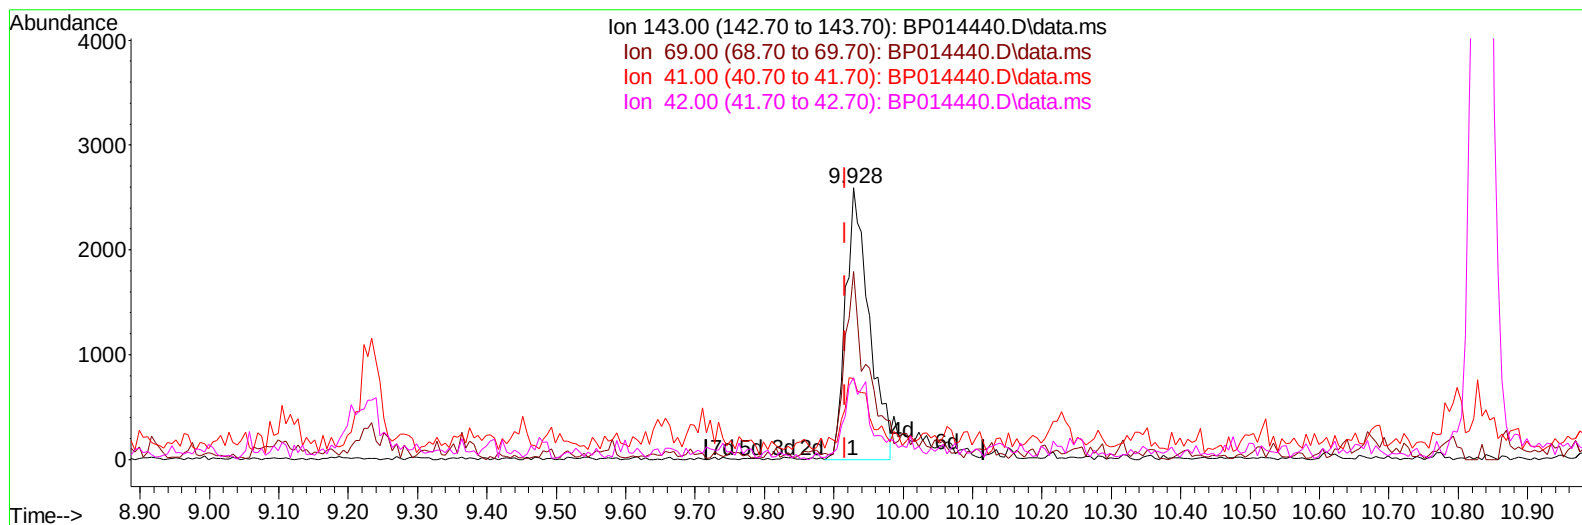

TIC: BP014440.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.928min (+ 0.012) 0.94 ng/ul

response 6109

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.40	69.16
41.00	24.10	29.76#
42.00	25.90	30.14




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

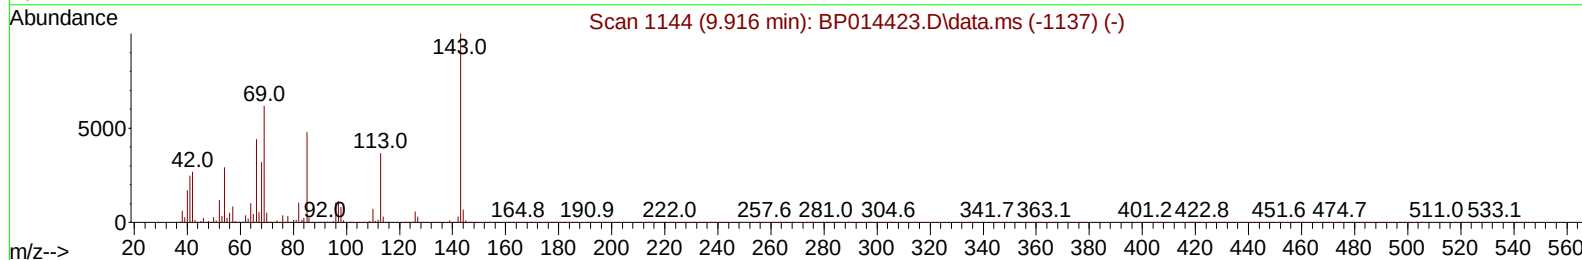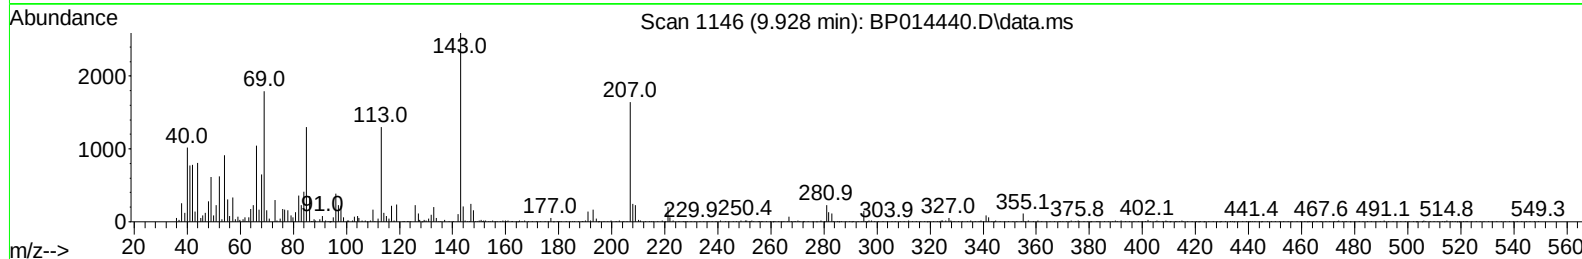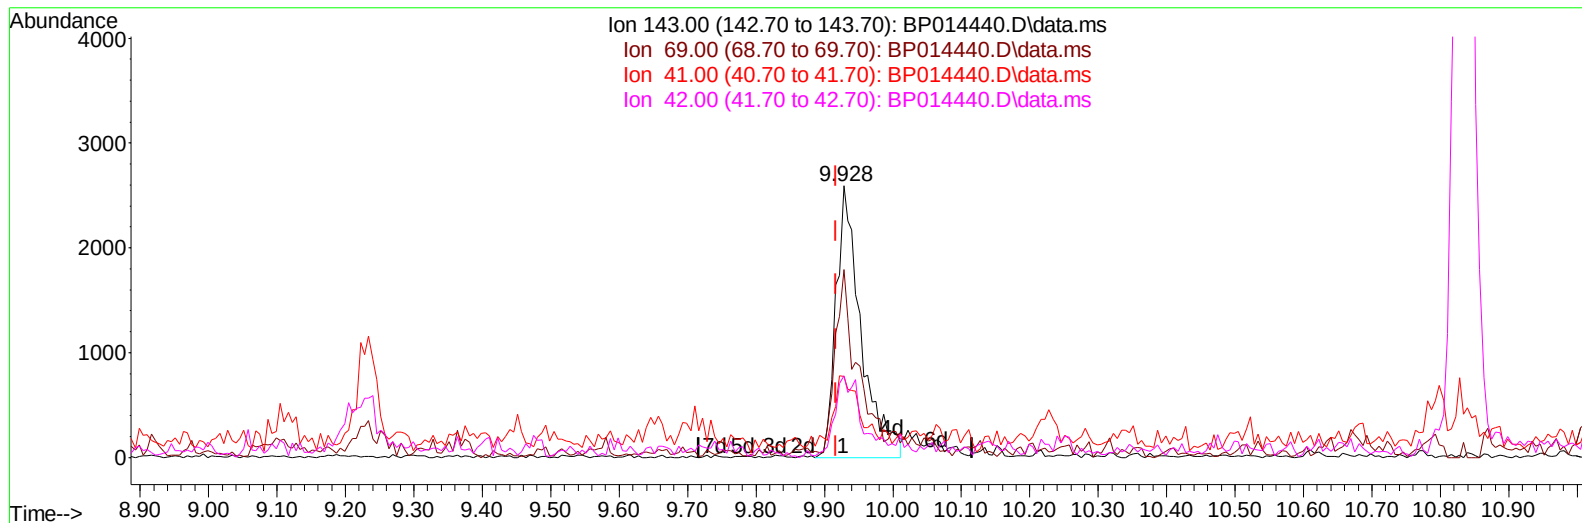

TIC: BP014440.D\data.ms

(24) 2-Nitrophenol-d4 (S)

9.928min (+ 0.012) 1.01 ng/ul m

response 6560

Ion	Exp%	Act%
143.00	100.00	100.00
69.00	62.40	69.16
41.00	24.10	29.76#
42.00	25.90	30.14




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

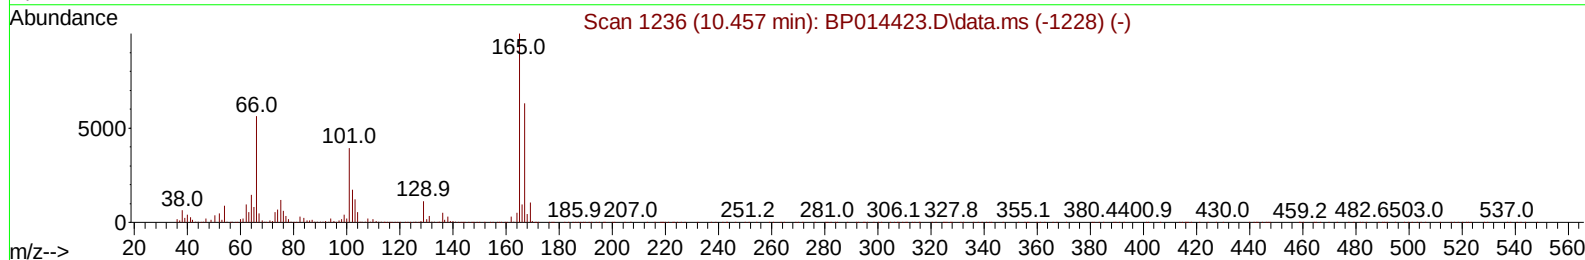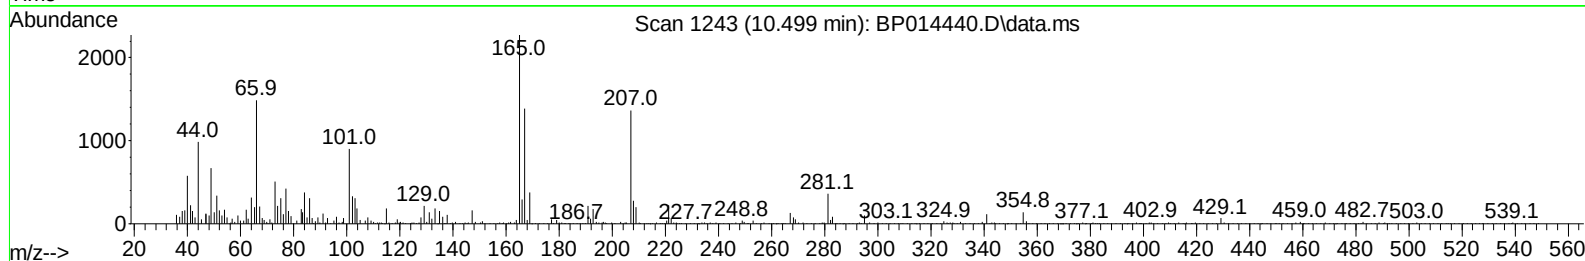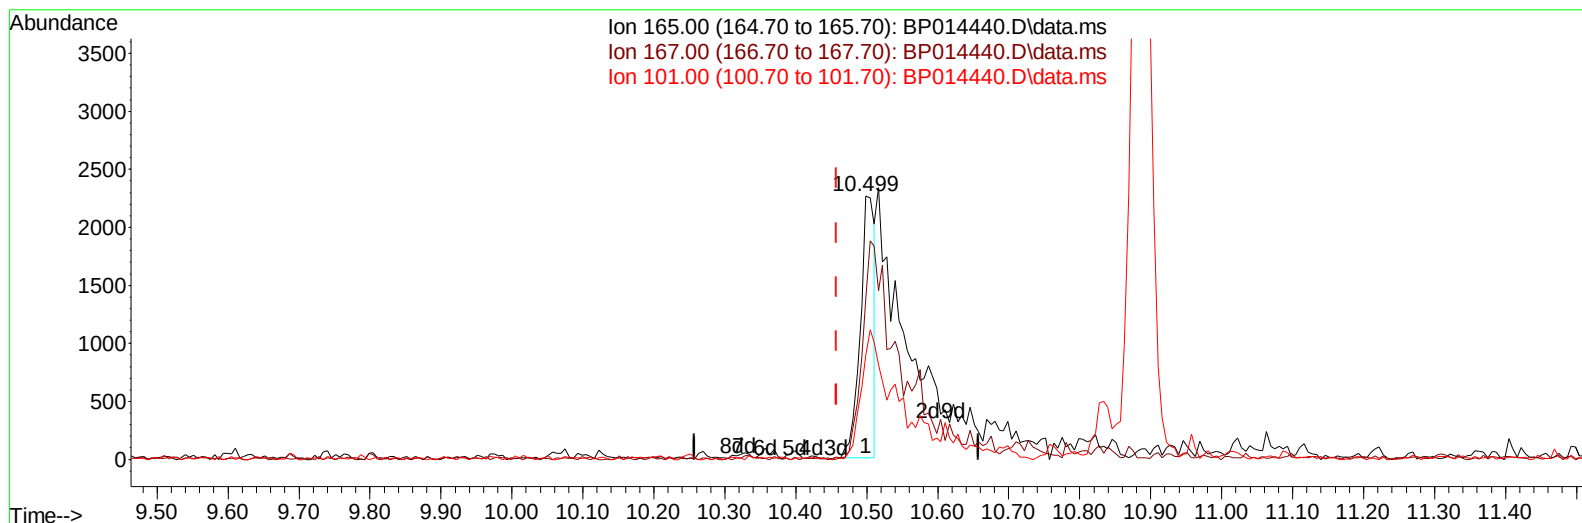

TIC: BP014440.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.499min (+ 0.041) 0.27 ng/ul

response 3209

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	60.93
101.00	39.20	39.55
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

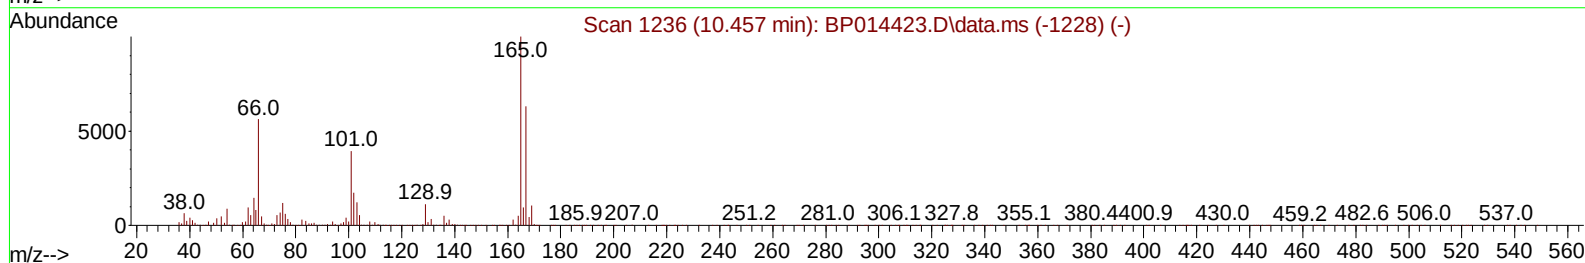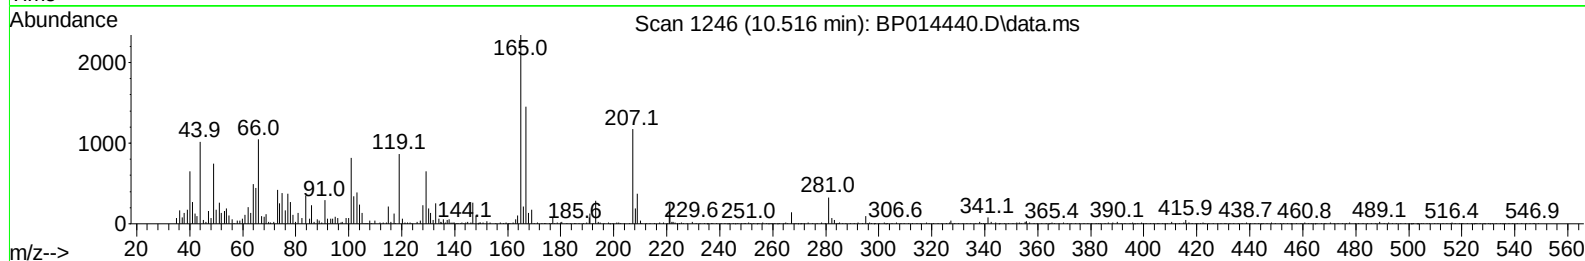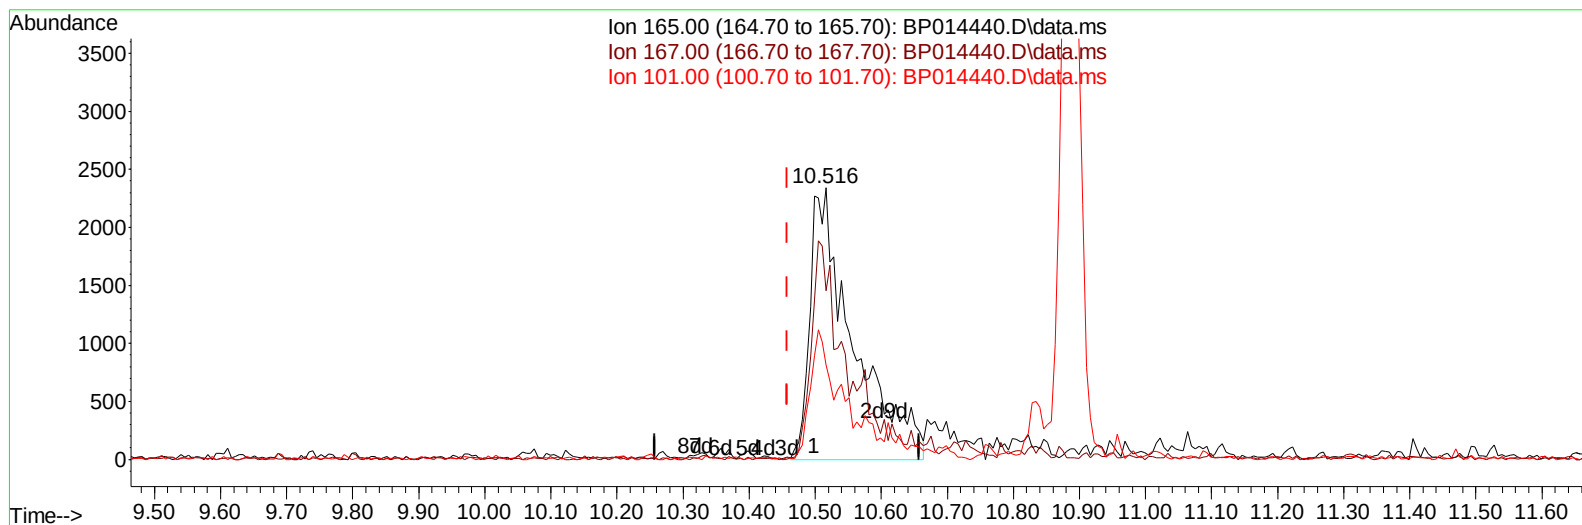

TIC: BP014440.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.516min (+ 0.059) 0.89 ng/ul m

response 10564

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	64.80	62.05
101.00	39.20	34.79
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

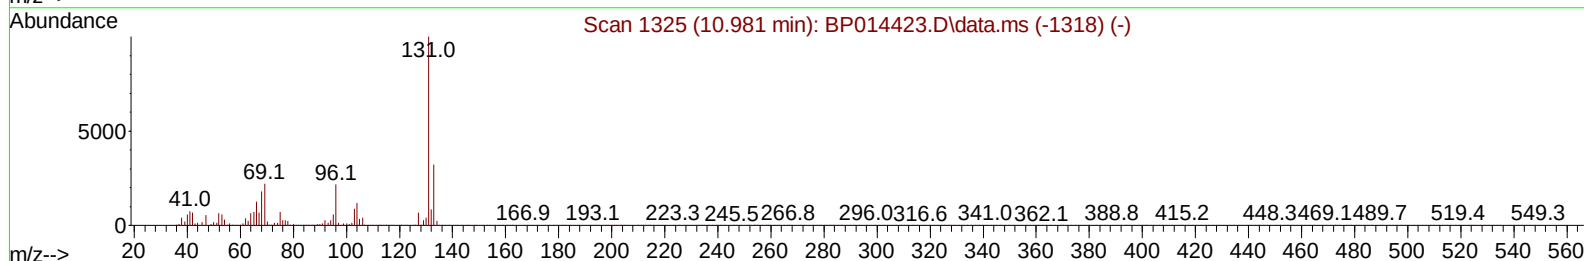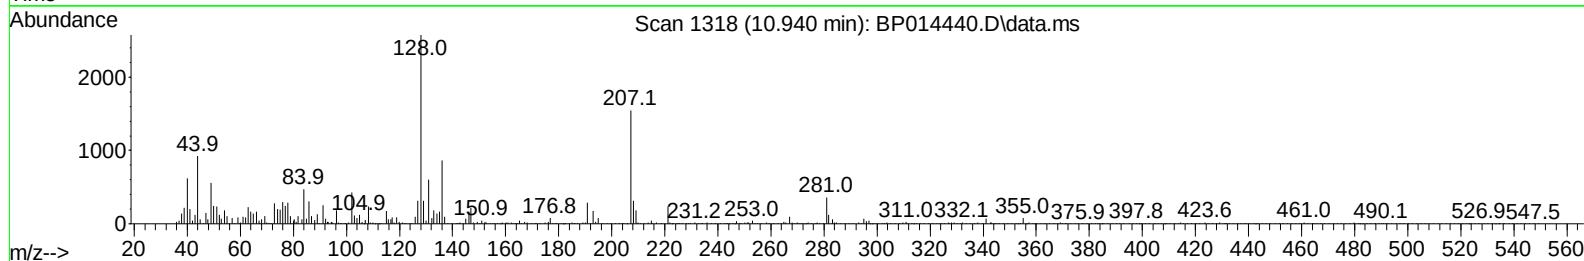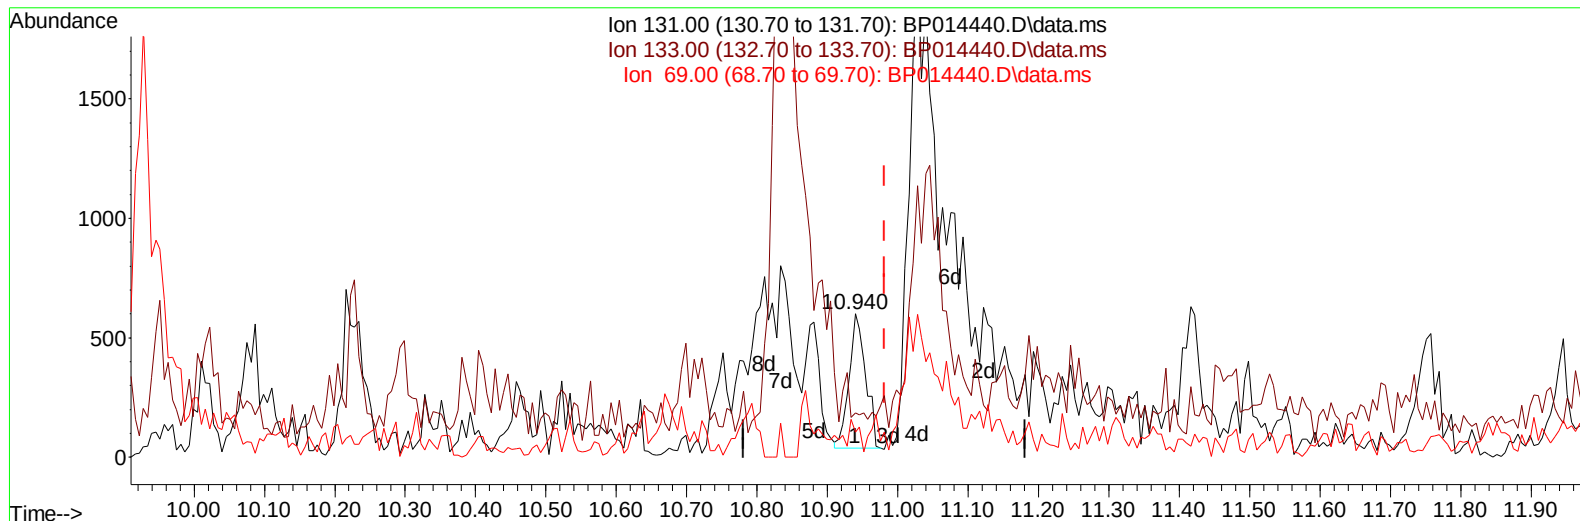

TIC: BP014440.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.940min (-0.041) 0.06 ng/ul

response 912

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	31.06
69.00	21.30	17.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

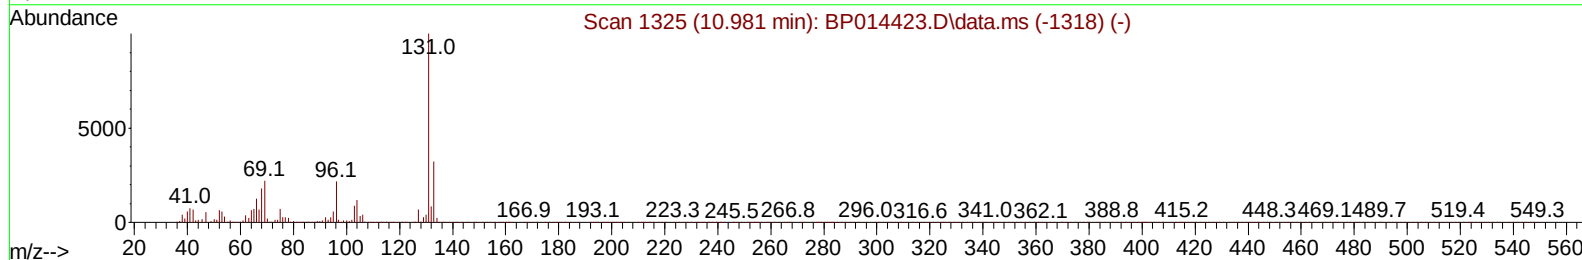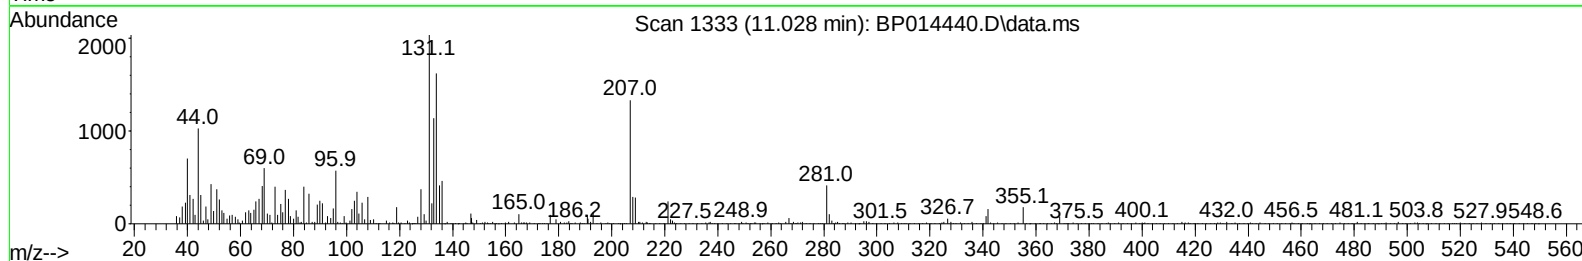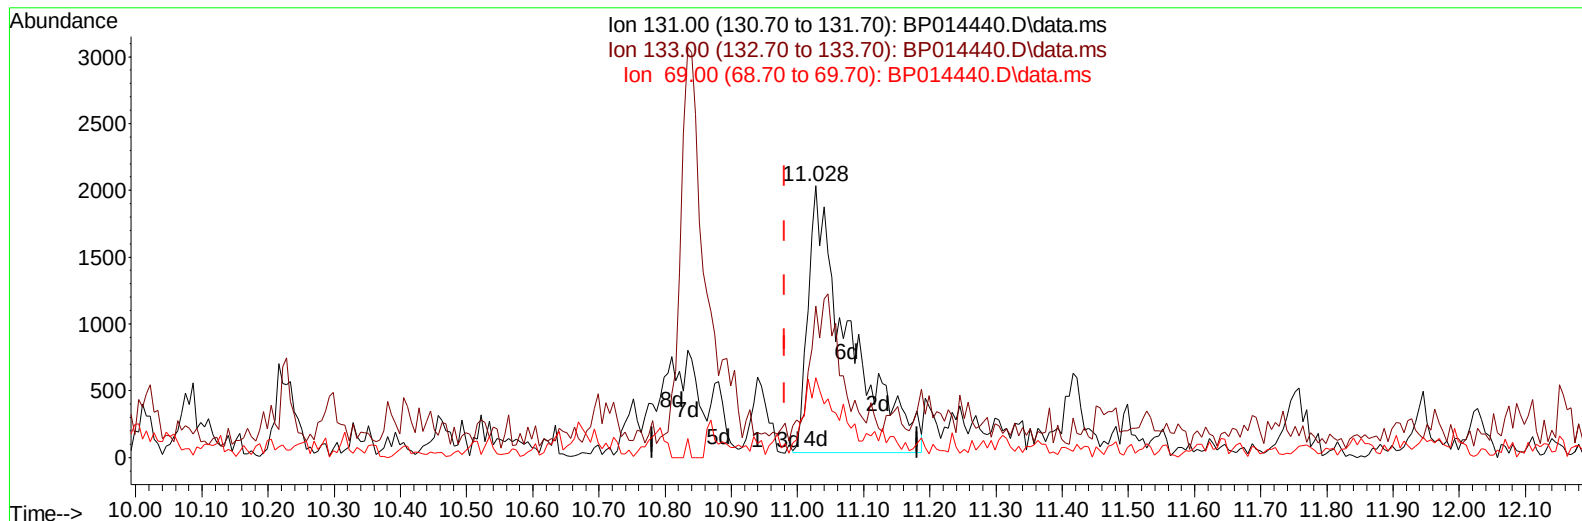

TIC: BP014440.D\data.ms

(31) 4-Chloroaniline-d4 (S)

11.028min (+ 0.047) 0.55 ng/ul m

response 8575

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	55.88#
69.00	21.30	29.41#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

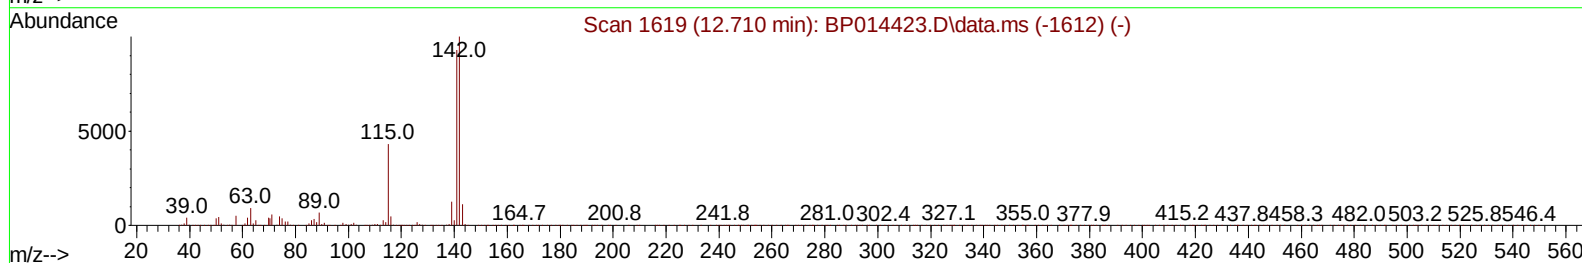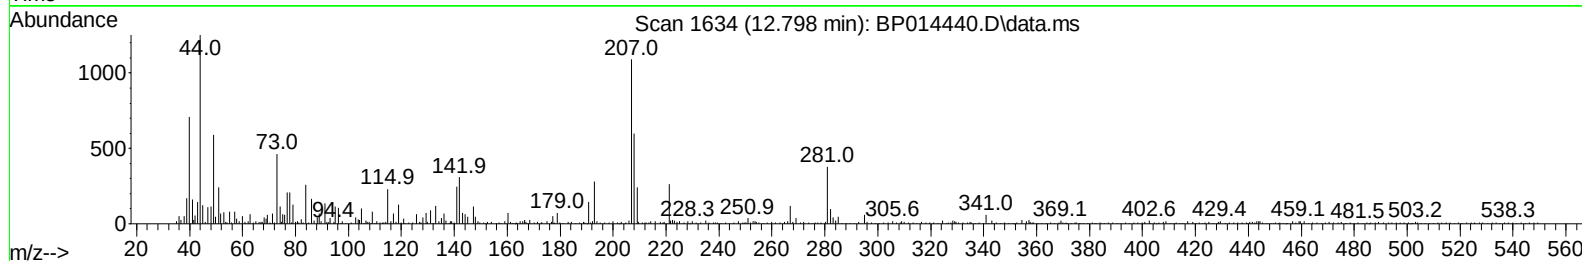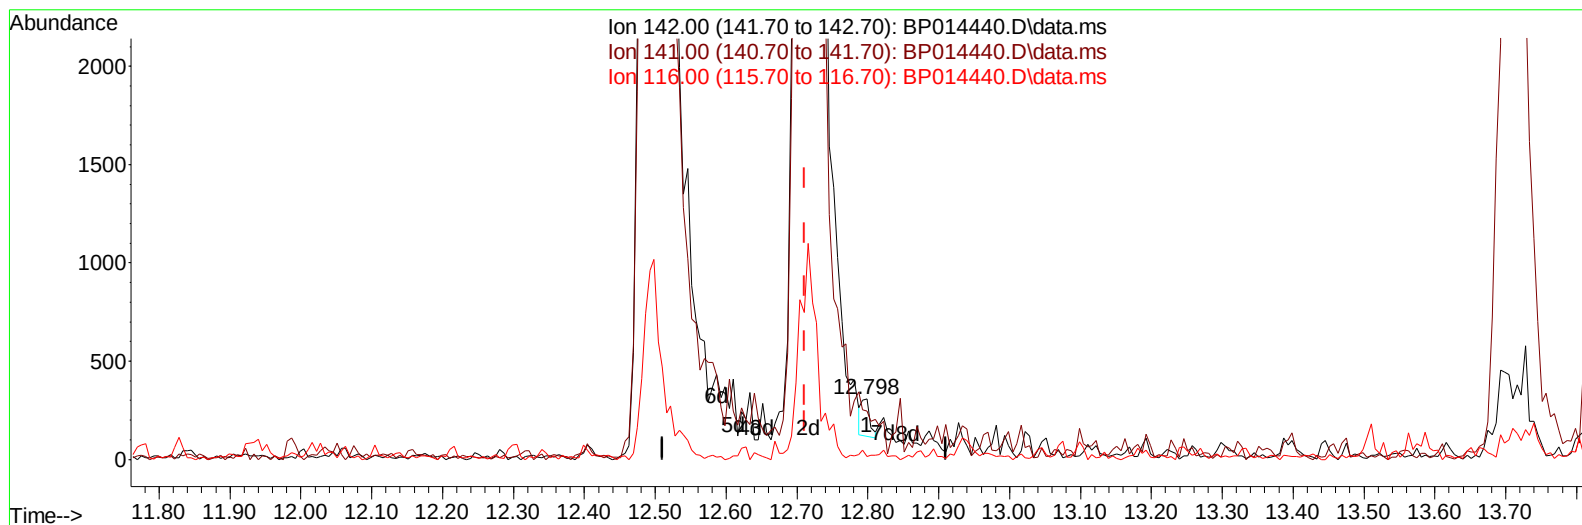

TIC: BP014440.D\data.ms

(37) 1-Methylnaphthalene

12.798min (+ 0.088) 0.01 ng/ul

response 156

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	95.70	79.94
116.00	4.50	4.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :

BNA_P




ClientSampleId :

C0QG7DL2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

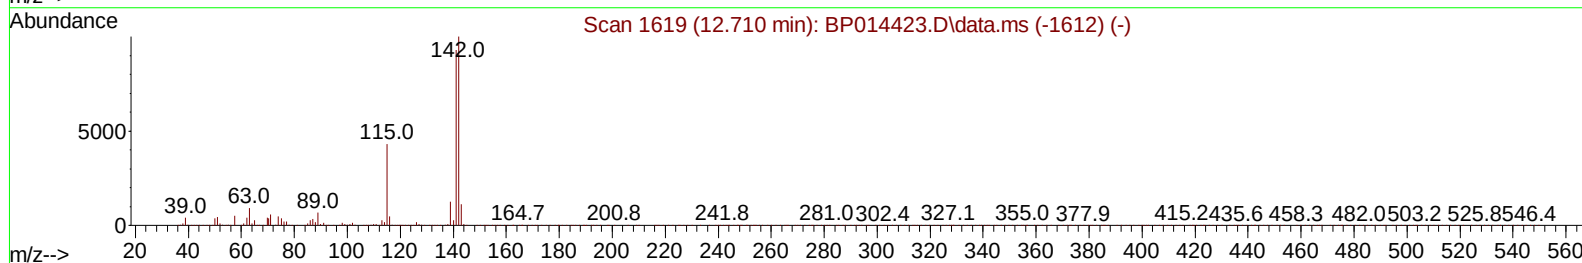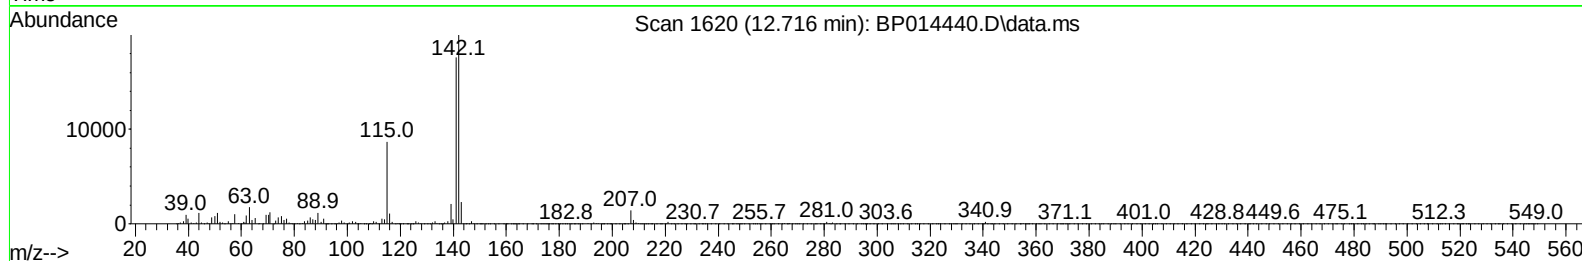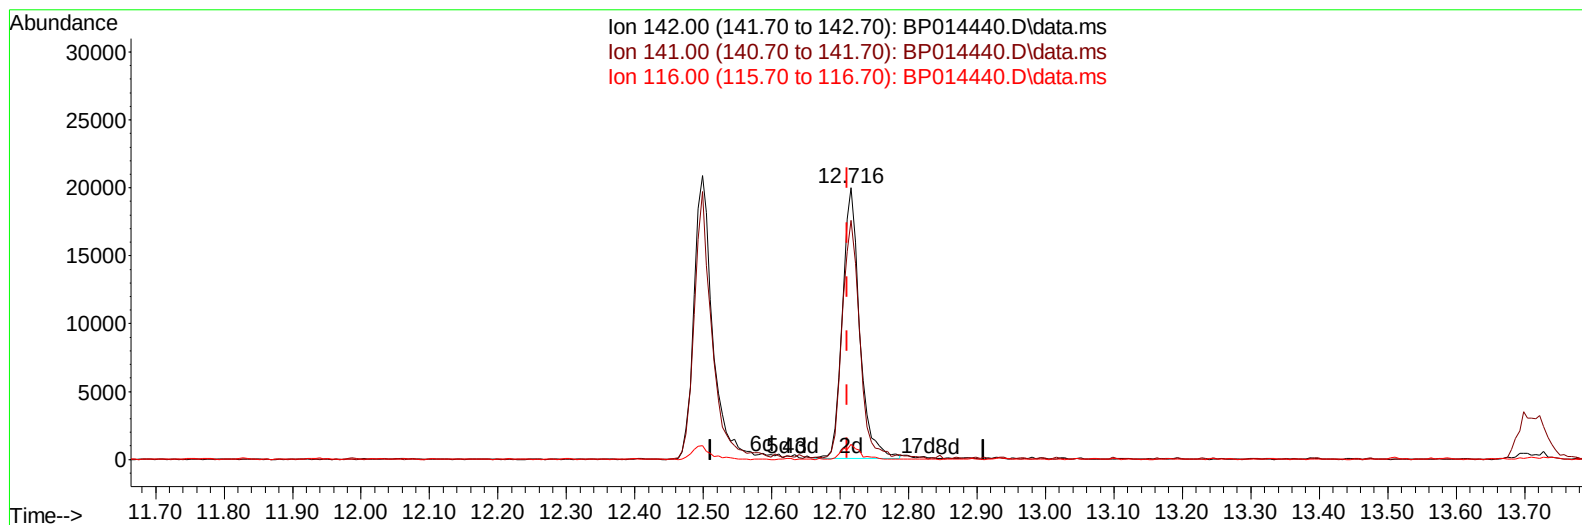

TIC: BP014440.D\data.ms

(37) 1-Methylnaphthalene

12.716min (+ 0.006) 1.32 ng/ul m

response 34718

Ion	Exp%	Act%
142.00	100.00	100.00
141.00	95.70	88.00
116.00	4.50	5.50#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

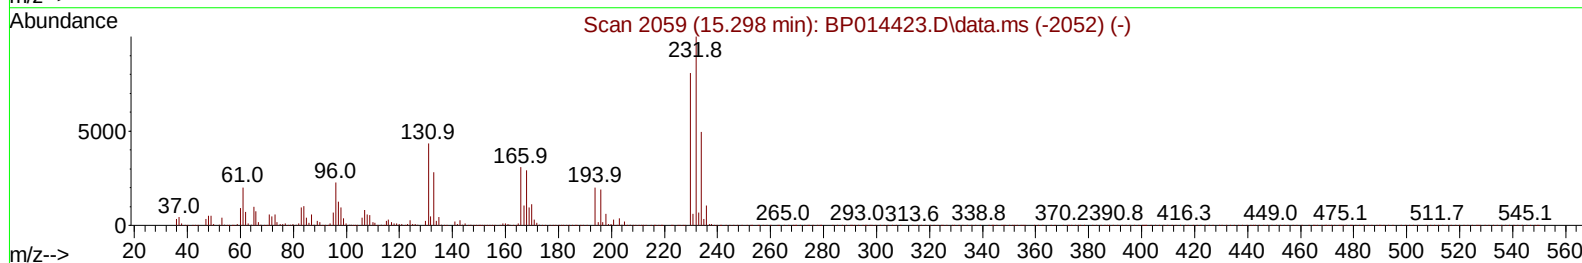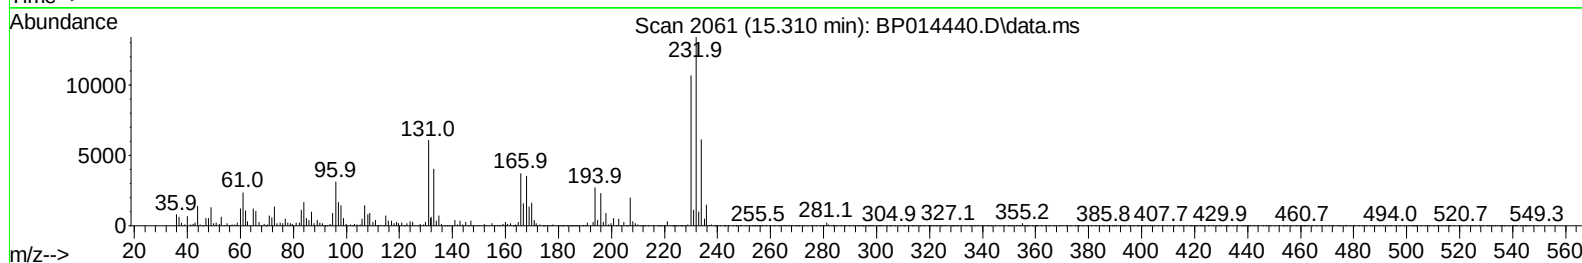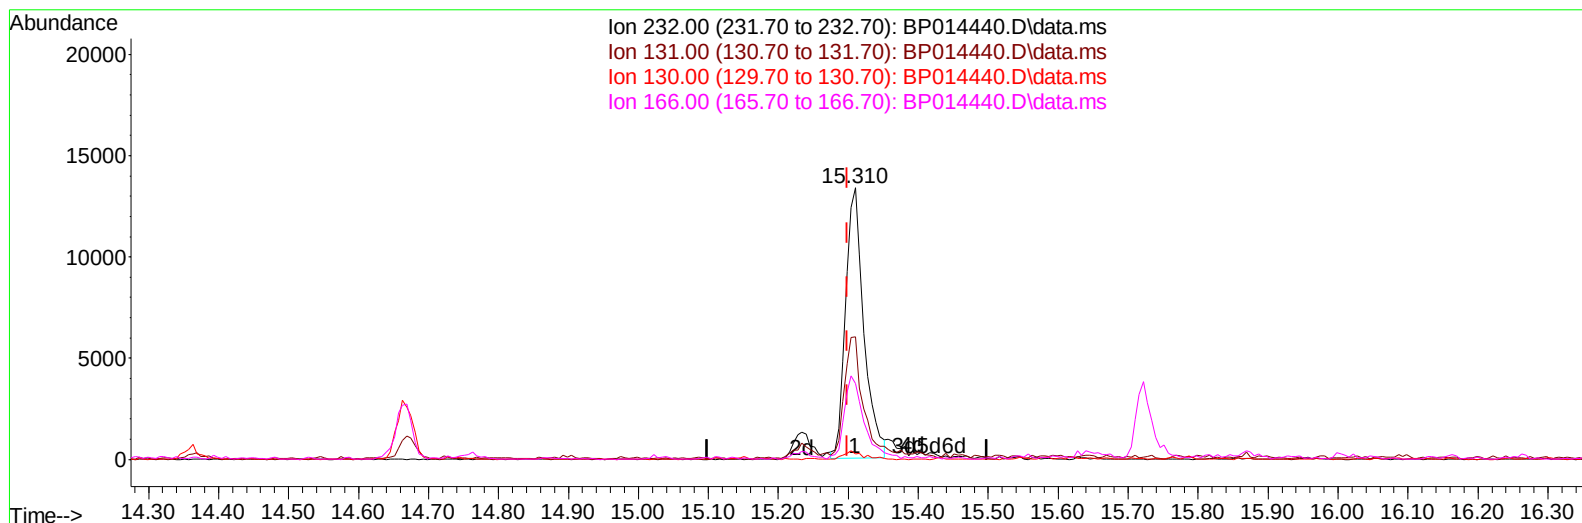

TIC: BP014440.D\data.ms

(58) 2,3,4,6-Tetrachlorophenol

15.310min (+ 0.012) 2.33 ng/ul

response 24008

Ion	Exp%	Act%
232.00	100.00	100.00
131.00	43.70	45.27
130.00	2.40	1.93
166.00	30.10	27.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

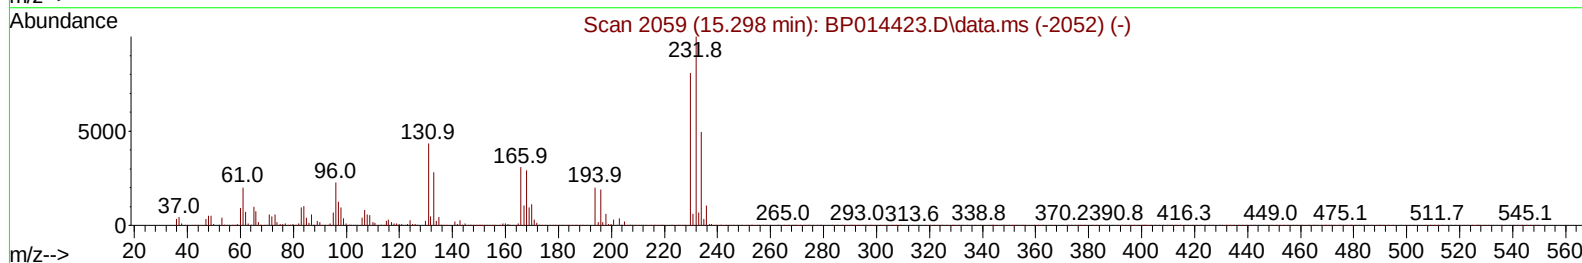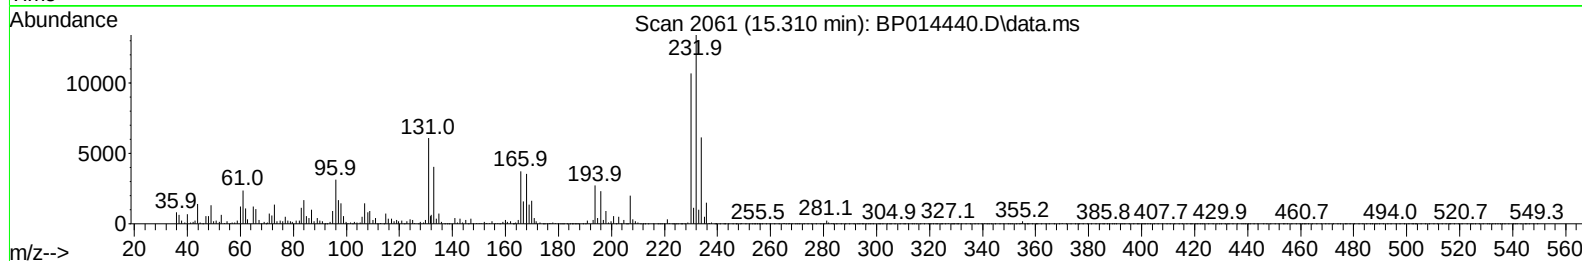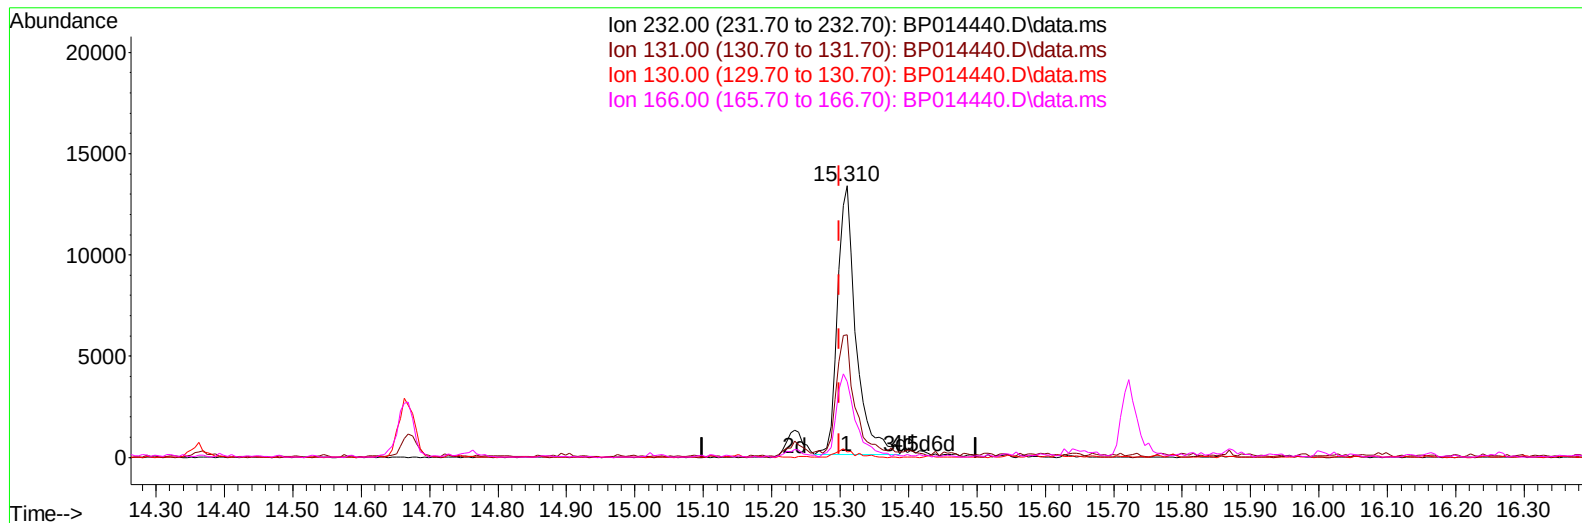

TIC: BP014440.D\data.ms

(58) 2,3,4,6-Tetrachlorophenol

15.310min (+ 0.012) 2.41 ng/ul m

response 24825

Ion	Exp%	Act%
232.00	100.00	100.00
131.00	43.70	45.27
130.00	2.40	1.93
166.00	30.10	27.95




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

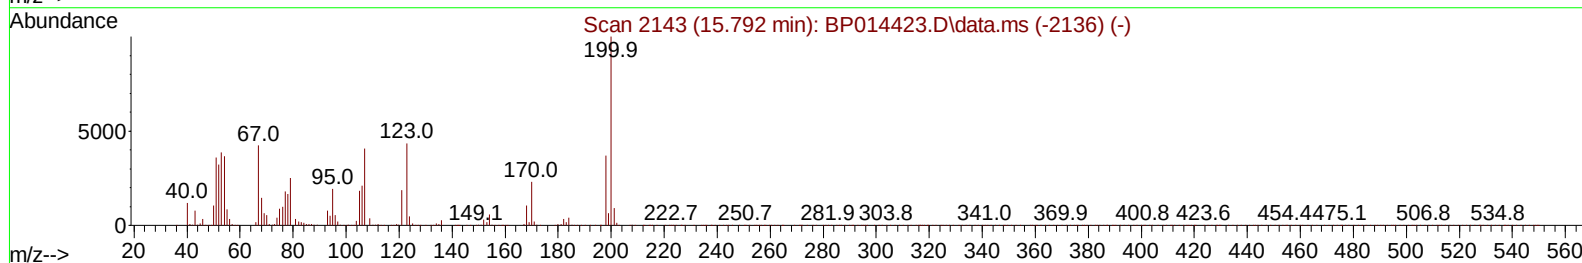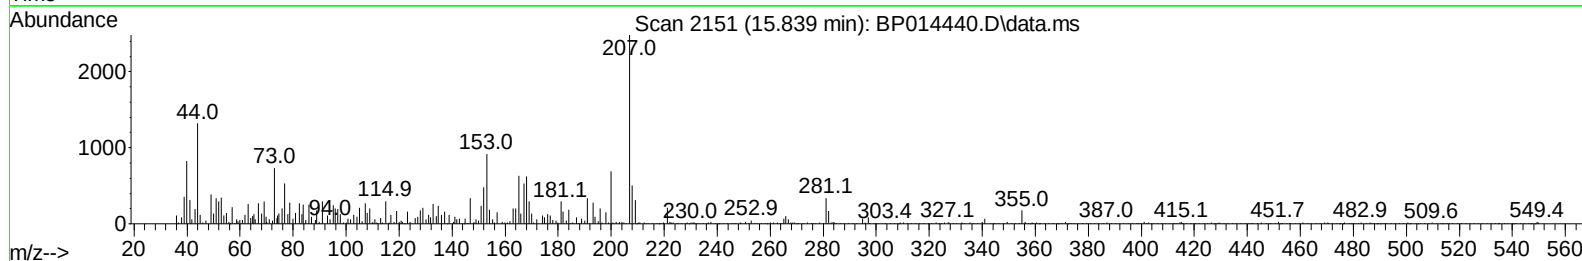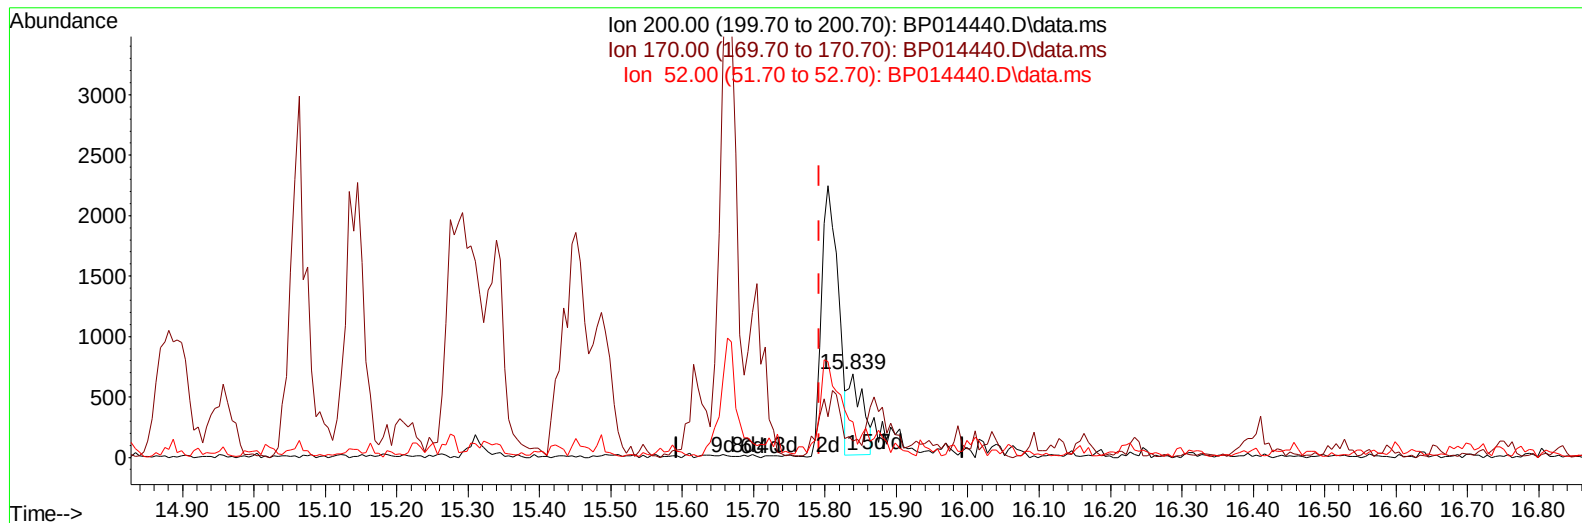

TIC: BP014440.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.839min (+ 0.047) 0.12 ng/ul

response 950

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	19.26
52.00	45.50	41.36
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

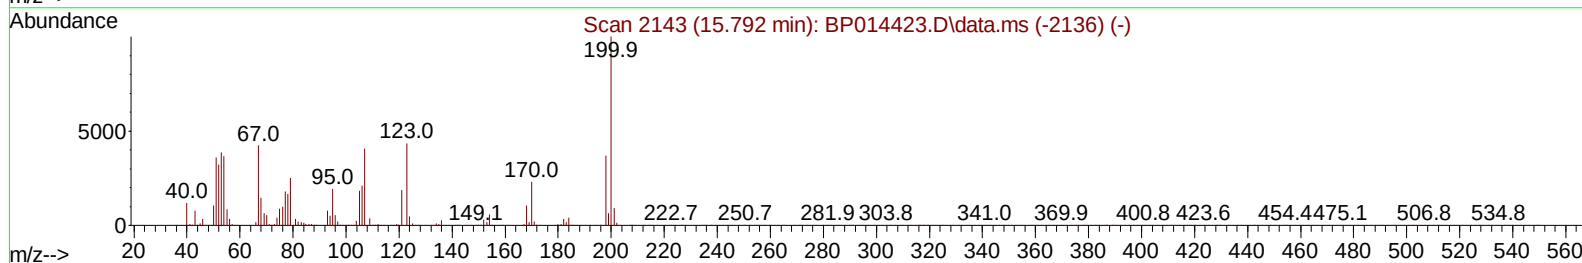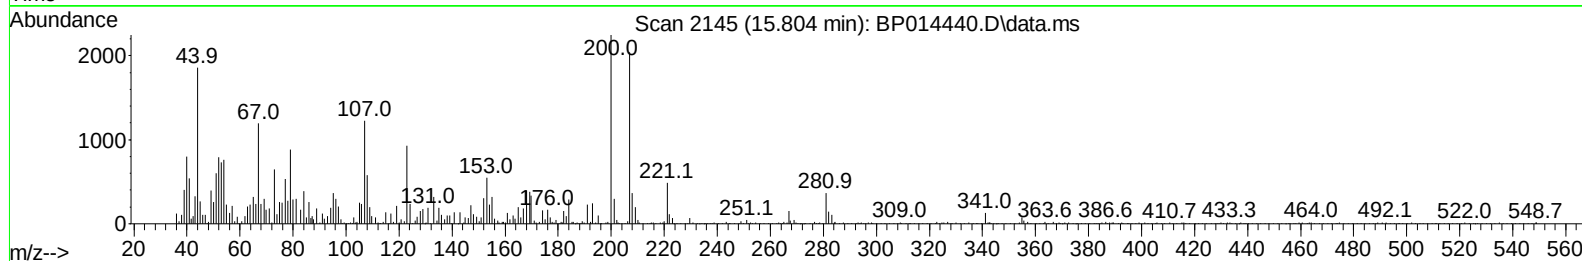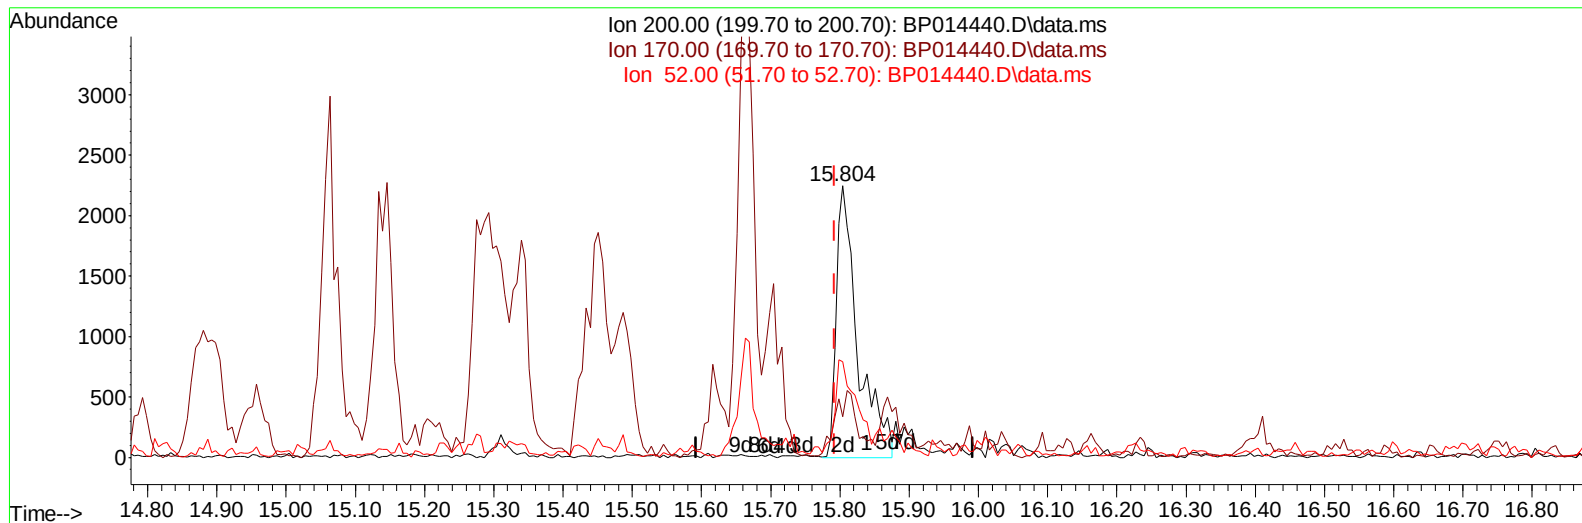

TIC: BP014440.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.804min (+ 0.012) 0.62 ng/ul m

response 4868

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	22.10	14.96#
52.00	45.50	35.31#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014440.D
 Acq On : 31 Mar 2023 13:07
 Operator : CG/JU
 Sample : 02131-02DL2 25X
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0QG7DL2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:53:06 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	152340	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	701358	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	488219	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1063799	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	728616	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	695115	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.393	96	968	0.246	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.240	99	2674m	0.190	ng/ul	0.06
9) Bis-(2-Chloroethyl)eth...	7.346	67	11578m	1.284	ng/ul	0.00
11) 2-Chlorophenol-d4	7.552	132	8983	0.885	ng/ul	0.01
15) 4-Methylphenol-d8	8.757	113	5984m	0.528	ng/ul	0.03
21) Nitrobenzene-d5	9.204	128	5173	0.914	ng/ul	0.01
24) 2-Nitrophenol-d4	9.928	143	6560m	1.012	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.516	165	10564m	0.895	ng/ul	0.06
31) 4-Chloroaniline-d4	11.028	131	8575m	0.551	ng/ul	0.05
46) Dimethylphthalate-d6	14.075	166	59329	1.499	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	57212	1.303	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	15.663	176	50785	1.538	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	4868m	0.622	ng/ul	0.01
73) Anthracene-d10	17.528	188	78612	1.527	ng/ul	0.00
81) Pyrene-d10	19.757	212	79545	1.625	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	53783	1.456	ng/ul	0.00
Target Compounds						
						Qvalue
30) Naphthalene	10.887	128	386806	9.901	ng/ul	98
36) 2-Methylnaphthalene	12.498	142	39703	1.500	ng/ul	95
37) 1-Methylnaphthalene	12.716	142	34718m	1.322	ng/ul	
58) 2,3,4,6-Tetrachlorophenol	15.310	232	24825m	2.409	ng/ul	
71) Pentachlorophenol	17.075	266	465126	52.802	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014440.D
Acq On : 31 Mar 2023 13:07
Operator : CG/JU
Sample : 02131-02DL2 25X
Misc :
ALS Vial : 49 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0QG7DL2

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:53:06 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

