




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014450.D
 Acq On : 31 Mar 2023 18:48
 Operator : CG/JU
 Sample : 02092-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB967

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:55:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

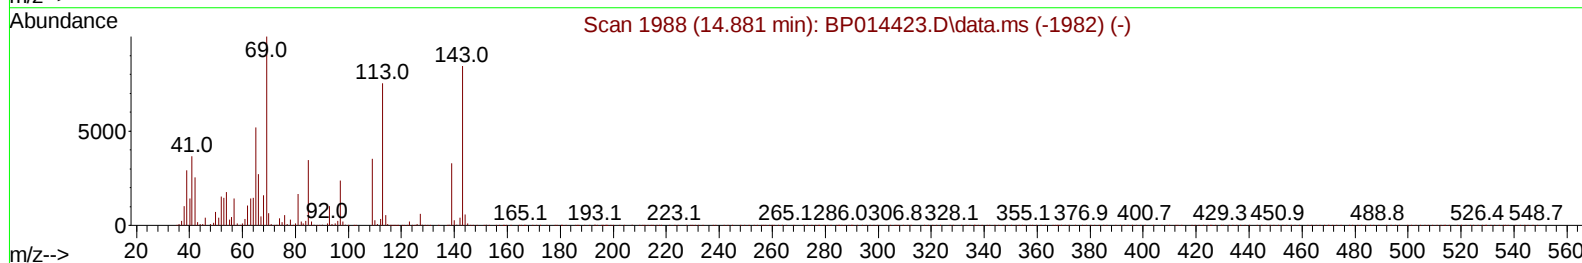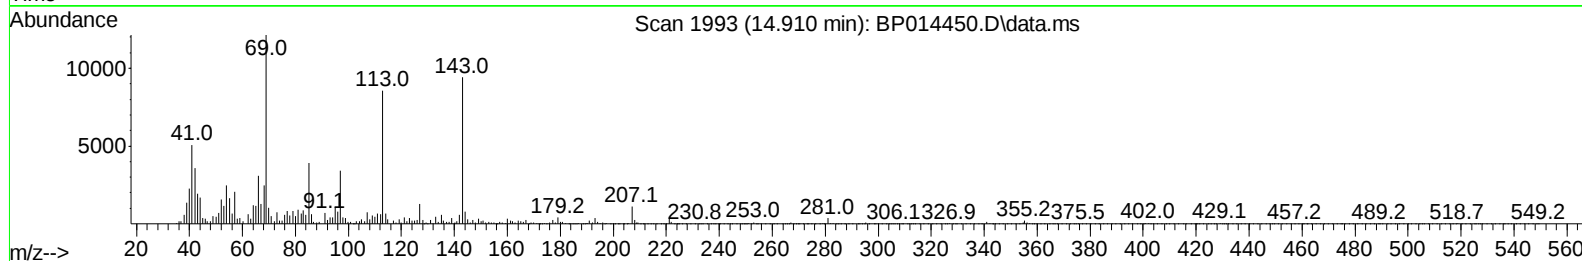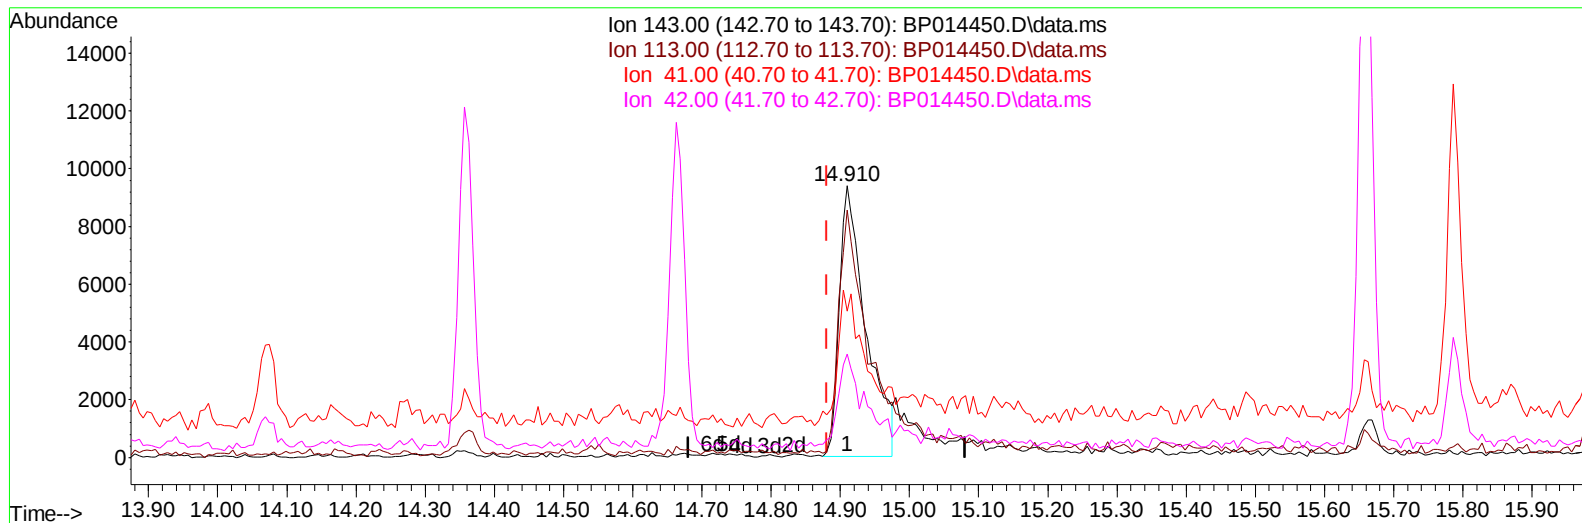

TIC: BP014450.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.029) 4.48 ng/u1

response 24851

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.10
41.00	44.20	53.83#
42.00	31.50	38.01#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014450.D
Acq On : 31 Mar 2023 18:48
Operator : CG/JU
Sample : 02092-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB967

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:55:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

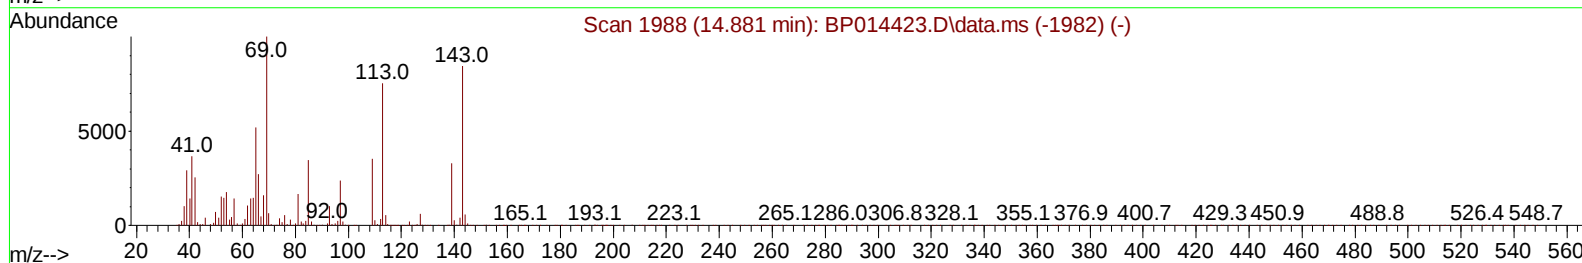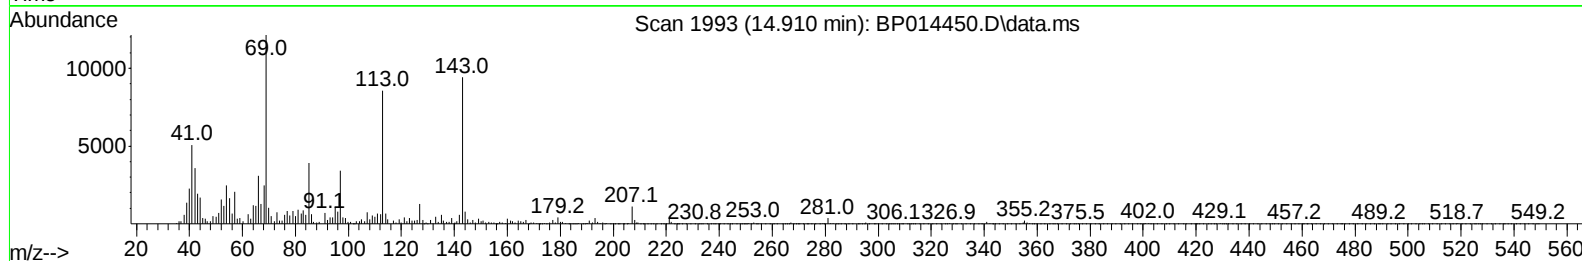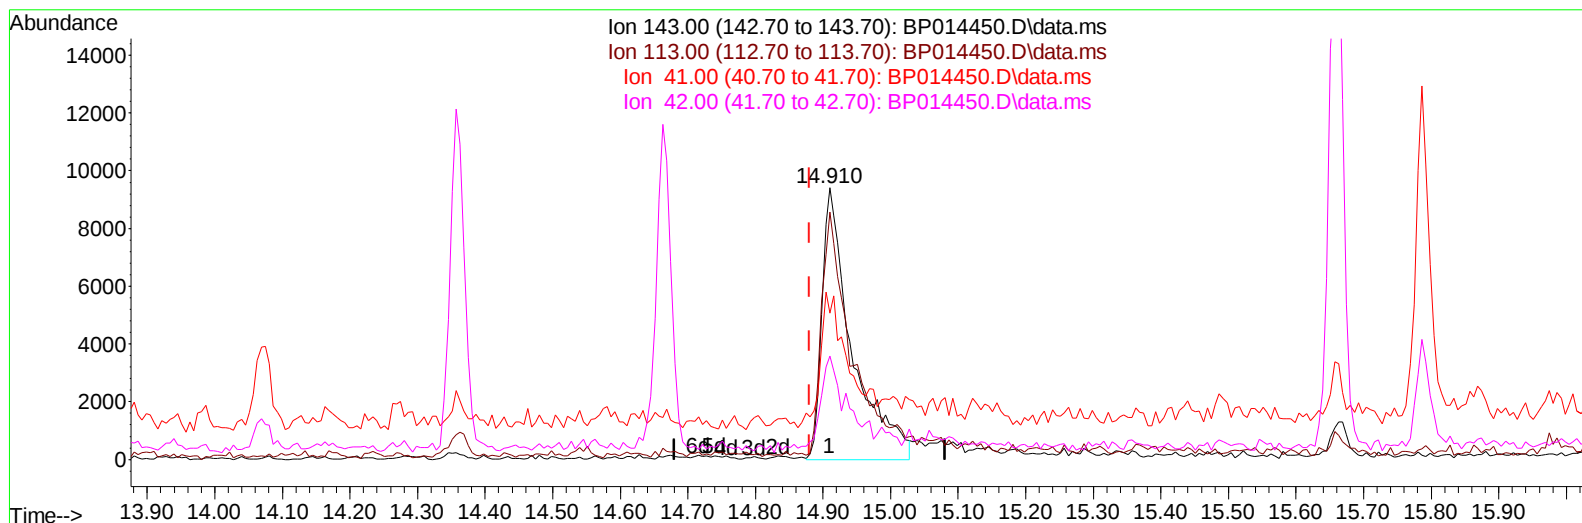

TIC: BP014450.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.029) 5.21 ng/ul m

response 28877

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	91.10
41.00	44.20	53.83#
42.00	31.50	38.01#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014450.D
 Acq On : 31 Mar 2023 18:48
 Operator : CG/JU
 Sample : 02092-05
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB967

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:55:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	188207	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	770205	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	452615	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.427	188	930782	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	934642	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	1087105	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	21028	4.333	ng/uL	0.00
4) Pyridine-d5	3.828	84	84906	6.827	ng/ul	0.01
7) Phenol-d5	7.175	99	108965	6.278	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	324966	29.180	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	289031	23.039	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	205005	14.642	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	183437	29.502	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	204579	28.734	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	329179	25.387	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	167087	9.783	ng/ul	0.00
46) Dimethylphthalate-d6	14.069	166	1158318	31.563	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1263111	31.019	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	28877m	5.209	ng/ul	0.03
60) Fluorene-d10	15.663	176	949706	31.032	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.786	200	176174	25.723	ng/ul	0.00
73) Anthracene-d10	17.528	188	1465364	32.531	ng/ul	0.00
81) Pyrene-d10	19.757	212	1746128	27.814	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	1901198	32.917	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014450.D
Acq On : 31 Mar 2023 18:48
Operator : CG/JU
Sample : 02092-05
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB967

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:55:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

