




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014451.D
Acq On : 31 Mar 2023 19:22
Operator : CG/JU
Sample : 02093-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB967

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:55:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

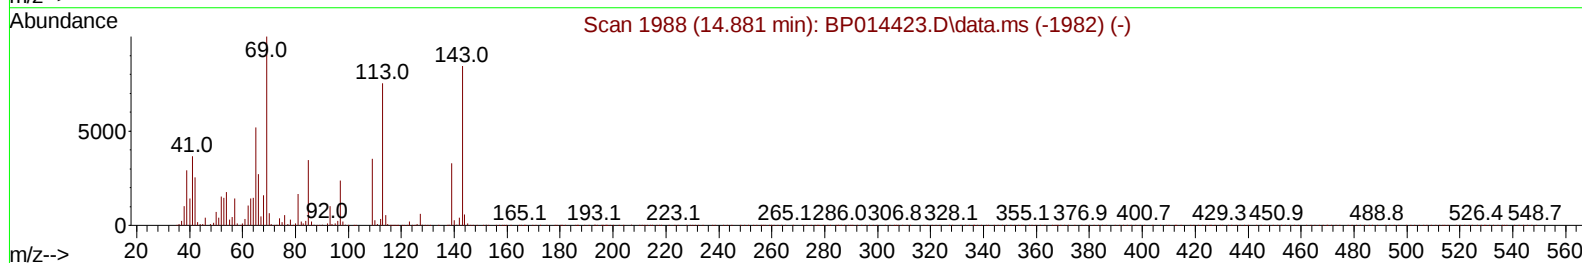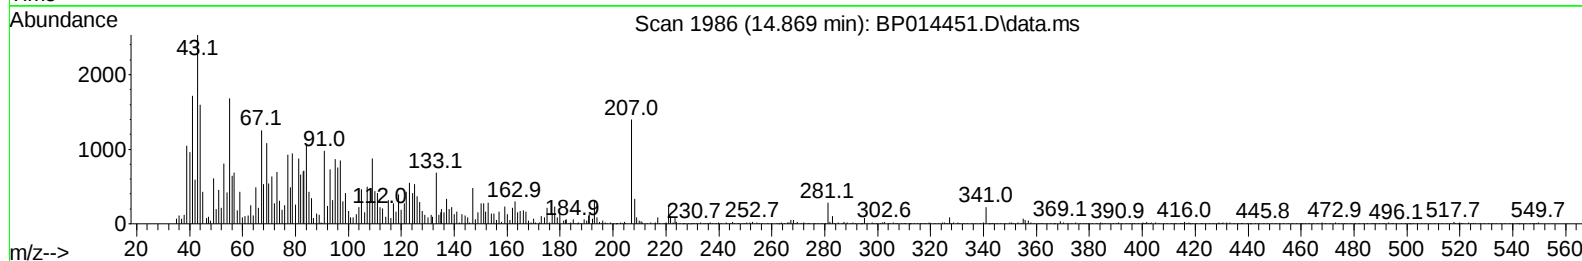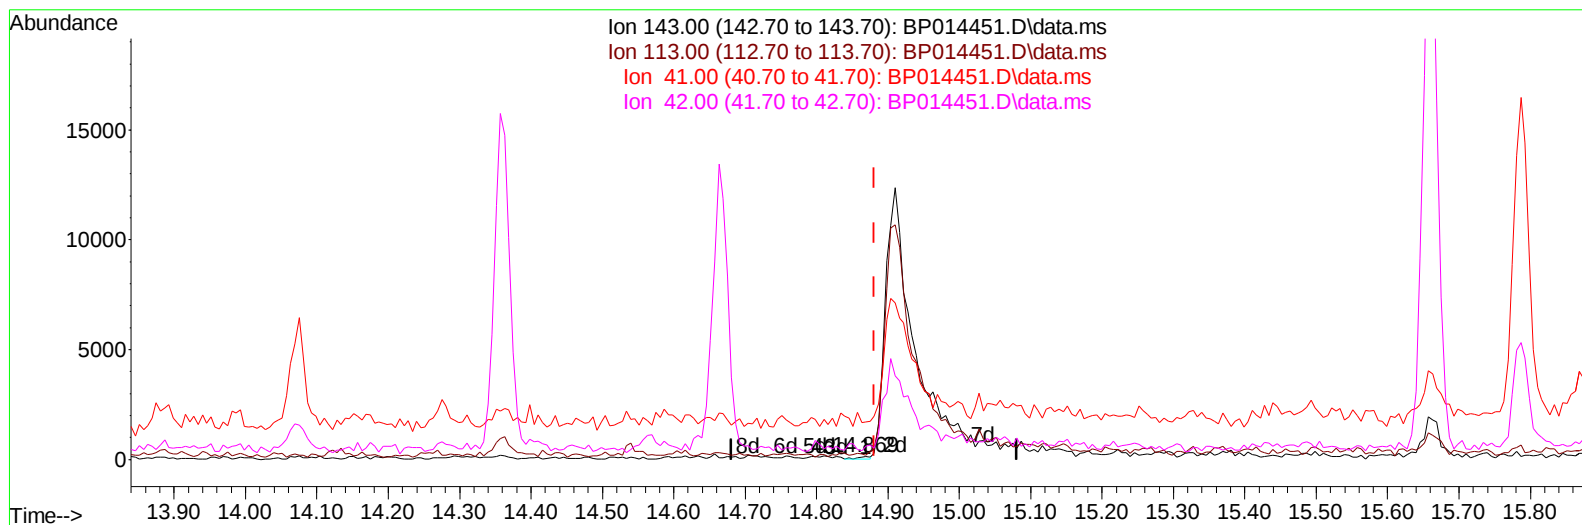

TIC: BP014451.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (-0.012) 0.02 ng/u1

response 150

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	156.92#
41.00	44.20	1317.69#
42.00	31.50	456.92#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014451.D
Acq On : 31 Mar 2023 19:22
Operator : CG/JU
Sample : 02093-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB967

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:55:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

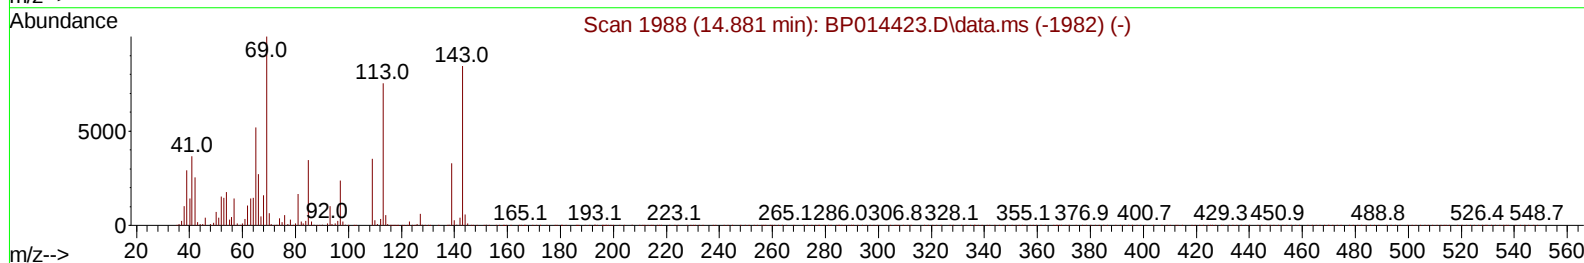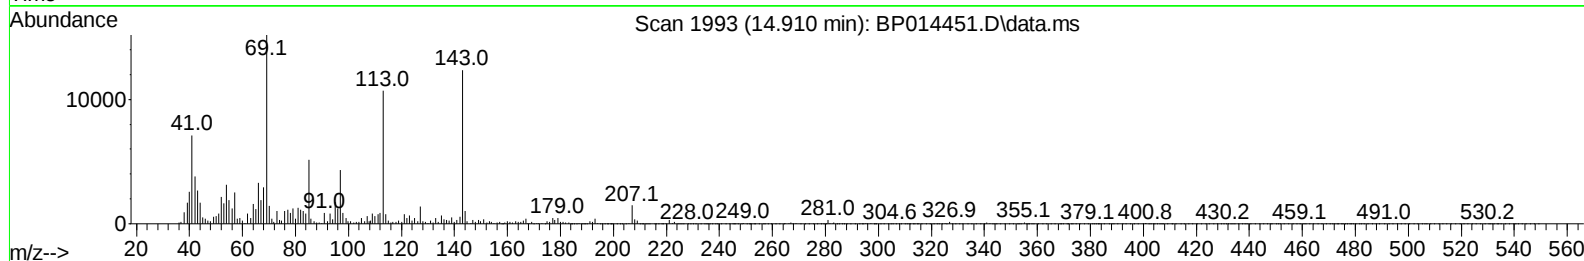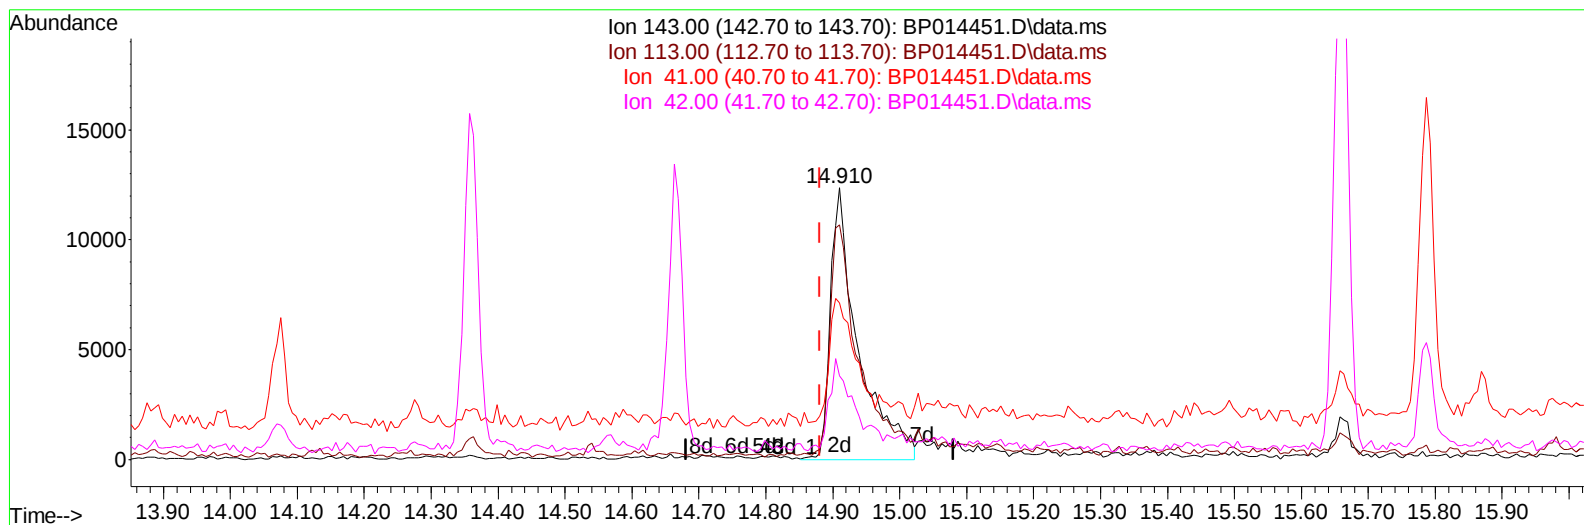

TIC: BP014451.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.910min (+ 0.029) 5.59 ng/ul m

response 35769

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	86.48
41.00	44.20	57.59#
42.00	31.50	30.88

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014451.D
 Acq On : 31 Mar 2023 19:22
 Operator : CG/JU
 Sample : 02093-03
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB967

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:55:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	176117	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	791353	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	522650	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1070012	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	710613	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	779580	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	19907	4.383	ng/uL	0.00
4) Pyridine-d5	3.828	84	95757	8.228	ng/ul	0.01
7) Phenol-d5	7.175	99	126980	7.818	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	356885	34.246	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	324981	27.683	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	250633	19.130	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	213714	33.453	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	244899	33.478	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.457	165	418713	31.429	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	198537	11.314	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1569215	37.030	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1668976	35.493	ng/ul	0.00
54) 4-Nitrophenol-d4	14.910	143	35769m	5.587	ng/ul	0.03
60) Fluorene-d10	15.663	176	1270129	35.941	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	244917	31.107	ng/ul	0.00
73) Anthracene-d10	17.528	188	1911727	36.917	ng/ul	0.00
81) Pyrene-d10	19.757	212	1874671	39.275	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.869	264	1543862	37.275	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014451.D
Acq On : 31 Mar 2023 19:22
Operator : CG/JU
Sample : 02093-03
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB967

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:55:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

