




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014452.D
Acq On : 31 Mar 2023 19:55
Operator : CG/JU
Sample : 02092-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:55:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

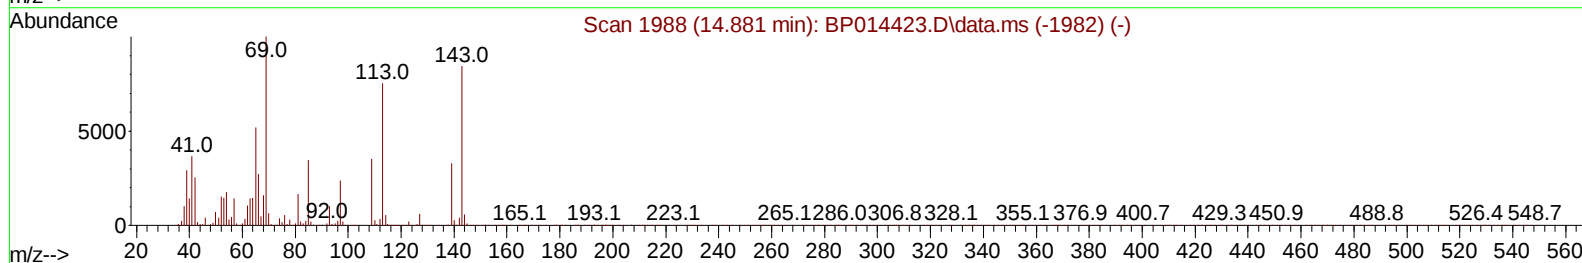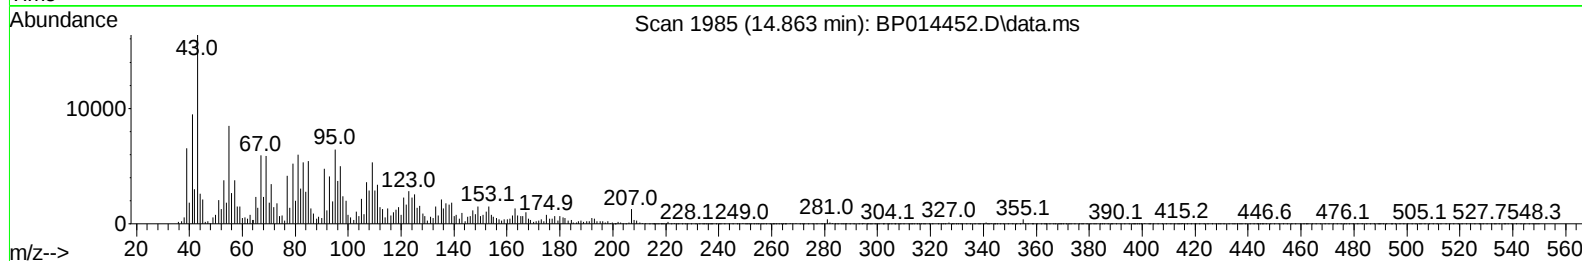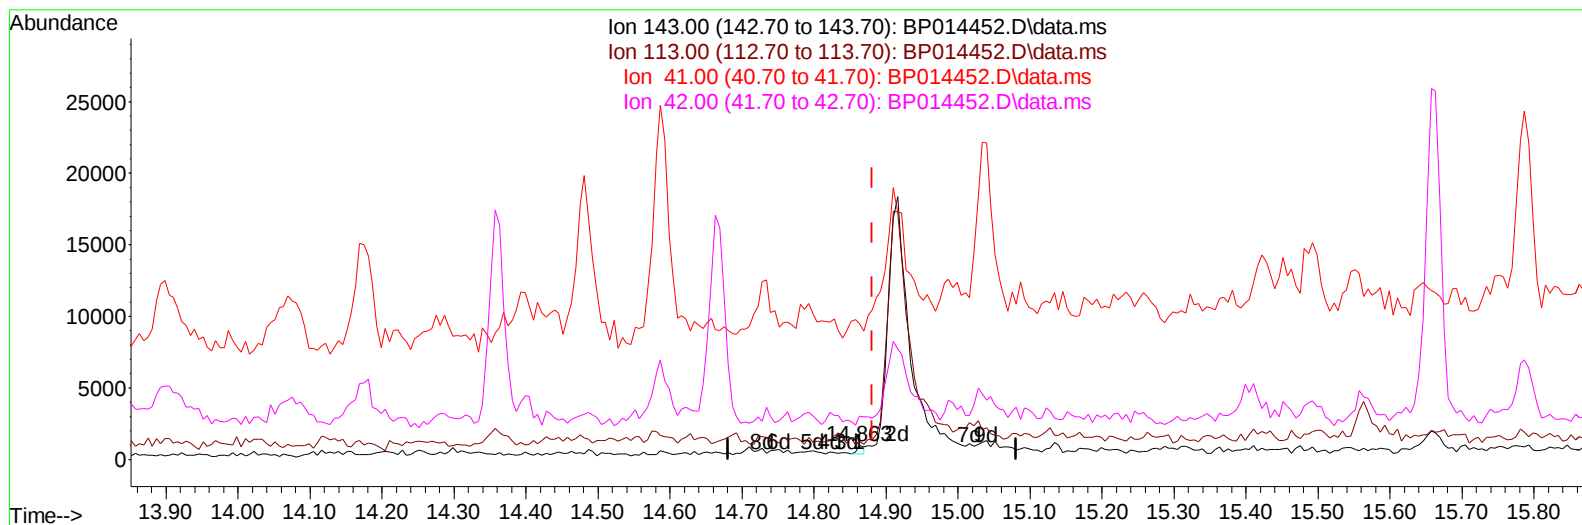

TIC: BP014452.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.863min (-0.018) 0.06 ng/u1

response 421

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	132.11#
41.00	44.20	994.25#
42.00	31.50	315.06#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014452.D
Acq On : 31 Mar 2023 19:55
Operator : CG/JU
Sample : 02092-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971

Manual IntegrationsAPPROVED

Quant Time: Mar 31 22:55:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

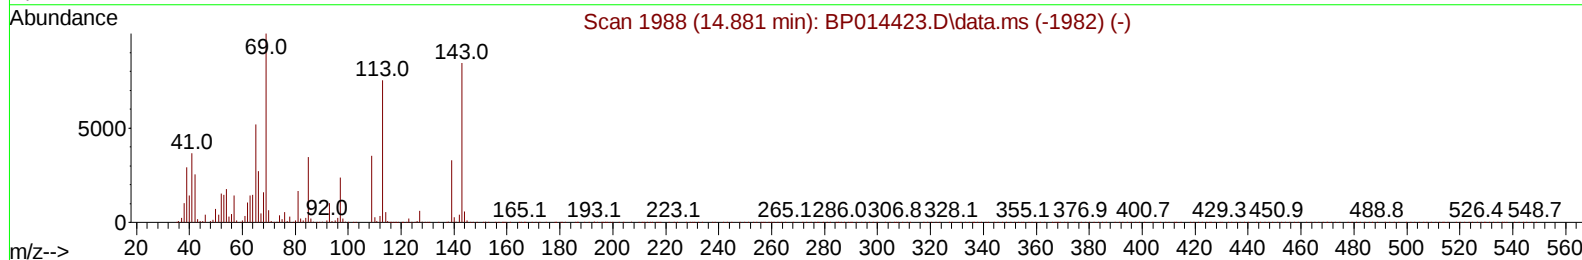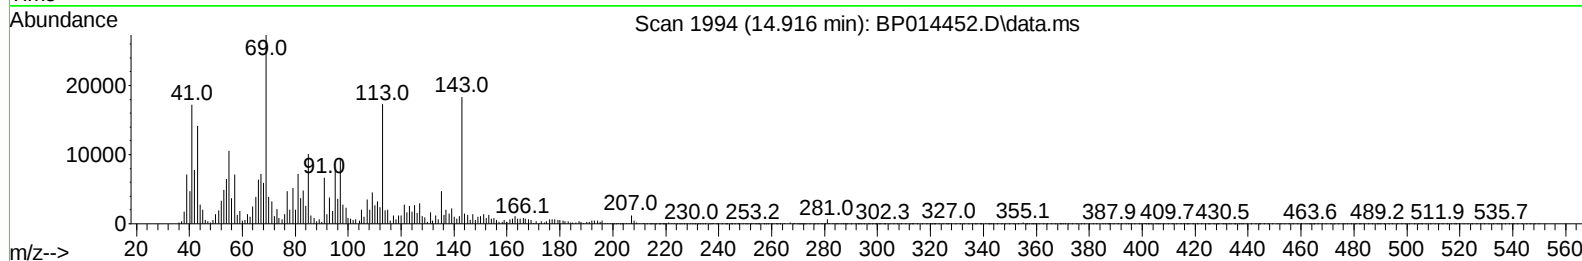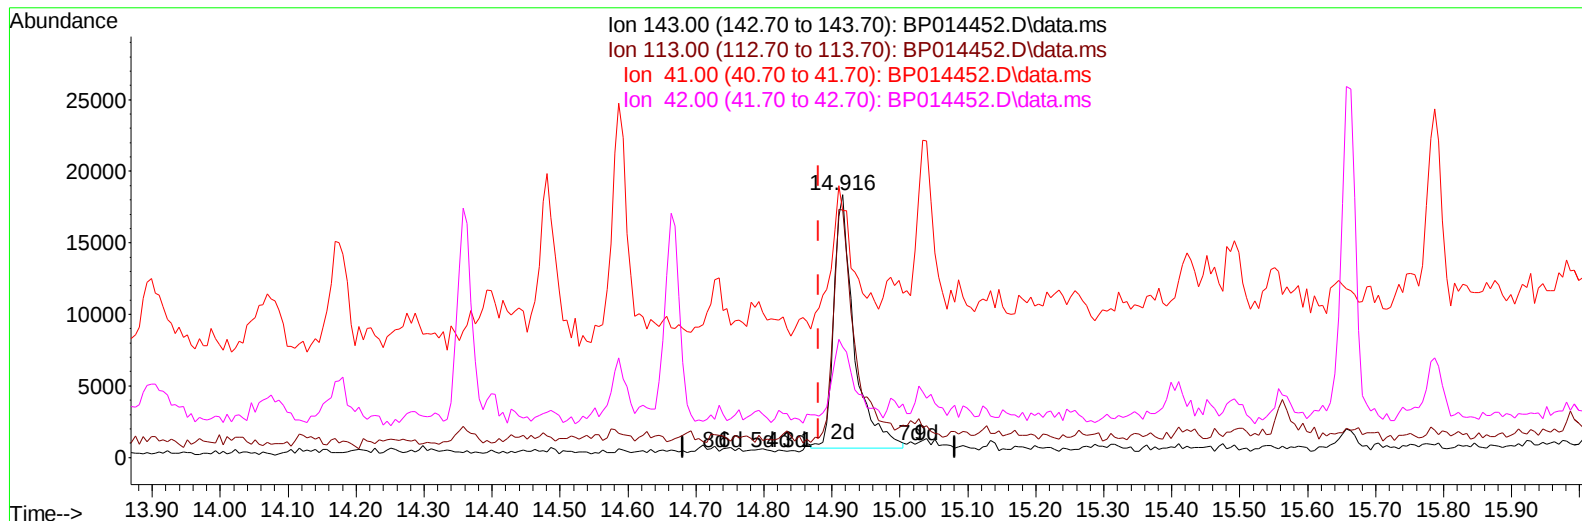

TIC: BP014452.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.035) 5.30 ng/ul m

response 37134

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	94.20
41.00	44.20	94.07#
42.00	31.50	42.15#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014452.D
 Acq On : 31 Mar 2023 19:55
 Operator : CG/JU
 Sample : 02092-08
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB971

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:55:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	218493	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	937298	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	571721	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1120072	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	750037	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	867555	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	22953	4.074	ng/uL	0.00
4) Pyridine-d5	3.823	84	123766	8.572	ng/ul	0.00
7) Phenol-d5	7.175	99	145967	7.244	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	378156	29.249	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	348164	23.906	ng/ul	0.00
15) 4-Methylphenol-d8	8.728	113	262235	16.134	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	226287	29.906	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	249279	28.771	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	413300	26.192	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	92524	4.452	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1443241	31.134	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	1589875	30.909	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	37134m	5.302	ng/ul	0.04
60) Fluorene-d10	15.663	176	1180484	30.537	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	218164	26.471	ng/ul	0.00
73) Anthracene-d10	17.528	188	1658073	30.588	ng/ul	0.00
81) Pyrene-d10	19.757	212	1573882	31.240	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	1393498	30.232	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014452.D
Acq On : 31 Mar 2023 19:55
Operator : CG/JU
Sample : 02092-08
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB971

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Mar 31 22:55:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

