




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014463.D
Acq On : 01 Apr 2023 02:40
Operator : CG/JU
Sample : 02092-12
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978

Manual IntegrationsAPPROVED

Quant Time: Apr 01 03:10:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

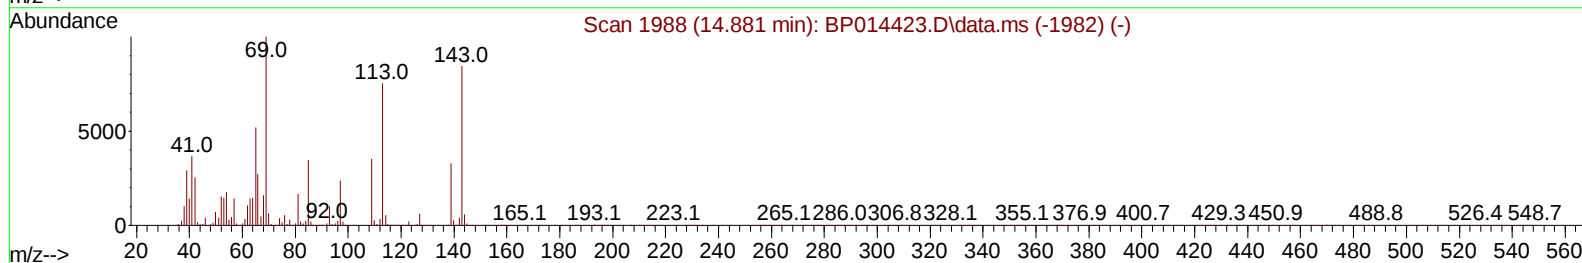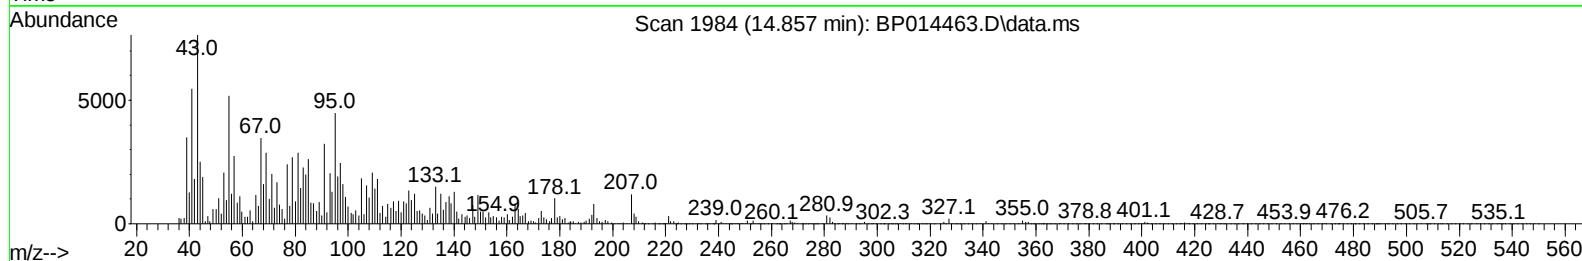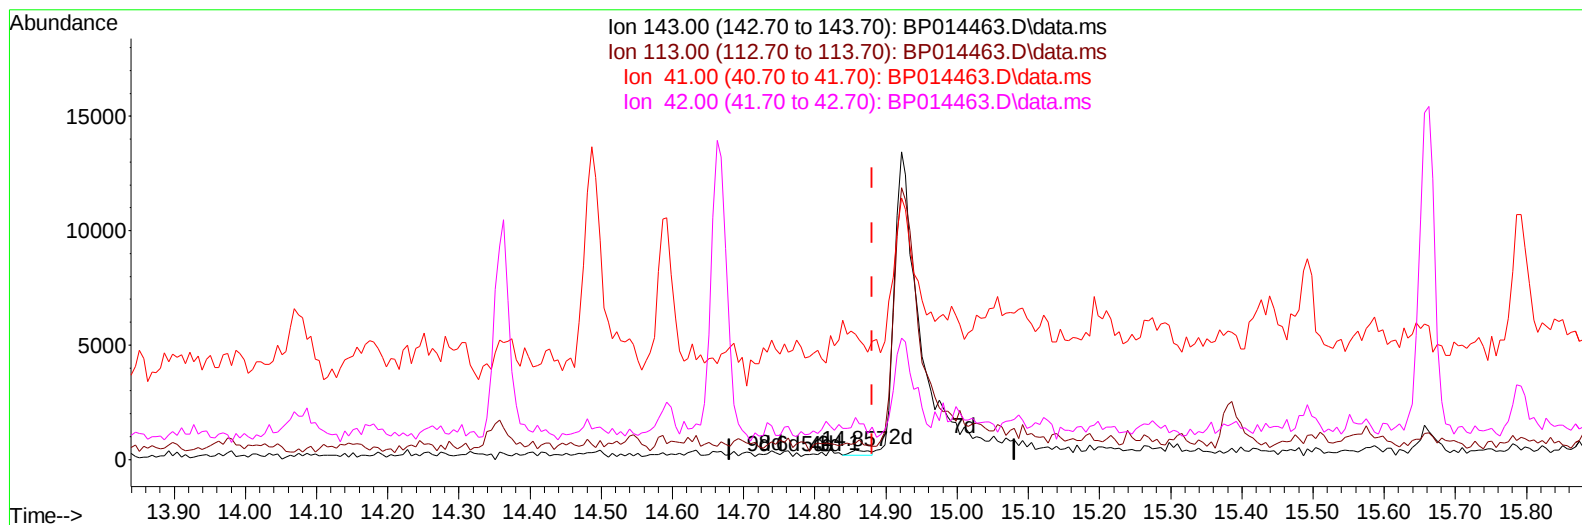

TIC: BP014463.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.857min (-0.024) 0.06 ng/u1

response 388

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	181.41#
41.00	44.20	1375.13#
42.00	31.50	458.54#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014463.D
Acq On : 01 Apr 2023 02:40
Operator : CG/JU
Sample : 02092-12
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978

Manual IntegrationsAPPROVED

Quant Time: Apr 01 03:10:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

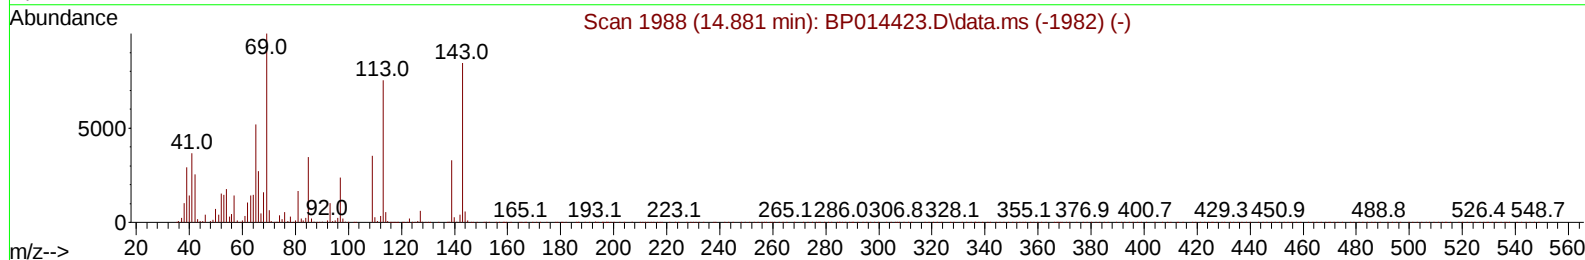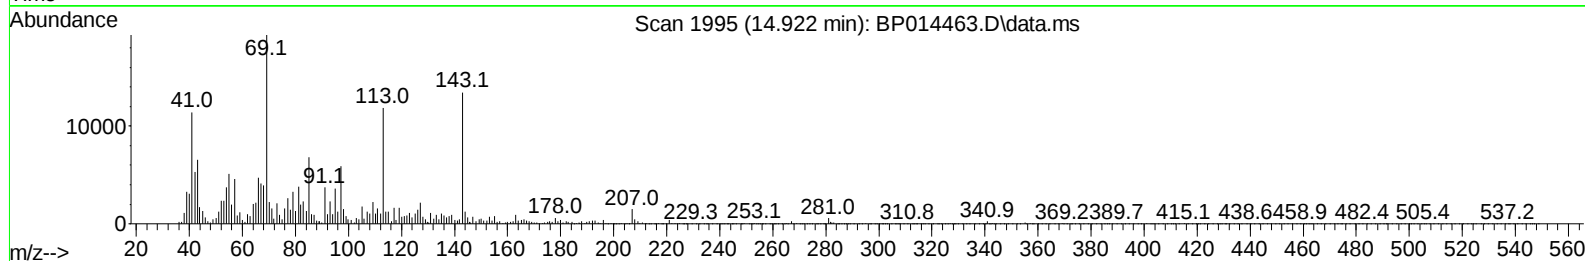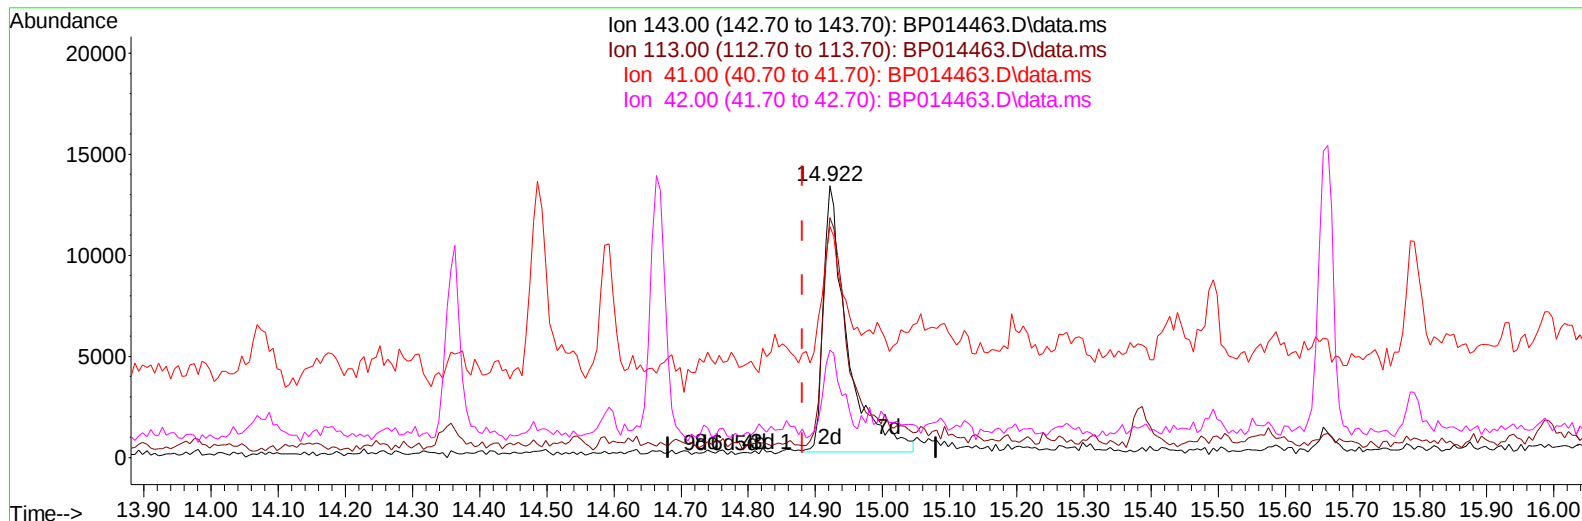

TIC: BP014463.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.041) 4.80 ng/ul m

response 33246

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	88.35
41.00	44.20	85.02#
42.00	31.50	39.55#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014463.D
 Acq On : 01 Apr 2023 02:40
 Operator : CG/JU
 Sample : 02092-12
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB978

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 03:10:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	182636	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	835412	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	566011	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.427	188	1205983	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	855004	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	832959	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	18654	3.961	ng/uL	0.00
4) Pyridine-d5	3.828	84	80415	6.663	ng/ul	0.01
7) Phenol-d5	7.187	99	107972	6.410	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	201659	18.660	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	188042	15.446	ng/ul	0.00
15) 4-Methylphenol-d8	8.740	113	162147	11.934	ng/ul	0.01
21) Nitrobenzene-d5	9.193	128	121124	17.960	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	130674	16.921	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	240140	17.075	ng/ul	0.00
31) 4-Chloroaniline-d4	10.987	131	95186	5.138	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	909260	19.813	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	959232	18.837	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	33246m	4.795	ng/ul	0.04
60) Fluorene-d10	15.663	176	750890	19.620	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	95436	10.755	ng/ul	0.00
73) Anthracene-d10	17.527	188	1170789	20.060	ng/ul	0.00
81) Pyrene-d10	19.757	212	1259667	21.934	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.868	264	886845	20.040	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014463.D
Acq On : 01 Apr 2023 02:40
Operator : CG/JU
Sample : 02092-12
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB978

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 03:10:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

