




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

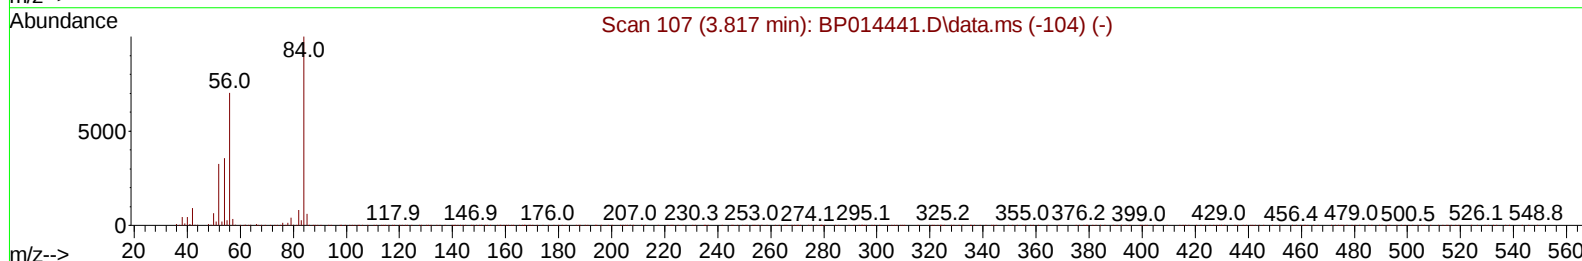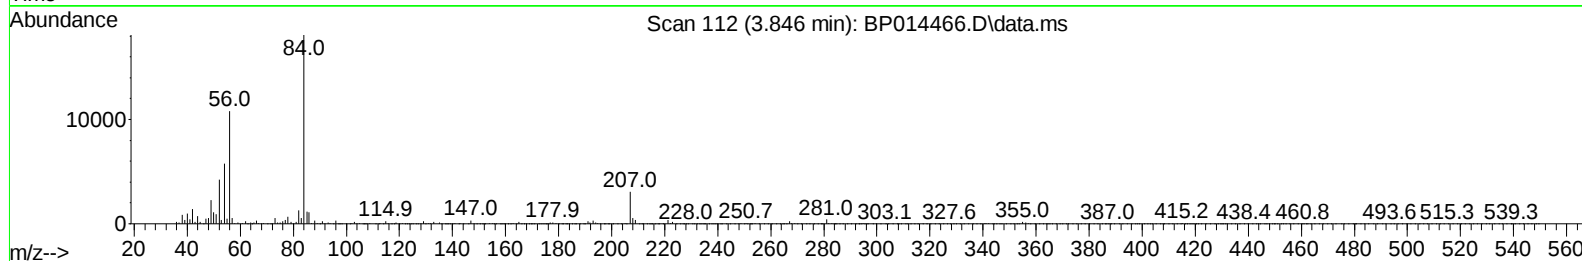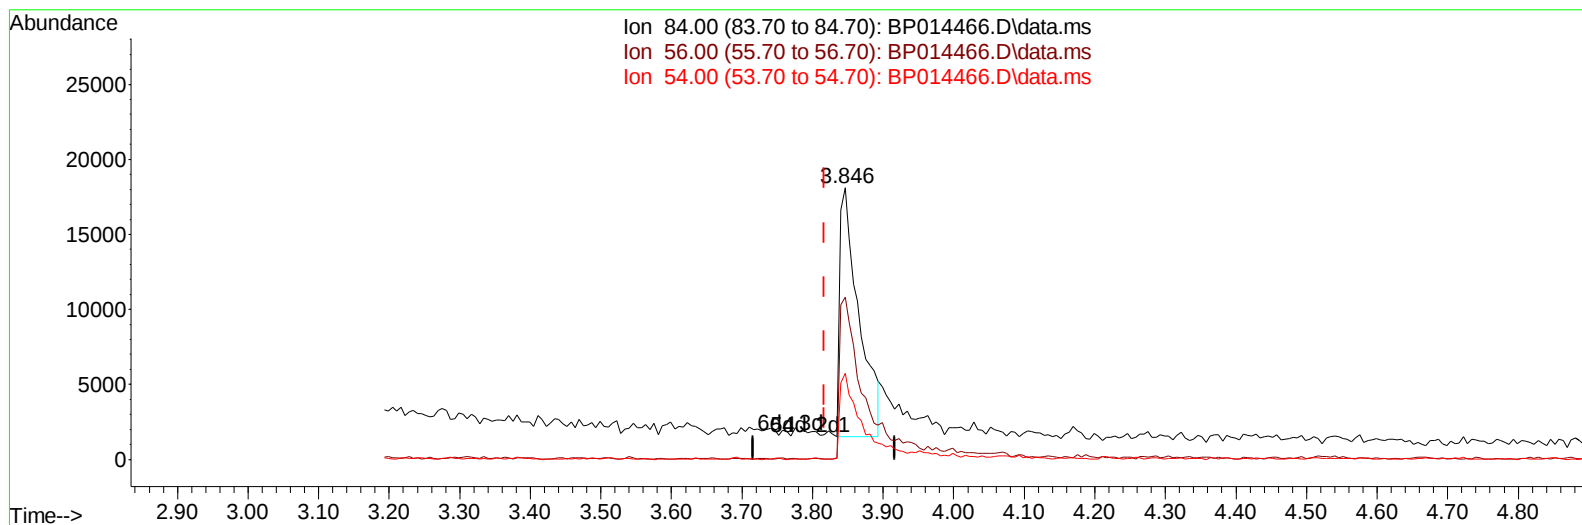

TIC: BP014466.D\data.ms

(4) Pyridine-d5 (S)

3.846min (+ 0.029) 3.01 ng/u1

response 31381

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	59.82
54.00	32.60	31.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014466.D
 Acq On : 01 Apr 2023 04:22
 Operator : CG/JU
 Sample : 02093-09
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB981

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:27:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

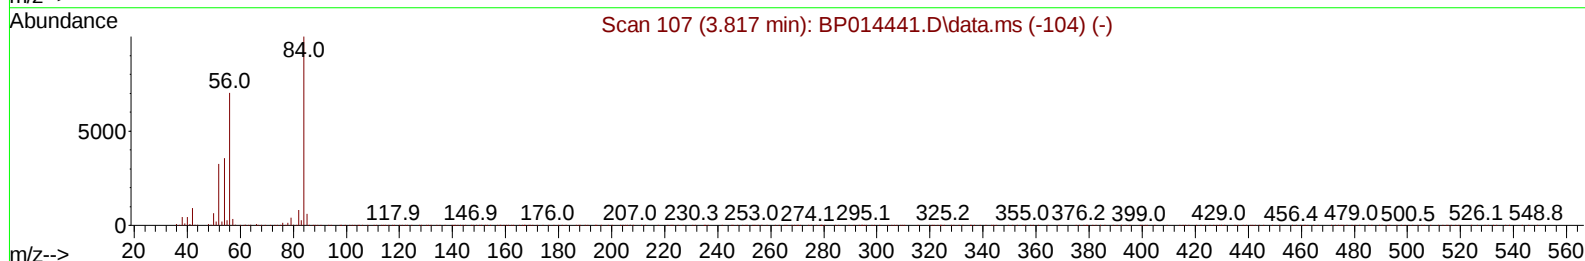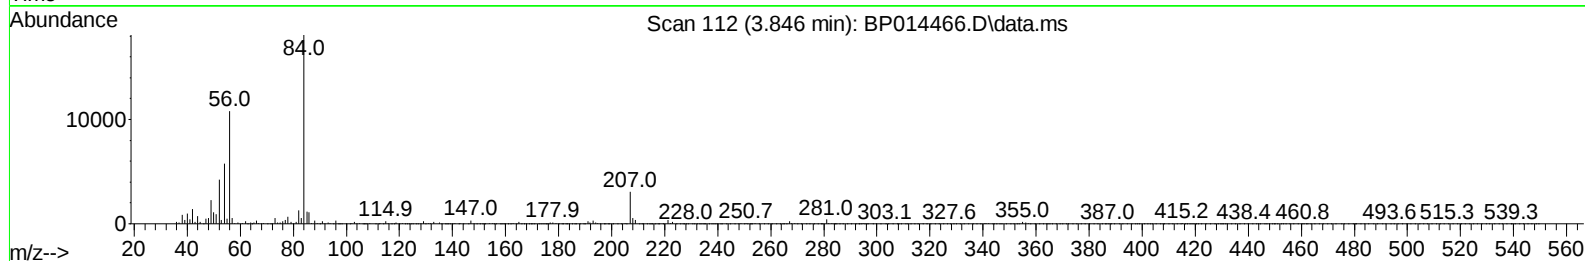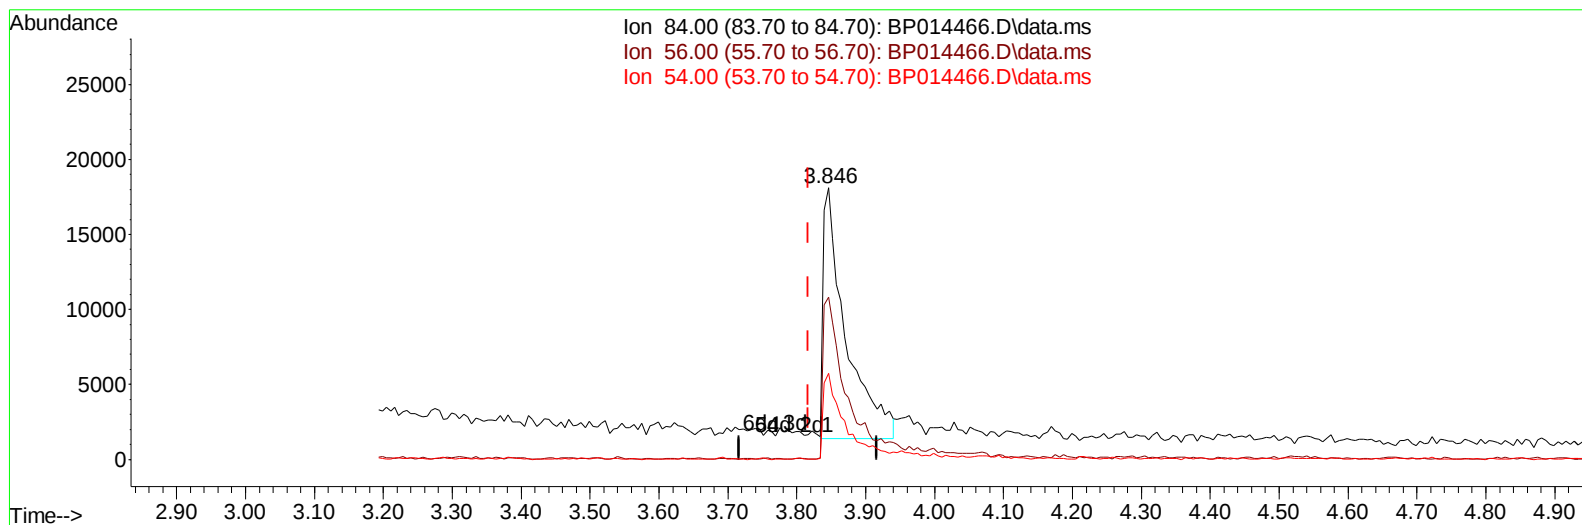

TIC: BP014466.D\data.ms

(4) Pyridine-d5 (S)

3.846min (+ 0.029) 3.65 ng/ul m

response 37978

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	65.70	59.82
54.00	32.60	31.72
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

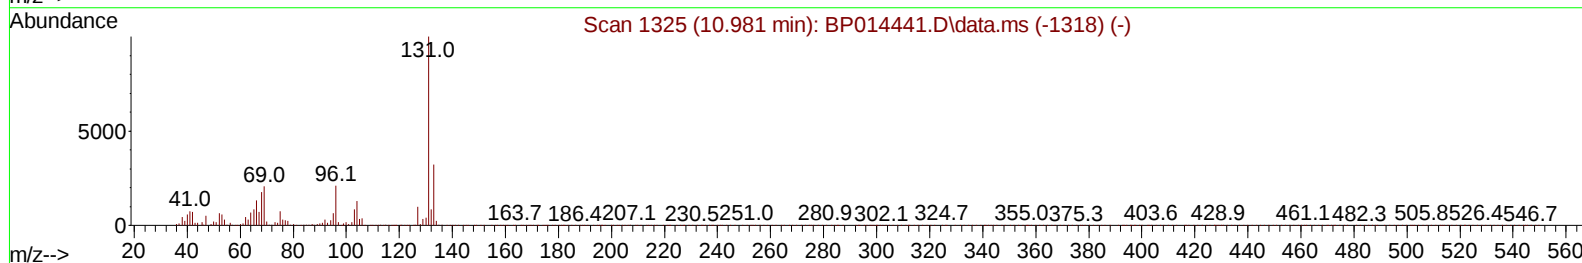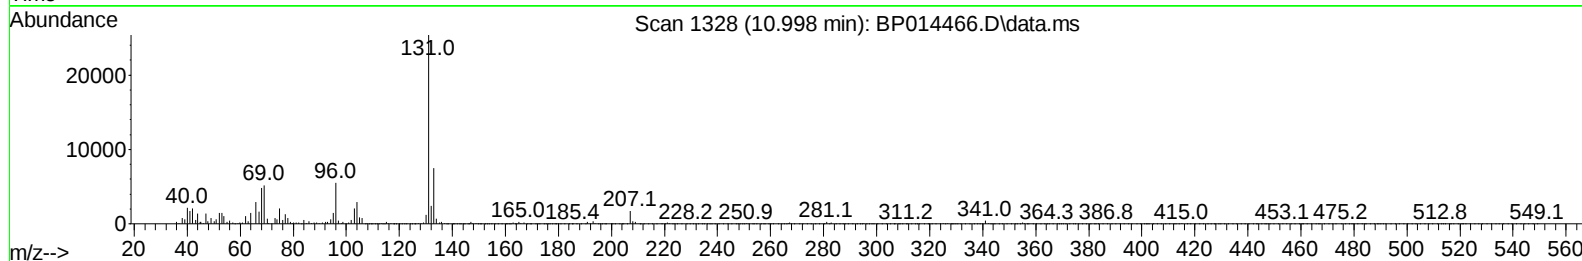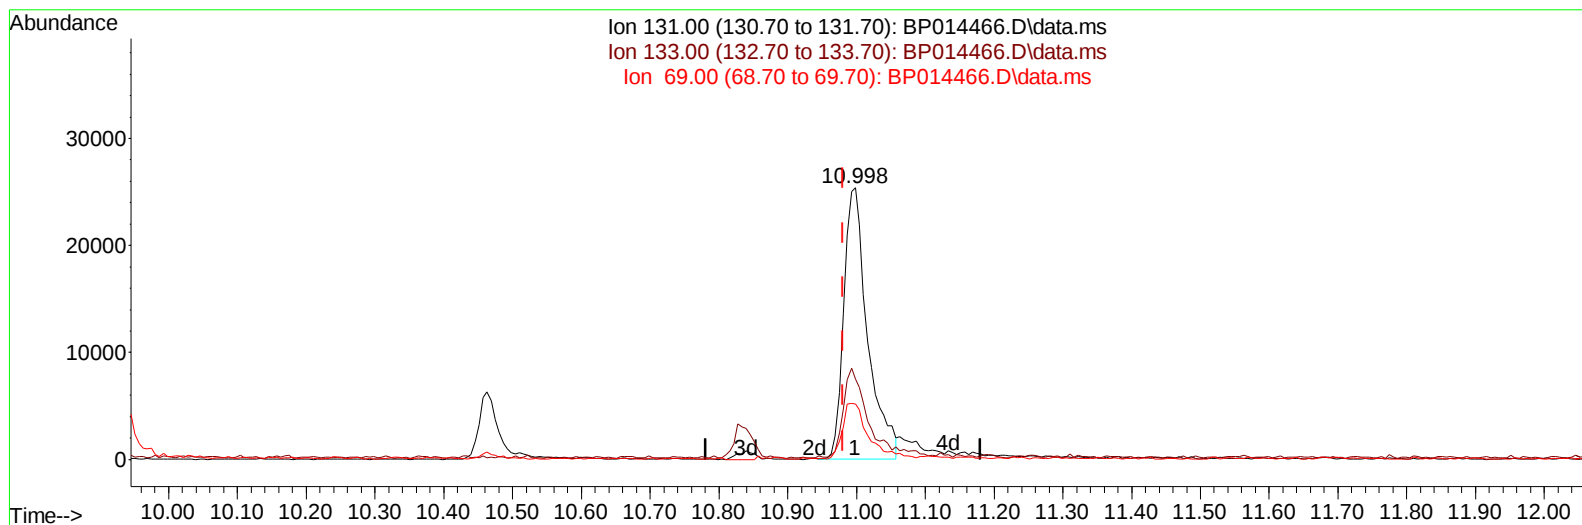

TIC: BP014466.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.998min (+ 0.018) 3.83 ng/ul

response 61334

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	29.59
69.00	21.30	20.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

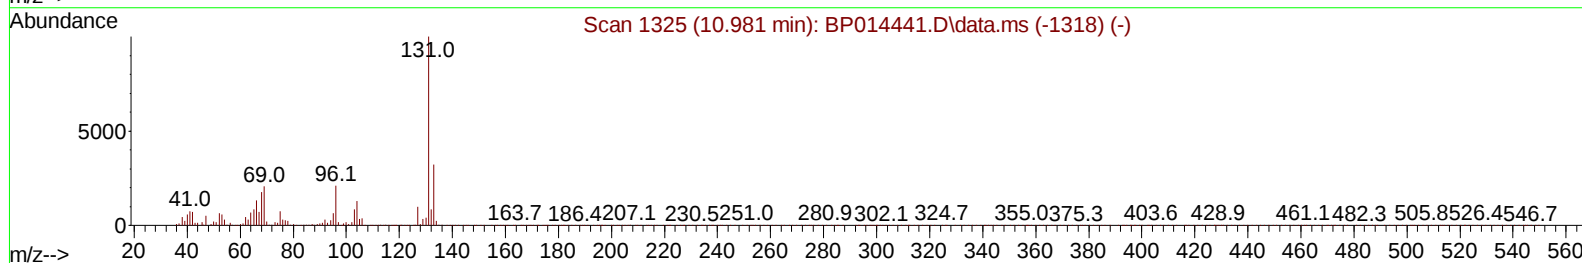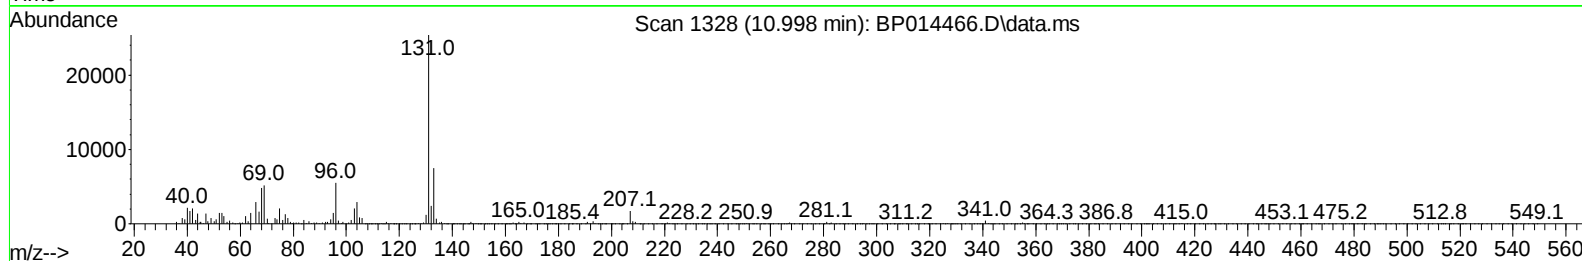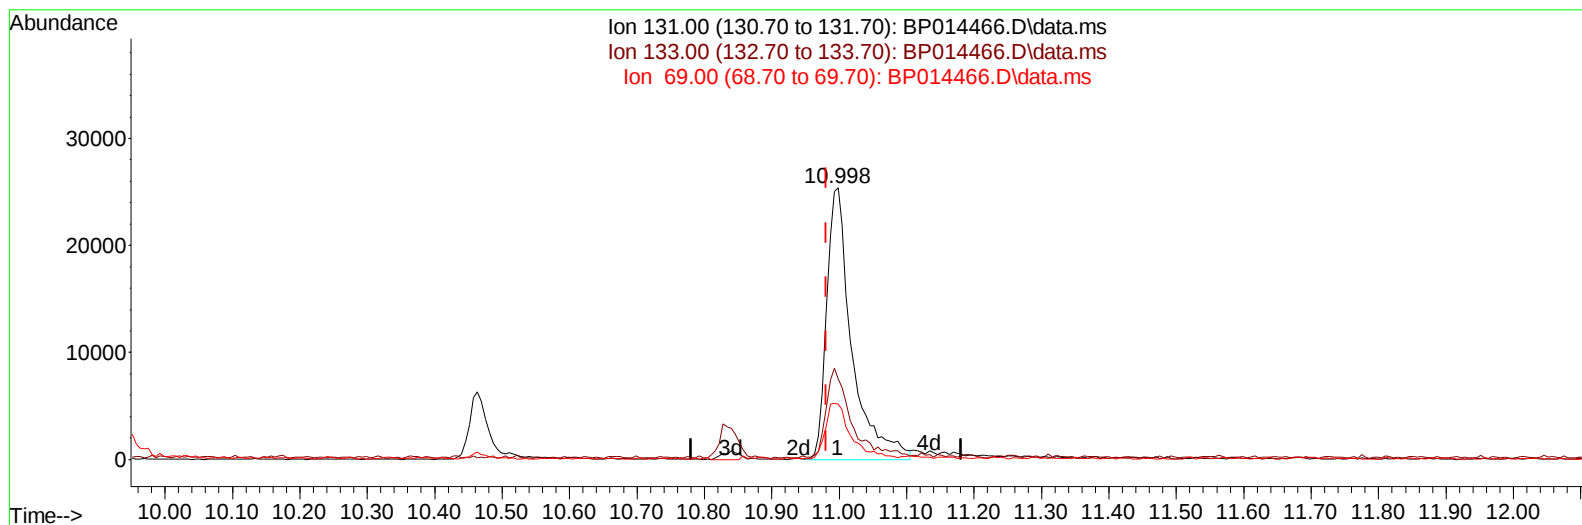

TIC: BP014466.D\data.ms

(31) 4-Chloroaniline-d4 (S)

10.998min (+ 0.018) 4.11 ng/ul m

response 65713

Ion	Exp%	Act%
131.00	100.00	100.00
133.00	32.20	29.59
69.00	21.30	20.45
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

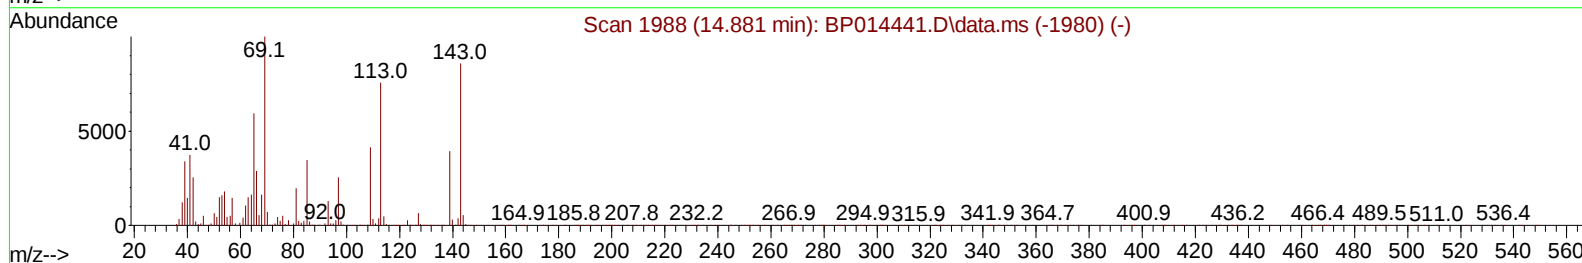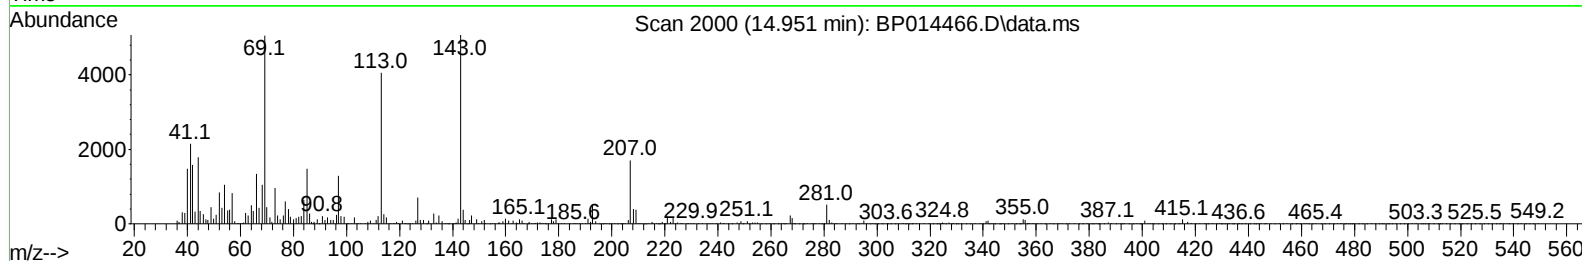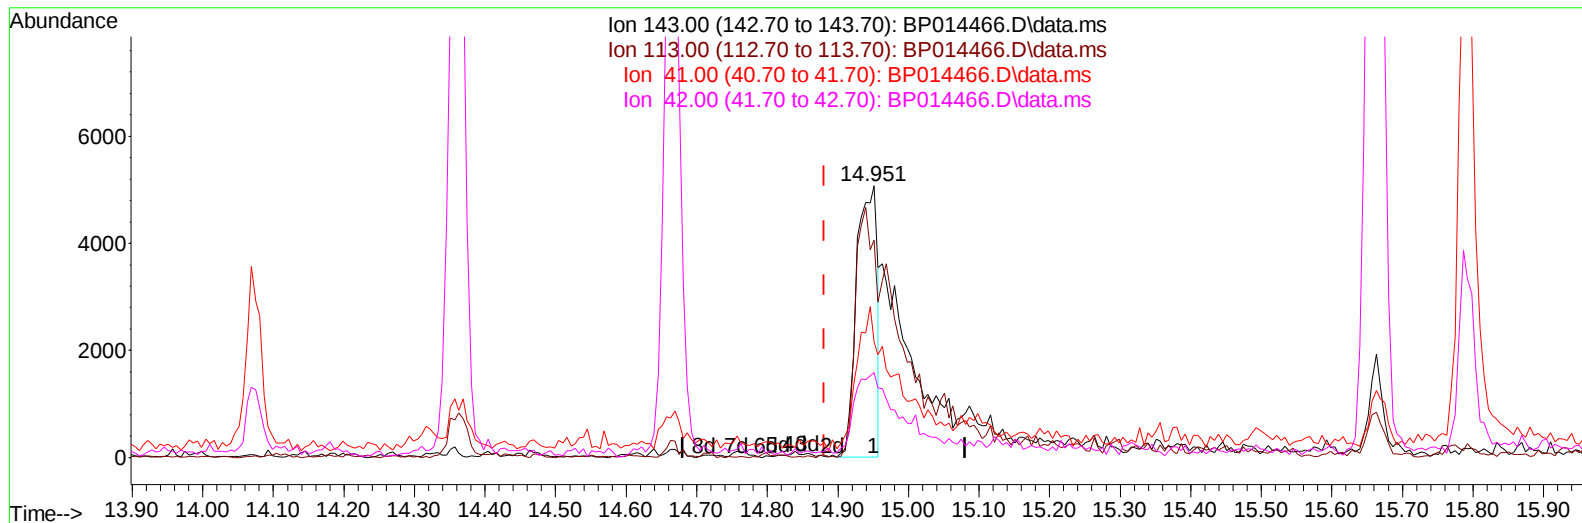

TIC: BP014466.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.951min (+ 0.070) 1.69 ng/u1

response 10462

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	80.07
41.00	44.20	42.46
42.00	31.50	31.15




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

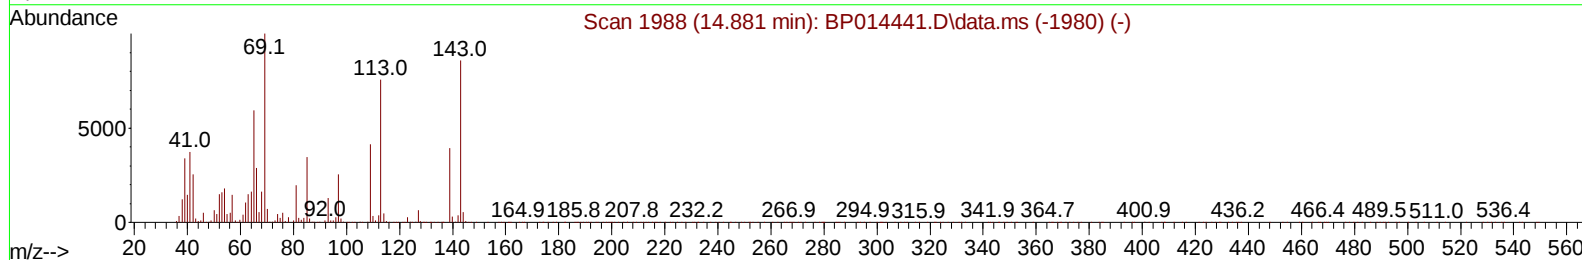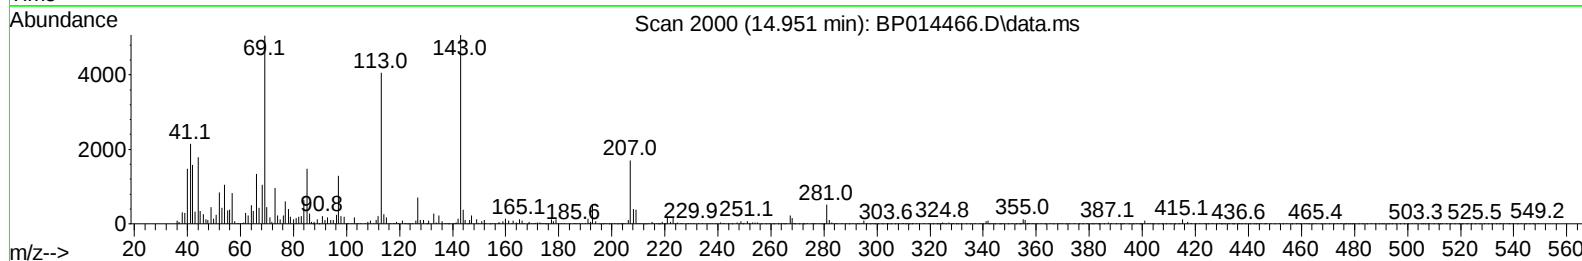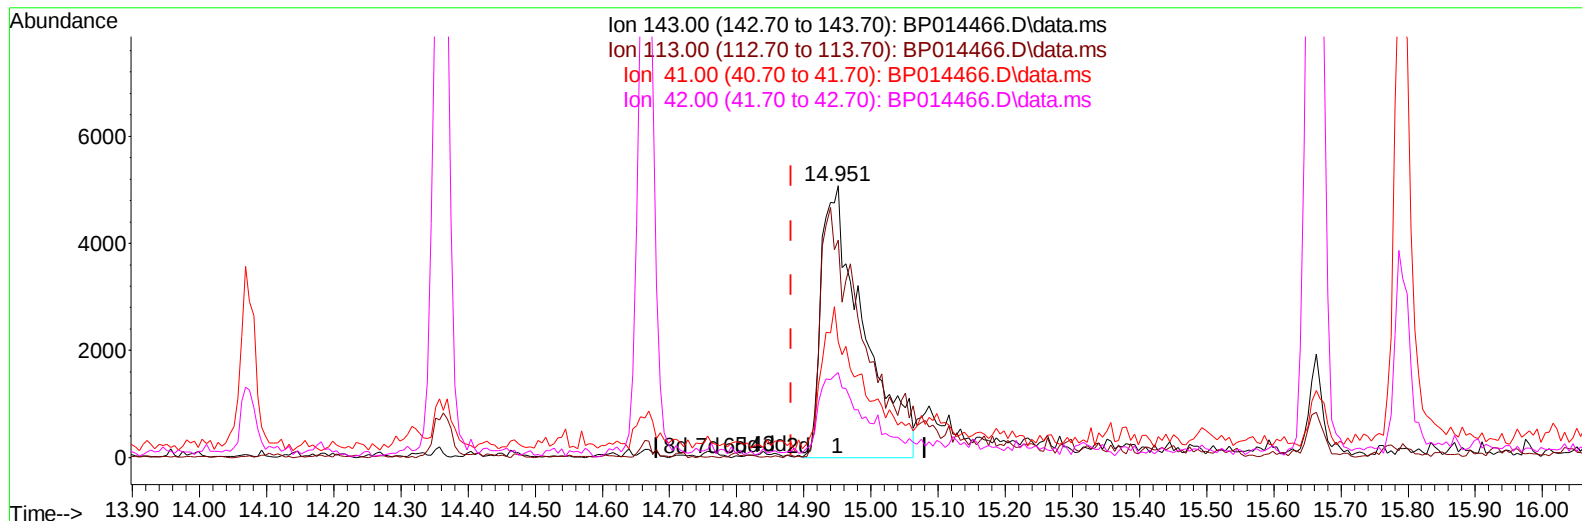

TIC: BP014466.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.951min (+ 0.070) 3.54 ng/ul m

response 21947

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	80.07
41.00	44.20	42.46
42.00	31.50	31.15

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014466.D
 Acq On : 01 Apr 2023 04:22
 Operator : CG/JU
 Sample : 02093-09
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB981

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 05:27:18 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	157589	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	721645	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	506185	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1084329	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	755918	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	776338	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	17473	4.300	ng/uL	0.00
4) Pyridine-d5	3.846	84	37978m	3.647	ng/ul	0.03
7) Phenol-d5	7.187	99	90296	6.213	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	313895	33.662	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	268033	25.516	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	186596	15.917	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	190721	32.738	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	215991	32.378	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	355932	29.297	ng/ul	0.00
31) 4-Chloroaniline-d4	10.998	131	65713m	4.106	ng/ul	0.02
46) Dimethylphthalate-d6	14.075	166	1418727	34.567	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1502469	32.992	ng/ul	0.00
54) 4-Nitrophenol-d4	14.951	143	21947m	3.540	ng/ul	0.07
60) Fluorene-d10	15.663	176	1176065	34.361	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	191995	24.064	ng/ul	0.00
73) Anthracene-d10	17.528	188	1957819	37.308	ng/ul	0.00
81) Pyrene-d10	19.757	212	2046949	40.314	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	1567641	38.007	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014466.D
Acq On : 01 Apr 2023 04:22
Operator : CG/JU
Sample : 02093-09
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB981

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 05:27:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

