




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014467.D
Acq On : 01 Apr 2023 04:55
Operator : CG/JU
Sample : 02092-15
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:30:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

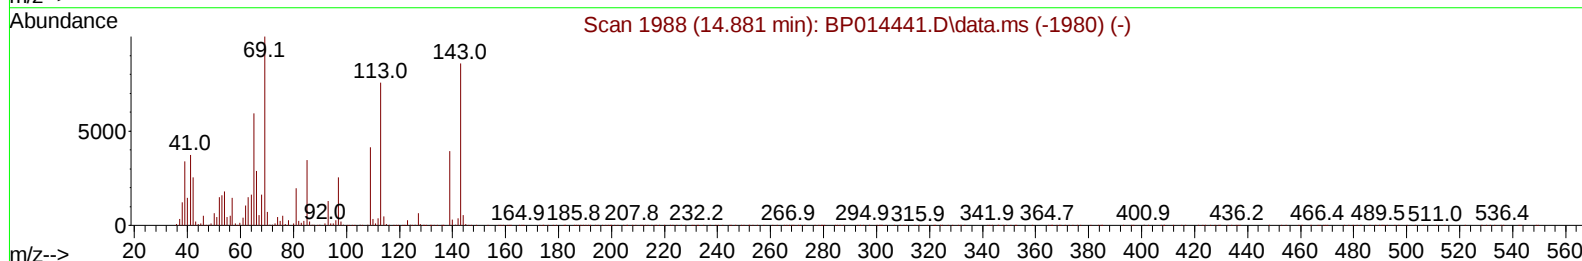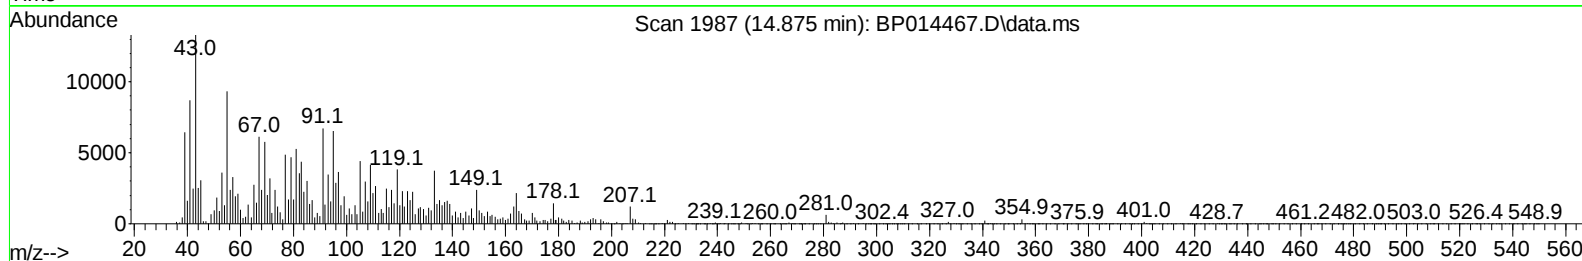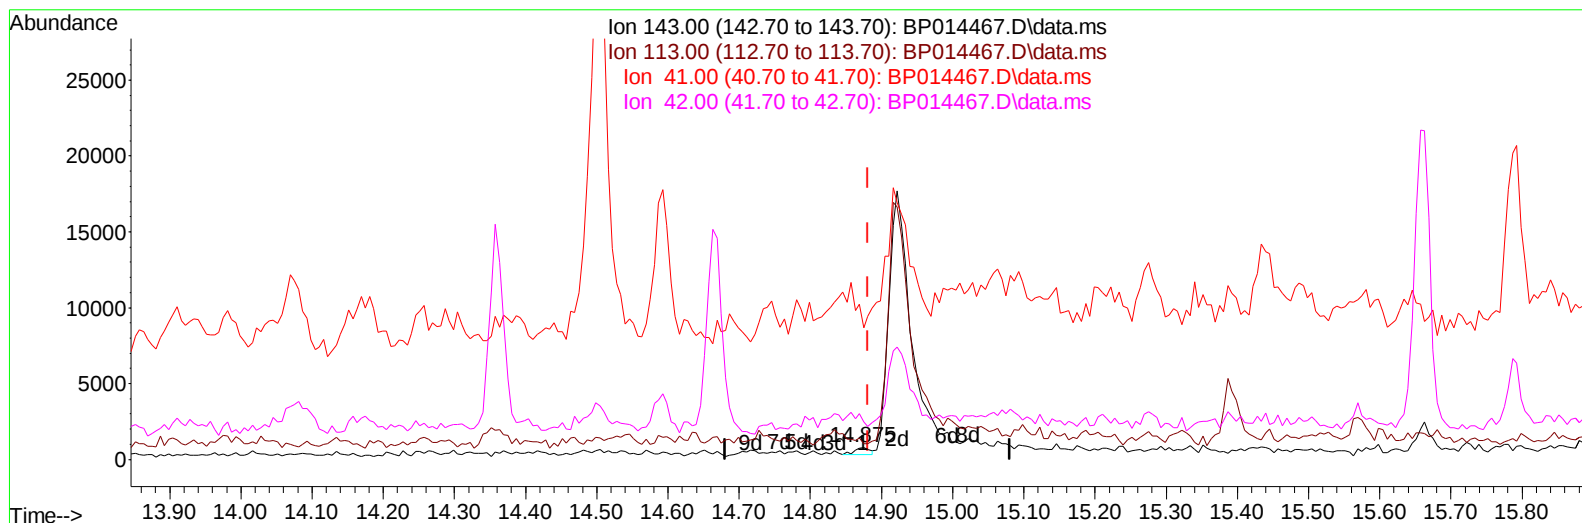

TIC: BP014467.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (-0.006) 0.10 ng/u1

response 704

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	133.50#
41.00	44.20	1105.22#
42.00	31.50	313.89#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014467.D
Acq On : 01 Apr 2023 04:55
Operator : CG/JU
Sample : 02092-15
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:30:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

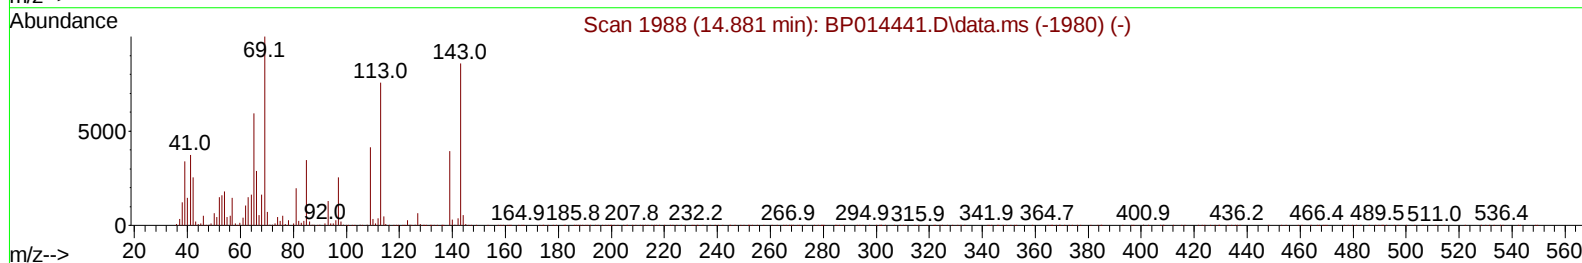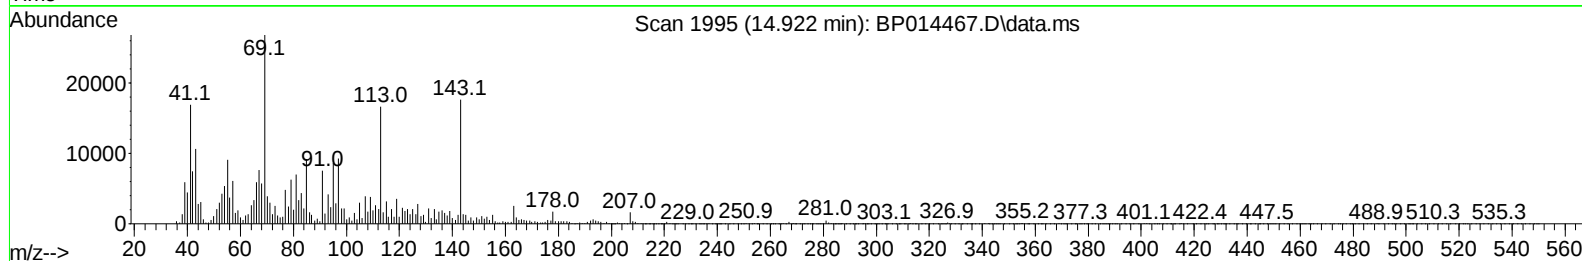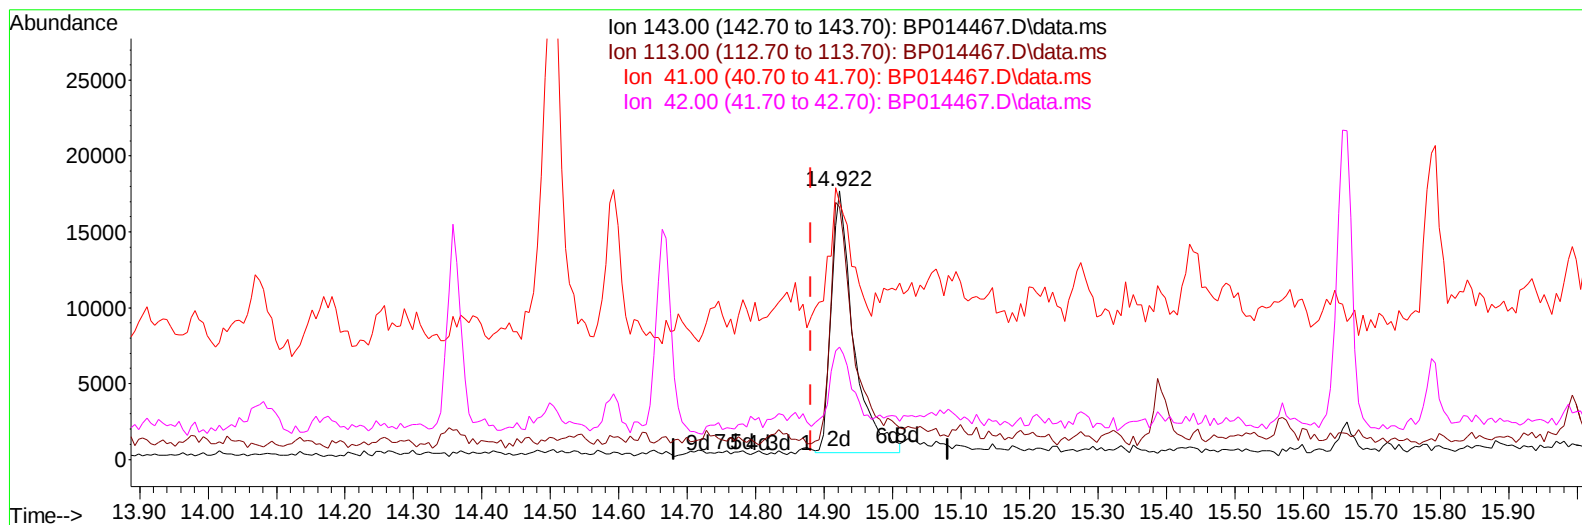

TIC: BP014467.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.041) 5.70 ng/ul m

response 39160

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	94.17
41.00	44.20	95.75#
42.00	31.50	41.97#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014467.D
 Acq On : 01 Apr 2023 04:55
 Operator : CG/JU
 Sample : 02092-15
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:30:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	198968	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	867261	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	561327	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1146863	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	760801	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	833280	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	20918	4.077	ng/uL	0.00
4) Pyridine-d5	3.834	84	79085	6.015	ng/ul	0.02
7) Phenol-d5	7.181	99	136224	7.424	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	322317	27.377	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	310287	23.396	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	239965	16.212	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	190895	27.266	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	216052	26.949	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	380968	26.093	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	264308	13.743	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1318240	28.964	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1400513	27.732	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	39160m	5.695	ng/ul	0.04
60) Fluorene-d10	15.663	176	1073200	28.276	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.793	200	194363	23.032	ng/ul	0.00
73) Anthracene-d10	17.528	188	1584624	28.550	ng/ul	0.00
81) Pyrene-d10	19.757	212	1606474	31.436	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	1288096	29.095	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014467.D
Acq On : 01 Apr 2023 04:55
Operator : CG/JU
Sample : 02092-15
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 05:30:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

