




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014468.D
Acq On : 01 Apr 2023 05:29
Operator : CG/JU
Sample : 02093-10
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:54:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

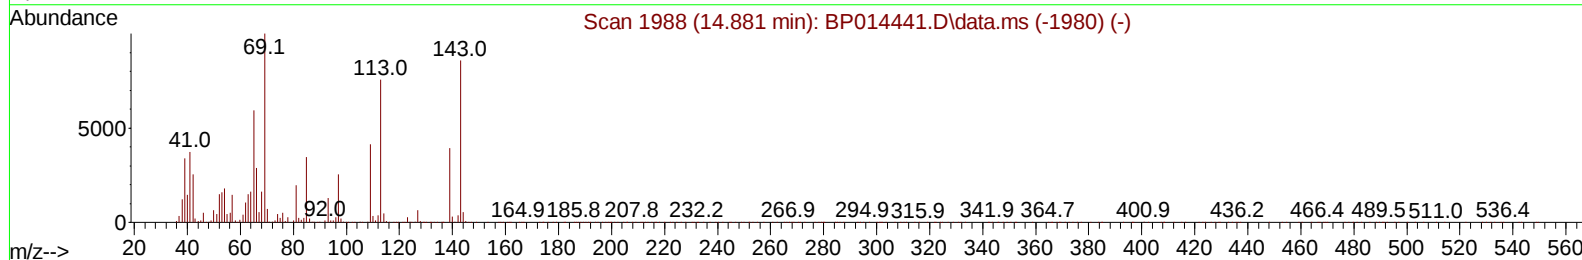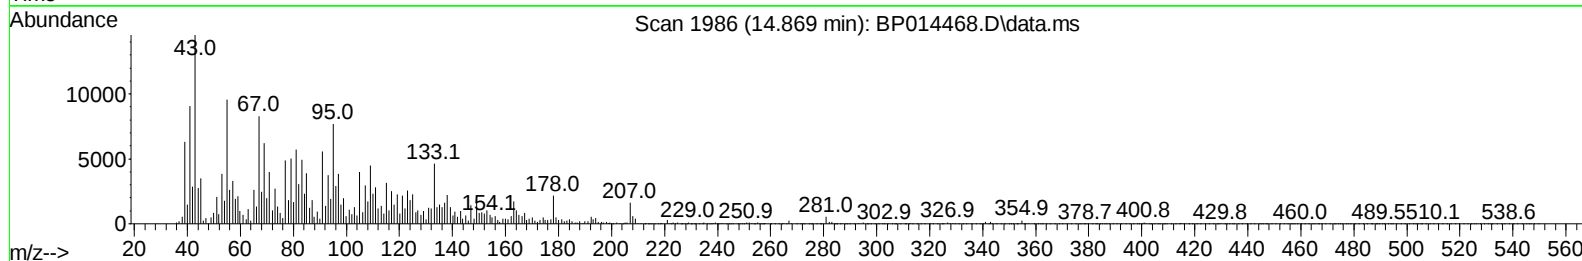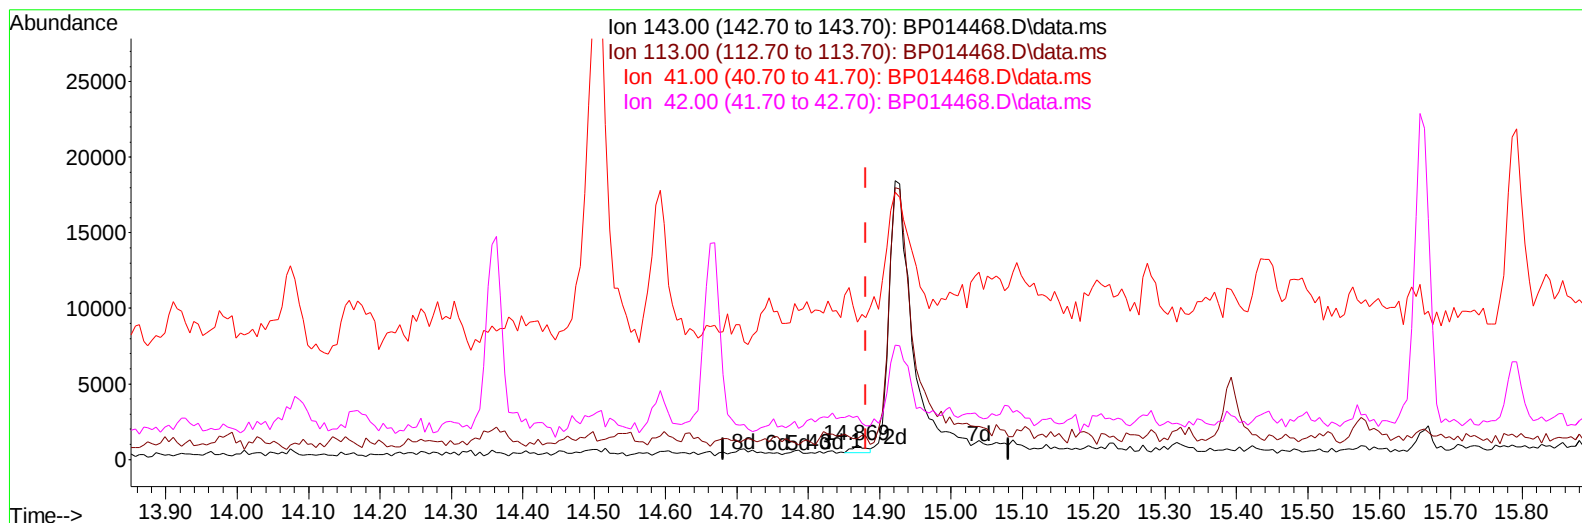

TIC: BP014468.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.869min (-0.012) 0.10 ng/u1

response 684

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	141.22#
41.00	44.20	939.26#
42.00	31.50	295.25#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014468.D
Acq On : 01 Apr 2023 05:29
Operator : CG/JU
Sample : 02093-10
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982

Manual IntegrationsAPPROVED

Quant Time: Apr 01 05:54:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

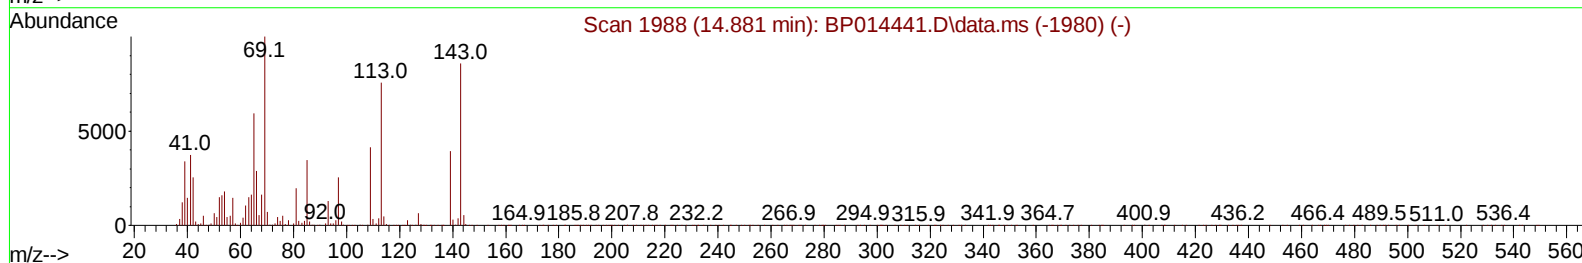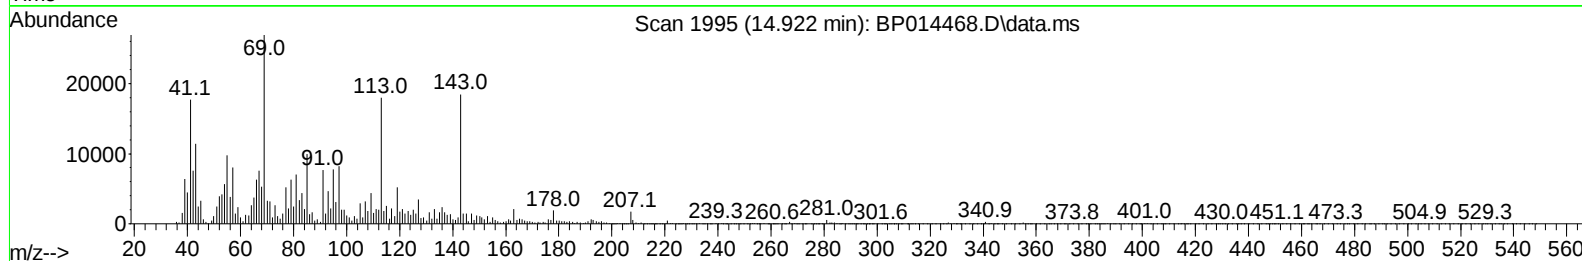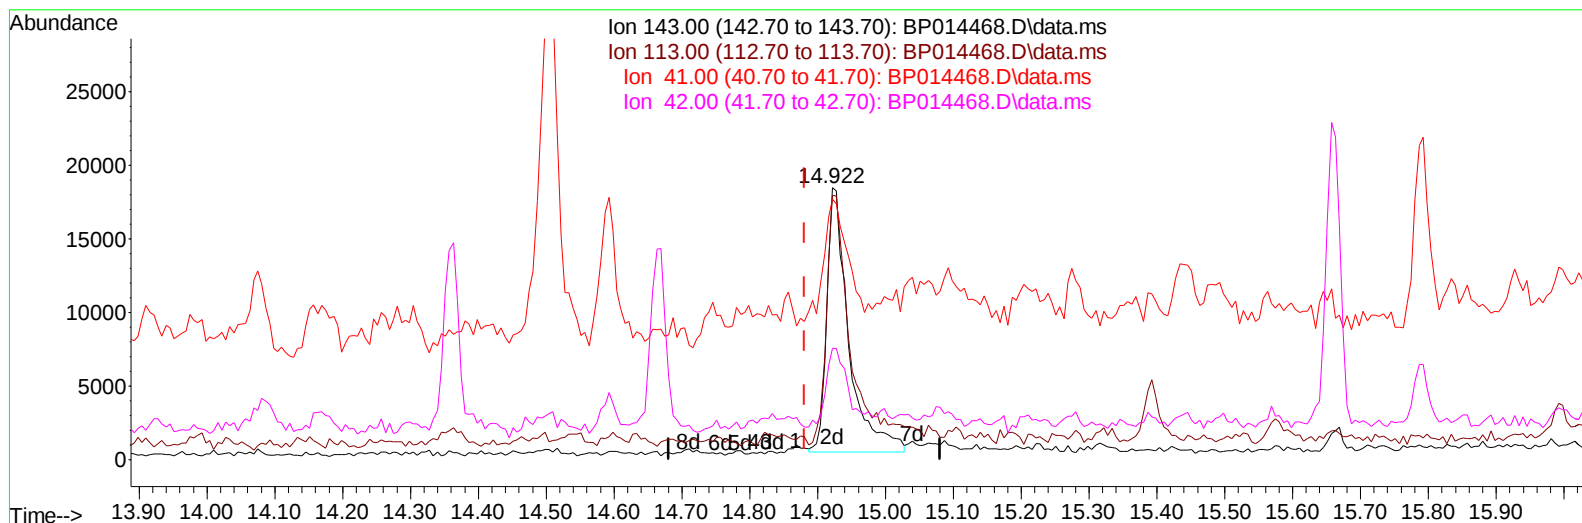

TIC: BP014468.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.041) 6.11 ng/ul m

response 40793

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	97.36
41.00	44.20	95.84#
42.00	31.50	40.95#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014468.D
 Acq On : 01 Apr 2023 05:29
 Operator : CG/JU
 Sample : 02093-10
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB982

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 05:54:57 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	192851	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	837027	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.669	164	544888	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.427	188	1124707	20.000	ng/ul	0.00
79) Chrysene-d12	21.515	240	766916	20.000	ng/ul	0.00
88) Perylene-d12	24.039	264	788001	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	20431	4.108	ng/uL	0.00
4) Pyridine-d5	3.834	84	78885	6.190	ng/ul	0.02
7) Phenol-d5	7.187	99	135147	7.599	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	7.334	67	312466	27.382	ng/ul	0.00
11) 2-Chlorophenol-d4	7.546	132	306739	23.862	ng/ul	0.00
15) 4-Methylphenol-d8	8.740	113	240355	16.754	ng/ul	0.01
21) Nitrobenzene-d5	9.187	128	191527	28.344	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	219324	28.346	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	376209	26.698	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	269307	14.509	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1321706	29.916	ng/ul	0.00
49) Acenaphthylene-d8	14.363	160	1396173	28.480	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	40793m	6.112	ng/ul	0.04
60) Fluorene-d10	15.663	176	1064079	28.881	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	196271	23.716	ng/ul	0.00
73) Anthracene-d10	17.527	188	1610963	29.596	ng/ul	0.00
81) Pyrene-d10	19.757	212	1669873	32.416	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.874	264	1245170	29.742	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.422	88	721874	132.089	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014468.D
Acq On : 01 Apr 2023 05:29
Operator : CG/JU
Sample : 02093-10
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB982

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 01 05:54:57 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

