




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014476.D
 Acq On : 01 Apr 2023 09:59
 Operator : CG/JU
 Sample : 02158-02
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-7D(20230329)

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 03 00:44:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

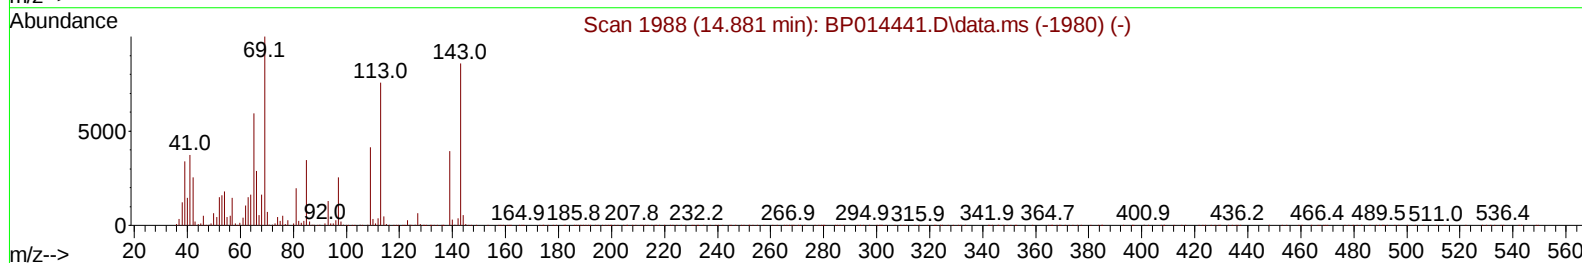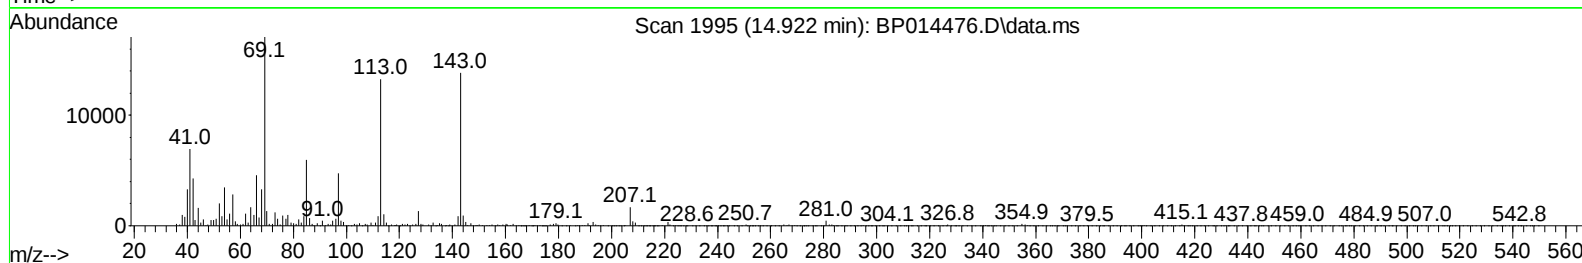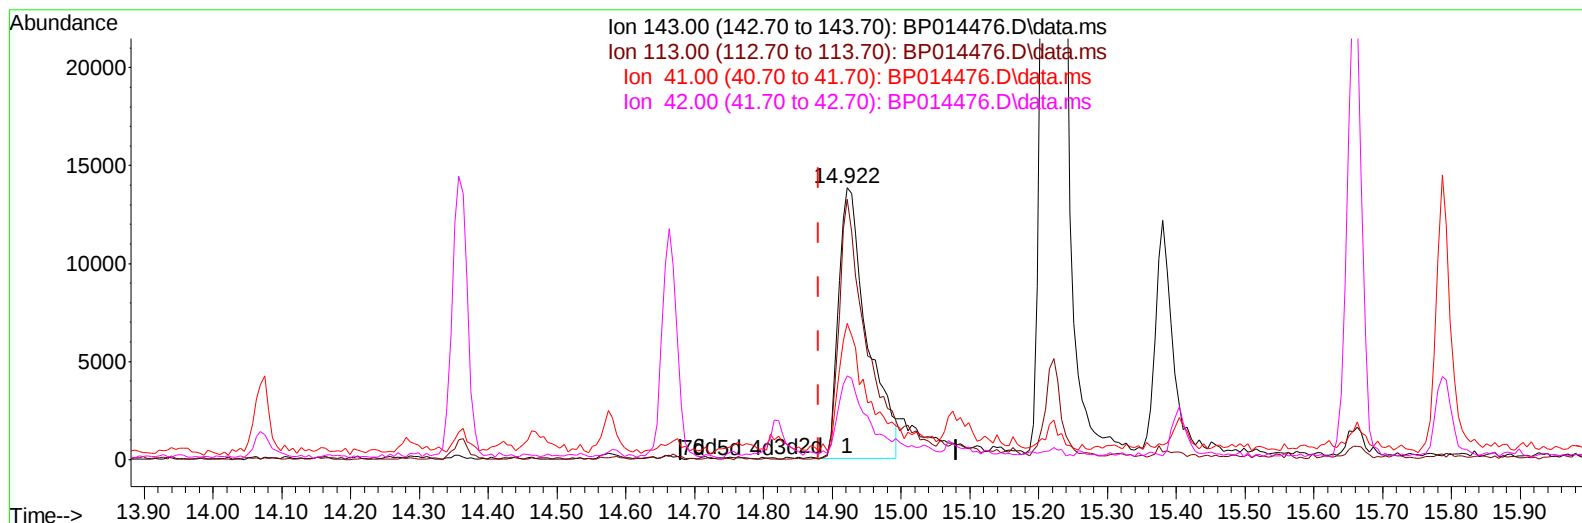

TIC: BP014476.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.041) 6.50 ng/ul

response 39957

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	95.78
41.00	44.20	50.14
42.00	31.50	30.89




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014476.D
 Acq On : 01 Apr 2023 09:59
 Operator : CG/JU
 Sample : 02158-02
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-7D(20230329)

Manual IntegrationsAPPROVED

Quant Time: Apr 03 00:44:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

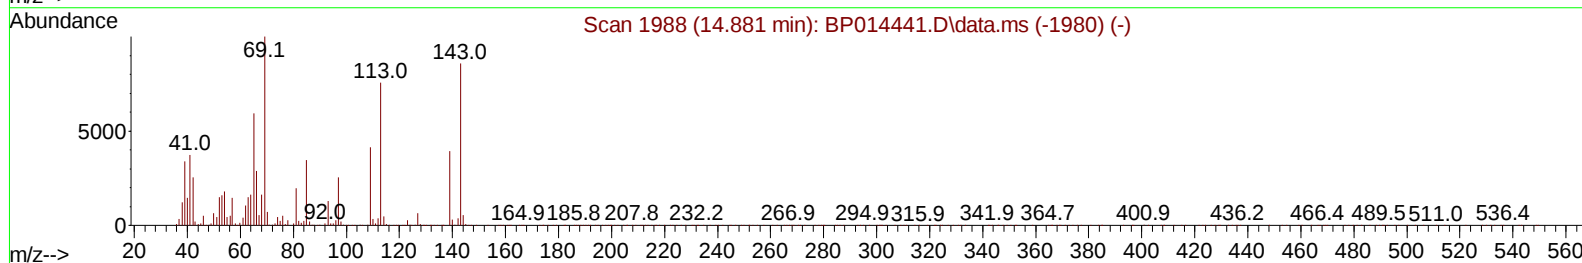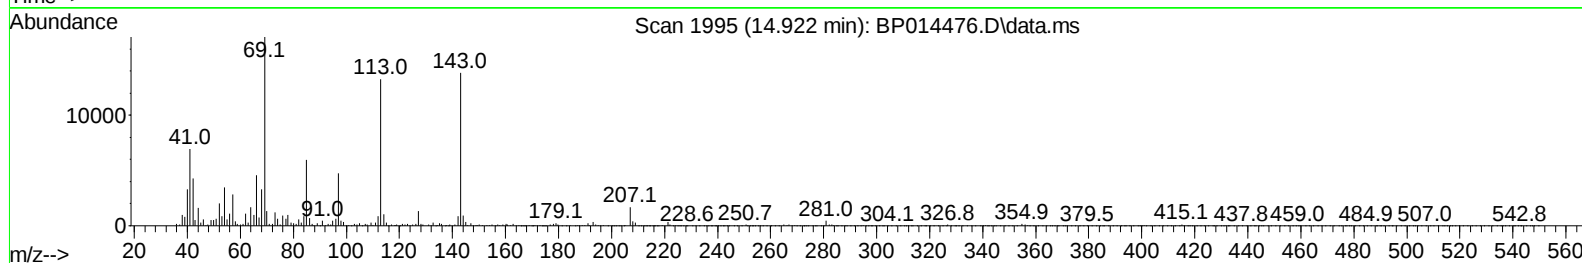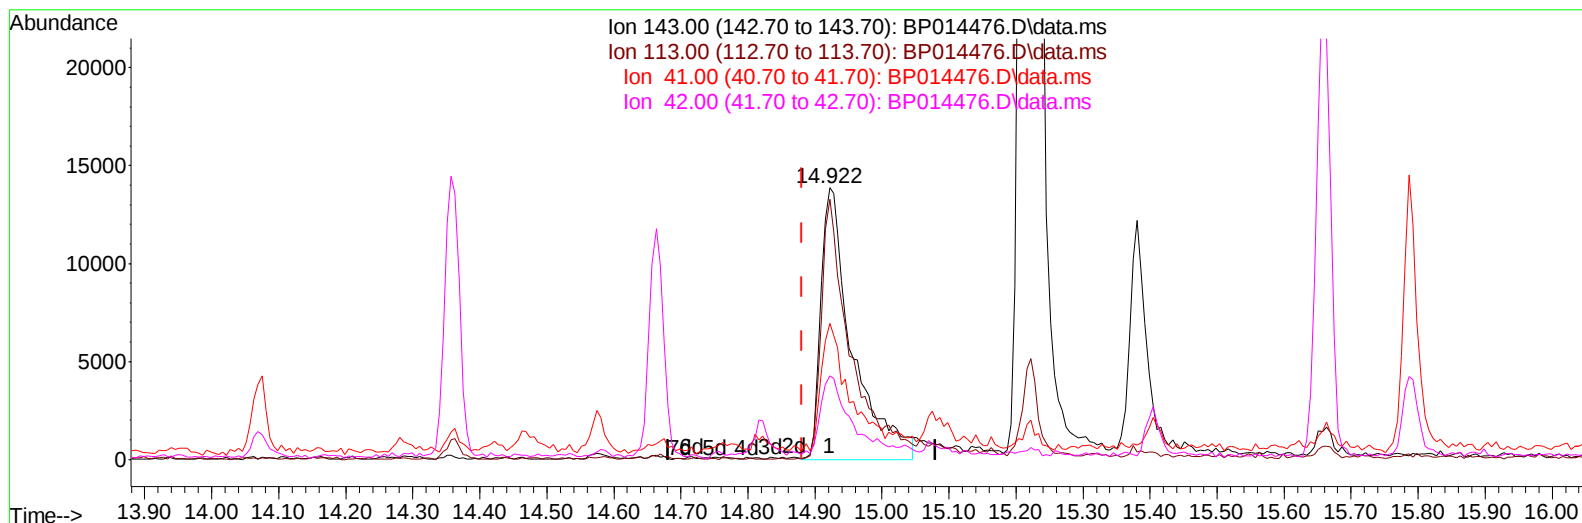

TIC: BP014476.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.922min (+ 0.041) 7.33 ng/ul m

response 45073

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	96.80	95.78
41.00	44.20	50.14
42.00	31.50	30.89

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014476.D
 Acq On : 01 Apr 2023 09:59
 Operator : CG/JU
 Sample : 02158-02
 Misc :
 ALS Vial : 86 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PMW-7D(20230329)

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/03/2023
 Supervised By :Jagrut Upadhyay 04/03/2023

Quant Time: Apr 03 00:44:28 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 31 04:41:29 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.011	152	157429	20.000	ng/ul	0.00
20) Naphthalene-d8	10.834	136	716083	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.663	164	502116	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.428	188	1113543	20.000	ng/ul	0.00
79) Chrysene-d12	21.516	240	871540	20.000	ng/ul	0.00
88) Perylene-d12	24.033	264	798406	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	19065	4.696	ng/uL	0.00
4) Pyridine-d5	3.828	84	70591	6.785	ng/ul	0.01
7) Phenol-d5	7.181	99	136796	9.422	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	344192	36.949	ng/ul	0.00
11) 2-Chlorophenol-d4	7.540	132	324684	30.941	ng/ul	0.00
15) 4-Methylphenol-d8	8.734	113	248648	21.231	ng/ul	0.00
21) Nitrobenzene-d5	9.187	128	209278	36.202	ng/ul	0.00
24) 2-Nitrophenol-d4	9.916	143	240792	36.376	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	416276	34.531	ng/ul	0.00
31) 4-Chloroaniline-d4	10.981	131	382730	24.102	ng/ul	0.00
46) Dimethylphthalate-d6	14.075	166	1528779	37.551	ng/ul	0.00
49) Acenaphthylene-d8	14.357	160	1656695	36.673	ng/ul	0.00
54) 4-Nitrophenol-d4	14.922	143	45073m	7.328	ng/ul	0.04
60) Fluorene-d10	15.663	176	1277705	37.634	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.787	200	225859	27.565	ng/ul	0.00
73) Anthracene-d10	17.528	188	2071932	38.447	ng/ul	0.00
81) Pyrene-d10	19.757	212	2331799	39.832	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.869	264	1669242	39.351	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014476.D
Acq On : 01 Apr 2023 09:59
Operator : CG/JU
Sample : 02158-02
Misc :
ALS Vial : 86 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PMW-7D(20230329)

Manual IntegrationsAPPROVED

Quant Time: Apr 03 00:44:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 31 04:41:29 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/03/2023
Supervised By :Jagrut Upadhyay 04/03/2023

