

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
 Data File : BP014399.D
 Acq On : 30 Mar 2023 13:38
 Operator : CG/JU
 Sample : 02092-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB984

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 03/31/2023
 Supervised By : Jagrut Upadhyay 03/31/2023

Quant Time: Mar 30 22:40:11 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 30 12:32:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.016	152	151617	20.000	ng/u1	0.00
20) Naphthalene-d8	10.839	136	647021	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.669	164	431087	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.433	188	954444	20.000	ng/u1	0.00
79) Chrysene-d12	21.521	240	768553	20.000	ng/u1	0.00
88) Perylene-d12	24.039	264	723095	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.387	96	18220	4.660	ng/uL	0.00
4) Pyridine-d5	3.857	84	24255m	2.421	ng/u1	0.04
7) Phenol-d5	7.181	99	82101	5.872	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.340	67	287314	32.025	ng/u1	0.00
11) 2-Chlorophenol-d4	7.545	132	241203	23.866	ng/u1	0.00
15) 4-Methylphenol-d8	8.734	113	164703	14.603	ng/u1	0.00
21) Nitrobenzene-d5	9.192	128	165681	31.720	ng/u1	0.00
24) 2-Nitrophenol-d4	9.922	143	185978	31.095	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.463	165	302579	27.778	ng/u1	0.00
31) 4-Chloroaniline-d4	10.998	131	66781m	4.654	ng/u1	0.01
46) Dimethylphthalate-d6	14.075	166	1132323	32.395	ng/u1	0.00
49) Acenaphthylene-d8	14.363	160	1222451	31.519	ng/u1	0.00
54) 4-Nitrophenol-d4	14.922	143	24238m	4.590	ng/u1	0.04
60) Fluorene-d10	15.669	176	960695	32.959	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.792	200	189218	26.943	ng/u1	0.00
73) Anthracene-d10	17.533	188	1552230	33.605	ng/u1	0.00
81) Pyrene-d10	19.762	212	1763443	34.160	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.880	264	1328668	34.585	ng/u1	0.00
Target Compounds					Qvalue	
59) Diethylphthalate	15.486	149	516576	14.874	ng/u1	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP033023\
Data File : BP014399.D
Acq On : 30 Mar 2023 13:38
Operator : CG/JU
Sample : 02092-16
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
CB984

Quant Time: Mar 30 22:40:11 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032823.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 30 12:32:14 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By : Christian Giraldo 03/31/2023
Supervised By : Jagrut Upadhyay 03/31/2023

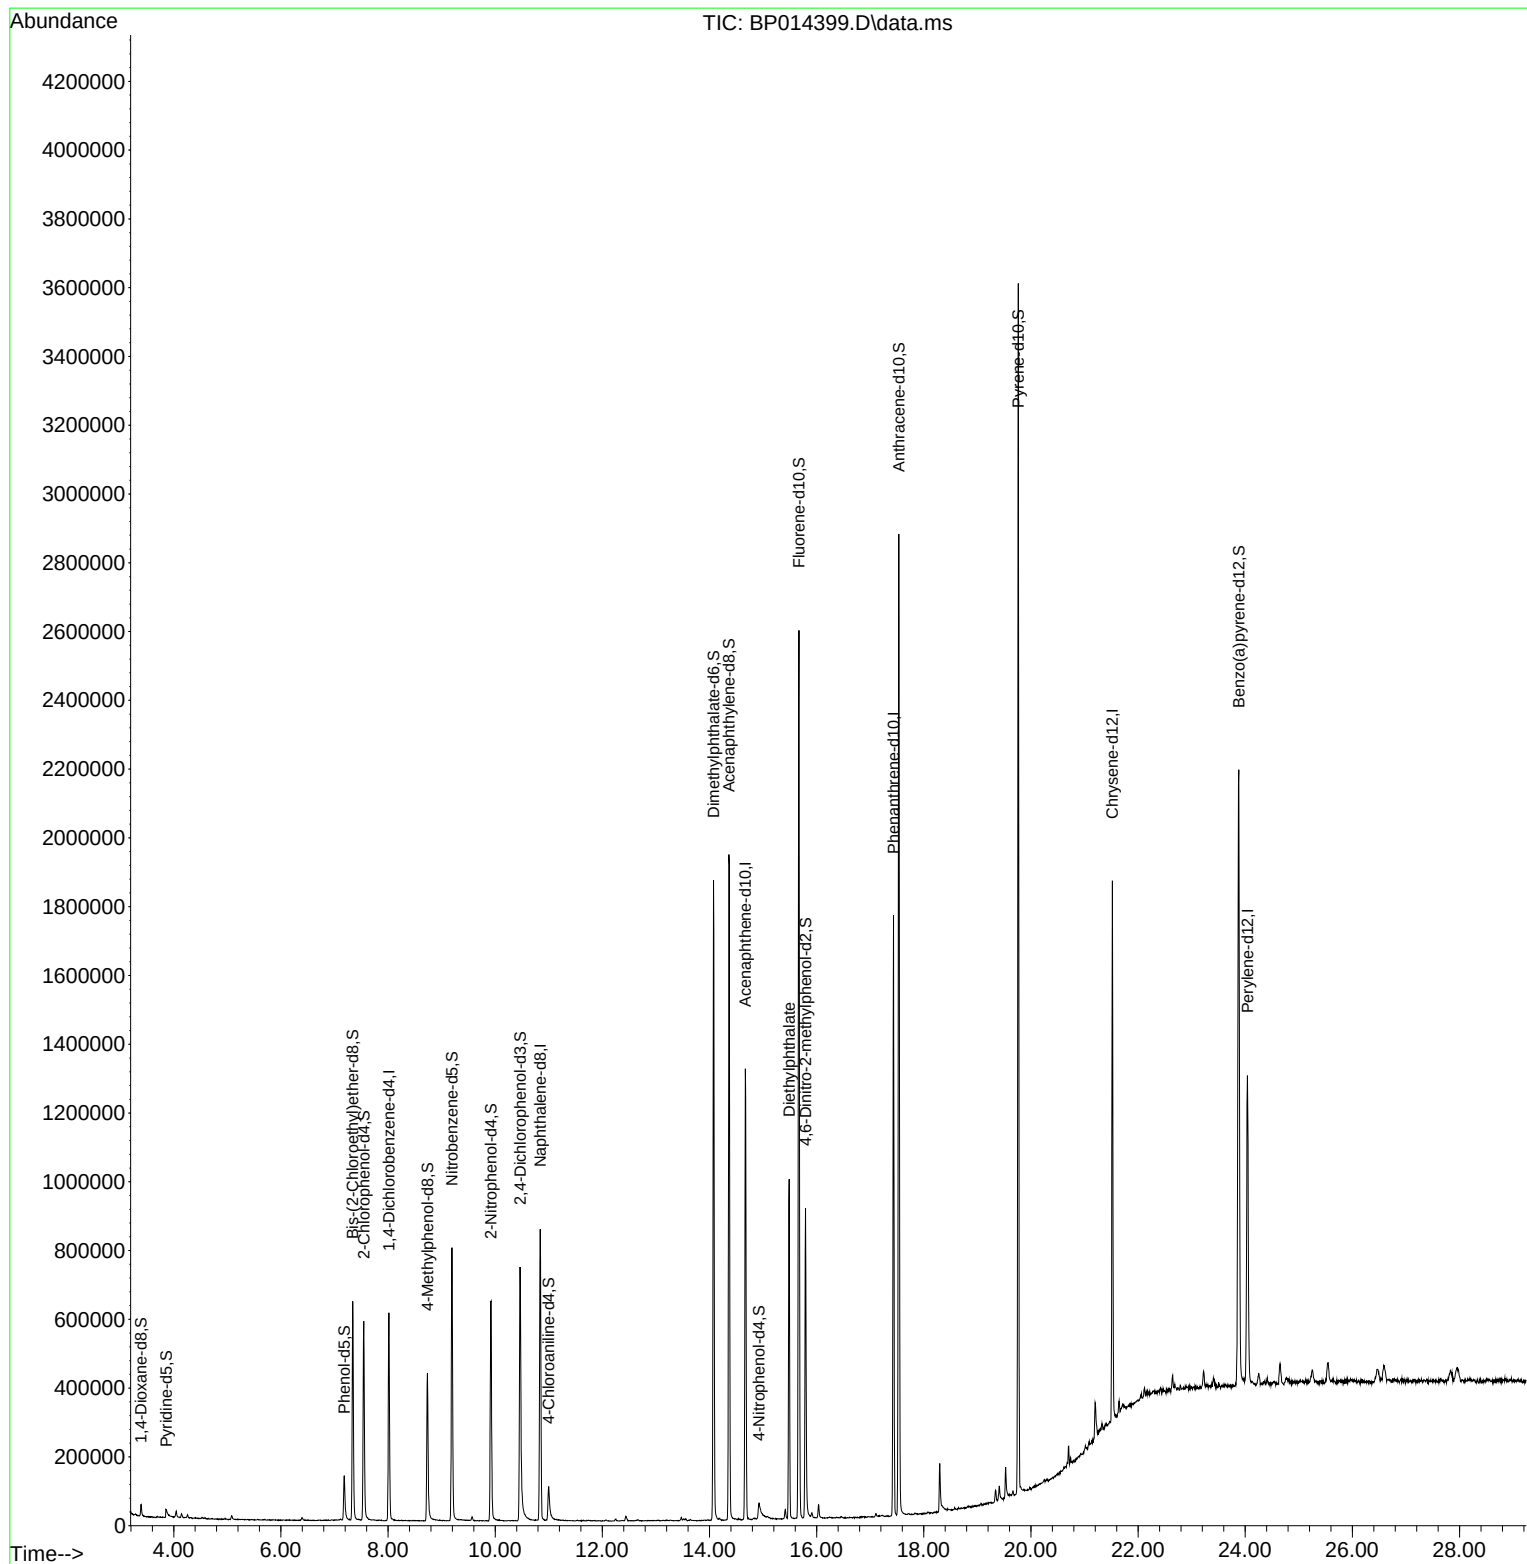

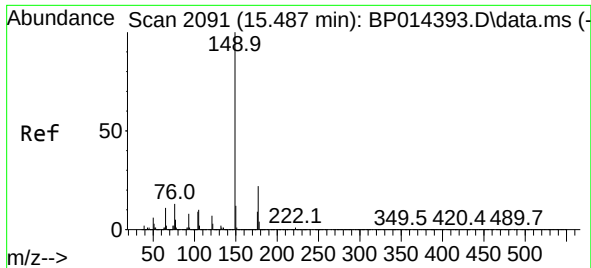

#59
 Diethylphthalate
 Concen: 14.874 ng/ul
 RT: 15.486 min Scan# 2091
 Delta R.T. -0.000 min
 Lab File: BP014399.D
 Acq: 30 Mar 2023 13:38

Instrument :
 BNA_P
 ClientSampleId :
 CB984

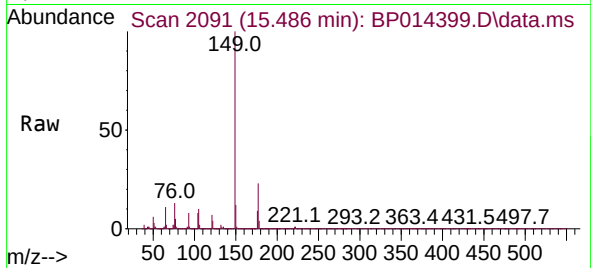

Tgt Ion:149 Resp: 516576
 Ion Ratio Lower Upper
 149 100
 177 22.7 18.2 27.2
 150 12.1 9.8 14.8

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 03/31/2023
 Supervised By :Jagrut Upadhyay 03/31/2023

